3875 Cypress Drive Petaluma, CA 94954 800.228.2555 707.773.1100 Fax 707.773.1180 www.gcx.com INSTRUMENT MOUNTING SYSTEM

# Installation Guide

Cable Management Hook Assembly for Vertically Mounted

Philips Flexible Module Server (FMS)

The purpose of this guide is to describe attachment of Hook Assembly.

### **Parts Reference**

The following parts and hardware are included in this installation kit (hardware not shown)


Item #	Description	Qty
1	Hook Assembly, Cable Management	1
2	M4 x 14 mm Pan Head Machine Screw (PHMS)	2
3	M4 x 12 mm PHMS	2

Tools required: Phillips screwdriver (not provided).

### Attaching Hook Assembly to FMS


The Hook Assembly is installed between the FMS and mounting clamp as shown below and on page 2.


## Attachment of Hook Assembly using Philips Clamp

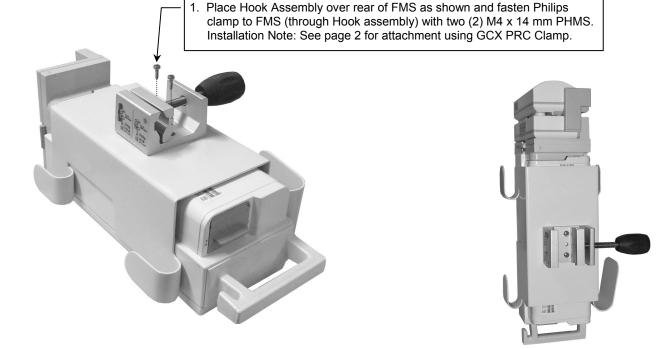







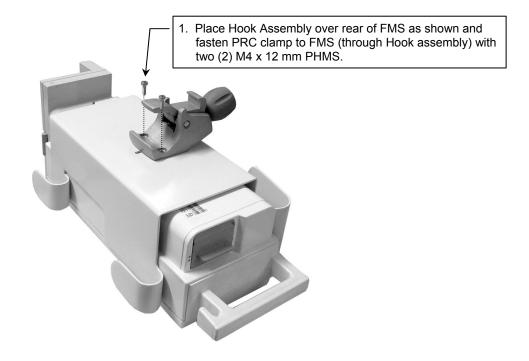

#### **Periodic Maintenance**

All fasteners associated with the mounting system should be inspected periodically and tightened or adjusted as necessary for optimal operation and safety.

#### **Cleaning the Mounting Assembly**

**CAUTION:** GCX makes no claims regarding the efficacy of the listed chemicals or processes as a means for controlling infection. Consult your hospital's infection control officer or epidemiologist. To clean or sterilize mounted devices or accessory equipment, refer to the specific instructions delivered with those products.

- 1. The mounting assembly may be cleaned with most mild, non-abrasive solutions commonly used in the hospital environment (e.g. diluted bleach, ammonia, or alcohol solutions).
- 2. The surface finish will be permanently damaged by strong chemicals and solvents such as acetone or trichloroethylene.
- 3. Steel wool or other abrasive material should never be used.
- 4. Damage caused by the use of unapproved substances or processes will not be warranted. We recommend testing of any cleaning solution on a small area of the arm that is not visible to verify compatibility.
- 5. Never submerge or allow liquids to enter the arm. Wipe any cleaning agents off the arm immediately using a waterdampened cloth. Dry mounting assembly thoroughly after cleaning.