

PHILIPS

OmniWire

Pressure guide wire



Solid core. No compromise.



Introducing Philips OmniWire,
the world's first solid core pressure wire¹

With an all new workhorse design, only OmniWire combines confidence in wire performance with proven iFR outcomes and iFR Co-registration, making it easy to benefit from physiology throughout the case.^{2,3,4}

Built like a contemporary workhorse guide wire


New design from tip-to-tail to improve navigation in complex anatomy

- New Nitinol distal core provides increased durability and shape recovery: ideal for use in multi-vessel disease and complex cases.
- Unique solid core for improved torque, pushability and kink resistance.
- Durable, integrated conductive bands for confidence during device delivery, reconnections and post-measurements.


More core. Less hypotube.

Until now, all pressure wires used a hollow hypotube to house electrical leads or optical fibers that carry the pressure signals. OmniWire uses a solid construction with conductive ribbons embedded in its outer layer. This innovation makes a larger solid core possible, similar to the design of your workhorse wire for improved durability, torque response and pushability, with a reduced risk of kinking.⁴


Traditional pressure wire

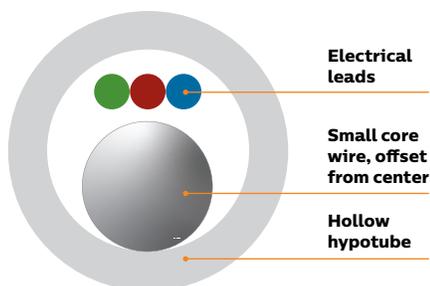

OmniWire with solid core

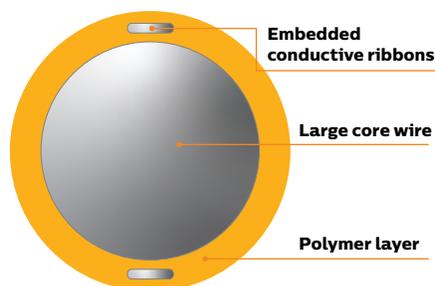


Workhorse guide wire*

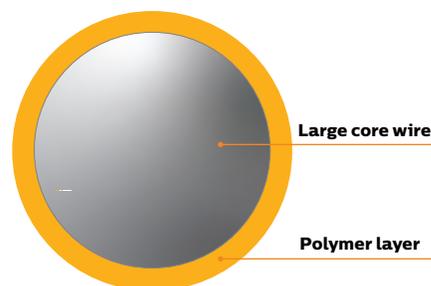

Order information

- 89185 OmniWire pressure guide wire, 185 cm, straight tip
- 89185J OmniWire pressure guide wire, 185 cm, j-tip

Technical specifications

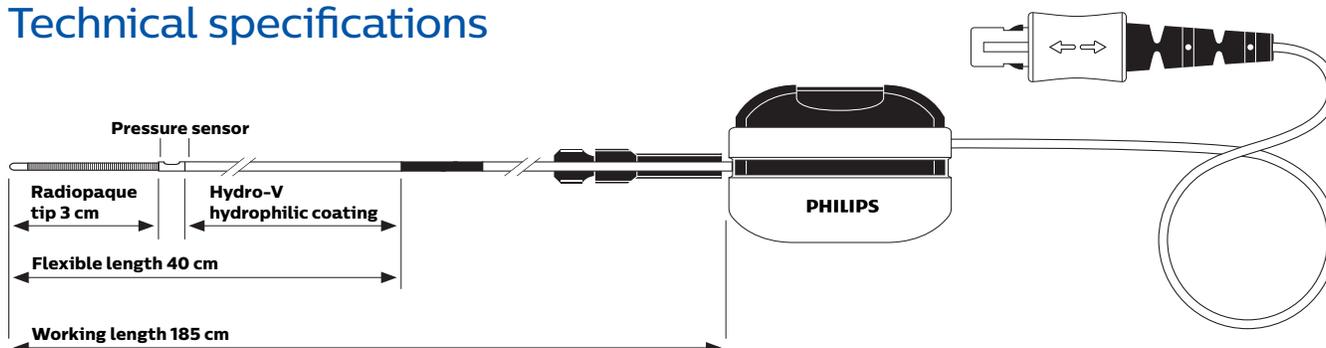

Learn more at www.philips.com/OmniWire

* Proximal cross-section. Not to scale, for illustration purposes only.

1. Data on file.
2. Davies JE, et al., Use of the Instantaneous Wave-free Ratio or Fractional Flow Reserve in PCI. N Engl J Med. 2017 May 11;376(19):1824-1834.
3. Gotberg M, et al., iFR-SWEDEHEART Investigators. Instantaneous Wave-free Ratio versus Fractional Flow Reserve to Guide PCI. N Engl J Med. 2017 May 11;376(19):1813-1823.
4. Comparisons to Verrata Plus. Data/report internally on file or internal company's data on file. Verification Report, D000410086/A

