

Magnetic Resonance

PHILIPS

Maintaining a clean environment for your patients

Before you begin



Cleaning and disinfecting

Clean and disinfect all patient contact points.






Always detach the coil before cleaning and disinfection.








Always use a cloth to apply cleaning and disinfection solution.

Always dry the coil and accessory after cleaning and disinfection.

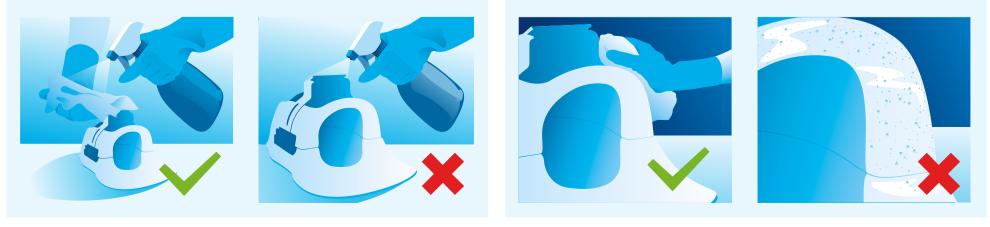

Find the right MRI coil for your system: www.philips.com/mrcoils

© 2024 Koninklijke Philips N.V. 4522 991 63691 * JUL 2024