

---

# DICOM

## Conformance Statement

ClearVue 350/550/650/850 3.1

000375000000073 Rev C

2015-06-08



---

© Koninklijke Philips Electronics N.V. 2014  
All rights are reserved.

**PHILIPS**

## 0.1 REVISION HISTORY

Document Version	Date of Issue	Author	Description
C	06-08-2015	Rupam Sarkar	Updated as per Opal R2 DCR
B	05-20-2015	Rupam Sarkar	Updated as per Opal R2 FRDR
A	03-23-2015	Rupam Sarkar	Initial Release

# 1 TABLE OF CONTENTS

0.1	REVISION HISTORY .....	2
1	TABLE OF CONTENTS .....	3
2	CONFORMANCE STATEMENT OVERVIEW .....	7
* Purchasable option. ....		8
3	INTRODUCTION.....	9
3.1	AUDIENCE .....	9
3.2	REMARKS .....	10
3.3	IMPORTANT NOTE TO THE READER .....	10
3.4	DEFINITIONS, TERMS AND ABBREVIATIONS.....	<b>ERROR! BOOKMARK NOT DEFINED.</b>
3.5	REFERENCES .....	<b>ERROR! BOOKMARK NOT DEFINED.</b>
4	NETWORKING .....	12
4.1	IMPLEMENTATION MODEL .....	12
4.1.1	Application Data Flow .....	12
4.1.2	Functional Definition of AEs.....	14
4.1.2.1	Functional Definition of Storage Application Entity .....	14
4.1.2.2	Functional Definition of Workflow Application Entity .....	14
4.1.2.3	Functional Definition of Hardcopy Application Entity .....	15
	Sequencing of Real-World Activities .....	16
4.2	AE SPECIFICATIONS .....	18
4.2.1	Storage Application Entity Specification .....	18
4.2.1.1	SOP Classes .....	18
4.2.1.2	Association Establishment Policy.....	18
4.2.1.2.1	General.....	18
4.2.1.2.2	Number of Associations .....	18
4.2.1.2.3	Asynchronous Nature.....	19
4.2.1.2.4	Implementation Identifying Information .....	19
4.2.1.3	Association Initiation Policy.....	19
4.2.1.3.1	Activity – Store Images, Loops and Structured Reports .....	19
4.2.1.3.1.1	Description and Sequencing of Activities .....	19
4.2.1.3.1.2	Proposed Presentation Contexts .....	21
4.2.1.3.1.3	SOP Specific Conformance for Image and Comprehensive Structured Report Storage SOP Classes .....	22
4.2.1.3.1.4	SOP Specific Conformance for Storage Commitment Push Model SOP Class 24	24
4.2.1.3.1.4.1	Storage Commitment Operations (N-ACTION).....	24
4.2.1.3.1.4.2	Storage Commitment Tags (N-ACTION) .....	24
4.2.1.3.1.4.3	Storage Commitment Notifications (N-EVENT-REPORT).....	25
4.2.1.3.1.4.4	Storage Commitment Tags (N-EVENT-REPORT).....	25
4.2.1.4	Association Acceptance Policy .....	26
4.2.1.4.1	Activity – Receive Storage Commitment Response .....	26
4.2.1.4.1.1	Description and Sequencing of Activities .....	26
4.2.1.4.1.2	Accepted Presentation Contexts.....	26
4.2.1.4.1.3	SOP Specific Conformance for Storage Commitment Push Model SOP Class 27	27
4.2.1.4.1.3.1	Storage Commitment Notifications (N-EVENT-REPORT).....	27
4.2.2	Workflow Application Entity Specification .....	28
4.2.2.1	SOP Classes .....	28
4.2.2.2	Association Establishment Policy.....	28

4.2.2.2.1	General.....	28
4.2.2.2.2	Number of Associations .....	28
4.2.2.2.3	Asynchronous Nature.....	28
4.2.2.2.4	Implementation Identifying Information .....	28
4.2.2.3	Association Initiation Policy.....	29
4.2.2.3.1	Activity – Worklist Update .....	29
4.2.2.3.1.1	Description and Sequencing of Activities.....	29
4.2.2.3.1.2	Proposed Presentation Contexts .....	30
4.2.2.3.1.3	SOP Specific Conformance for Modality Worklist.....	30
4.2.2.3.2	Activity –Acquire Images.....	34
4.2.2.3.2.1	Description and Sequencing of Activities.....	34
4.2.2.3.2.2	Proposed Presentation Contexts .....	35
4.2.2.3.2.3	SOP Specific Conformance for MPPS.....	36
4.2.2.4	Association Acceptance Policy .....	40
4.2.3	Hardcopy Application Entity Specification .....	41
4.2.3.1	SOP Classes .....	41
4.2.3.2	Association Establishment Policy.....	41
4.2.3.2.1	General.....	41
4.2.3.2.2	Number of Associations .....	41
4.2.3.2.3	Asynchronous Nature.....	42
4.2.3.2.4	Implementation Identifying Information .....	42
4.2.3.3	Association Initiation Policy.....	42
4.2.3.3.1	Activity – Film Images .....	42
4.2.3.3.1.1	Description and Sequencing of Activities.....	42
4.2.3.3.1.2	Proposed Presentation Contexts .....	44
4.2.3.3.1.3	Common SOP Specific Conformance for all Print SOP Classes..	44
4.2.3.3.1.4	SOP Specific Conformance for the Printer SOP Class.....	44
4.2.3.3.1.4.1	Printer SOP Class Operations (N-GET).....	44
4.2.3.3.1.4.2	Printer SOP Class Notifications (N-EVENT-REPORT)....	45
4.2.3.3.1.5	SOP Specific Conformance for the Film Session SOP Class.....	46
4.2.3.3.1.5.1	Film Session SOP Class Operations (N-CREATE) .....	46
4.2.3.3.1.5.2	Film Session SOP Class Operations (N-DELETE) .....	47
4.2.3.3.1.6	SOP Specific Conformance for the Film Box SOP Class .....	47
4.2.3.3.1.6.1	Film Box SOP Class Operations (N-CREATE) .....	47
4.2.3.3.1.6.2	Film Box SOP Class Operations (N-ACTION) .....	48
4.2.3.3.1.7	SOP Specific Conformance for the Image Box SOP Class .....	49
4.2.3.3.1.7.1	Basic Grayscale Image Box SOP Class Operations (N-SET)	
4.2.3.3.1.7.2	Basic Color Image Box SOP Class Operations (N-SET)	50
4.2.3.4	Association Acceptance Policy .....	51
4.2.4	Verification Application Entity specification.....	51
4.2.4.1	SOP Class.....	51
4.2.4.2	Association Establishment Policy.....	51
4.2.4.2.1	General.....	51
4.2.4.2.2	Number of Associations .....	52
4.2.4.2.3	Asynchronous Nature.....	52
4.2.4.2.4	Implementation Identifying Information .....	52
4.2.4.3	Association Initiation Policy.....	52
4.2.4.3.1	Activity – Verify as SCU and SCP.....	52
4.2.4.3.2	Description and Sequencing of Activities.....	52
4.2.4.3.3	Proposed Presentation Contexts .....	55
4.2.4.3.4	SOP Specific Conformance for Verification .....	55
4.2.4.3.4.1	Verification SOP Class Operations (C-ECHO) .....	55
4.2.4.3.5	Association Acceptance Policy .....	55

4.2.4.3.5.1	Verification SOP Class Notifications .....	55	
4.3	PHYSICAL NETWORK INTERFACES.....	56	
4.3.1	Supported Communication Stacks .....	56	
4.3.1.1	TCP/IP Stack.....	56	
4.3.2	Physical Network Interface .....	56	
4.4	CONFIGURATION.....	56	
	AE Title/Presentation Address Mapping.....	56	
	4.4.1.1	Local AE Title .....	57
	4.4.1.2	Remote AE Title/Presentation Address Mapping.....	57
	4.4.1.2.2	Workflow .....	57
	4.4.1.2.3	Hardcopy.....	58
5	MEDIA STORAGE .....	59	
5.1	IMPLEMENTATION MODEL .....	59	
5.1.1	Application Data Flow .....	59	
5.1.2	Functional Definition of AEs.....	59	
5.1.2.1	Functional Definition of Media Application Entity .....	59	
5.1.3	Sequencing of Real-World Activities.....	59	
5.1.4	File Meta Information Options.....	59	
5.2	AE SPECIFICATIONS .....	60	
5.2.1	Media Application Entity Specification .....	60	
	Reading a DICOM study from removable media.....	60	
	5.2.1.1	File Meta Information for the Application Entity .....	61
	5.2.1.2	Real-World Activities .....	61
	5.2.1.2.1	Activity – Send to Media – “Export” .....	61
	5.2.1.2.2	Activity – Import from Media – “Import” .....	61
	5.2.1.2.3	Activity – Update to Media – Export” .....	61
	5.2.1.2.3.1	Media Storage Application Profiles .....	61
	5.2.1.2.3.2	Options .....	61
	Directory Information Module.....	62	
	Patient Directory Record.....	62	
	Study Directory Record .....	62	
	Series Directory Record .....	62	
	Image Directory Record .....	63	
	SR Document Directory Record .....	63	
6	SUPPORT OF CHARACTER SETS .....	64	
6.1	SUPPORT FOR RUSSIAN MARKETS .....	65	
6.2	SUPPORT FOR CHINESE MARKETS .....	65	
7	SECURITY .....	65	
8	ANNEXES .....	66	
8.1	CREATED IOD INSTANCES.....	66	
8.1.1	US or US Multiframe Image IOD.....	66	
8.1.2	Comprehensive Structured Report IOD .....	67	
8.1.3	Common Modules .....	67	
8.1.4	US or Multiframe Image Modules .....	73	
8.1.5	Comprehensive Structured Report Modules.....	81	
8.2	USED FIELDS IN RECEIVED IOD BY APPLICATION .....	83	
8.3	ATTRIBUTE MAPPING .....	83	
8.4	COERCED/MODIFIED FIELDS.....	85	
8.5	CONTROLLED TERMINOLOGY.....	85	
8.6	GRAYSCALE IMAGE CONSISTENCY .....	85	

8.7	EXTENSIONS / SPECIALIZATIONS / PRIVATIZATIONS .....	85
8.7.1	Standard Extended / Specialized / Private SOPs .....	85
8.7.2	2D.....	85
8.7.4	PRIVATE TRANSFER SYNTAXES.....	86
APPENDIX A – Structured Reports.....		87
A.1	STRUCTURED REPORTS.....	87
A.2	OB – GYN STRUCTURED REPORT TEMPLATE.....	87
A.2.1	Template specific conformance for TID 5000 .....	87
A.2.1.1	OB-GYN Patient Characteristics (TID 5001).....	89
A.2.1.2	OB-GYN Procedure Summary (TID 5002).....	90
A.2.1.2.1	OB-GYN Fetus Summary (TID 5003) .....	90
A.2.1.3	Fetal Biometry Ratio Section (TID 5004) .....	92
A.2.1.3.1	Fetal Biometry Ratios (CID 12004) .....	93
A.2.1.4	Fetal Biometry Section (TID 5005).....	93
A.2.1.4.1	Fetal Biometry Measurements (CID 12005) .....	93
A.2.1.5	Fetal Long Bones Section (TID 5006).....	94
A.2.1.6	Fetal Cranium Section (TID 5007) .....	95
A.2.1.6.1	Fetal Biometry Group (TID 5008).....	95
A.2.1.7	Fetal Biophysical Profile Section (TID5009) .....	96
A.2.1.8	Early Gestation Section (TID 5011) .....	97
A.2.1.9	Amniotic Sac Section (TID 5010) .....	97
A.2.1.10	Pelvis and Uterus Section (TID 5015).....	98
A.2.1.10.1	CID 12011 Ultrasound Pelvis And Uterus.....	101
A.2.1.11	Ovaries Section (TID 5012).....	102
A.2.1.12	Follicles Section (TID 5013) .....	103
A.2.1.13	OB-GYN Fetus Vascular Ultrasound Measurement Group (TID 5025) .....	104
A.2.1.13.1	Fetal Vascular Measurements .....	104
A.2.1.14	OB-GYN Pelvic Vascular Ultrasound Measurement Group (TID 5026) .....	108
A.2.1.14.1	Pelvic Vascular Measurements.....	109
A.2.1.15	Gestation Age Equations & Tables (CID 12013) .....	111
A.2.1.15.1	Gestational Age Equations and Tables Not Exported in DICOM SR .....	113
A.2.1.16	OB Fetal Body Weight Equations & Tables .....	113
A.3	VASCULAR ULTRASOUND STRUCTURED REPORT TEMPLATE .....	114
A.3.1	Template specific conformance for TID 5100 .....	114
A.3.2	TID 5100 Vascular Ultrasound Report.....	114
A.3.3	Vascular Patient Characteristics (TID 5101).....	117
A.3.4	Vascular Procedure Summary (TID 5102).....	118
A.3.5	eDCS – Vascular Template Support.....	118
A.3.5.1	eDCS Table.....	119
A.4	ADULT ECHOCARDIOGRAPHY STRUCTURED REPORT TEMPLATE .....	168
A.4.1	Template specific conformance for TID 5200 .....	168
A.4.2	Echocardiography Patient Characteristics (TID 5201) .....	169
A.4.3	Echo Procedure Summary Section (TID 5200-03) .....	170
A.4.4	Echo Section (TID 5202).....	170
A.4.5	Echo Measurement (TID 5203).....	171
A.4.6	Hepatic Veins (T-48720) .....	172
A.4.7	eDCS – Adult Echocardiography Template Support .....	174
A.4.7.1	eDCS Table.....	174
A.4.8	Cardiac (Adult Echo) Meas/Calcs NOT exported in Dicom .....	206
A.4.9	Units Codes.....	209
A.5	PEDIATRIC ECHOCARDIOGRAPHY STRUCTURED REPORT TEMPLATE .....	210

A.5.1	Template specific conformance for TID 5220 .....	210
A.5.1.1	Cardiovascular Patient Characteristics (TID 3606).....	211
A.5.1.2	Cardiac Ultrasound Pediatric Echo Measurement Section (TID 5221).....	214
A.5.1.3	Pediatric, Fetal and Congenital Cardiac Ultrasound Section (TID 5222).....	215
A.5.1.4	Pediatric, Fetal and Congenital Cardiac Ultrasound Measurement (TID 5223)...	215
A.5.1.5	Cardiac Ultrasound Fetal Characteristics (TID 5225) .....	216
A.5.1.6	Cardiac Ultrasound Summary Section (TID 5226).....	216
A.5.1.7	Cardiac Ultrasound FetalSummary Section (TID 5227).....	217
A.5.1.8	Cardiac Ultrasound Fetal Measurement Section (TID 5228) .....	217
A 5.2	eDCS – Pediatric Echocardiography Template Support.....	217
A 5.2.1	eDCS Table.....	218
A.5.3	Pediatric Echo Meas/Calcs NOT exported in Dicom .....	276
APPENDIX B	– BULK PRIVATE TAGS .....	277
B.1	BULK PRIVATE TAGS .....	277
APPENDIX C	– Generic Angle Measurements .....	278
C.1	GENERIC ANGLE MEASUREMENTS.....	278

## **2 CONFORMANCE STATEMENT OVERVIEW**

The Philips ClearVue 350/550/650/850 3.1 Ultrasound systems implement the necessary DICOM® services to download worklists from an information system, save acquired US Images and Structured Reports to a network

---

<sup>®</sup> DICOM is the registered trademark of the National Electrical Manufacturers Association for its standards publications relating to digital communications of medical information.

storage device, CD/DVD or USB, print to a networked hardcopy device and inform the information system about the work actually done.

NOTE: This DICOM Conformance Statement applies to ClearVue 350 3.1, ClearVue 550 3.1, ClearVue 650 3.1 and ClearVue 850 3.1 systems unless a note is present describing any different behavior or support.

Table 1 provides an overview of the supported network services.

**Table 1  
NETWORK SERVICES**

Networking SOP Classes	User of Service (SCU)	Provider of Service (SCP)
<b>Transfer</b>		
Ultrasound Image Storage	Yes*	No
Ultrasound Multiframe Image Storage	Yes*	No
Storage Commitment Push Model	Yes*	No
Comprehensive SR	Yes*	No
<b>Workflow Management</b>		
Modality Worklist	Yes*	No
Modality Performed Procedure Step	Yes*	No
<b>Print Management</b>		
Basic Grayscale Print Management	Yes*	No
Basic Color Print Management	Yes*	No

\* Purchasable option.

Table 2 below specifies the Media Storage Application Profiles supported.

**Table 2  
MEDIA SERVICES**

Media Storage Application Profile	Write Files (FSC or FSU)	Read Files (FSR)
<b>Compact Disk – Recordable</b>		
STD-US-SC-MF <sup>(1)</sup> -CD-R	Yes / Yes <sup>(2)</sup>	Yes <sup>(3)</sup>

for Ultrasound images, compressed and uncompressed		
STD-GEN-CD for Structured Reports	Yes / Yes <sup>(2)</sup>	No
<b>DVD</b>		
STD-US-SC-MF <sup>(1)</sup> -DVD for Ultrasound images, compressed and uncompressed	Yes / Yes <sup>(2)</sup>	Yes <sup>(3)</sup>
STD-GEN-DVD for Structured Reports	Yes / Yes <sup>(2)</sup>	No
<b>USB Devices</b>		
STD-GEN-USB-JPEG for Ultrasound images, compressed and uncompressed and Structured Reports	Yes / Yes	Yes <sup>(4)</sup>

(1) Note that the "MF" designator includes both Single Frame (SF) and Multi-frame (MF) ultrasound images.

(2) Only acts as a FSU for media that may be written to multiple times.

(3) Philips ClearVue 650 3.1 reads and imports data from Philips ClearVue 650 3.0 and ClearVue 650 1.0 system. Philips ClearVue 350 3.1 reads and imports data from ClearVue 350 3.0, ClearVue 350 2.0 and ClearVue 350 1.0. Philips ClearVue 550 3.1 reads and imports data from ClearVue 550 1.0, ClearVue 550 2.0 and ClearVue 550 3.0.

(4) Yes, but not for importing Structured Reports.

**Table 3**  
**SUPPORTED STRUCTURED REPORT TEMPLATES**

Concept Name
OB-GYN Ultrasound Procedure Report (Template ID 5000)
Vascular Ultrasound Procedure Report (Template ID 5100)
Adult Echocardiography Procedure Report (Template ID 5200)
Pediatric Echocardiography Procedure Reports (Template ID 5220)

## 3 INTRODUCTION

### 3.1 AUDIENCE

This document is intended for hospital staff, health care system integrators, software designers or implementers. It is assumed that the reader has a working understanding of DICOM.

### **3.2 REMARKS**

DICOM, by itself, does not guarantee interoperability. However, the Conformance Statement facilitates a first-level validation for interoperability between different applications supporting the same DICOM functionality.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.

The scope of this Conformance Statement is to facilitate communication between the Philips Healthcare ClearVue 350/550/650/850 3.1 ultrasound systems and other vendors' Medical equipment. The Conformance Statement should be read and understood in conjunction with the DICOM Standard [DICOM]. However, by itself it is not guaranteed to ensure the desired interoperability and successful interconnectivity.

The user should be aware of the following important issues:

- The comparison of different conformance statements is the first step towards assessing interconnectivity between Philips Healthcare and non - Philips Healthcare equipment.
- Test procedures should be defined to validate the desired level of connectivity.
- The DICOM standard will evolve to meet the users' future requirements. Philips Healthcare is actively involved in developing the standard further and therefore reserves the right to make changes to its products or to discontinue its delivery.

### **3.3 IMPORTANT NOTE TO THE READER**

#### **Interoperability**

Interoperability refers to the ability of application functions, distributed over two or more systems, to work successfully together. The integration of medical devices into an IT environment may require application functions that are not specified within the scope of DICOM. Consequently, using only the information provided by this Conformance Statement does not guarantee interoperability of Philips equipment with non-Philips equipment. It is the user's responsibility to analyze thoroughly the application requirements and to specify a solution that integrates Philips equipment with non-Philips equipment.

#### **Validation**

Philips equipment has been carefully tested to assure that the actual implementation of the DICOM interface corresponds with this Conformance Statement. Where Philips equipment is linked to non-Philips equipment, the first step is to compare the relevant Conformance Statements. If the Conformance Statements indicate that successful information exchange should be possible, additional validation tests will be necessary to ensure the functionality, performance, accuracy and stability of image and image related data. It is the responsibility of the user (or user's agent) to specify the appropriate test suite and to carry out the additional validation tests.

#### **New versions of the DICOM Standard**

The DICOM Standard will evolve in future to meet the user's growing requirements and to incorporate new features and technologies. Philips is actively involved in this evolution and plans to adapt its equipment to future versions of the DICOM Standard. In order to do so, Philips reserves the right to make changes to its products or to discontinue its delivery. The user should ensure that any non-Philips provider linking to Philips equipment also adapts to future versions of the DICOM Standard. If not, the incorporation of DICOM enhancements into Philips equipment may lead to loss of connectivity (in case of networking) and incompatibility (in case of media).

### **3.4 DEFINITIONS, TERMS AND ABBREVIATIONS**

Definitions, terms and abbreviations used in this document are defined within the different parts of the DICOM standard.

Abbreviations and terms are as follows:

AE	DICOM Application Entity
AET	Application Entity Title
CD-R	Compact Disk Recordable
DICOM	Digital Imaging and Communications in Medicine
FSC	File-Set Creator
FSU	File-Set Updater
FSR	File-Set Reader
GSDF	Grayscale Standard Display Function
IOD	(DICOM) Information Object Definition
ISO	International Standard Organization
LOINC	Logical Observation Identifiers Names and Codes
MPPS	Modality Performed Procedure Step
MWL	Modality Worklist
R	Required Key Attribute for Modality Worklist Query Matching
O	Optional Key Attribute for Modality Worklist Query Matching
PDU	DICOM Protocol Data Unit
PDE	Patient Data Entry
SCP	DICOM Service Class Provider (DICOM server)
SCU	DICOM Service Class User (DICOM client)
SOP	DICOM Service-Object Pair
SNOMED	Systematized Nomenclature of Medicine (SRT)
U	Unique Key Attribute for Modality Worklist Query Matching, or Optional Attribute
US	Ultrasound

### 3.5 REFERENCES

[DICOM] Digital Imaging and Communications in Medicine (DICOM), NEMA PS 3.1-3.18, 2008

Integrating the Healthcare Enterprise (IHE) Radiology Technical Framework, Vol. 1, Integration Profiles, Revision 8.0 Final Text, August 30, 2007

Integrating the Healthcare Enterprise (IHE) Radiology Technical Framework, Vol. 2, Transactions, Revision 8.0 Final Text, August 30, 2007

Integrating the Healthcare Enterprise (IHE) Radiology Technical Framework, Vol. 3, Transactions (Continued), Revision 8.0 Final Text August 30, 2007

Integrating the Healthcare Enterprise (IHE) Cardiology Technical Framework, Year 2: 2005-2006, Volume 1, Integration Profiles, Revision 2.1, June 9, 2006


Integrating the Healthcare Enterprise (IHE) Cardiology Technical Framework, Year 2: 2005-2006, Volume 2, Transactions, Revision 2.1, June 8, 2006

Integrating the Healthcare Enterprise (IHE) Cardiology Technical Framework, Supplement 2007, Evidence Documents Profile Cardiology Options: Stress Testing CT/MR Angiography, <Trial Implementation Version 0.06>, June 6, 2007

## 4 NETWORKING

### 4.1 IMPLEMENTATION MODEL

#### 4.1.1 Application Data Flow

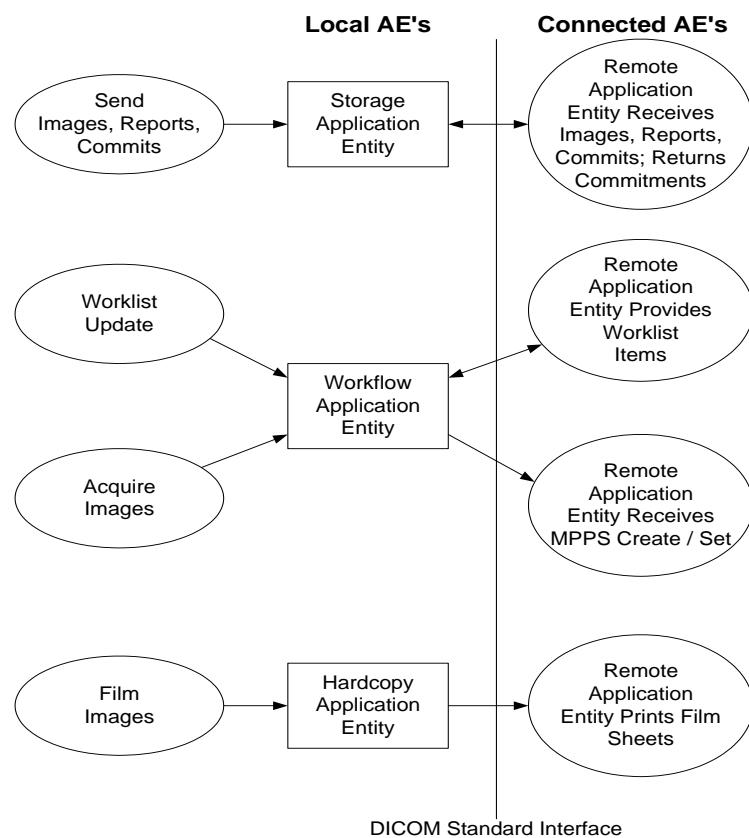

**Figure 1**  
APPLICATION DATA FLOW DIAGRAM

- The **Storage Application Entity** sends **Images** to one or two remote AEs and **Structured Reports** to a single remote AE. Acquisition of images is associated with the local real-world activity “Freeze” then “Acquire” for single frame and “Acquire” for loops or clips. Sending or exporting of images depends on user configuration, either “Send as you go” as and when the image is acquired (or) “Batch” when End Exam is pressed, (or) Manual. An exam may be exported by user selecting from “Review”. A storage commitment server is configured for one of the two image storage servers. Storage Commitment for Structured Reports requires a separate commit server configuration entry. If the remote AE is configured for **Storage Commitment**, the Storage AE will request Storage Commitment after successful storage of the image(s) and Structured Reports, if sent. If a commitment response is successfully obtained, there will be no job remaining in the queue (viewed using CNTL-J) signaling the Auto-delete function that the exam qualifies for deletion.
- The **Workflow Application Entity** receives Worklist information from and sends MPPS information to remote AEs. It is associated with the local real-world activities “Refresh Now” or automatic polling. When either the “Refresh Now” or automatic polling are performed, the Workflow Application Entity queries a remote AE for worklist items that provides the set of worklist items matching the query request.  
Modality Performed Procedure Step (MPPS) messages are sent from the system under the following circumstances:
  - MPPS N-Create, Status = IN PROGRESS:
    - Closing the Patient Data Entry screen will result in automated creation of an MPPS Instance managed by a remote AE.
  - MPPS N-Set, Status = COMPLETE
    - Completion of the MPPS is performed as the result of an operator action of ending the exam.
  - MPPS N-Set, Status = DISCONTINUED
    - “Cancel” causes the “Discontinued” status to be sent.
- An Ended Exam may be ‘appended’ with images and SRs within 24 hours of the beginning of the exam. There are two fundamental methods to perform append:
  - *Note: The system will notify the user that it is “Restarting” the study. If beyond 24 hours, the system will not allow new images to be acquired.*
  - Append from Patient Data Entry
    - Press the “Patient” hardkey. If Modality Worklist is configured, press the “Manual Entry” button and/or select the “Restart” button to get a list of exams that are less than 24 hours old. Select an exam and ‘OK’ to close Patient Data Entry to return to scanning.
  - Append from Image Review
    - Press the “Review” hardkey then select the “Search for Study” icon to see the list of performed studies. Select the exam and hit “Open Study” to return to live scanning to acquire images and measurements.
- The **Hardcopy Application Entity** sends DICOM print pages to a remote AE (Printer or print server). It is associated with the local real-world activity Acquire when a DICOM Printer is configured for Batch Mode in the current preset, or “DICOM print” is selected with Right Button on the Exam in the system Patient Directory.
- Additionally, individual images can be selected in Review and sent with the selection of “Print selected still images to DICOM Printer” icon.

- Either action creates a print queue containing one or more virtual film sheets composed from images acquired by the user. It creates and sends fully rendered pages already containing the user's selected formatting choices. Only a single image object per sheet is sent to the printer. This print object is rather large compared to sending individual Image Box objects to the printer. If the user has both a BW and Color DICOM printer configured and selected, and is using "Send as you go", the images containing no Color Flow or Chroma data will be sent to the BW printer, all others will be sent to the Color printer.
- Exam data is sent to all selected Store, Print and Workflow destinations simultaneously in accordance with system configuration of "Send as you go" or "Batch" at end of exam or Manual.

#### **4.1.2 Functional Definition of AEs**

##### **4.1.2.1 Functional Definition of Storage Application Entity**

A Network Store queue with associated network destination will activate the Storage AE. An association request is sent to the destination AE and upon successful negotiation of a Presentation Context the image transfer is started. If the association cannot be opened, the related queue's Status is set to RETRY as displayed in the Job Manager (CNTL-J). The user may select "Retry Job" to attempt re-send.. After the automatic retries have failed, the job is set to ERROR. The user may "Delete Job" and re-send manually. Deleting a job does not remove the data, as it is still present on the system. Only the request to transfer the data is removed. Once any communication issues have been resolved, "Retry Job" may be selected or if the jobs were deleted, they may be queued again from the Review directory.

Storage Commitment messages are structured and sent depending on the user configuration for sending data. If the system is set for "Send as you go", then commit requests are sent when the images are exported. Several images may be contained in a single request. When the system is set to "Batch mode" all images are exported at the end of the exam, a Storage Commitment queue is established and remains in the Job Manager window until the N-Event-Report-Request message is received.

Studies sent manually from "Review" will also send Storage Commitment requests.

##### **4.1.2.2 Functional Definition of Workflow Application Entity**

"Refresh Now" attempts to download a Modality Worklist from a Modality Worklist server with studies matching the search criteria by sending a C-Find Request containing user-definable Query parameters. There could be additional attributes that the ClearVue system can send depending on the transport layer being used. Query parameters are stored in the "Advanced" tab adjacent to the MWL SCP selection in the "Servers and Roles" setup page. 10 Customizable Queries may be used, 5 are factory defaults.

Settings that may be customized are:

- Query Name (not sent in the DICOM data)
- Start Date (All Dates, Today or Date Range)
- AE Title (This system, Any or Another specific)
- Modality (Ultrasound or All Modalities)

When the Workflow AE establishes an association to a remote AE, a MWL C-Find-Rq message is sent to the MWL server. The server will transfer all matching worklist items via the open association. The results of a successful Worklist Update will overwrite the data in the Worklist display. There is no queue management for Worklist.

The Workflow AE creates a MPPS Instance when the PDE (Patient Data Entry screen) is closed. An MPPS N-Create-Rq message is sent to the MPPS server with the status of "IN PROGRESS". At the end of the exam, when "Completed" or "Cancel" are selected, an MPPS N-Set- Rq message is sent with "COMPLETED" or "DISCONTINUED" respectively. MPPS message queues are listed in the Job Manager (CNTL-J) window.


#### **4.1.2.3 Functional Definition of Hardcopy Application Entity**

A print queue will activate the Hardcopy AE. An association is established with the printer(s) and the printer's status is determined. If the printer is operating normally, the film sheet print requests will be sent. If the printer is not operating normally, the print queue status is set to "Failed" and can be restarted by the user via the queue management interface.

When both a BW and a Color DICOM printer are configured, the images that contain color data, i.e., Color Flow Doppler or "Chroma" will be sent to the Color printer only, and all other images will be sent to the BW printer. Otherwise, all images will be sent to the selected printer.

There is an embedded retry mechanism that retries based on the individual server's settings as configured by the user. Default values are: 3 Retries with 300 seconds (5 minutes) Interval.

## Sequencing of Real-World Activities

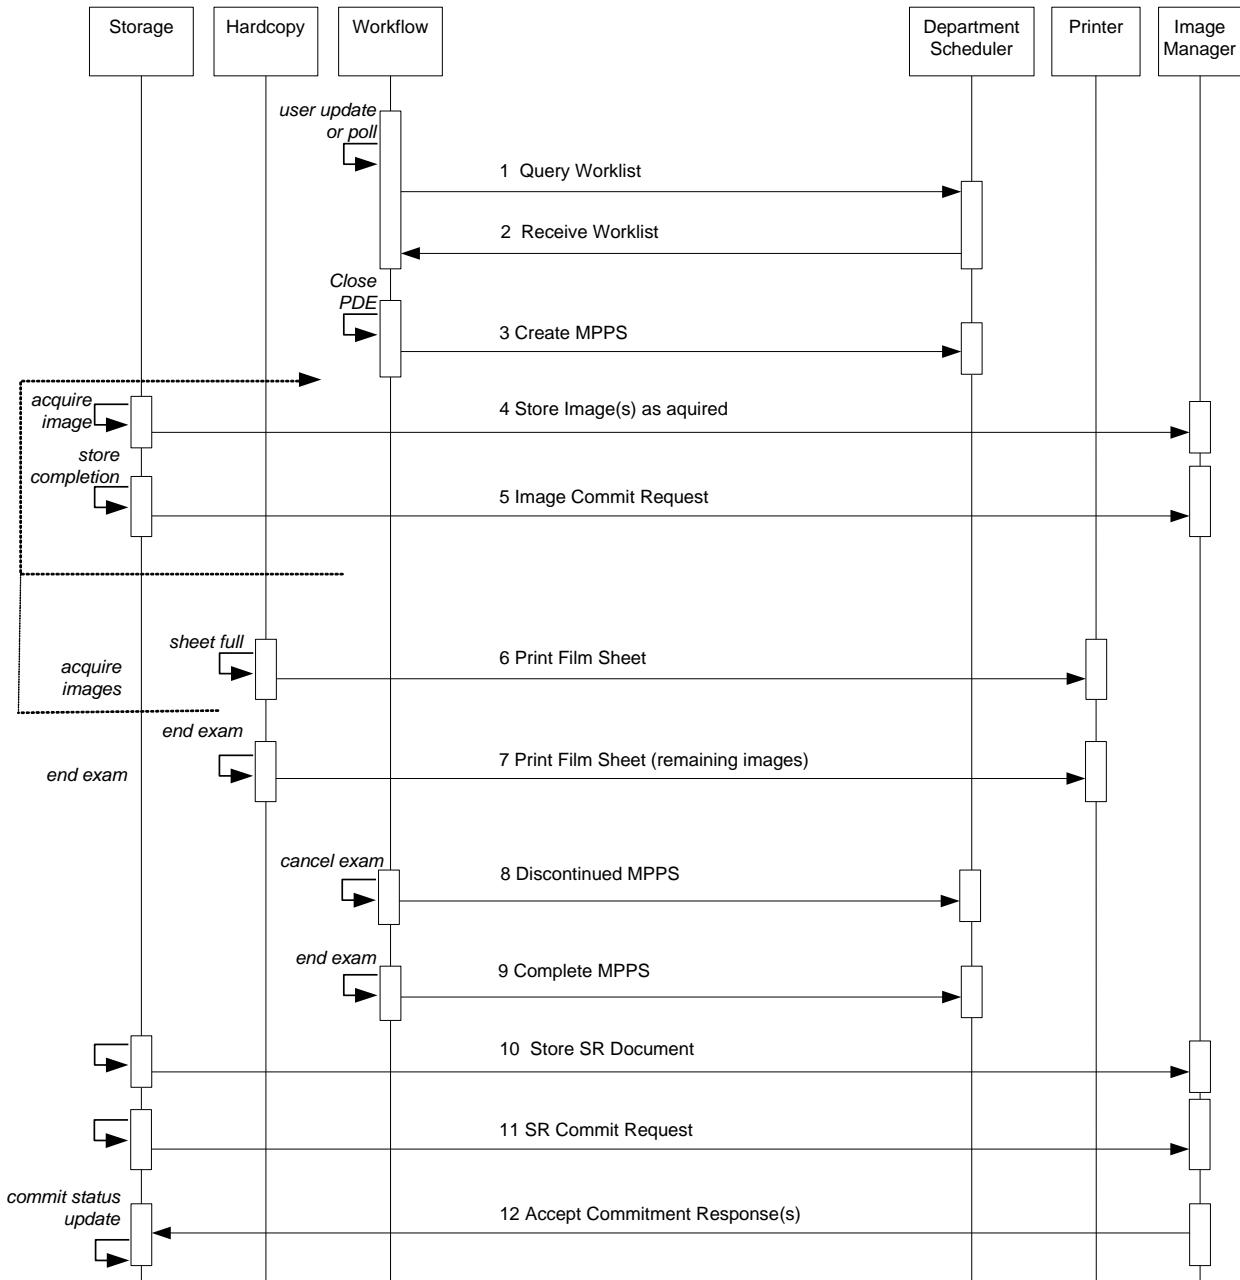


**FIGURE 2A:**  
SEQUENCING CONSTRAINTS – SEND AS YOU GO CONFIGURATION

Figures 2a and 2b illustrate normal scheduled workflow conditions.

Notes:

- Printing to DICOM printers may occur independent of any other DICOM activity.
- All selected store, print and workflow devices are sent data during the exam when configured for “Send as you go”, at the end of exam “Batch” or from Review when set for Manual.
- Selecting a study from Review for export will send to selected devices.

Other workflow situations (e.g. unscheduled procedure steps) will have other sequencing constraints. Printing or storage could equally take place after image acquisition. Printing could be omitted completely if no printer is connected or hardcopies are not required.

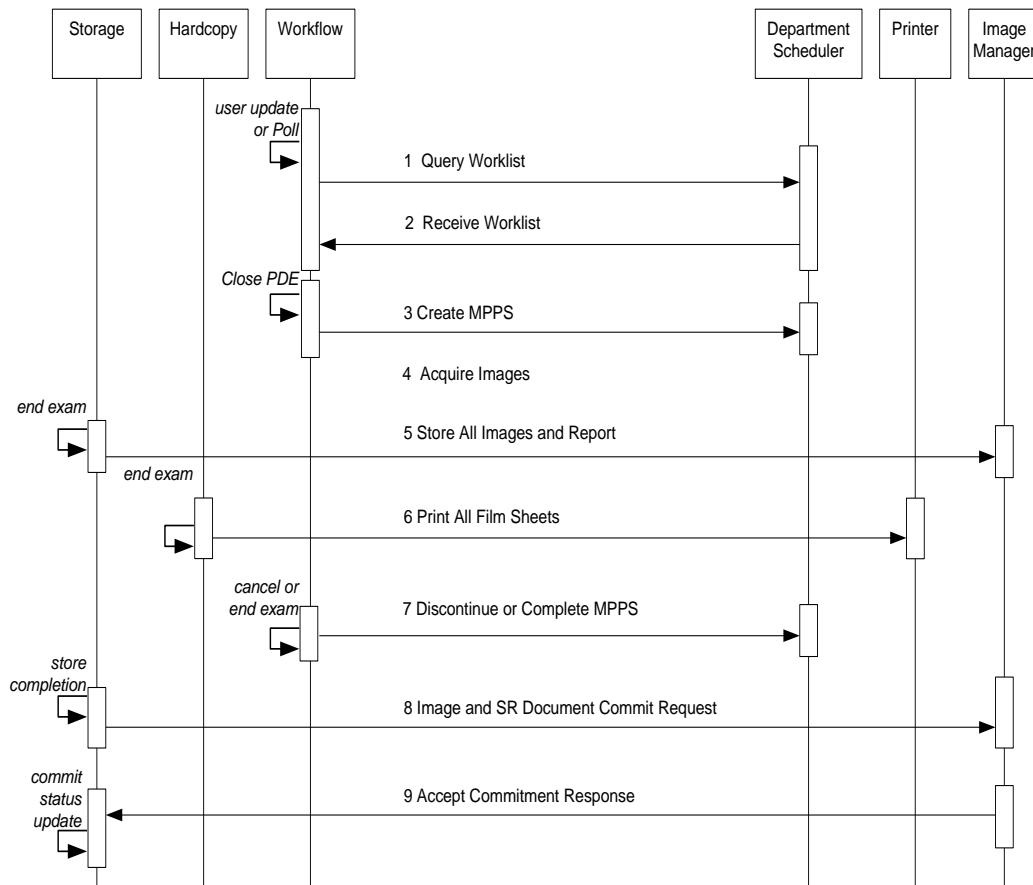

**FIGURE 2B:**  
SEQUENCING CONSTRAINTS – END EXAM CONFIGURATION

## 4.2 AE SPECIFICATIONS

### 4.2.1 Storage Application Entity Specification

#### 4.2.1.1 SOP Classes

ClearVue 350/550/650/850 3.1 provide Standard Extended<sup>1</sup> Conformance to the following SOP Classes:

**Table 3  
SOP CLASSES FOR AE STORAGE**

SOP Class Name	SOP Class UID	SCU	SCP
US Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Yes	No
US Multiframe Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Yes	No
Comprehensive Structured Report Storage	1.2.840.10008.5.1.4.1.1.88.33	Yes	No
Storage Commitment Push Model	1.2.840.10008.1.20.1	Yes	No

#### 4.2.1.2 Association Establishment Policy

##### 4.2.1.2.1 General

The DICOM standard application context name for DICOM 3.0 is always proposed:

**Table 4  
DICOM APPLICATION CONTEXT FOR AE STORAGE**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

The PDU size is configurable with a minimum size of 100 and a maximum size of 16,000. The default PDU size is 16,000.

##### 4.2.1.2.2 Number of Associations

ClearVue 350/550/650/850 3.1 initiates one Association at a time for each destination to which a transfer request is being processed in the active job queue list. Two Storage SCPs may be selected, but only one job will be active at a time, the other(s) remain pending until the active job is completed or failed.

**Table 5  
NUMBER OF ASSOCIATIONS INITIATED FOR AE STORAGE**

Maximum number of simultaneous Associations	5, 1 for each configured storage device
---	---

One Primary Storage Server, one Secondary Storage Server, one Storage Commitment Server, one SR Storage Server and one SR Storage Commitment Server.

ClearVue 350/550/650/850 3.1 accepts Associations for N-EVENT-REPORT notifications for the Storage Commitment Push Model SOP Class on a separate association.

**Table 6  
NUMBER OF ASSOCIATIONS ACCEPTED FOR AE STORAGE**

<sup>1</sup> See section 8.7 for information on the Standard Extended SOP Class

Maximum number of simultaneous Associations	1
---	---

#### 4.2.1.2.3 Asynchronous Nature

ClearVue 350/550/650/850 3.1 does not support asynchronous communication (multiple outstanding transactions over a single Association).

**Table 7  
ASYNCHRONOUS NATURE AS A SCU FOR AE STORAGE**

Maximum number of outstanding asynchronous transactions	1
---	---

#### 4.2.1.2.4 Implementation Identifying Information

The implementation information for this Application Entity is:

**Table 8  
DICOM IMPLEMENTATION CLASS AND VERSION FOR AE STORAGE**

Implementation Version Name	Implementation Class UID
ClearVue 350_3.1	1.3.46.670589.14.5000.310
ClearVue 550_3.1	1.3.46.670589.14.6000.310
ClearVue 650_3.1	1.3.46.670589.14.9002.310
ClearVue 850_3.1	1.3.46.670589.14.9004.310

#### 4.2.1.3 Association Initiation Policy

##### 4.2.1.3.1 Activity – Store Images, Loops and Structured Reports

###### 4.2.1.3.1.1 Description and Sequencing of Activities

Images and Reports may be sent from the selected studies from the Review directory. When the “Send as you go” option is active, the queue is serviced continuously during the exam. Each image is sent in its own association that is opened and closed. Additional images acquired during the exam will be sent using subsequent associations.

If the C-STORE response from the remote application contains a status other than Success or Warning, the association is retried until switched to a failed state.


When a system configured with network destinations is used without the network connected, it is considered to be in “Portable” mode. When returning from portable, reconnecting the network cable will initiate transfer.

The Storage Commitment service is implemented to handle image commitment separately from Structured Reports. For Images, only the Primary Store SCP may be associated with a commitment server. For Structured Reports, the SR Store SCP may be configured with its own commit server. In each case, the Storage AE will transmit a Storage Commitment request (N-ACTION) over a separate Association from the storage of image or report objects. Outstanding Commit Requests (those that have not received an N-Event-Report) will remain in the Job Manager (CNTL-J) until the report is received.

The Storage AE can only receive an N-EVENT-REPORT request in a separate subsequent association initiated by the SCP employing PDU 54H SCP/SCU Role Negotiation in the SCP’s Association Request. It cannot receive N-Event-Report-Rq messages on the same association as the N-Action-Rq.

Structured Reports will contain only supported measurements and calculations created by ClearVue 350/550/650/850 3.1. This may exclude some entries displayed in the on-system report. Measurements or calculations that are not supported for export are listed in Appendix A.

- The OB and Gyn Study types create OB-GYN Ultrasound Procedure Reports.
- The Vascular Study type creates Vascular Ultrasound Procedure Reports.
- The Cardiac (Adult Echo) Study type creates Adult Echocardiography Reports.
- The Cardiac (Ped Echo) Study type creates Pediatric Echocardiography Reports.

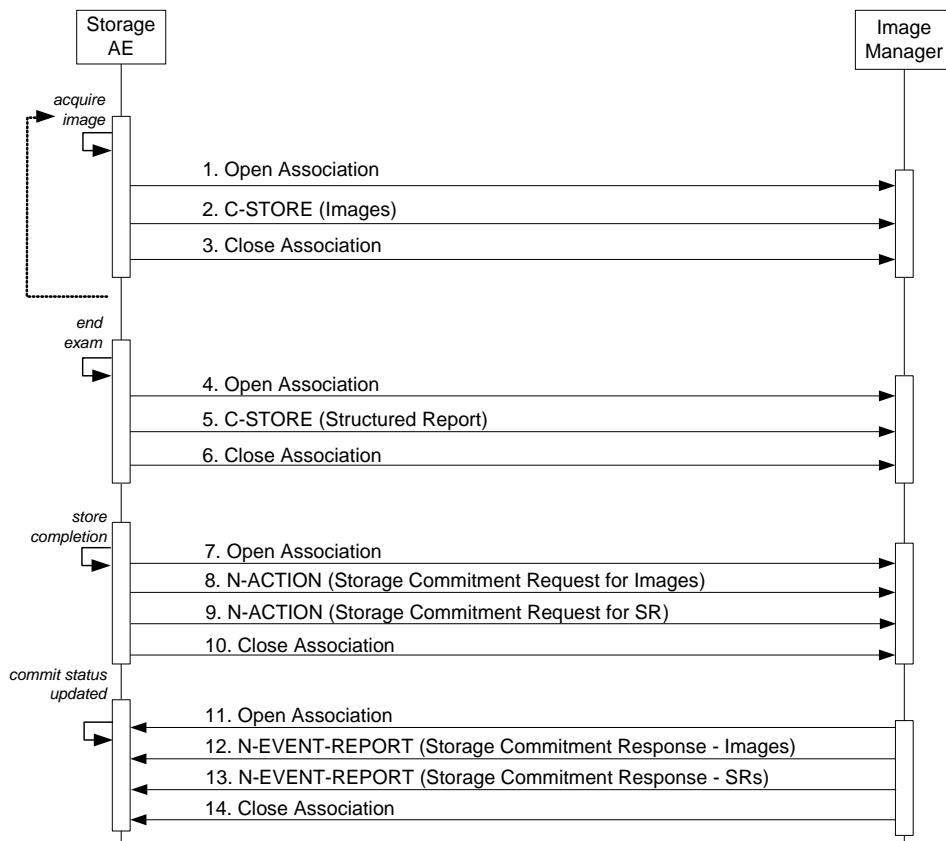

**Figure 3**  
SEQUENCING OF ACTIVITY – SEND IMAGES AND STRUCTURED REPORT

The sequence of interactions between the Storage AE and an Image Manager is illustrated in Figure 3 for the “Store” configuration option “Send as you go.” The alternative option, “Batch mode” differs only in the removal of the loop symbol on the ‘acquire images’ activity

NOTES: The N-EVENT-REPORT must be sent over a separate association initiated by the Image Manager (see Section 4.2.1.4.1 on Activity – Receive Storage Commitment Response).

#### 4.2.1.3.1.2 Proposed Presentation Contexts

ClearVue 350/550/650/850 3.1 is capable of proposing the Presentation Contexts shown in the following table:

**Table 9  
PROPOSED PRESENTATION CONTEXTS FOR ACTIVITY SEND IMAGES**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
US Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Implicit VR LittleEndian* Explicit VR LittleEndian JPEG Lossy Baseline RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.5	SCU	None
US Multiframe Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Implicit VR LittleEndian Explicit VR LittleEndian JPEG Lossy Baseline RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.5	SCU	None
Comprehensive Structured Report Storage	1.2.840.10008.5.1.4.1.1.88.33	Implicit VR LittleEndian	1.2.840.10008.1.2	SCU	None
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR LittleEndian Explicit VR LittleEndian	1.2.840.10008.1.2 1.2.840.10008.1.2.1	SCU	None

\*The following applies to both US Image and US Multiframe Images

JPEG used if image Photometric Interpretation is

YBR\_FULL\_422

RLE Lossless is used if image formats are any of

Palette Color, RLE Compressed

RGB, RLE Compressed

MONOCHROME2, RLE Compressed

Implicit LittleEndian (ILE) transfer Syntax is used when:

Palette Color, Uncompressed ILE

RGB, Uncompressed ILE

MONOCHROME2, Uncompressed ILE

Explicit LittleEndian (ELE) transfer syntax is used when:

Palette Color, Uncompressed ELE

RGB, Uncompressed ELE

MONOCHROME2, Uncompressed ELE

**Storage Commitment N-Action Requests** are only sent to the image storage device that is configured as the Storage Commitment server and associated with the Primary SCP. SRs are sent to their own configured SCP and Storage Commitment for SRs are handled separately from images.

#### 4.2.1.3.1.3 SOP Specific Conformance for Image and Comprehensive Structured Report Storage SOP Classes

All Image and Comprehensive Structured Report Storage SOP Classes supported by the Storage AE exhibit the same behavior, except where stated, and are described together in this section.

Table 10 describes C-Store response behavior.

The following Default Settings and Ranges may be used where applicable in Table 10:

Setting	Default	Range
Connect Timeout	30 sec	10 – 999 sec
Read Timeout	300 sec	30 – 999 sec
Write Timeout	300 sec	30 – 999 sec
Maximum Retries	3	0 – 999

**Table 10**  
**STORAGE C-STORE RESPONSE STATUS HANDLING BEHAVIOR**

Establishing the Association with Default settings

Condition (After C-Store)	Status Codes (C-Store- RSP)	Response
Could not establish the association within 30-second time window (Connect Timeout) due to NO RESPONSE from the Storage Server	Not Applicable	<p>The association attempt is aborted, and after 5-minutes a new association is attempted. ClearVue 350/550/650/850 3.1 will make three attempts to open an association with the configured Storage SCP before aborting the storage request and placing the job in an error state. The user can then manually restart the job at some later date. The failure is logged to the DICOM log file as an error.</p> <p>The 5-minute timeout and the number of retries are configurable by the user from the DICOM Setup screens. The 5-minute timeout is mapped to the 'Retry Interval' input control on the DICOM Setup screen and the number of retries is mapped to 'Maximum Retries' on the DICOM Setup screen.</p>
Refused	A7xx	<p>If the Storage SCP server refuses the association, then the association attempt is aborted. ClearVue 350/550/650/850 3.1 will wait 5-minutes and then reattempt the association. ClearVue 350/550/650/850 3.1 will make three attempts to establish the association before aborting the storage request and placing the job in an error state. The user can then manually restart the job at some later date. The failure is logged to the DICOM log file as an error.</p> <p>As an example, the association would be refused if the storage server employs a high security mechanism whereby it only accepts association requests from DICOM Servers that it knows about and the ClearVue 350/550/650/850 3.1's AE Title was not in the PACS database.</p> <p>See the timeout and retry settings above.</p>

During Image or SR Transfer

Service Status	Error Code	Behavior
After association has been accepted, there is no response to a request within 5-minute time window (Read Timeout).	Not Applicable	If the association is lost during active image transfer to the Storage SCP server, ClearVue 350/550/650/850 3.1 will initiate a new association after 5 minutes, and attempt to store all the images. If during transfer, the association is again lost, ClearVue 350/550/650/850 3.1 will wait another 5 minutes and try again. ClearVue 350/550/650/850 3.1 will make three attempts to send all the images before aborting the storage request and placing the job in an error state. The user can then manually restart the job at some later date. The failure is logged to the DICOM log file as an error.  See the timeout and retry settings above.
Error	A9xx, Cxxx, 0122, Other	ClearVue 350/550/650/850 3.1 will treat all errors as failure of Storage request (also called as Job). A failed job is automatically retried after 5 minutes. If the job fails even after three attempts, ClearVue 350/550/650/850 3.1 will abort this request and place the job in an Error state. The user can then manually restart the job at some later date. The failure is logged to the DICOM log file as an error.
Warning	D000, B000, B006, B007	If the Storage SCP issues a warning on a particular image (perhaps it had to use coercion), ClearVue 350/550/650/850 3.1 logs the warning to the DICOM log file as an informational event and continues on as if the image was successfully stored to the PACS (see row below).
Success	0000	When an image is successfully stored to the Storage SCP (PACS), ClearVue 350/550/650/850 3.1 will keep a record of the successful storage. If all the images in the job are successfully stored, ClearVue 350/550/650/850 3.1 will notify the user (through an icon on the list of studies), and the job will be removed from the job manager.
*	Any other status code.	The Association is aborted using A-ABORT and the transfer fails. The status is logged.

The behavior of Storage AE during communication failure is summarized in Table 11.

**Table 11**  
**STORAGE COMMUNICATION FAILURE BEHAVIOR**

Exception	Behavior
Timeout	Same as Service Status timeouts in Table 10 above.
Association aborted by the SCP or network layers	Same as Service Status in Table 10 above.

The contents of US Image, US Multiframe Storage and Comprehensive Structured Report Storage SOP Instances conform to the DICOM IOD definitions described in Section 8.1.

#### **4.2.1.3.1.4 SOP Specific Conformance for Storage Commitment Push Model SOP Class**

##### **4.2.1.3.1.4.1 Storage Commitment Operations (N-ACTION)**

The Storage AE will request storage commitment for the configured device.

Table 12 summarizes the behavior of Storage AE when receiving response status codes.

**Table 12  
STORAGE COMMITMENT N-ACTION RESPONSE STATUS HANDLING BEHAVIOR**

<b>Service Status</b>	<b>Further Meaning</b>	<b>Error Code</b>	<b>Behavior</b>
Success	Success	0000	The system waits for the N-Event-Report.
*	*	Any other status code.	The commit status remains incomplete for all objects.

Table 13 summarizes the behavior of Storage AE during communication failure.

**Table 13  
STORAGE COMMITMENT COMMUNICATION FAILURE BEHAVIOR**

<b>Exception</b>	<b>Behavior</b>
Timeout	Same as non-success status in Table 12.
Association aborted by the SCP or network layers	Same as non-success status in Table 12.

##### **4.2.1.3.1.4.2 Storage Commitment Tags (N-ACTION)**

The Storage AE will request storage commitment using the following tags

NOTE: Storage Commitment may only be automatically requested by the system at the end of a study.

**Table 13a  
STORAGE COMMITMENT N-ACTION-REQUEST MESSAGE CONTENTS**

<b>Action Type Name</b>	<b>Action Type ID</b>	<b>Attribute</b>	<b>Tag</b>	<b>Requirement Type SCU</b>
Request Storage Commitment	1	Transaction UID	(0008,1195)	1
		Referenced SOP Sequence	(0008,1199)	1
		>Referenced SOP Class UID	(0008,1150)	1
		>Referenced SOP Instance UID	(0008,1155)	1

Subsequently, ClearVue 350/550/650/850 3.1 expects N-EVENT-REPORT messages from the storage commit server although ClearVue 350/550/650/850 3.1 does not assume that the event will arrive at any particular time. ClearVue 350/550/650/850 3.1 does not wait but will process the event whenever it arrives.

ClearVue 350/550/650/850 3.1 might be either powered down or disconnected from the network and used in portable mode, it is possible for the N-EVENT-REPORT to arrive from the Storage Commitment SCP while ClearVue 350/550/650/850 3.1 cannot receive it. If an outstanding N-EVENT-REPORT does not arrive within 96 hours, then

ClearVue 350/550/650/850 3.1 will reissue the same Storage Commitment request. When the event arrives, ClearVue 350/550/650/850 3.1 returns an N-EVENT-REPORT response primitive with one of the following status codes.

#### 4.2.1.3.1.4.3 Storage Commitment Notifications (N-EVENT-REPORT)

The Storage AE can receive an N-EVENT-REPORT notification received from the SCP via Reverse-role negotiation.

Table 14 summarizes the behavior of Storage AE when receiving Event Types within the N-EVENT-REPORT.

**Table 14  
STORAGE COMMITMENT N-EVENT-REPORT BEHAVIOUR**

Event Type Name	Event Type ID	Behavior
Storage Commitment Request Successful	1	The commit status is set to complete for each object.
Storage Commitment Request Complete – Failures Exist	2	The commit status remains incomplete. The commit comment for each object is logged.

The reasons for returning specific status codes in an N-EVENT-REPORT response are summarized in Table 15.

**Table 15  
STORAGE COMMITMENT N-EVENT-REPORT RESPONSE STATUS REASONS**

Service Status	Further Meaning	Error Code	Reasons
Success	Success	0000	The storage commitment result has been successfully received.

#### 4.2.1.3.1.4.4 Storage Commitment Tags (N-EVENT-REPORT)

Tags supported for receiving an N-Event-Report message.

Table 16 lists the tags that may be received within the N-EVENT-REPORT.

**Table 16  
STORAGE COMMITMENT N-EVENT-REPORT MESSAGE CONTENTS**

Event Type Name	Event Type ID	Attribute	Tag	Requirement Type SCP
Storage Commitment Request Successful	1	Transaction UID	(0008,1195)	1
		Retrieve AE Title	(0008,0054)	3
		Storage Media File-Set ID	(0088,0130)	3
		Storage Media File-Set UID	(0088,0140)	3
		Referenced SOP Sequence	(0008,1199)	1
		>Referenced SOP Class UID	(0008,1150)	1
		>Referenced SOP Instance UID	(0008,1155)	1

		> <i>Retrieve AE Title</i>	(0008,0054)	3
		> <i>Storage Media File-Set ID</i>	(0088,0130)	3
		> <i>Storage Media File-Set UID</i>	(0088,0140)	3
Storage Commitment Request Complete – Failures Exist	2	Transaction UID	(0008,1195)	1
		<i>Retrieve AE Title</i>	(0008,0054)	3
		<i>Storage Media File-Set ID</i>	(0088,0130)	3
		<i>Storage Media File-Set UID</i>	(0088,0140)	3
		Referenced SOP Sequence	(0008,1199)	1
		>Referenced SOP Class UID	(0008,1150)	1
		>Referenced SOP Instance UID	(0008,1155)	1
		> <i>Retrieve AE Title</i>	(0008,0054)	3
		> <i>Storage Media File-Set ID</i>	(0088,0130)	3
		> <i>Storage Media File-Set UID</i>	(0088,0140)	3
		Failed SOP Sequence	(0008,1198)	1
		>Referenced SOP Class UID	(0008,1150)	1
		>Referenced SOP Instance UID	(0008,1155)	1
		>Failure Reason	(0008,1197)	1

In Table 16 above, the attributes in *italics* may be sent from the server, handled and ignored by HD15.

#### 4.2.1.4 Association Acceptance Policy

##### 4.2.1.4.1 Activity – Receive Storage Commitment Response

###### 4.2.1.4.1.1 Description and Sequencing of Activities

The Storage AE accepts associations for pending responses to a Storage Commitment Request only using SCP/SCU Role Negotiation; explicitly stating that the association is initiated by the SCP to the SCU. Any other will be rejected.

###### 4.2.1.4.1.2 Accepted Presentation Contexts

Table 17 summarizes Presentation Contexts that the Storage AE accepts.

**Table 17**  
**ACCEPTABLE PRESENTATION CONTEXTS FOR**  
**ACTIVITY RECEIVE STORAGE COMMITMENT RESPONSE**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Storage Commitment Push Model	1.2.840.10008.1.20 .1	Implicit VR Little Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1	SCU	None

#### 4.2.1.4.1.3 SOP Specific Conformance for Storage Commitment Push Model SOP Class

##### 4.2.1.4.1.3.1 Storage Commitment Notifications (N-EVENT-REPORT)

Upon receipt of an N-EVENT-REPORT the timer associated with the Transaction UID will be canceled.

Table 14 summarizes the behavior of Storage AE when receiving Event Types within the N-EVENT-REPORT.

The Storage AE may reject association attempts as shown in the Table below. The Result, Source and Reason/Diag columns represent the values returned in the appropriate fields of an ASSOCIATE-RJ PDU. The contents of the Source column is abbreviated to save space and the meaning of the abbreviations are:

- a) 1 – DICOM UL service-user
- b) 2 – DICOM UL service-provider (ASCE related function)
- c) 3 – DICOM UL service-provider (Presentation related function)

Table 17b summarizes the reasons for returning specific status codes in an N-EVENT-REPORT response.

**Table 17b  
ASSOCIATION REJECTION REASONS**

Result	Source	Reason/Diag	Explanation
2 – Rejected Transient	c	2 – Local Limit Exceeded	The (configurable) maximum number of simultaneous associations has been reached. An association request with the same parameters may succeed at a later time.
2 – Rejected Transient	c	1 – Temporary Congestion	No associations can be accepted at this time. An association request with the same parameters may succeed at a later time.
1 – Rejected Permanent	a	2 – Application Context Name Not Supported	The association request contained an unsupported Application Context Name. An association request with the same parameters will not succeed at a later time.
1 – Rejected Permanent	a	7 – Called AE Title Not Recognized	The association request contained an unrecognized Called AE Title. A successful association request will require configuration changes. This rejection reason normally occurs when the association initiator is incorrectly configured and attempts to address the association acceptor using the wrong AE Title. Make sure the Commit Server has the correct AE Title and IP Address for the ultrasound system.
1 – Rejected Permanent	a	3 – Calling AE Title Not Recognized	The association request contained an unrecognized Calling AE Title. An association request with the same parameters will not succeed at a later time unless configuration changes are made. This rejection reason normally occurs when the association acceptor has not been configured to recognize the AE Title of the association initiator. Ensure

			there is no variation in Case in this system's AE Title on the Commit Server.
1 – Rejected Permanent	b	1 – No Reason Given	The association request could not be parsed. An association request with the same format will not succeed at a later time.

#### 4.2.2 Workflow Application Entity Specification

##### 4.2.2.1 SOP Classes

ClearVue 350/550/650/850 3.1 provide Standard Conformance to the following SOP Classes:

**Table 18  
SOP CLASSES FOR AE WORKFLOW**

SOP Class Name	SOP Class UID	SCU	SCP
MWL Information Model – FIND	1.2.840.10008.5.1.4.31	Yes	No
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Yes	No

##### 4.2.2.2 Association Establishment Policy

###### 4.2.2.2.1 General

The DICOM standard application context name for DICOM 3.0 is always proposed:

**Table 19  
DICOM APPLICATION CONTEXT FOR AE WORKFLOW**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

###### 4.2.2.2.2 Number of Associations

ClearVue 350/550/650/850 3.1 initiate one Association at a time for a Worklist request and a separate association for Modality Performed Procedure Step messages.

**Table 20  
NUMBER OF ASSOCIATIONS INITIATED FOR AE WORKFLOW**

Maximum number of simultaneous Associations	1
---	---

###### 4.2.2.2.3 Asynchronous Nature

ClearVue 350/550/650/850 3.1 does not support asynchronous communication.

**Table 21  
ASYNCHRONOUS NATURE AS A SCU FOR AE WORKFLOW**

Maximum number of outstanding asynchronous transactions	1
---	---

###### 4.2.2.2.4 Implementation Identifying Information

The implementation information for this Application Entity is:

**Table 22**  
**DICOM IMPLEMENTATION CLASS AND VERSION FOR AE WORKFLOW**

Implementation Version Name	Implementation Class UID
ClearVue 350_3.1	1.3.46.670589.14.5000.310
ClearVue 550_3.1	1.3.46.670589.14.6000.310
ClearVue 650_3.1	1.3.46.670589.14.9002.310
ClearVue 850_3.1	1.3.46.670589.14.9004.310

#### **4.2.2.3 Association Initiation Policy**


##### **4.2.2.3.1 Activity – Worklist Update**

###### **4.2.2.3.1.1 Description and Sequencing of Activities**

Worklist queries for Modality (US) or All Modalities may be initiated by the user or will occur at a preset interval set as one of the following:

- The user may press “Refresh Now” to send a query: using search keys: Start Date, Modality and AE Title selections made in the Set Modality Worklist Queries configuration page.
- The user may configure the system to search for studies scheduled for its AE Title, or it may be set to search for a different AE Title’s studies, or all.
- The system may be set\* to periodically poll the worklist server. Default is 10 minutes, adjustable in one minute increments from 1 to 32,767 minutes.

\* Follow Setups > System > DICOM > DICOM Preset > Change Settings for current preset > Modify in Roles > MWL SCP – Advanced > MWL Polling Frequency.

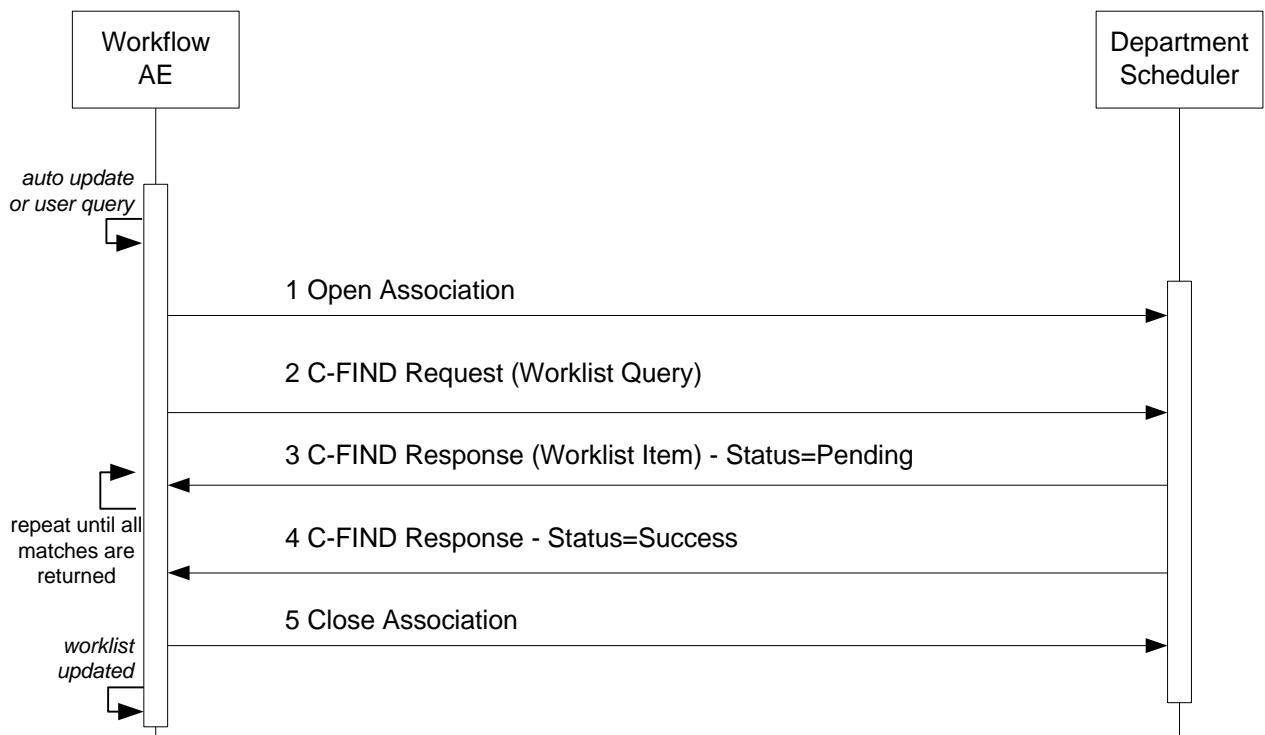

**Figure 5**  
SEQUENCING OF ACTIVITY – WORKLIST UPDATE

A possible sequence of interactions between the Workflow AE and a Departmental Scheduler (e.g. a device such as a RIS or HIS which supports the MWL SOP Class as an SCP) is illustrated in Figure 5:

#### 4.2.2.3.1.2 Proposed Presentation Contexts

ClearVue 350/550/650/850 3.1 will propose Presentation Contexts as shown in the following table:

**Table 23**  
PROPOSED PRESENTATION CONTEXTS FOR ACTIVITY WORKLIST UPDATE

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Modality Worklist Information Model – FIND	1.2.840.10008.5.1 .4.31	Explicit VR LittleEndian* Implicit VR LittleEndian	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None

\*Note: If the worklist server accepts Explicit VR LittleEndian and Implicit VR LittleEndian then ClearVue 350/550/650/850 3.1 will use Explicit VR LittleEndian Transfer Syntax.

#### 4.2.2.3.1.3 SOP Specific Conformance for Modality Worklist

Table 24 summarizes the behavior of ClearVue 350/550/650/850 3.1 when encountering status codes in a MWL C-FIND response.

Additional attributes sent by RIS SCP, other than the ones listed in the following table, will be ignored by the ClearVue system. A message “query failed” will appear on the user interface if ClearVue 350/550/650/850 3.1 receives any other SCP response status than “Success” or “Pending.”

**Table 24  
MODALITY WORKLIST C-FIND RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Error Code	Behavior
Success	Matching is complete	0000	The system replaced the worklist from the response.
Refused	Out of Resources	A700	The Association is aborted using A-ABORT. The worklist is not replaced.
Failed	Identifier does not match SOP Class	A900	Same as “Refused” above.
Failed	Unable to Process	C000 – CFFF	Same as “Refused” above.
Cancel	Matching terminated due to Cancel request	FE00	The retrieved items are ignored.
Pending	Matches are continuing	FF00	Continue.
Pending	Matches are continuing – Warning that one or more Optional Keys were not supported	FF01	Continue.
*	*	Any other status code.	Same as “Refused” above.

Table 25 summarizes the behavior of ClearVue 350/550/650/850 3.1 during communication failure.

**Table 25  
MODALITY WORKLIST COMMUNICATION FAILURE BEHAVIOR**

Exception	Behavior
Timeout	Same as Service Status “Refused” in the table above.
Association aborted by the SCP or network layers	Same as Service Status “Refused” in the table above.

Table 26 describes the ClearVue 350/550/650/850 3.1 Worklist Matching Keys and requested attributes. Unexpected attributes returned in a C-FIND response are ignored.

Non-matching responses returned by the SCP due to unsupported optional matching keys are ignored.

**Table 26  
WORKLIST MATCHING KEYS**

<b>Module Name</b> Attribute Name	<b>Tag</b>	<b>VR</b>	<b>M</b>	<b>R</b>	<b>D</b>	<b>IOD</b>
<b>Scheduled Procedure Step</b>						
Scheduled Procedure Step Sequence	(0040,0100)	SQ		x		
> Scheduled Station AE Title	(0040,0001)	AE	S, *	x		x
> Scheduled Procedure Step Start Date	(0040,0002)	DA	S, R	x		x
> Scheduled Procedure Step Start Time	(0040,0003)	TM		x	x	x
> Scheduled Procedure Step End Date	(0040,0004)	DA		x		
> Scheduled Procedure Step End Time	(0040,0005)	TM		x		
> Modality	(0008,0060)	CS	S, *	x		x
> Scheduled Performing Physician's Name <sup>1</sup>	(0040,0006)	PN		x		x
> Scheduled Procedure Step Description <sup>2</sup>	(0040,0007)	LO		x	x	x
> Scheduled Protocol Code Sequence <sup>3</sup>	(0040,0008)	SQ		x		x
> Scheduled Station Name	(0040,0010)	SH		x		
> Scheduled Procedure Step Location <sup>4</sup>	(0040,0011)	SH		x	x	x
> Pre-Medication	(0040,0012)	LO		x		
> Scheduled Procedure Step ID	(0040,0009)	SH		x		x
> Requested Contrast Agent	(0032,1070)	LO		x		
> Scheduled Procedure Step Status	(0040,0020)	CS		x		x
> Comments on the Scheduled Procedure Step	(0040,0400)	LT		x		
<b>Requested Procedure</b>						
Requested Procedure ID <sup>5</sup>	(0040,1001)	SH		x		x
Reason for the Requested Procedure <sup>6</sup>	(0040,1002)	LO		x		
Requested Procedure Description	(0032,1060)	LO		x		x
Study Instance UID	(0020,000D)	UI		x		x
Referenced Study Sequence	(0008,1110)	SQ		x		x
Requested Procedure Code Sequence	(0032,1064)	SQ		x		
Names of Intended Recipients of Results	(0040,1010)	PN		x		
Requested Procedure Comments	(0040,1400)	LT		x		
<b>Imaging Service Request</b>						
Accession Number <sup>7</sup>	(0008,0050)	SH		x	x	x
Requesting Physician	(0032,1032)	PN		x		
Requesting Service	(0032,1033)	LO		x		
Referring Physician's Name <sup>8</sup>	(0008,0090)	PN		x	x	x
Reason for the Imaging Service Request <sup>9</sup>	(0040,2001)	LO		x	x	
Imaging Service Request Comments	(0040,2400)	LT		x		
<b>Module Name</b> Attribute Name	<b>Tag</b>	<b>VR</b>	<b>M</b>	<b>R</b>	<b>D</b>	<b>IOD</b>
<b>Visit Admission</b>						
Current Patient Location	(0038,0300)	LO		x		
<b>Patient Identification</b>						
Patient's Name	(0010,0010)	PN		x	x	x
Patient ID	(0010,0020)	LO		x	x	x
Other Patient IDs <sup>10</sup>	(0010,1000)	LO		x	x	x

<b>Patient Demographic</b>						
Patient's Birth Date <sup>11</sup>	(0010,0030)	DA		x	x	x
Patient's Birth Time <sup>11</sup>	(0010,0032)	TM	x	x		
Patient's Sex <sup>12</sup>	(0010,0040)	CS	x	x	x	
Patient's Age <sup>13</sup>	(0010,1010)	AS				
Patient Size <sup>14</sup>	(0010,1020)	DS	x	x	x	
Ethnic Group	(0010,2160)	SH	x			
Patient's Weight <sup>15</sup>	(0010,1030)	DS	x	x	x	
Patient Comments	(0010,4000)	LT	x	x		
Referenced Patient Sequence	(0008,1120)	SQ	x			x
<b>Patient Medical</b>						
Medical Alerts	(0010,2000)	LO		x		
Additional Patient's History	(0010,21B0)	LT	x			
Pregnancy Status	(0010,21C0)	US	x			

\* = Wildcard matching

The above table should be read as follows:

Module Name: The name of the associated module for supported worklist attributes.

Attribute Name: Attributes supported to build a ClearVue 350/550/650/850 3.1 Worklist Request Identifier.

Tag: DICOM tag for this attribute.

VR: DICOM VR for this attribute.

M: Matching keys for (automatic) Worklist Update. An "S" indicates that ClearVue 350/550/650/850 3.1 supplies an attribute value for Single Value Matching, "R" indicates a Range Value and "\*" is for Wildcard matching. See section 4.2.2.3.1.1 for setup location.

R: Return keys. An "x" indicates that ClearVue 350/550/650/850 3.1 supplies this attribute as a Return Key with zero length for Universal Matching.

D: Displayed keys. An "x" indicates that this worklist attribute is displayed to the user in the Patient Data Entry screen or Worklist Directory.

IOD: An "x" indicates that this Worklist attribute's data is included into applicable Image, SR or MPPS Object Instances created during performance of the related Procedure Step.

Notes:

1 Scheduled Performing Physician's Name is set in MPPS, sets the "Performed by" field in the Patient ID screen.

2 Scheduled Procedure Step Description is set in MPPS and images. May be used to set "Description" field in the Patient Selection screen and is mapped to "Study Description" in images. 2<sup>nd</sup> Configuration choice for "Study Description" in images.

3 Returned Scheduled Protocol Code Sequence contents are mapped to Scheduled Action Item Code Sequence and Performed Action Item Code Sequence in MPPS. If Code Meaning is present it is the 3<sup>rd</sup> Configuration option for Study description in images.

4 Scheduled Procedure Step Location sets the "Location" field in the Patient Selection Screen.

5 Requested Procedure Description value is set in the "Description" field of the Patient Selection screen and "Study Description" of the Patient ID screen. Manual entry to Study Description field is also sent in Image and MPPS messages.

6 May be used to set "Indication" field on Patient Selection screen. 1<sup>st</sup> choice, configurable. Not exported in DICOM.

7 Displayed on Patient ID screen and sent in MPPS and Images.

8 Sets the "Referring Physician" in Patient ID and Patient Selection screens.

9 May be used to set "Indication" field on Patient Selection screen. 2<sup>nd</sup> choice, configurable.

- 10              Displayed in “Alternate ID Number” field of Patient ID screen. Sent only in Images.
- 11              Birth Date and Birth Time can populate the ‘DOB’ field of Patient ID screen. Birth Date only is sent in MPPS messages.
- 12              Populates the “Gender” field in the Patient Selection screen.
- 13              Populates the “Age” field in the Patient Selection screen.
- 14              Populates “Height” fields in “Patient ID” and “Patient Selection” screens.
- 15              Populates “Weight” fields in “Patient ID” and “Patient Selection” screens.

#### **4.2.2.3.2 Activity –Acquire Images**

##### **4.2.2.3.2.1     Description and Sequencing of Activities**

An association to the configured MPPS SCP system is established immediately after the closing the Patient Data Entry screen, sending the MPPS N-Create message with status of “IN PROGRESS”.

The “End Exam” button causes a “COMPLETED” status in the N-Set message. An exam for which an MPPS Instance is sent with a state of “COMPLETED” can no longer be updated; however, it may be appended. See section 4.1.1, Application Data Flow for details on append.

Pressing the “Cancel” button causes a “DISCONTINUED” message. An exam for which an MPPS Instance is sent with a state of “DISCONTINUED” can also no longer be updated; however, it may be appended. See section 4.1.1, Application Data Flow for details on append.

The system supports creation of “unscheduled cases” by allowing MPPS instances to be communicated for locally registered Patients.


The system performs a single Performed Procedure Step at a time per Scheduled Procedure Step.

ClearVue 350/550/650/850 3.1 will initiate an Association to issue an:

- N-CREATE request according to the CREATE Modality Performed Procedure Step SOP Instance operation or a
- N-SET request to finalize the contents and state of the MPPS according to the SET Modality Performed Procedure Step Information operation.

The opening of a study marks the beginning of a new Modality Performed Procedure Step (MPPS). At this time, a MPPS record is created on the MPPS SCP through the use of the N-CREATE service. If the MPPS SCP is unavailable at this time, the request is queued and will be sent when the MPPS SCP is available.

When the user ends the scheduled procedure by closing the study and saving any changes, the MPPS status is “Completed”. Alternatively, the user may choose to cancel acquisition, the study is saved in local storage and the MPPS status becomes “Discontinued”. At this time, the Study Management AE attempts to modify the MPPS on the MPPS SCP through the use of the N-SET service. If the MPPS SCP is unavailable, the request is queued and will be sent when the MPPS SCP is available.

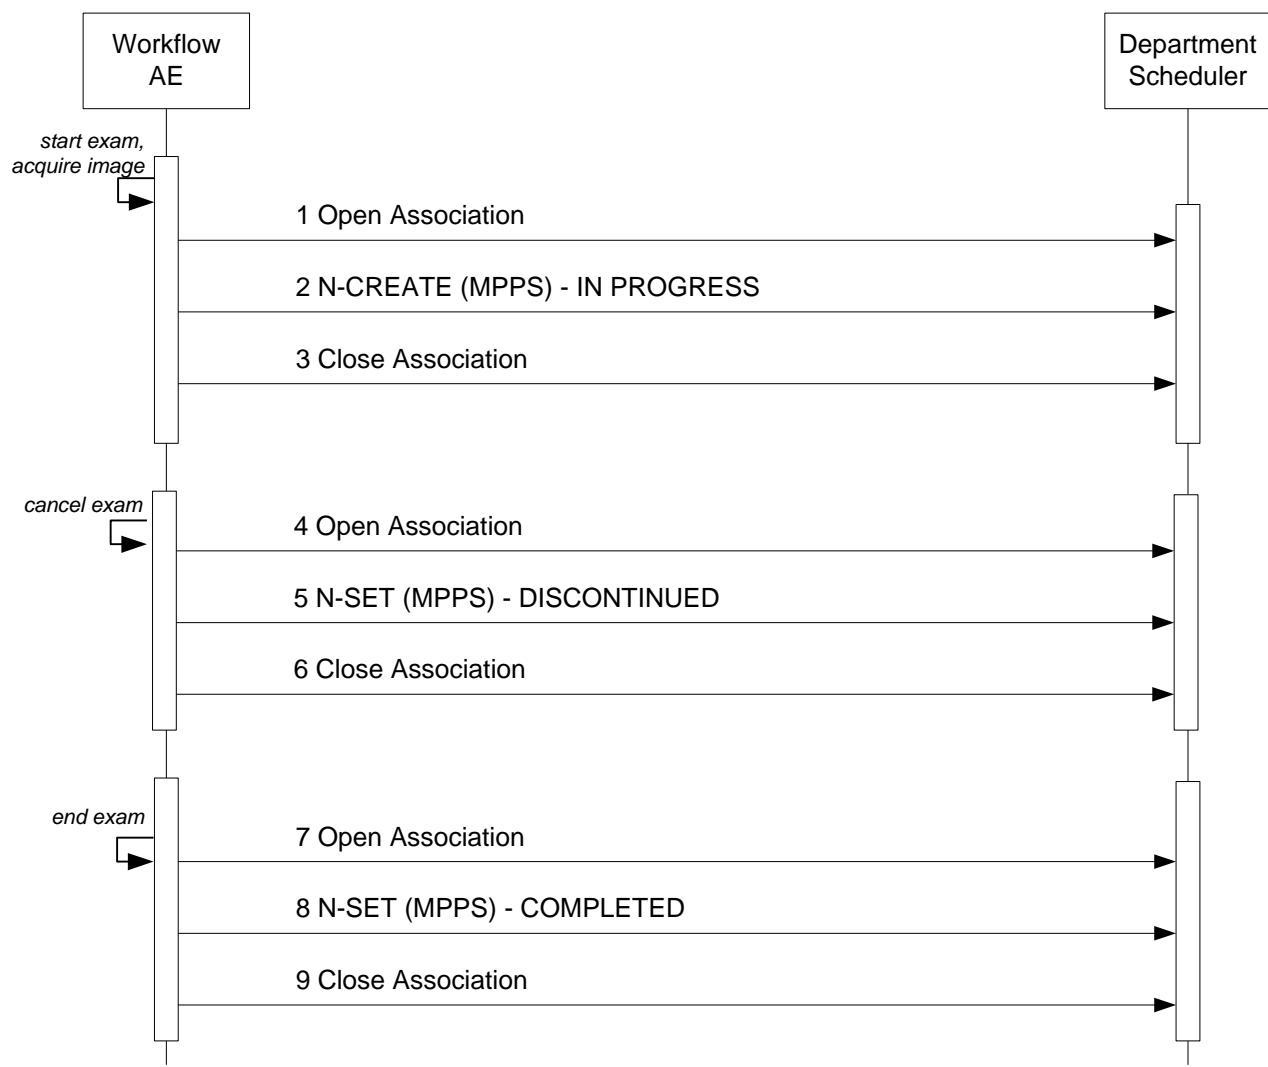

**Figure 6**  
SEQUENCING OF ACTIVITY – ACQUIRE IMAGES

A possible sequence of interactions between the Workflow AE and a Departmental Scheduler (e.g. a device such as a RIS or HIS which supports the MPPS SOP Class as an SCP) is illustrated in Figure 6.

Note: The Cancel and End Exam commands are mutually exclusive. They are both represented here for illustration purposes only. Actual workflow uses one or the other for a given exam.

#### 4.2.2.3.2.2 Proposed Presentation Contexts

ClearVue 350/550/650/850 3.1 will propose Presentation Contexts as shown in the following table:

**Table 27**  
**PROPOSED PRESENTATION CONTEXTS FOR REAL-WORLD ACTIVITY ACQUIRE IMAGES**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Modality Performed Procedure Step	1.2.840.10008.3.1 .2.3.3	Explicit VR Little Endian* Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None

\*Note: If the worklist server accepts Explicit VR Little Endian and Implicit VR Little Endian then ClearVue 350/550/650/850 3.1 will use Explicit VR Little Endian Transfer Syntax.

#### 4.2.2.3.2.3 SOP Specific Conformance for MPPS

Table 28 summarizes the behavior of ClearVue 350/550/650/850 3.1 when encountering status codes in an MPPS N-CREATE or N-SET response.

The updated attributes are shown in Table 30 below. The “N\_CREATE Usage” column shows the attributes transmitted when the status of the study changes to “IN\_PROGRESS”. The “N-SET Usage” column shows the attributes transmitted when the status of the study changes to “COMPLETED” or “DISCONTINUED”.

Note: The following fields are copied from the selected MWL entry to the Patient ID screen:

Accession Number

Patient's Name

Patient's ID

Patient's Birth Date

Patient's Sex

Referring Physician's Name

Study description

Usually, the performing physician will accept the information in the Patient ID Screen, as is, however the physician has the option of editing the information before starting the study. If the physician edits this information then the MPPS N-CREATE command that is sent to the MPPS server on study start will use the edited information and not the original MWL information.

**Table 28**  
**MPPS N-CREATE / N-SET RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.
Failure	Processing Failure – Performed Procedure Step Object may no longer be updated	0110	The Association is aborted.
Warning	Attribute Value Out of Range	0116H	The error message is displayed.

*	*	Any other status code.	Same as "Failure" above.
---	---	------------------------	--------------------------

Table 29 summarizes the behavior of ClearVue 350/550/650/850 3.1 during communication failure.

**Table 29**  
**MPPS COMMUNICATION FAILURE BEHAVIOR**

Exception	Behavior
Timeout	Same as "Failure" above.
Association aborted by the SCP or network layers	Same as "Failure" above.

Table 30 provides a description of the MPPS N-CREATE and N-SET request identifiers. Empty cells in the N-CREATE and N-SET columns indicate that the attribute is not sent.

**Table 30**  
**MPPS N-CREATE / N-SET REQUEST IDENTIFIER**

Attribute Name	Tag	VR	N-CREATE	N-SET
Specific Character Set	(0008,0005)	CS	See Section 6 for details.	
Modality	(0008,0060)	CS	US	
Referenced Patient Sequence	(0008,1120)	SQ	If available from MWL, else NULL	
> Referenced SOP Class UID	(0008,1150)	UI	1.2.840.10008.3.1.2.1.1 No value sent for unscheduled study.	
>Referenced SOP Instance UID	(0008,1155)	UI	No value sent for unscheduled study.	
Patient's Name	(0010,0010)	PN	As received from MWL or entered in PDE.	
Patient ID	(0010,0020)	LO	From Modality Worklist or user input to the "MRN" field. MWL value may be edited.	
Patient's Birth Date	(0010,0030)	DA	Same as above, except "Patient's Birth Date" field.	
Patient's Sex	(0010,0040)	CS	Same as above, except "Gender" field.	
Study ID	(0020,0010)	SH	System Generated, starting with 1 and incrementing for each study,	
Performed Station AE Title	(0040,0241)	AE	AE Title from configuration (requires power cycle to use updated setting)	

<b>Attribute Name</b>	<b>Tag</b>	<b>VR</b>	<b>N-CREATE</b>	<b>N-SET</b>
Performed Station Name	(0040,0242)	SH	Same as ‘Performed Station AE Title’ tag above.	
Performed Location	(0040,0243)	SH	If available from MWL, else NULL	
Performed Procedure Step Start Date	(0040,0244)	DA	Actual start date (on close of PDE screen)	
Performed Procedure Step Start Time	(0040,0245)	TM	Actual start time (on close of PDE screen)	
Procedure Code Sequence	(0008,1032)	SQ	Mapped from Requested Procedure Code Sequence (0032,1064) from MWL No value sent for unscheduled study.	As received from MWL No value sent for unscheduled study.
>Code Value	(0008,0100)	SH	As received from MWL No value sent for unscheduled study.	As received from MWL No value sent for unscheduled study.
>Coding Scheme Designator	(0008,0102)	SH	As received from MWL No value sent for unscheduled study.	As received from MWL No value sent for unscheduled study.
>Coding Scheme Version	(0008,0103)	SH	As received from MWL No value sent for unscheduled study.	As received from MWL No value sent for unscheduled study.
>Code Meaning	(0008,0104)	LO	As received from MWL No value sent for unscheduled study.	As received from MWL No value sent for unscheduled study.
Performed Procedure Step End Date	(0040,0250)	DA	Zero length	Actual end date
Performed Procedure Step End Time	(0040,0251)	TM	Zero length	Actual end time
Performed Procedure Step Status	(0040,0252)	CS	IN PROGRESS	COMPLETED or DISCONTINUED
Performed Procedure Step ID	(0040,0253)	SH	Auto generated in the format, <YYYYMMDD.HHMMSS>	
Performed Procedure Step Description	(0040,0254)	LO	Set from “Study Description” field in PDE, else mapped from Requested Procedure Description in MWL.	
Performed Procedure Type Description	(0040,0255)	LO	If present in MWL, else “Indication” field in PDE.	
Performed Protocol Code Sequence	(0040,0260)	SQ	Zero length, or mapped from MWL Scheduled Protocol Code Sq (0040,0008)	Same
>Code Value	(0008,0100)	SH	As received from MWL	As received from MWL

<b>Attribute Name</b>	<b>Tag</b>	<b>VR</b>	<b>N-CREATE</b>	<b>N-SET</b>
			No value sent for unscheduled study.	No value sent for unscheduled study.
>Coding Scheme Designator	(0008,0102)	SH	As received from MWL No value sent for unscheduled study.	As received from MWL No value sent for unscheduled study.
>Code Meaning	(0008,0104)	LO	As received from MWL No value sent for unscheduled study.	As received from MWL No value sent for unscheduled study.
Scheduled Step Attributes Sequence	(0040,0270)	SQ		
> Accession Number	(0008,0050)	SH	From MWL or user PDE input. MWL value may be edited.	
> Referenced Study Sequence	(0008,1110)	SQ	One item per item in the MWL Reference Study Sequence. Absent if unscheduled.	
>> Referenced SOP Class UID	(0008,1150)	UI	Same value as in of the Reference Study Sequence in the MWL	
>> Referenced SOP Instance UID	(0008,1155)	UI	Same value as in of the Reference Study Sequence in the MWL	
> Study Instance UID	(0020,000D)	UI	Same value as in MWL attribute or auto generated	
> Requested Procedure Description	(0032,1060)	LO	Same value as in MWL attribute, 1 <sup>st</sup> Choice, from "Study Description" in PDE, else NULL	
> Scheduled Procedure Step Description	(0040,0007)	LO	Same value as in MWL attribute, else NULL	
> Scheduled Protocol Code Sequence	(0040,0008)	SQ	Same value as in MWL attribute, else NULL	
>>Code Value	(0008,0100)	SH	Same value as in MWL attribute, else NULL	
>>Coding Scheme Designator	(0008,0102)	SH	Same value as in MWL attribute, else NULL	
>>Code Meaning	(0008,0104)	LO	Same value as in MWL attribute, else NULL	
> Scheduled Procedure Step ID	(0040,0009)	SH	Same value as in MWL attribute, else NULL	
> Requested Procedure ID	(0040,1001)	SH	Same value as in MWL attribute, else NULL	
Performed Series Sequence	(0040,0340)	SQ		One item per acquired series

<b>Attribute Name</b>	<b>Tag</b>	<b>VR</b>	<b>N-CREATE</b>	<b>N-SET</b>
> Retrieve AE Title	(0008,0054)	AE	Zero Length	Same
> Series Description	(0008,103E)	LO	Zero Length	Same
> Performing Physician's Name	(0008,1050)	PN	From the "Performed by" field in PDE	From the "Performed by" field in PDE
> Operator's Name	(0008,1070)	PN	From the "Performed by" field in PDE	Same
> Referenced Image Sequence	(0008,1140)	SQ	Zero Length	Zero Length
>> Referenced SOP Class UID	(0008,1150)	UI		
>> Referenced SOP Instance UID	(0008,1155)	UI		
> Protocol Name	(0018,1030)	LO	"Free Form"	"Free Form"
> Series Instance UID	(0020,000E)	UI	Auto Generated	Same
> Referenced Non-Image Composite SOP Instance Sequence	(0040,0220)	SQ	Zero Length	Zero Length

#### **4.2.2.4 Association Acceptance Policy**

The Workflow Application Entity does not accept Associations.

#### 4.2.3 Hardcopy Application Entity Specification

##### 4.2.3.1 SOP Classes

ClearVue 350/550/650/850 3.1 provide Standard Conformance to the following SOP Classes:

**Table 31  
SOP CLASSES FOR AE HARDCOPY**

SOP Class Name	SOP Class UID	SCU	SCP
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Yes	No
Basic Color Print Management Meta	1.2.840.10008.5.1.1.18	Yes	No

The Print Meta SOP Classes are defined by the following set of supported SOP Classes:

- Basic Film Session SOP Class
- Basic Film Box SOP Class
- Basic Grayscale ( or Color) Image Box SOP Class
- Printer SOP Class

Important note about printing by ClearVue 350/550/650/850 3.1:

- The number of Film Boxes per session is one
- The number of images per Film Box is one
- Most image formatting and layout is performed by ClearVue 350/550/650/850 3.1 resulting in a single rather large dataset sent to the printer
- ClearVue 350/550/650/850 3.1 will release the associations after the print command (N-Action-Rq) is sent. It will not hold the association open to receive the printer's N-Event-Report message.

##### 4.2.3.2 Association Establishment Policy

###### 4.2.3.2.1 General

The DICOM standard application context name for DICOM 3.0 is always proposed:

**Table 32  
DICOM APPLICATION CONTEXT FOR AE HARDCOPY**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

###### 4.2.3.2.2 Number of Associations

ClearVue 350/550/650/850 3.1 initiates one Association at a time for each configured hardcopy device. Multiple hardcopy devices can be configured.

**Table 33  
NUMBER OF ASSOCIATIONS INITIATED FOR AE HARDCOPY**

Maximum number of simultaneous Associations	2
---	---

Note: One Black and White only Printer/Server and one Color Printer/Server.

#### **4.2.3.2.3 Asynchronous Nature**

ClearVue 350/550/650/850 3.1 does not support asynchronous communication (multiple outstanding transactions over a single Association).

**Table 34  
ASYNCHRONOUS NATURE AS A SCU FOR AE HARDCOPY**

Maximum number of outstanding asynchronous transactions	1
---	---

#### **4.2.3.2.4 Implementation Identifying Information**

The implementation information for this Application Entity is:

**Table 35  
DICOM IMPLEMENTATION CLASS AND VERSION FOR AE HARDCOPY**


Implementation Version Name	Implementation Class UID
ClearVue 350_3.1	1.3.46.670589.14.5000.310
ClearVue 550_3.1	1.3.46.670589.14.6000.310
ClearVue 650_3.1	1.3.46.670589.14.9002.310
ClearVue 850_3.1	1.3.46.670589.14.9004.310

#### **4.2.3.3 Association Initiation Policy**

##### **4.2.3.3.1 Activity – Film Images**

###### **4.2.3.3.1.1 Description and Sequencing of Activities**

The system composes images onto film sheets and sends print requests to job queue.

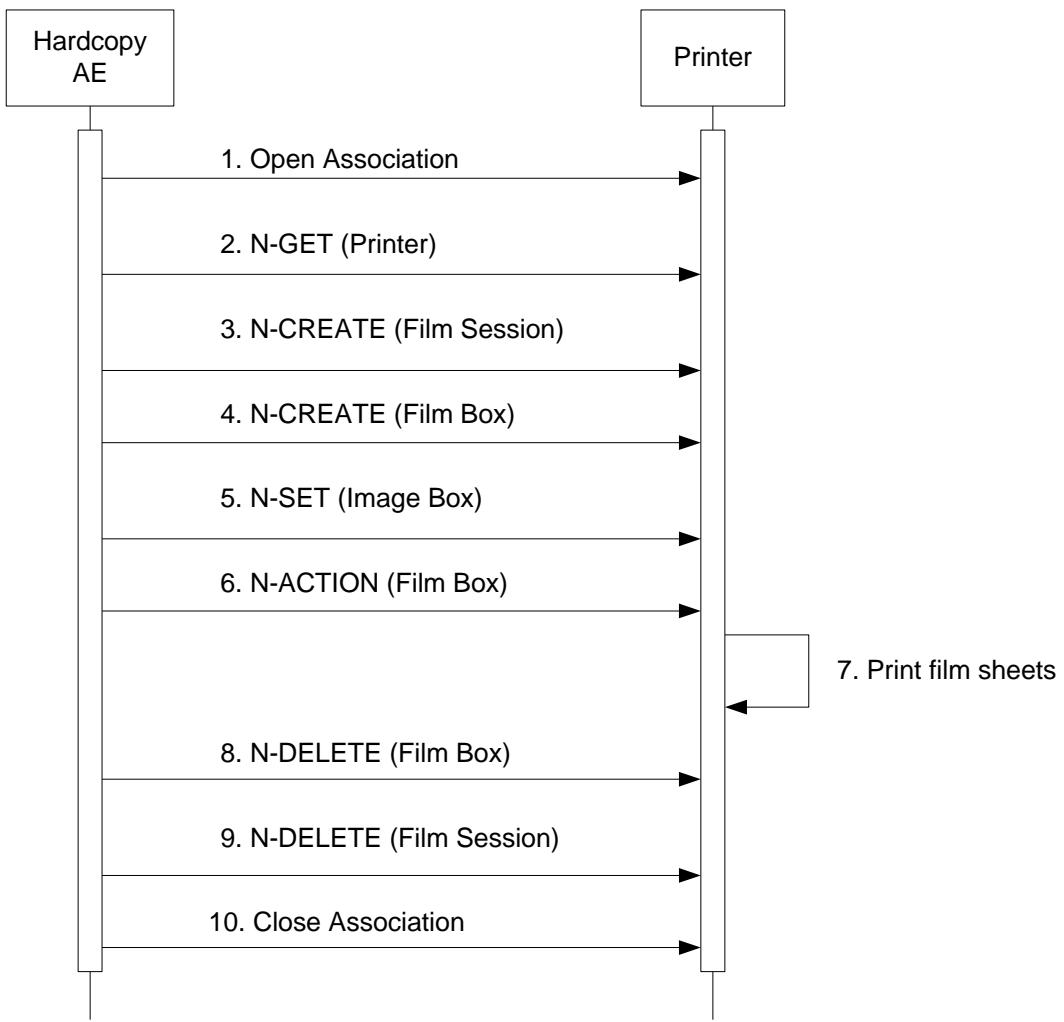

**Figure 7**  
SEQUENCING OF ACTIVITY – PRINT IMAGES

Figure 7 illustrates a typical sequence of DIMSE messages sent over an association between Hardcopy AE and a Printer. Two DICOM Printers may be simultaneously configured, one for BW and one for Color prints.

If both BW and Color printers are configured and selected, the images that contain color data, i.e., Color Flow Doppler or "Chroma" will be sent to the Color printer, and all other images will be sent to the BW printer.

In "Send as you go", images will be sent to the printer when the number needed to fill the configured format is met, until "End Exam" is pressed when page(s) that have not been exported will be sent. In "Batch mode" or "Manual", each formatted page is sent as soon as it is composed by the system. If fewer images than a full page are sent, the remaining blank spaces will be sent black.

Status of the print-job is reported through the Job Manager (CNTL-J). Only one job will be active at a time for each separate hardcopy device. If any response from the remote application contains a status other than Success or Warning, the association is aborted and the related job is switched to a failed state. It can be restarted any time by user interaction.

#### 4.2.3.3.1.2 Proposed Presentation Contexts

Table 36 shows the Presentation Contexts ClearVue 350/550/650/850 3.1 is capable of proposing.

**Table 36  
PROPOSED PRESENTATION CONTEXTS FOR ACTIVITY FILM IMAGES**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Basic Grayscale Print Management Meta	1.2.840.10008.5.1 .1.9	Explicit VR LittleEndian* Implicit VR LittleEndian	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Basic Color Print Management Meta	1.2.840.10008.5.1 .1.18	Explicit VR LittleEndian* Implicit VR LittleEndian	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None

\* Note: If the worklist server accepts Explicit VR LittleEndian and Implicit VR LittleEndian then ClearVue 350/550/650/850 3.1 will use Explicit VR LittleEndian Transfer Syntax.

#### 4.2.3.3.1.3 Common SOP Specific Conformance for all Print SOP Classes

Table 37 summarizes the general behavior of Hardcopy AE during communication failure. This behavior is common for all SOP Classes supported by Hardcopy AE.

**Table 37  
HARDCOPY COMMUNICATION FAILURE BEHAVIOR**

Exception	Behavior
Timeout	The Association is aborted and reported as "Failed."
Association aborted by the SCP or network layers	"Network Communication Failure" is reported.

#### 4.2.3.3.1.4 SOP Specific Conformance for the Printer SOP Class

Hardcopy AE supports the following DIMSE operations and notifications for the Printer SOP Class:

- N-GET

Details of the supported attributes and status handling behavior are described in the following subsections.

##### 4.2.3.3.1.4.1 Printer SOP Class Operations (N-GET)

Hardcopy AE uses the Printer SOP Class N-GET operation to obtain information about the current printer status. Table 38 lists the attributes obtained via N-GET.

**Table 38**  
**PRINTER SOP CLASS N-GET RESPONSE ATTRIBUTES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Printer Status	(2110,0010)	CS	Provided by Printer	ALWAYS	Printer
Printer Status Info	(2110,0020)	CS	Provided by Printer	ALWAYS	Printer

The Printer Status information is evaluated as follows:

1. If Printer status (2110,0010) is NORMAL, the print-job continues to be printed.
2. If Printer status (2110,0010) is FAILURE, the print-job is retried as configured then is marked as failed.
3. If Printer status (2110,0010) is WARNING, the print-job continues to be printed.

Table 39 summarizes the behavior of Hardcopy AE when encountering status codes in an N-GET response.

**Table 39**  
**PRINTER SOP CLASS N-GET RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The request to get printer status information was success.
*	*	Any other status code.	Same as Timeout above.

#### **4.2.3.3.1.4.2 Printer SOP Class Notifications (N-EVENT-REPORT)**

Hardcopy AE is capable of receiving an N-EVENT-REPORT request at any time during an association.

Table 40 summarizes the behavior of Hardcopy AE when receiving Event Types within the N-EVENT-REPORT.

**Table 40**  
**PRINTER SOP CLASS N-EVENT-REPORT BEHAVIOUR**

Event Type Name	Event Type ID	Behavior
Normal	1	The print-job continues to be printed.
Warning	2	The print-job. For user-recoverable warnings, the job retries as configured. Then marked as failed.
Failure	3	The job retries as configured print then is marked as failed.
*	*	Status code of 0113H

Table 41 summarizes the reasons for returning specific status codes in an N-EVENT-REPORT response.

**Table 41**  
**PRINTER SOP CLASS N-EVENT-REPORT RESPONSE STATUS REASONS**

Service Status	Further Meaning	Error Code	Reasons
Success	Success	0000	The notification event has been successfully received.
Failure	No Such Event Type	0113H	An invalid Event Type ID was supplied in the N-EVENT-REPORT request.
Failure	Processing Failure	0110H	An internal error occurred during processing of the N-EVENT-REPORT. A short description of the error will be returned in Error Comment (0000,0902).

#### 4.2.3.3.1.5 SOP Specific Conformance for the Film Session SOP Class

Hardcopy AE supports the following DIMSE operations for the Film Session SOP Class:

- N-CREATE

Details of the supported attributes and status handling behavior are described in the following subsections.

##### 4.2.3.3.1.5.1 Film Session SOP Class Operations (N-CREATE)

Table 42 lists the attributes supplied in an N-CREATE Request.

**Table 42**  
**FILM SESSION SOP CLASS N-CREATE REQUEST ATTRIBUTES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Number of Copies	(2000,0010)	IS	Default 1. Range is 1 – 99.	ALWAYS	USER
Print Priority	(2000,0020)	CS	HIGH	ALWAYS	AUTO
Medium Type	(2000,0030)	CS	BLUE FILM, CLEAR FILM or PAPER and 'Printer Specific' options*	VNAP	USER
Film Destination	(2000,0040)	CS	MAGAZINE or PROCESSOR and 'Printer Specific' options *	ALWAYS	USER
Film Session Label	(2000,0050)	LO	Philips Medical Systems	ALWAYS	AUTO

\*Dependent on the specific printer selected

Table 43 summarizes the behavior of Hardcopy AE when encountering status codes in an N-CREATE response.

**Table 43**  
**FILM SESSION SOP CLASS N-CREATE RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.
Warning	Attribute Value Out of Range	0116H	System continues operations.
Warning	Attribute List Error	0107H	Same as above.
*	*	Any other status	The Association is aborted and the print-job fails.

Service Status	Further Meaning	Error Code	Behavior
		code.	

#### 4.2.3.3.1.5.2 Film Session SOP Class Operations (N-DELETE)

The behavior of Hardcopy AE when encountering status codes in an N-DELETE response is summarized in the Table below:

**Table 44  
PRINTER SOP CLASS N-DELETE RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.
*	*	Any other status code.	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.

#### 4.2.3.3.1.6 SOP Specific Conformance for the Film Box SOP Class

Hardcopy AE supports the following DIMSE operations for the Film Box SOP Class:

- N-CREATE
- N-ACTION

Details of the supported attributes and status handling behavior are described in the following subsections.

#### 4.2.3.3.1.6.1 Film Box SOP Class Operations (N-CREATE)

Table 47 lists the attributes supplied in an N-CREATE Request.

**Table 47  
FILM BOX SOP CLASS N-CREATE REQUEST ATTRIBUTES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Image Display Format	(2010,0010)	ST	STANDARD\1,1	ALWAYS	AUTO
Referenced Film Session Sequence	(2010,0500)	SQ		ALWAYS	AUTO
>Referenced SOP Class UID	(0008,1150)	UI	1.2.840.10008.5.1.1.1	ALWAYS	AUTO
>Referenced SOP Instance UID	(0008,1155)	UI	From created Film Session SOP Instance	ALWAYS	AUTO
Referenced Image Box Sequence	(2010,0510)	SQ		ALWAYS	AUTO

Attribute Name	Tag	VR	Value	Presence of Value	Source
>Referenced SOP Class UID	(0008,1150)	UI	1.2.840.10008.5.1.1.1	ALWAYS	AUTO
>Referenced SOP Instance UID	(0008,1155)	UI	From created Film Session SOP Instance	ALWAYS	AUTO
Film Orientation	(2010,0040)	CS	Default = PORTRAIT, or LANDSCAPE	ALWAYS	AUTO/USER
Film Size ID	(2010,0050)	CS	Default – 8INX10IN and DICOM Defined Terms: 8INX10IN, 8_5INX11IN, 10INX12IN, 10INX14IN, 11INX14IN, 11INX17IN, 14INX14IN, 14INX17IN, 24CMX24CM, 24CMX30CM, A4, A3 and ‘Printer Specific’ options.	ALWAYS	AUTO/USER
Magnification Type	(2010,0060)	CS	NONE, CUBIC, BILINEAR, REPLICATE, ‘Printer Specific’ options	ALWAYS	USER
Min Density	(2010,0120)	US	User editable 0-999	ANAP	USER
Max Density	(2010,0130)	US	User editable 0-999	ALWAYS	USER
Trim	(2010,0140)	CS	NO	ALWAYS	AUTO
Configuration Information	(2010,0150)	ST	DICOM supports a “config ID#” or a “config string”. Check “Printer Catalog” for appropriate data.	ALWAYS	USER

Table 48 summarizes the behavior of Hardcopy AE when encountering status codes in an N-CREATE response.

**Table 48**  
**FILM BOX SOP CLASS N-CREATE RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.
Warning	Requested Max Density outside of printer’s operating range	B605H	The N-CREATE operation is considered successful but the status meaning is logged.
*	*	Any other status code.	The Association is aborted and the job failed.

#### 4.2.3.3.1.6.2 Film Box SOP Class Operations (N-ACTION)

The Hardcopy AE issues an N-ACTION Request to instruct the Print SCP to print the contents of the Film Box.

Table 49 summarizes the behavior of Hardcopy AE when encountering status codes in an N-ACTION response.

**Table 49**  
**FILM BOX SOP CLASS N-ACTION RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully. The film has been accepted for printing.
Warning	Film Box SOP Instance hierarchy does not contain Image Box SOP Instances (empty page)	B603H	The Association is aborted and the job is failed.
Failure	Unable to create Print Job SOP Instance; print queue is full.	C602	Same as B603H above.
*	*	Any other status code.	Same as B603H above.

#### 4.2.3.3.1.7 SOP Specific Conformance for the Image Box SOP Class

Hardcopy AE supports the following DIMSE operations for the Image Box SOP Class:

- N-SET

Details of the supported attributes and status handling behavior are described in the following subsections.

##### 4.2.3.3.1.7.1 Basic Grayscale Image Box SOP Class Operations (N-SET)

Table 50 lists the attributes supplied in an N-SET Request for Basic Grayscale Image Box SOP Class.

**Table 50**  
**IMAGE BOX SOP CLASS N-SET REQUEST ATTRIBUTES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Image Box Position	(2020,0010)	US	1	ALWAYS	AUTO
Basic Grayscale Image Sequence	(2020,0110)	SQ	Used for BW (Monochrome2) print	ALWAYS*	AUTO
>Samples Per Pixel	(0028,0002)	US	1 for Monochrome2 3 for RGB	ALWAYS	AUTO
>Photometric Interpretation	(0028,0004)	CS	MONOCHROME2 RGB	ALWAYS	AUTO
>Rows	(0028,0010)	US	Depends on film size	ALWAYS	See Printer Catalog
>Columns	(0028,0011)	US	Depends on film size	ALWAYS	See Printer Catalog
>Pixel Aspect Ratio	(0028,0034)	US	Depends on aspect ratio	ANAP	AUTO
>Bits Allocated	(0028,0100)	US	8	ALWAYS	AUTO
>Bits Stored	(0028,0101)	US	8	ALWAYS	AUTO
>High Bit	(0028,0102)	US	7	ALWAYS	AUTO

>Pixel Representation	(0028,0103)	US	0		ALWAYS	AUTO
>Pixel Data	(7FE0,0010)	OW	Pixels of rendered film sheet.		ALWAYS	AUTO
Polarity	(2020,0020)	CS	NORMAL		ALWAYS	AUTO

\* Mutually exclusive attributes

Table 51 summarizes the behavior of Hardcopy AE when encountering status codes in an N-SET response.

**Table 51  
IMAGE BOX SOP CLASS N-SET RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.
Failure	Insufficient memory in printer to store the image.	C605	The Association is aborted and the job is failed.
*	*	Any other status code.	Same as C605 above.

#### 4.2.3.3.1.7.2 Basic Color Image Box SOP Class Operations (N-SET)

Table 52 lists the attributes supplied in an N-SET Request for Basic Color Image Box SOP Class.

**Table 52  
IMAGE BOX SOP CLASS N-SET REQUEST ATTRIBUTES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Image Box Position	(2020,0010)	US	1	ALWAYS	AUTO
Basic Color Image Sequence	(2020,0111)	SQ	Used for Color (RGB) print	ALWAYS*	AUTO
>Samples Per Pixel	(0028,0002)	US	1 for Monochrome2 3 for RGB	ALWAYS	AUTO
>Photometric Interpretation	(0028,0004)	CS	MONOCHROME2 RGB	ALWAYS	AUTO
>Planar Configuration	(0028,0006)	US	“01” for Color-by-plane “00” for Color-by-Pixel, Used only for RGB print.	ANAP	USER
>Rows	(0028,0010)	US	Depends on film size	ALWAYS	See Printer Catalog
>Columns	(0028,0011)	US	Depends on film size	ALWAYS	See Printer Catalog
>Pixel Aspect Ratio	(0028,0034)	US	Depends on aspect ratio	ANAP	AUTO
>Bits Allocated	(0028,0100)	US	8	ALWAYS	AUTO

>Bits Stored	(0028,0101)	US	8		ALWAYS	AUTO
>High Bit	(0028,0102)	US	7		ALWAYS	AUTO
>Pixel Representation	(0028,0103)	US	0		ALWAYS	AUTO
>Pixel Data	(7FE0,0010)	OW	Pixels of rendered film sheet.		ALWAYS	AUTO
Polarity	(2020,0020)	CS	NORMAL		ALWAYS	AUTO

\* Mutually exclusive attributes

Table 53 summarizes the behavior of Hardcopy AE when encountering status codes in an N-SET response.

**Table 53  
IMAGE BOX SOP CLASS N-SET RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.
Failure	Insufficient memory in printer to store the image.	C605	The Association is aborted and the job is failed.
*	*	Any other status code.	Same as C605 above.

#### 4.2.3.4 Association Acceptance Policy

The Hardcopy Application Entity does not accept Associations.

#### 4.2.4 Verification Application Entity specification

##### 4.2.4.1 SOP Class

ClearVue 350/550/650/850 3.1 provide Standard Conformance to the following SOP Class:

**Table 54.1  
SOP CLASSES FOR AE VERIFICATION**

SOP Class Name	SOP Class UID	SCU	SCP
Verification	1.2.840.10008.1.1	Yes	Yes

#### 4.2.4.2 Association Establishment Policy

##### 4.2.4.2.1 General

The DICOM standard application context name for DICOM 3.0 is always proposed:

**Table 54.2  
DICOM APPLICATION CONTEXT FOR AE VERIFICATION**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

#### 4.2.4.2.2 Number of Associations

ClearVue 350/550/650/850 3.1 initiates one Association at a time for a Verification request.

**Table 54.3  
NUMBER OF ASSOCIATIONS INITIATED FOR AE VERIFICATION**

Maximum number of simultaneous Associations	Up to 10, one for each configured remote device
---	---

**Table 54.4  
NUMBER OF ASSOCIATIONS ACCEPTED FOR AE VERIFICATION**

Maximum number of simultaneous Associations	Unlimited - calling AE must be already configured in ClearVue 350/550/650/850 3.1.
---	--

#### 4.2.4.2.3 Asynchronous Nature

ClearVue 350/550/650/850 3.1 does not support asynchronous communication (multiple outstanding transactions over a single Association).

**Table 54.5  
ASYNCHRONOUS NATURE AS A SCU FOR AE VERIFICATION**

Maximum number of outstanding asynchronous transactions	1
---	---

#### 4.2.4.2.4 Implementation Identifying Information

The implementation information for this Application Entity is:

**Table 54.6  
DICOM IMPLEMENTATION CLASS AND VERSION FOR AE VERIFICATION**

Implementation Version Name	Implementation Class UID
ClearVue 350_3.1	1.3.46.670589.14.5000.310
ClearVue 550_3.1	1.3.46.670589.14.6000.310
ClearVue 650_3.1	1.3.46.670589.14.9002.310
ClearVue 850_3.1	1.3.46.670589.14.9004.310

#### 4.2.4.3 Association Initiation Policy

##### 4.2.4.3.1 Activity – Verify as SCU and SCP

##### 4.2.4.3.2 Description and Sequencing of Activities


**SCU:** The user can verify the existence of a DICOM server on the hospitals network, through a button in the 'DICOM Setup' screen. When the user presses this button, ClearVue 350/550/650/850 3.1 will initiate the association.

Only one association is established for each verification attempt. However, the proposed presentation contexts not only includes the 'Verification SOP class' but also includes all the SOP classes that ClearVue 350/550/650/850 3.1 could possibly be connected to as Servers. This is done in order to retrieve the capabilities of the remote Server.

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Implicit VR LittleEndian	1.2.840.10008.1.2	SCU /SCP	None
US Image Storage	1.2.840.10008.5.1. 4.1.1.6.1	Implicit VR LittleEndian* Explicit VR LittleEndian JPEG Lossy Baseline RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.4. 50 1.2.840.10008.1.2.5	SCU	None
US Multiframe Image Storage	1.2.840.10008.5.1. 4.1.1.3.1	Implicit VR LittleEndian Explicit VR LittleEndian JPEG Lossy Baseline RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.4. 50 1.2.840.10008.1.2.5	SCU	None
Comprehensive Structured Report Storage	1.2.840.10008.5.1. 4.1.1.88.33	Implicit VR LittleEndian Explicit VR LittleEndian	1.2.840.10008.1.2 1.2.840.10008.1.2.1	SCU	None
Storage Commitment Push Model	1.2.840.10008.1.20. .1	Implicit VR LittleEndian Explicit VR LittleEndian	1.2.840.10008.1.2 1.2.840.10008.1.2.1	SCU	None
Modality Worklist Information Model – FIND	1.2.840.10008.5.1. 4.31	Explicit VR LittleEndian* Implicit VR LittleEndian	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Modality Performed Procedure Step	1.2.840.10008.3.1. 2.3.3	Explicit VR LittleEndian* Implicit VR LittleEndian	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Basic Grayscale Print Management Meta	1.2.840.10008.5.1. 1.9	Explicit VR LittleEndian* Implicit VR LittleEndian	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None
Basic Color Print Management Meta	1.2.840.10008.5.1. 1.18	Explicit VR LittleEndian* Implicit VR LittleEndian	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU	None


ClearVue 350/550/650/850 3.1 initiates an Association in order to issue:

- C-ECHO request according to the Verification SOP Class.

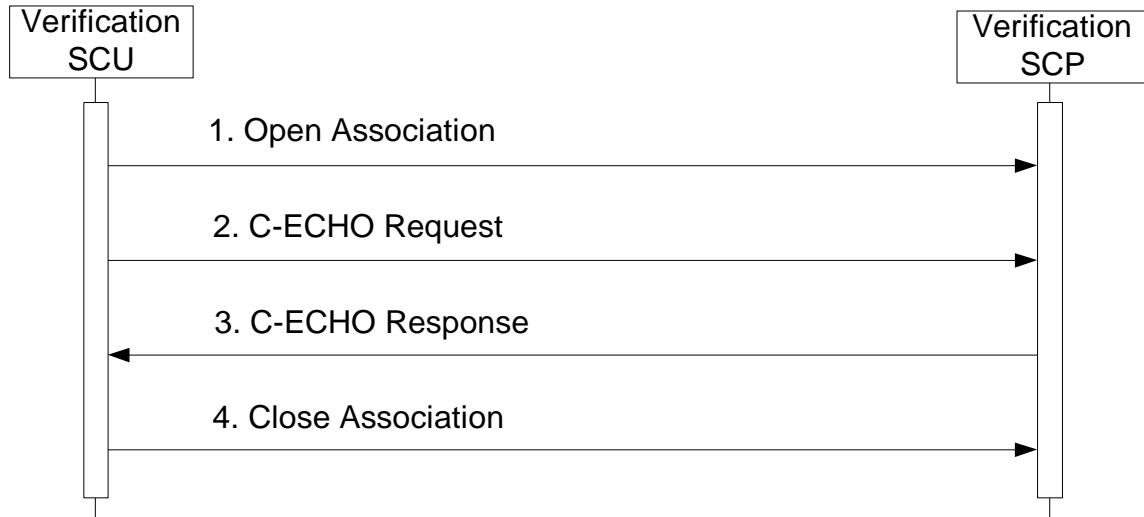

**Figure 8a**  
SEQUENCING OF ACTIVITY – ISSUE VERIFY

**SCP:** The system listens on the port configured on the “This System” Configuration screen for Verification requests initiated by other remote devices. The calling device AE must already be configured as a remote device in ClearVue 350/550/650/850 3.1 or the association is rejected.

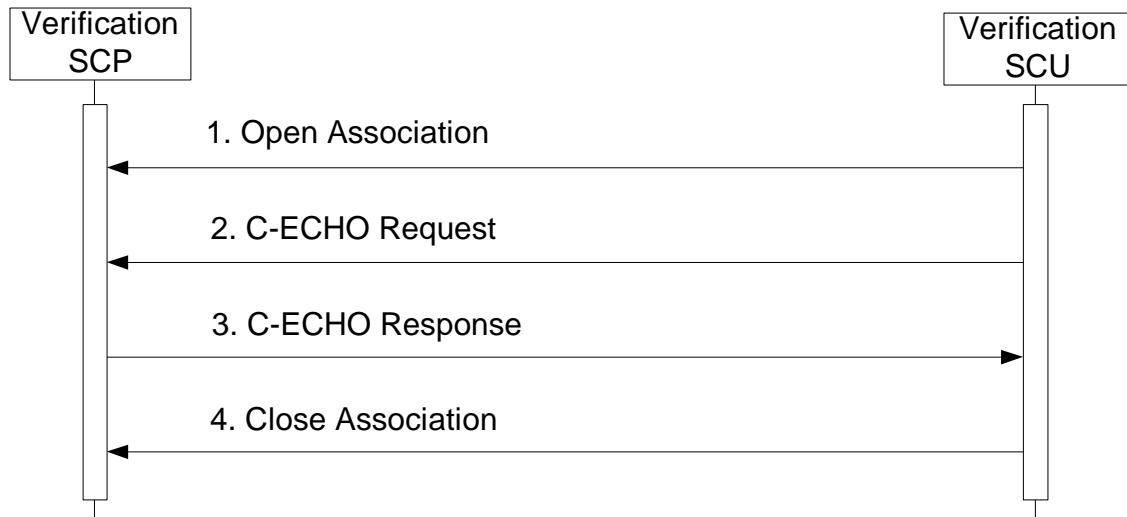

**Figure 8b**  
SEQUENCING OF ACTIVITY – RECEIVE VERIFY

#### 4.2.4.3.3 Proposed Presentation Contexts

ClearVue 350/550/650/850 3.1 will propose Presentation Contexts as shown in the following table:

**Table 54.7  
PROPOSED PRESENTATION CONTEXTS FOR ACTIVITY VERIFICATION**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Explicit VR Little Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2	SCU /SCP	None

#### 4.2.4.3.4 SOP Specific Conformance for Verification

Table 54.8 summarizes the behavior of ClearVue 350/550/650/850 3.1 when receiving status codes in a C-ECHO response.

A message will appear on the user interface if ClearVue 350/550/650/850 3.1 receives any other SCP response status than "Success."

**Table 54.8  
VERIFICATION C-ECHO RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Error Code	Behavior
Success		0000	Device Status is set to: Verified
Refused	Out of Resources	A700	Device Status is set to: Not Verified
Failed	Unable to Process	C000 – CFFF	Same as "Refused" above.
*	*	Any other status code.	Same as "Refused" above.

#### 4.2.4.3.4.1 Verification SOP Class Operations (C-ECHO)

#### 4.2.4.3.5 Association Acceptance Policy

#### 4.2.4.3.5.1 Verification SOP Class Notifications

Association Negotiation Request message contents for each DICOM device:

Device Type	SOP Classes Requested	Additional Notes
Primary or Secondary Storage SCP	US Image Storage US Multiframe Storage Verification	
Storage Commit SCP	Storage Commitment Verification	
SR Storage SCP	Comprehensive Structured Report Storage	

	Verification	
SR Storage Commit SCP	Storage Commitment Verification	
B&W Printer SCP	Basic Grayscale META Print Verification	Color images may be sent to a bw printer if it supports converting to BW.
Color Printer SCP	Basic Color META Print Verification	May be the same printer if color is also supported.
MWL SCP	Modality Worklist Verification	MWL query settings are located in Setups > System > DICOM > DICOM Preset > Change Settings for current preset > Modify in Roles > MWL SCP – Advanced > Set Modality Worklist Query page.
PPS SCP	Modality Performed Procedure Step Verification	

## 4.3 PHYSICAL NETWORK INTERFACES

### 4.3.1 Supported Communication Stacks

#### 4.3.1.1 TCP/IP Stack

ClearVue 350/550/650/850 3.1 provides DICOM TCP/IP Network Communication Support as defined in Part 8 of the DICOM Standard.

### 4.3.2 Physical Network Interface

The ClearVue 350/550/650/850 3.1 system supports one network interface at a time. The following physical network interfaces are available:

**Table 52  
SUPPORTED PHYSICAL NETWORK INTERFACE**

1) Ethernet 10/100/1000BaseT, RJ-45, UTP, STP; AutoDetect Speed, Full or Half Duplex
--

## 4.4 CONFIGURATION

### AE Title/Presentation Address Mapping

The DICOM setup screen allows the user to configure a significant number of options including (but not limited to):

- For the ClearVue 350/550/650/850 3.1 system, its AE Title, IP Address and Port number, Wired or Wireless connection.
- For DICOM servers, their AE Title, Port number, IP address.
- For Storage SCP's and for media storage, the image format.

Advanced settings (including Photometric Interpretation settings: MONOCHROME2, RGB, Palette color and YBR\_FULL\_422 and Transfer Syntaxes: Implicit LittleEndian, Explicit LittleEndian, RLE and JPEG for images), loop timing, pixel spacing, and display compensation.

- For DICOM Printers, many DICOM configuration settings

- For a MWL server, the query parameters: scheduled procedure start range, modality, AE Title.
- ClearVue 350/550/650/850 3.1 also supports QLAB where the user can perform QLAB quantification on the system of images acquired by the system.

The Devices Configuration section allows the following device types to be configured:

Device Type	Supported SOPs
Primary or Secondary Storage SCP	Ultrasound Store Ultrasound Multiframe Store
Storage Commit SCP	Storage Commitment Push Model
SR Storage SCP	Comprehensive Structured Report Store
SR Storage Commit SCP	Storage Commitment Push Model
B&W Printer SCP	Basic Grayscale Print Meta
Color Printer SCP	Basic Color Print Meta
MWL SCP	Modality Worklist
PPS SCP	Modality Performed Procedure Step

To configure a single server that supports image store, commitment and PPS, then a “Server” entry must be configured under “Setups>DICOM...>Change Settings for DICOM Preset>Servers and Roles>Servers”. Enter a Name (an ‘alias’ used in the system UI only), the appropriate AE Title, IP Address, Port number and timeout values. “Ping” sends an ICMP ping message to the address and a DICOM Verification Association message is sent to the Port and AE Title. A success message is displayed if all is configured correctly at this level. If not, an error message dialog is displayed indicating possible reasons and suggested corrective actions. Hit “Done” to continue to Role definition.

Once the server data is defined, then its role and options are configured. For each role, as in Primary Storage SCP, MPPS SCP, etc, select the server’s alias name from the list. If “Advanced” options are available, select the “Advanced” button to access them,

When Role configuration is completed and “Done” is selected under “Roles”, then another set of Verification messages are sent to each server confirming network connectivity and DICOM role support. A dialog box updates as the tasks are in progress. No error messages indicates successful configuration.

#### 4.4.1.1 Local AE Title

All local AEs use the same AE Title and TCP/IP Port configured via the Setups>DICOM...>Change Settings for DICOM Setup>This System screen. The system listens on the configured Port only for Verification requests and Storage Commitment N-Event reports. The system supports Static Addressing or DHCP to receive its IP Address, Subnet Mask and Default Gateway address.

#### 4.4.1.2 Remote AE Title/Presentation Address Mapping

The AE Titles, IP Addresses and Port numbers of remote applications are manually configured using the Setups>DICOM...>Change Settings for DICOM Preset>Servers and Roles>. The remote system’s IP Address may be entered manually if known or the Host Name of the remote device may be entered and resolved by the DNS if the network includes this service.

#### 4.4.1.2.2 Workflow

Setup is used to set the AE Title, Port number and IP Address the remote MWL SCP. Multiple MWL SCPs may be defined, but only a single remote MWL SCP can be selected at a time.

The default MWL query uses Modality = “US”. This may be changed in the “Set Modality Worklist Query Customizable Queries” definition page. Alternately, “ANY” modality may be selected.

“AE Title” may be selected as the system’s or a custom query value may be defined for a different AE Title or for “ANY”.

The Start Date defaults to “Today” but may be modified to be “All Dates”, or a Date Range that may be 0 - 99 days (or hours) Prior plus the next 0 -99 days.

The automated polling interval range for sending MWL queries is between 1 and 32,767 minutes, defaulting to 10 minutes.

Setup is used to set the AE Title, Port number and IP Address of the remote MPPS SCP. Multiple MPPS SCPs may be defined, but only a single remote MPPS SCP can be selected at a time.

#### **4.4.1.2.3 Hardcopy**

Setup is used to set the AE Titles, Port numbers and IP Addresses for the remote Print SCPs.


Multiple remote Print SCPs can be defined, but up to one Grayscale and one Color Print SCP may be selected at a time.

Automatic sending of color images to the color printer and BW images to the BW printer is selectable in the Setups>DICOM...>Change Settings for DICOM Preset>Servers and Roles>BW or Color Printer SCP Advanced settings.

## 5 MEDIA STORAGE

### 5.1 IMPLEMENTATION MODEL

#### 5.1.1 Application Data Flow

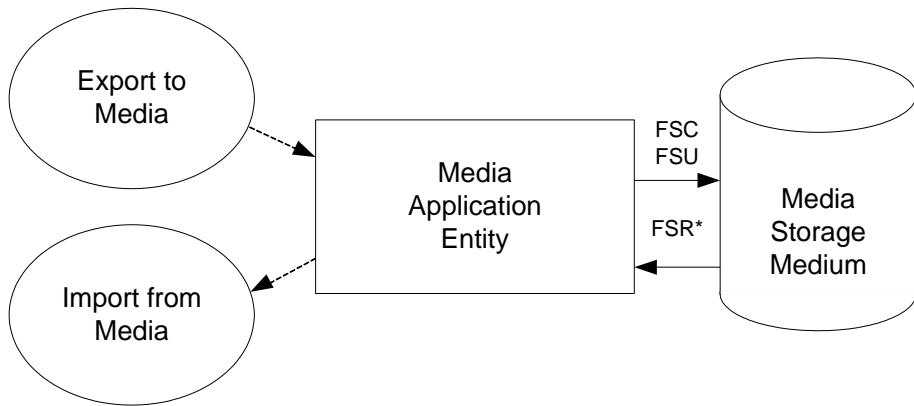

**Figure 9**  
APPLICATION DATA FLOW DIAGRAM FOR MEDIA STORAGE

- The Media Application Entity exports Images and Structured Reports to a removable storage medium. It is associated with the local real-world activity “Export” using the configured export selection parameters for selected patients’ data (images and / or Structured Reports). For “Import”, the system will not read in Structured Reports.
- Throughout this section, the term “Media” refers to any of the media listed below which is in use.

ClearVue 350/550/650/850 3.1 will support the use of most writable media including CD-R, CD-RW, DVD-R, DVD+R, DVD-RW, DVD+RW, and USB devices. The DICOM structure will be the same regardless of media used.

#### 5.1.2 Functional Definition of AEs

##### 5.1.2.1 Functional Definition of Media Application Entity

Using “Export” will pass the currently selected patients’ exams or individually selected images to the Media Application Entity. The contents of each export job will be written to the selected media destination. The size of the selected media is used to determine and display the number of media required for the export. When a device is filled to capacity, the system will prompt the user for addition media and continue.

##### 5.1.3 Sequencing of Real-World Activities

At least one image must exist and be selected before the Media Application Entity can be invoked. The operator can insert new media at any time. The Media Application Entity will wait indefinitely for media to be inserted before starting to write to the device.

##### 5.1.4 File Meta Information Options

The implementation information written to the File Meta Header in each file is:

**Table 65**  
DICOM IMPLEMENTATION CLASS AND VERSION FOR MEDIA STORAGE

Implementation Version Name	Implementation Class UID

ClearVue 350_3.1	1.3.46.670589.14.5000.310
ClearVue 550_3.1	1.3.46.670589.14.6000.310
ClearVue 650_3.1	1.3.46.670589.14.9002.310
ClearVue 850_3.1	1.3.46.670589.14.9004.310

## 5.2 AE SPECIFICATIONS

### 5.2.1 Media Application Entity Specification

The Media Application Entity provides standard conformance to the DICOM Interchange Option of the Media Storage Service Class. The Application Profiles and roles are listed in

**Table 66  
APPLICATION PROFILES, ACTIVITIES AND ROLES FOR OFFLINE-MEDIA**

Application Profiles Supported	Real World Activity	Role	SC Option
STD-US-SC-MF-CDR STD-GEN-CD*	Send to....Media	FSC	Interchange
STD-US-SC-MF-DVD STD-GEN-DVD STD-GEN-USB-JPEG		FSC, U**	
STD-US-SC-MF-CDR STD-US-SC-MF-DVD STD-GEN-USB-JPEG		R***	

\* Note that Ultrasound-specific Application Profiles do not include Structured Report SOP Class, necessitating addition of the STD-GEN CDR and DVD Application Profiles.

\*\* Update functionality requires DVD+RW, or USB

\*\*\* File Set Reader functionality may be limited only to media created by other ClearVue 350/550/650/850 3.1 systems.

For previously imported studies, ClearVue 350/550/650/850 3.1 will export the IODs using the transfer syntax and tags that were used when ClearVue 350/550/650/850 3.1 originally imported the study.

Transfer Syntax and Photometric Interpretation options for removable media

Transfer Syntax	Photometric Interpretation
Uncompressed (DICOM Explicit VR LittleEndian)	Palette Color
Uncompressed (DICOM Explicit VR LittleEndian)	RGB
Uncompressed (DICOM Explicit VR LittleEndian)	MONOCHROME2
RLE (Lossless) Compression	Palette Color
RLE (Lossless) Compression	RGB
RLE (Lossless) Compression	MONOCHROME2
JPEG (Lossy) Compression	YBR_FULL_422

### Reading a DICOM study from removable media

When requested to read the media directory, the ClearVue 350/550/650/850 3.1 Application Entity acts as FSR using the Interchange Option.

Choosing the Import operation from a menu initiates importing images. See the system user manuals for a description of the specific user interface capabilities. ClearVue 350/550/650/850 3.1 doesn't support FSR role for DICOM SR.

### **5.2.1.1 File Meta Information for the Application Entity**

The File-Set Identifier included in the File Meta Header is “”.

### **5.2.1.2 Real-World Activities**

#### **5.2.1.2.1 Activity – Send to Media – “Export”**

The Media Application Entity acts as an FSC using the interchange option when requested to export SOP Instances from the local database to media.

The contents of the export job will be written together with a corresponding DICOMDIR to media. The user can cancel an export job in the job queue.

#### **5.2.1.2.2 Activity – Import from Media – “Import”**

The Media Application Entity acts as an FSR using the interchange option when requested to import SOP Instances from media to the local database.

The Import Studies icon presents the directory of the system or the offline media. Selected exams are transferred from the media to the system for review. Objects transferred to the system retain their original SOP Instance UIDs.

Note: Structured Reports may not be read back into ClearVue 350/550/650/850 3.1.

#### **5.2.1.2.3 Activity – Update to Media – Export”**

The Media Application Entity acts as an FSU using the interchange option when requested to export SOP Instances from the local database to media upon which DICOM data already resides.

The system user selects exams from the system’s directory for transfer to media that already contains data. The DICOMDIR is updated allowing access to original and new data.

#### **5.2.1.2.3.1 Media Storage Application Profiles**

See Table 66 for supported Application Profiles.

#### **5.2.1.2.3.2 Options**

The Media Application Entity supports the SOP Classes and Transfer Syntaxes listed in Table 67.

**Table 67  
IODS, SOP CLASSES AND TRANSFER SYNTAXES FOR OFFLINEMEDIA**

Information Object Definition	SOP Class UID	Transfer Syntax	Transfer Syntax UID
Media Storage Directory Storage	1.2.840.10008.1.3.10	Explicit VR LittleEndian	1.2.840.10008.1.2.1
US Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR LittleEndian JPEG Lossy Baseline RLE	1.2.840.10008.1.2.1 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.5
US Multiframe Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR LittleEndian JPEG Lossy Baseline RLE	1.2.840.10008.1.2.1 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.5
Comprehensive Structured Report Storage*	1.2.840.10008.5.1.4.1.1.88.33	Explicit VR LittleEndian	1.2.840.10008.1.2.1

\* Export only.

## Directory Information Module

All data elements are used as described in DICOM 3.0 Part 3 for Basic Directory Object Definitions. As stated in the Ultrasound Application Profile, “The (DICOMDIR) Directory shall include Directory Records of PATIENT, STUDY, SERIES, IMAGE and SR DOCUMENT corresponding to the information object files in the File-set”. These are present when writing media. Given this requirement, ClearVue 350/550/650/850 3.1 uses these directory records to identify the study to import with the exception of SR DOCUMENT. If there are DICOM image files on the import media that do not appear in the DICOMDIR Directory Information Module (either because references to these files were omitted or because the Directory Information Module, optional in DICOM but required in the Ultrasound Application Profile, does not exist), these files are not recognized by the system.

ClearVue 350/550/650/850 3.1 ignores directory Record Types other than those above.

ClearVue 350/550/650/850 3.1 also ignores the “File-set consistency Flag” (0004, 1212).

### Patient Directory Record

Attribute Name	Tag	Type	Usage
Specific Character Set	0008,0005	1C	The default DICOM character set and optional set ISO-IR 100 (Latin 1) are supported. See Section 6 for details.
Patient Name	0010,0010	2	Displayed to help the user identify the patient folder in which to place the studies for this patient.
Patient ID	0010,0020	1	Displayed to help the user identify the patient folder in which to place the studies for this patient.

### Study Directory Record

Attribute Name	Tag	Type	Usage
Specific Character Set	0008,0005	1C	The Default DICOM character set and optional set ISO-IR 100 (Latin 1) are supported. See Section 6 for details.
Study Date	0008,0020	1	Used in displaying list of studies to user
Study Time	0008,0030	1	Used in displaying list of studies to user
Accession Number	0008,0050	2	Stored in the system database
Study Description	0008,1030	2	Generated
Study Instance UID	0020,000D	1C	Stored in the system database
Study ID	0020,0010	1	Stored in the system database

### Series Directory Record

Attribute Name	Tag	Type	Usage
Specific Character Set	0008,0005	1C	The default DICOM character set and optional set ISO-IR 100 (Latin 1) are supported. See Section 6 for details.
Modality	0008,0060	1	Only US is supported. Other modalities are ignored.
Series Instance UID	0020,000E	1	Stored

Series Description	0008,103E	3	Stored
Series Number	0020,0011	1	Stored

#### Image Directory Record

Attribute Name	Tag	Type	Usage
Specific Character Set	0008,0005	1C	The default DICOM character set and optional set ISO-IR 100 (Latin 1) are supported. See Section 6 for details.
Instance Number	0020,0013	1	Used
Referenced File ID	0004,1500	1C	Used
Referenced SOP Class UID in File	0004,1510	1C	Used
Referenced SOP UID in File	0004,1511	1C	Used
Referenced Transfer Syntax UID in File	0004,1512	1C	Used
Content Date	0008,0023	3	Used for ordering the thumbnail display. On Export, comes from the image.
Content Time	0008,0033	3	Used for ordering the thumbnail display. On Export, comes from the image.

#### SR Document Directory Record

Attribute Name	Tag	Type	Usage
Specific Character Set	0008,0005	1C	The default DICOM character set and optional set ISO-IR 100 (Latin 1) are supported. See Section 6 for details.
Instance Number	0020,0013	1	Used
Referenced File ID	0004,1500	1C	Used
Referenced SOP Class UID in File	0004,1510	1C	Used
Referenced SOP UID in File	0004,1511	1C	Used
Referenced Transfer Syntax UID in File	0004,1512	1C	Used
Content Date	0008,0023	3	Used for ordering the thumbnail display. On Export, comes from the image.
Content Time	0008,0033	3	Used for ordering the thumbnail display. On Export, comes from the image.
Concept Name Code Sequence	(0040,A043)	1	Code describing the concept represented by the root Content Item (Document Title).
>Code Value	0008,0100		Used to identify SR Template value
>Coding Scheme Designator	0008,0102		DCM
>Code Meaning	0008,0104		Name of the SR template
Completion Flag	0040,A491		"PARTIAL"
Verificaiton Flag	0040,A493		"UNVERIFIED"

## **6 SUPPORT OF CHARACTER SETS**

All ClearVue 350/550/650/850 3.1 DICOM applications support the

ISO\_IR 100 (ISO 8859-1:1987 Latin Alphabet No. 1 supplementary set)

ClearVue 350/550/650/850 3.1 will offer support for Chinese and Russian. This includes translating system text into these languages and allowing the user to input Chinese and Cyrillic characters into the system. One important aspect of this is that the user will be able to enter these special characters into the Patient ID screen.

The present DICOM standard allows Code Extension Techniques for multi-byte characters. Therefore, as well as the default character set (ISO-IR 6), ClearVue 350/550/650/850 3.1 supports the following extended character sets:

ISO-IR 100	Latin Alphabet No. 1
ISO-IR 144	Russian Cyrillic

Important Note:

When an Application Entity which, does not support Code Extension Techniques, receives a Data Set, which includes multi-byte characters from a ClearVue 350/550/650/850 3.1 system, misrepresentation of characters may occur.

The DICOM standard states that it is the responsibility of the Application Entity, which receives the Data Sets to take whatever action is considered necessary to minimize the effect of misrepresented characters. It is not the responsibility of the ClearVue 350/550/650/850 3.1 system to take such action.

## **6.1 SUPPORT FOR RUSSIAN MARKETS**

ClearVue 350/550/650/850 3.1 uses "Code-extension techniques" to encode Russian Cyrillic characters in DICOM tags with value representations of SH, LO, ST, LT, UT, and PN.

The technique requires two things in a DICOM file that contains these characters:

1. Add the Optional Specific Character Set tag (0008,0005) and set the value to the list of identifiers for all the non-standard character sets that will appear in any string in the file separated by backslashes. For example:

For Russian systems:

(0008,0005) = "ISO 2022 IR 144\ISO 2022 IR 100"

For English systems:

(0008,0005) = "ISO 2022 IR 100"

2. Embed escape sequences in the strings that contain Cyrillic characters to cause the DICOM interpreting code to switch from one character set to another.

The escape sequences to be used are defined as:

"<ESC>(B" ISO - IR 6 ASCII - DICOM default character set

"<ESC>(J" ISO - IR 144 Russian Cyrillic

## **6.2 SUPPORT FOR CHINESE MARKETS**

The current DICOM standard as of this release of ClearVue 350/550/650/850 3.1 does not support Chinese character sets. ClearVue 350/550/650/850 3.1 however provides support for Chinese customers so that they can enter text using Chinese characters.

If the system is set up for Chinese, then the user can enter just one version of the patient name. This would make Chinese systems work in the same way as Russian, English, French, Italian, and Spanish systems. The Chinese user will be able to enter the patient name using a combination of Chinese and Roman characters – all of the characters will appear wherever the system displays the patient name (image, report, Search for Study window, etc.).

Since the DICOM Standard does not offer support for Chinese characters, all Chinese characters entered into the Patient ID screen will be lost if a user exports or backs up a study to media. This will be noticed when the study is imported back into the system; upon import, each Chinese character will be replaced with a question mark ("?") character. The question marks will make it obvious to the user that the characters were lost.

If the user enters a patient name that consists entirely of Chinese characters, then the name will come back as "??????". In this case, the user will have to identify the study in the "Import Study" and "Search for Study" windows by the MRN. If the user enters a patient name that consists of a combination of Roman and Chinese characters, then Roman characters will be preserved, and the name will come back as something like "Lee ???????". This will give users who like to back up their studies the flexibility of entering a patient name with a combination of Roman and Chinese characters, and have at least part of the name come back during import.

**Note** that the original Chinese name will be "burned into" study images that are exported to media.

## **7 SECURITY**

DICOM security is not implemented on ClearVue 350/550/650/850 3.1 at this time.

ClearVue 350/550/650/850 3.1 incorporates an internal firewall that only accepts incoming traffic on the designated listening port, as configured in the "This System" tab of the DICOM setups screen. Changes to this port value require a power cycle to become effective.

## 8 ANNEXES

### 8.1 CREATED IOD INSTANCES

Table 69 specifies the attributes of an Ultrasound Image transmitted by the ClearVue 350/550/650/850 3.1 storage application.

Table 70 specifies the attributes of a Comprehensive Structured Reports transmitted by the ClearVue 350/550/650/850 3.1 storage application. Please note that there are differences between which Structured Report Templates are used in each product.

The following tables use a number of abbreviations. The abbreviations used in the “Presence of ...” column are:

VNAP	Value Not Always Present (attribute sent zero length if no value is present)
ANAP	Attribute Not Always Present
ALWAYS	Always Present
EMPTY	Attribute is sent without a value

The abbreviations used in the “Source” column:

MWL	the attribute value source Modality Worklist Unless otherwise noted, values returned from worklist may be overridden by User input.
USER	the attribute value source is from User input
AUTO	the attribute value is generated automatically
MPPS	the attribute value is the same as the Modality Performed Procedure Step service
CONFIG	the attribute value source is a configurable parameter

#### 8.1.1 US or US Multiframe Image IOD

**Table 69**  
**IOD OF CREATED US OR US MULTIFRAME SOP INSTANCES**

IE	Module	Reference	Presence of Module
Patient	Patient	Table 71	ALWAYS
Study	General Study	Table 72	ALWAYS
	Patient Study	Table 73	ALWAYS
Series	General Series	Table 74	ALWAYS
Equipment	General Equipment	Table 75	ALWAYS
Image	General Image	Table 76	ALWAYS
	Image Pixel	Table 77	ALWAYS

Palette Color Lookup Table	Table 77-a	ANAP
Cine	Table 78	Only if Multi-frame
Multi-frame	Table 79	Only if Multi-frame
US Region Calibration	Table 80	ANAP
US Image	Table 81	ALWAYS
VOI LUT	Table 82	ANAP
SOP Common	Table 83	ALWAYS

### 8.1.2 Comprehensive Structured Report IOD

**Table 70**  
**IOD OF CREATED COMPREHENSIVE STRUCTURED REPORT SOP INSTANCES**

IE	Module	Reference	Presence of Module
Patient	Patient	Table 71	ALWAYS
Study	General Study	Table 72	ALWAYS
	Patient Study	Table 73	ALWAYS
Series	SR Document Series	Table 84	ALWAYS
Equipment	General Equipment	Table 75	ALWAYS
Document	SR Document General	Table 85	ALWAYS
	SR Document Content	Table 86	ALWAYS
	SOP Common	Table 87	ALWAYS

### 8.1.3 Common Modules

**Table 71**  
**PATIENT MODULE OF CREATED SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Patient's Name	(0010,0010)	PN	Same attribute of MWL or PDE input	ALWAYS	MWL/ USER/ AUTO

Attribute Name	Tag	VR	Value	Presence of Value	Source
Patient ID	(0010,0020)	LO	From MWL, user input or system generated.	ALWAYS	MWL/USER/AUTO
Patient's Birth Date	(0010,0030)	DA	Same attribute of MWL or PDE input	VNAP	MWL/USER
Patient's Sex	(0010,0040)	CS	Same attribute of MWL or PDE input User Input may be: M = male F = female O = other If "Unknown", an empty string is sent.	VNAP	MWL/USER
Other Patient IDs	(0010,1000)	LO	Same attribute of MWL or PDE input to Alternate ID number.	ANAP	MWL/USER

**Table 72**  
**GENERAL STUDY MODULE OF CREATED SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Study Instance UID	(0020,000D)	UI	Same value as in MWL or auto generated If non-Worklist, format is: 1.3.46.670589.14.<model>.<version>.4. <serno>.<datetime>.<n> <model> is 5000 for ClearVue 350, 6000 for ClearVue 550 and 9002 for ClearVue 650. <version> is 300 for ClearVue 350/550/650. <serno> is system serial number <datetime> is date time when the uid was requested in yyyyymmddhhmmss format <n> is the nth image generated at the <datetime>th second	ALWAYS	MWL/AUTO
Study Date	(0008,0020)	DA	Study's Start Date (0040,0244).	ALWAYS	AUTO
Study Time	(0008,0030)	TM	Study's Start Time (0040,0245).	ALWAYS	AUTO
Referring Physician's Name	(0008,0090)	PN	User Input from Patient ID screen. From MWL, only Last, First and Middle names sent as "Last, First, Middle" in the Last name field.	VNAP	MWL/USER
Study ID	(0020,0010)	SH	Auto-generated starting at 1	ALWAYS	AUTO

Attribute Name	Tag	VR	Value	Presence of Value	Source
Accession Number	(0008,0050)	SH	Same attribute of MWL or user PDE input.	VNAP	MWL/USER
Study Description	(0008,1030)	LO	'Study Description' in PDE or, Configurable by the user through setup. Can either be a fixed list or (for users with a MWL server), can be obtained from the MWL Server.  The string used will be the first non-empty string from the following list: Requested Procedure description tag (0032,1060), Scheduled Procedure Step description tag (0040,0007) Scheduled Procedure Step, "Code Meaning" tag (0008,0104) Reason for the requested procedure tag (0040,1002) Reason for imaging service request tag (0040,2001)	ANAP	MWL/USER

**Table 73  
PATIENT STUDY MODULE OF CREATED SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Patient Size	(0010,1020)	DS	Same value as MWL attribute or PDE input.	ANAP	MWL/USER
Patient's Weight	(0010,1030)	DS	Same value as MWL attribute or PDE input.	ANAP	MWL/USER
Additional Patient's History	(0010,21B0)	LT	Only from User Input	ANAP	USER

**Table 74  
GENERAL SERIES MODULE OF CREATED IMAGE SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Modality	(0008,0060)	CS	"US"	ALWAYS	AUTO

Attribute Name	Tag	VR	Value	Presence of Value	Source
Series Instance UID	(0020,000E )	UI	<p>A system generated Unique Identifier of the form: 1.3.46.670589.14.&lt;model&gt;.&lt;version&gt;.3.&lt;serno&gt;.&lt;datetime&gt;.&lt;n&gt;</p> <p>&lt;model&gt; is 5000 for ClearVue 350, 6000 for ClearVue 550 and 9002 for ClearVue 650.</p> <p>&lt;version&gt; is 300 for ClearVue 350/550/650.</p> <p>&lt;serno&gt; is system serial number</p> <p>&lt;datetime&gt; is date time when the uid was requested in yyyyymmddhhmmss format</p> <p>&lt;n&gt; is the nth image generated at the &lt;datetime&gt;th second</p> <p>Note:</p> <p>If a study is reopened, a new SeriesInstUID would be generated and all newly acquired images would be part of the new series. Also the MPPS messages (if applicable) that would be sent when the study is restarted would contain the newly generated SeriesInstUID.</p>	ALWAYS	AUTO
Series Number	(0020,0011)	IS	Always 1 for images	ALWAYS	AUTO
Performing Physician's Name	(0008,1050)	PN	PDE input, 'Performed by'.	ANAP	USER
Protocol Name	(0018,1030)	LO	<p>"Free Form"</p> <p>"Exercise 2 Stage"</p> <p>"Exercise 3 Stage"</p> <p>"Pharmacological 4 Stage"</p> <p>user defined</p>	ANAP	AUTO
Series Description	(0008,103E )	LO	User entry in the 'Study Description' field of the Patient ID screen. If the user does not enter a value, this tag is not sent.	ANAP	MWL/USER
Operator's Name	(0008,1070)	PN	User entry in the 'Performed by' field of the Patient ID screen. If the user does not enter a value, this tag is not sent.	ANAP	MWL/USER
Referenced Performed Procedure Step Sequence	(0008,1111)	S Q	<p>Identifies the MPPS SOP Instance this image is related to</p> <p>* Will be present when an MPPS Server is configured.</p>	ANAP*	AUTO
>Referenced SOP Class UID	(0008,1150)	UI	<p>PPS SOP Class = "1.2.840.10008.3.1.2.3.3"</p> <p>* Will be present when an MPPS Server is configured.</p>	ANAP*	AUTO
>Referenced SOP Instance UID	(0008,1155)	UI	<p>PPS Instance UID of the PPS generating this image</p> <p>* Will be present when an MPPS Server is configured.</p>	ANAP*	AUTO

Attribute Name	Tag	VR	Value	Presence of Value	Source
Request Attributes Sequence	(0040,0275)	S Q	This sequence will be present only for scheduled study. In case of unscheduled study, this sequence will not be present. This sequence will not be present if attributes 'Requested Procedure ID' and/or 'Scheduled Procedure Step ID' is/are missing.	ANAP	AUTO / MWL
>Requested Procedure ID	(0040,1001)	SH	Auto-generated=Study ID or value from MWL. One item.	ANAP	AUTO / MWL
>Requested Procedure Description	0032,1060	LO	Set with the value entered or selected in "Study Description" field of Patient ID screen. If the study is started from MWL, the "Study Description" field of Patient ID screen is populated from 'Requested Procedure Description' attribute of MWL. (1st choice, configurable)	ANAP	USER/ MWL
>Scheduled Procedure Step ID	(0040,0009)	SH	Auto-generated=Study ID or value from MWL. One item.	ANAP	AUTO / MWL
>Scheduled Procedure Step Description	(0040,0007)	LO	Same value as MWL attribute.	ANAP	MWL
>Scheduled Protocol Code Sequence	(0040,0008)	S Q	Same value as MWL attribute.	ANAP	MWL
Performed Procedure Step ID	(0040,0253)	SH	Set as current date and time in the format yyyyymmdd.hhmmss.	ANAP	AUTO
Performed Procedure Step Start Date	(0040,0244)	DA	Date on which the Performed Procedure Step started on close of Patient Data Entry Screen	ANAP	AUTO
Performed Procedure Step Start Time	(0040,0245)	T M	Time on which the Performed Procedure Step started on close of Patient Data Entry Screen	ANAP	AUTO
Performed Procedure Step Description	(0040,0254)	LO	Set with the value entered or selected in 'Study Description' field of Patient ID screen. If the study is started from MWL, the "Study Description" field of Patient ID screen is populated from 'Requested Procedure Description' attribute of MWL. (1st choice, configurable).	ANAP	USER / MWL
Performed Protocol Code Sequence	(0040,0260)	S Q	Zero length, or mapped from MWL Scheduled Protocol Code Sq (0040,0008)	ANAP	MWL

**Table 75**  
**GENERAL EQUIPMENT MODULE OF CREATED SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Manufacturer	(0008,0070)	LO	Philips Medical Systems	ALWAYS	AUTO
Institution Name	(0008,0080)	LO	<p>Entered by the user from the 'System' tab in the 'Setup' screen ('Top Border' button). Note: If the user imports an EnVisor or ClearVue 350/550/650/850 3.1 study that was generated at another institution and opens the study the institution name displayed along the top border of the system screen is the institution viewing the images not the institution where the image was acquired. The institution name where the image was acquired can however be burned into the image. Also, if the user exports the study to removable media or to a networked PACS and changes the format of the image data in some way either by exporting it in a different image format from the internal format (Palette Color, RLE) or by applying a display compensation curve, then the institution name is changed to the current institution.</p> <p>'Philips Healthcare' default.</p>	VNAP	CONFIG
Station Name	(0008,1010)	SH	The AE Title of ClearVue 350/550/650/850 3.1 system on which the image is acquired. The user can configure the AE Title of the system through 'Setup'.	VNAP	CONFIG
Software Version(s)	(0018,1020)	LO	<p>This is a multi-valued tag which contains the following components:</p> <p>Model Name ClearVue 350_300 or CleareVue 550_300 or ClearVue 650_300</p> <p>Then the part number and version of</p> <p>PRINTERS Ultrasound Application DRIVERS Operating System.</p>	ALWAYS	AUTO
Manufacturer's Model Name	(0008,1090)	LO	ClearVue 350 or ClearVue 550 or ClearVue 650	ALWAYS	AUTO

#### 8.1.4 US or Multiframe Image Modules

**Table 76**  
**GENERAL IMAGE MODULE OF CREATED US SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Instance Number	(0020,0013)	IS	Generated by device, increments from “1” in each series. Gaps in values may exist if images are deleted on the system prior to export.	ALWAYS	AUTO
Patient Orientation	(0020,0020)	CS	The system sends the empty tag for 2D/3D and is not used for PanView images.	VNAP	AUTO
Content Date	(0008,0023)	DA	<yyyymmdd>	VNAP	AUTO
Content Time	(0008,0033)	TM	<hhmmss>	VNAP	AUTO
Image Type	(0008,0008)	CS	<p>The system computes this value as the four component multi-value attribute:</p> <p>“&lt;Pixel Data Characteristics&gt; / &lt;Patient Examination Characteristics&gt; / &lt;Modality Specific Characteristics&gt; / &lt;Implementation Specific Identifiers&gt;”</p> <p>&lt;Pixel Data Characteristics&gt;</p> <p>Palette Color &amp; RGB: “ORIGINAL” denotes original source-data</p> <p>YBR:</p> <p>“DERIVED” denotes pixels that have been derived from the original – in this case by lossy compression.</p> <p>MONOCHROME2:</p> <p>“DERIVED” denotes pixels that have been derived from the original – in this case by grayscale transformations.</p> <p>&lt;Patient Examination Characteristics&gt;</p> <p>Always “PRIMARY”</p> <p>&lt;Modality Specific Characteristics&gt;</p> <p>This is based on the user-selected entry in the drop down list ‘Additional Data Type’ on the Patient Id screen. It is mapped to the most appropriate value from the DICOM standard (Ex: “ABDOMINAL”).</p> <p>&lt;Implementation Specific Identifiers&gt; Always blank.</p>	VNAP	CONFIG
Acquisition Date	(0008,0022)	DT	The system uses the same value as the Content Date, tag 0008,0023.	VNAP	AUTO

Attribute Name	Tag	VR	Value	Presence of Value	Source
Acquisition Time	(0008,0032)	TM	The system uses the same value as the Content time, tag 0008,0033.	VNAP	AUTO
Acquisition Datetime	(0008,002A)	DT	The system generates this as a combination of Acquisition Date and Acquisition Time. The format is yyyyymmddhhmmss.ffffff	VNAP	AUTO
Lossy Image Compression	(0028,2110)	CS	"01" if image is lossy compressed, "00" if not.	VNAP	AUTO
Image Comments	(0020,4000)	LT	Not used with images. For reports, contains: "Report Version x Page x of x"	ANAP	AUTO
Presentation LUT Shape	(2050,0020)	CS	"IDENTITY". Only if "Image Export Format" is GSDF.	ANAP	AUTO

**Table 77**  
**IMAGE PIXEL MODULE OF CREATED US OR US MULTIFRAME SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Samples per Pixel	(0028,0002)	US	1 for MONOCHROME2 1 for PALETTE COLOR 3 for RGB 3 for YBR_FULL_422	ALWAYS	CONFIG
Photometric Interpretation	(0028,0004)	CS	MONOCHROME2 PALETTE COLOR RGB YBR_FULL_422	ALWAYS	CONFIG
Rows	(0028,0010)	US	2D B/W & Color stills/loops, acquired with top & right border: 600 2D B/W & Color quad-sized loops from stress: 300 Reports: 600 QLAB from IMT plug-in: 600 QLAB (all others): 600	ALWAYS	CONFIG
Columns	(0028,0011)	US	2D B/W & Color stills/loops, acquired with top & right border: 800 2D B/W & Color quad-sized loops from stress: 336 Reports: 800 QLAB from IMT plug-in: 936 QLAB: 800	ALWAYS	CONFIG
Bits Allocated	(0028,0100)	US	Based on the 'Image Format' that is set by the user in DICOM Setup. Palette Color Mode:	ALWAYS	AUTO

Attribute Name	Tag	VR	Value	Presence of Value	Source
			2D B&W: 8 bits 2D Color, Reports & QLAB: 16 bits RGB Mode: 2D B&W,: 8 bits 2D Color, Reports & QLAB: 8 bits YBR_FULL_422 Mode: 2D B&W: 8 bits 2D Color, Reports & QLAB: 8 bits MONOCHROME2 Mode: 8 bits		
Bits Stored	(0028,0101)	US	Always the same numbers as Bits Allocated.	ALWAYS	AUTO
High Bit	(0028,0102)	US	The High Bit is always (Bits Allocated -1).	ALWAYS	AUTO
Pixel Representation	(0028,0103)	US	“0” pixels are Unsigned integers	ALWAYS	AUTO
Pixel Data	(7FE0,0010)	OW / OB		ALWAYS	AUTO
Planar Configuration	(0028,0006)	US	Palette Color Images: Not present RGB Images: Zero (color-by-pixel) YBR: Images: Always zero (color-by-pixel) MONOCHROME2 Images: Not present	ALWAYS	AUTO
Red Palette Color Lookup Table Descriptor	(0028,1101)	IC	See Table 77-a.	ANAP	CONFIG
Green Palette Color Lookup Table Descriptor	(0028,1102)	IC	See Table 77-a.	ANAP	CONFIG
Blue Palette Color Lookup Table Descriptor	(0028,1103)	IC	See Table 77-a.	ANAP	CONFIG
Red Palette Color Lookup Table Data	(0028,1201)	IC	See Table 77-a.	ANAP	CONFIG
Green Palette Color Lookup Table Data	(0028,1202)	IC	See Table 77-a.	ANAP	CONFIG
Blue Palette Color Lookup Table Data	(0028,1203)	IC	See Table 77-a.	ANAP	CONFIG

**Table 77-a**  
**PALETTE COLOR LOOKUP TABLE MODULE**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Red Palette Color Lookup Table Descriptor	(0028,1101)	US	Used only for 2D and REPORT acquired as image. B&W stills & loops: 256, 0, 16 Color stills & loops: 0, 0, 16 REPORT (acquired as image): xx, 0, 16 where 'xx' is a variable value.	ALWAYS	CONFIG
Green Palette Color Lookup Table Descriptor	(0028,1102)	US	Used only for 2D and REPORT acquired as image. B&W stills & loops: 256, 0, 16 Color stills & loops: 0, 0, 16 REPORT (acquired as image): xx, 0, 16 where 'xx' is a variable value.	ALWAYS	CONFIG
Blue Palette Color Lookup Table Descriptor	(0028,1103)	US	Used only for 2D and REPORT acquired as image. B&W stills & loops: 256, 0, 16 Color stills & loops: 0, 0, 16 REPORT (acquired as image): xx, 0, 16 where 'xx' is a variable value.	ALWAYS	CONFIG
Red Palette Color Lookup Table Data	(0028,1201)	OW	Used only for 2D and REPORT acquired as image.	VNAP	CONFIG
Green Palette Color Lookup Table Data	(0028,1202)	OW	Used only for 2D and REPORT acquired as image.	VNAP	CONFIG
Blue Palette Color Lookup Table Data	(0028,1203)	OW	Used only for 2D and REPORT acquired as image.	VNAP	CONFIG

**Table 78**  
**CINE MODULE OF CREATED US MULTIFRAME SOP**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Recommended Display Frame Rate	(0008,2144)	IS	Used for Multiframe	ANAP	AUTO
Cine Rate	(0018,0040)	IS	Used for Multiframe	ANAP	AUTO
Effective Duration	(0018,0072)	DS	Used for Multiframe	ANAP	AUTO

Attribute Name	Tag	VR	Value	Presence of Value	Source
Frame Time	(0018,1063)	DS	Nominal time (in msec) per individual frame. Present if Frame Increment Pointer (0028,0009) points to Frame Time.  Note: If you export a study to removable media using Average Frame Time, on import back into the system only the images up to but not including the loop will be imported. However the study on media is fine and can be imported onto a PACS without any problems.	ANAP	CONFIG
Frame Time Vector	(0018,1065)	DS	An array that contains the real time increments (in msec) between frames for a Multi-frame image. Present if Frame Increment Pointer (0028,0009) points to Frame Time Vector.	ANAP	CONFIG

**Table 79  
MULTI-FRAME MODULE OF CREATED US MULTIFRAME SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Number of Frames	(0028,0008)	IS	# of frames in object	ANAP	AUTO
Frame Increment Pointer	(0028,0009)	AT	Configurable by the user in DICOM Setup. If the user selects a loop timing preference where each frame in a loop has the same duration then Frame Increment Pointer takes the value 0018,1063 (Frame Time). If the user selects a loop timing preference where each frame in a loop has the different duration then Frame Increment Pointer takes the value 0018,1065 (Frame Time Vector).	ANAP	CONFIG

**Table 80  
US REGION CALIBRATION MODULE OF CREATED US IMAGE OR US MULTIFRAME IMAGE SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Sequence of Ultrasound Regions	(0018,6011)	SQ	A sequence is present for each region on the system display	ANAP	AUTO
>Region Location Min x <sub>0</sub>	(0018,6018)	UL	Top Left position of region.	ALWAYS	AUTO
>Region Location Min y <sub>0</sub>	(0018,601A)	UL	Top Left position of region	ALWAYS	AUTO
>Region Location	(0018,601C)	UL	Bottom Right position of region	ALWAYS	AUTO

Attribute Name	Tag	VR	Value	Presence of Value	Source
Max x <sub>1</sub>					
>Region Location Max y <sub>1</sub>	(0018,601E)	UL	Bottom Right position of region	ALWAYS	AUTO
>Physical Units X Direction	(0018,6024)	US	Enumerated Value. 2D Image = 0003H = CM MMode / Doppler = 0004H = SEC	ALWAYS	AUTO
>Physical Units Y Direction	(0018,6026)	US	Enumerated Value. ECG Region = 0000H = None 2D Image = 0003H = CM MMode = 0003H = CM Doppler = 0007H = CM / SEC	ALWAYS	AUTO
>Physical Delta X	(0018,602C)	FD	The physical value per pixel increment	ALWAYS	AUTO
>Physical Delta Y	(0018,602E)	FD	The physical value per pixel increment	ALWAYS	AUTO
>Reference Pixel X <sub>0</sub>	(0018,6020)	SL	The X pixel value of baseline	ALWAYS	AUTO
>Reference Pixel Y <sub>0</sub>	(0018,6022)	SL	The Y pixel value of baseline	ALWAYS	AUTO
>Reference Pixel Physical Value X	(0018,6028)	FD	For each region, the X coordinate of the reference point for measurements within that region.	ALWAYS	AUTO
>Reference Pixel Physical Value Y	(0018,602A)	FD	For each region, the Y coordinate of the reference point for measurements within that region.	ALWAYS	AUTO
>Region Spatial Format	(0018,6012)	US	Enumerated Value. 2D (tissue or flow) = 0001H MMode (tissue or flow) = 0002H Spectral (CW or PW Doppler) = 0003H ECG (waveform) = 0004H	ALWAYS	AUTO
>Region Data Type	(0018,6014)	US	Enumerated Value. Tissue = 0001H (2D, MMode) PW Spectral Doppler = 0003H CW Spectral Doppler = 0004H ECG (waveform) = 000AH	ALWAYS	AUTO
>Region Flags	(0018,6016)	UL	Always set to 3.	ALWAYS	AUTO

**Table 81**  
**US IMAGE MODULE OF CREATED US IMAGE OR US MULTIFRAME IMAGE SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Samples Per Pixel	(0028,0002)	US	See 'Image Pixel Module'	ALWAYS	AUTO
Photometric Interpretation	(0028,0004)	CS	See 'Image Pixel Module'	ALWAYS	CONFIG
Bits Allocated	(0028,0100)	US	See 'Image Pixel Module'	ALWAYS	AUTO
Bits Stored	(0028,0101)	US	See 'Image Pixel Module'	ALWAYS	AUTO
High Bit	(0028,0102)	US	See 'Image Pixel Module'	ALWAYS	AUTO
Planar Configuration	(0028,0006)	US	See 'Image Pixel Module'	ALWAYS	AUTO
Pixel Representation	(0028,0103)	US	"0" Pixels are Unsigned integers	ALWAYS	AUTO
Frame Increment Pointer	(0028,0009)	AT	(0018,1063) "Frame Time" or (0018,1065) "Frame Time Vector"	ANAP	CONFIG
Image Type	(0008,0008)	CS	See 'General Image Module'	VNAP	CONFIG
Lossy Image Compression	(0028,2110)	CS	"01" if image is lossy compressed, "00" if not.	ALWAYS	AUTO
Ultrasound Color Data Present	(0028,0014)	US	0 or 1	ANAP	AUTO
Acquisition Datetime	(0008,002A)	DT	The date and time that the acquisition of data that resulted in this image started.	VNAP	AUTO
Transducer Data	(0018,5010)	LO	Transducer name. VM = 3, the last two fields are written as "UNUSED".	ALWAYS	AUTO
Transducer Type	(0018,6031)	LO	SECTOR_PHASED, LINEAR, CURVED LINEAR Only used for 2D images; not used for Doppler-only images (i.e. pencil probes)	ANAP	AUTO
Processing Function	(0018,5020)	LO	The factory-defined exam/preset that was active when the image was acquired even if a user-defined preset.	ALWAYS	AUTO

**Table 82**  
**VOI LUT MODULE OF CREATED US SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Window Center	(0028,1050)	DS	$2^{n-1}$ where n is the number of bits per pixel n = 8 Center = 128 n= 16 Center = 32768 Value only meaningful with MONOCHROME2.	ANAP	AUTO

Attribute Name	Tag	VR	Value	Presence of Value	Source
Window Width	(0028,1051)	DS	2 <sup>n</sup> where n is the number of bits per pixel n = 8 Width = 256 n= 16 Width = 65336 Value only meaningful with MONOCHROME2.	ANAP	AUTO

**Table 83**  
**SOP COMMON MODULE OF CREATED US IMAGE OR US MULTIFRAME IMAGE SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
SOP Class UID	(0008,0016)	UI	1.2.840.10008.5.1.4.1.1.6.1 for US Image 1.2.840.10008.5.1.4.1.1.3.1 for US Multiframe Image	ALWAYS	AUTO
SOP Instance UID	(0008,0018)	UI	Generated by device in the format: For ClearVue 350_300 – 1.3.46.670589.14.5000.300.2.xxxxxx.yyyymmddhhmmsss.v For ClearVue 550_300 – 1.3.46.670589.14.6000.300.2.xxxxxx.yyyymmddhhmmsss.v For ClearVue 650_300 – 1.3.46.670589.14.9002.300.2.xxxxxx.yyyymmddhhmmsss.v where 2 indicates a SOP Instance UID, x indicates the system serial number, then date and time and v is a counter of the instances.	ALWAYS	AUTO
Specific Character Set	(0008,0005)	CS	The attribute contains all the character sets used (this is a multi-value attribute). See Section 6 for more information on the character sets that this system uses. ISO_IR 100 and possibly more. The most likely scenario that would require a non Basic Character set would be when the system has been set to a locale that uses non Basic characters (e.g. Russia) AND the user has entered one of these characters into the Patient Identification screen,	ALWAYS	AUTO

### 8.1.5 Comprehensive Structured Report Modules

**Table 84**  
**SR DOCUMENT SERIES MODULE OF CREATED COMPREHENSIVE SR SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Modality	(0008,0060)	CS	“SR”	ALWAYS	AUTO
Series Instance UID	(0020,000E)	UI	Auto-generated	ALWAYS	AUTO
Series Number	(0020,0011)	IS	A number unique within the Study starting with 2.	ALWAYS	AUTO
Referenced Performed Procedure Step Sequence	(0008,1111)	SQ	Identifies the MPPS SOP Instance to which this image is related	ANAP	MPPS
>Referenced SOP Class UID	(0008,1150)	UI	PPS SOP Class = “1.2.840.10008.3.1.2.3.3”	ANAP	MPPS
> Referenced SOP Instance UID	(0008,1155)	UI	PPS Instance UID of the PPS generating this document	ANAP	MPPS

**Table 85**  
**SR DOCUMENT GENERAL MODULE OF CREATED COMPREHENSIVE SR SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Instance Number	(0020,0013)	IS	Unique number starting with “0” zero.	ALWAYS	AUTO
Completion Flag	(0040,A491)	CS	PARTIAL	ALWAYS	AUTO
Verification Flag	(0040,A493)	CS	UNVERIFIED	ALWAYS	AUTO
Content Date	(0008,0023)	DA	Date content created.	ALWAYS	AUTO
Content Time	(0008,0033)	TM	Time content created.	ALWAYS	AUTO
Referenced Request Sequence	(0040,A370)	SQ	Identifies Requested Procedures being fulfilled (completely or partially) by creation of this Document. Null string if unscheduled.	VNAP	AUTO
>Study Instance UID	(0020,000D)	UI	Same value as in MWL or auto generated	ALWAYS	MWL/AUTO
>Referenced Study Sequence	(0008,1110)	SQ	1 item per item in MWL, absent if unscheduled	ANAP	MWL
>>Referenced SOP Class UID	(0008,1150)	UI	Identifies the Referenced SOP Class	ANAP	MWL
>>Referenced SOP Instance UID	(0008,1155)	UI	Instance UID	ANAP	MWL
>Accession Number	(0008,0050)	SH	Same attribute of MWL or user PDE input.	VNAP	MWL/USER

Attribute Name	Tag	VR	Value	Presence of Value	Source
>Placer Order Number/Imaging Service Request	(0040,2016)	LO	Order Number of Imaging Service Request assigned by placer	VNAP	MWL
>Filler Order Number/Imaging Service Request	(0040,2017)	LO	Order Number of Imaging Service Request assigned by filler	VNAP	MWL
>Requested Procedure ID	(0040,1001)	SH	1 item per item in MWL, absent if unscheduled	ANAP	MWL
>Requested Procedure Description	(0032,1060)	LO	1 item per item in MWL, absent if unscheduled	ANAP	MWL
>Requested Procedure Code Sequence	(0032,1064)	SQ	1 item per item in MWL, absent if unscheduled	ANAP	MWL

**Table 86**

**SR DOCUMENT CONTENT MODULE OF CREATED COMPREHENSIVE SR SOP INSTANCES**

This table describes the template-specific data summarized from the following tables in the DICOM Standard:  
Document Content Macro, Document Relationship Macro, Numeric Measurement Macro and Code Macro

Attribute Name	Tag	VR	Value	Presence of Value	Source
Content Template Sequence	(0040,A504)	SQ		ALWAYS	AUTO
>Template Identifier	(0040,DB00)	CS	The Root Content Item identifies TID 5000 (OB-GYN) 5100 (Vascular) 5200 (Adult Echo) 5220 (Ped Echo)	ALWAYS	AUTO
>Mapping Resource	(0008,0105)	CS	DCMR	ALWAYS	AUTO
Content Sequence	(0040,A730)	SQ		ALWAYS	AUTO
>Relationship Type	(0040,A010)	CS	See <a href="#">Template ID 5000</a> for OB-GYN See <a href="#">Template ID 5100</a> for Vascular See <a href="#">Template ID 5200</a> for Adult Echo See <a href="#">Template ID 5220</a> for Ped Echo	ALWAYS	AUTO
Document Relationship Macro Table			See <a href="#">Template ID 5000</a> for OB-GYN See <a href="#">Template ID 5100</a> for Vascular See <a href="#">Template ID 5200</a> for Adult Echo See <a href="#">Template ID 5220</a> for Ped Echo	ANAP	AUTO
Document Content Macro			See <a href="#">Template ID 5000</a> for OB-GYN See <a href="#">Template ID 5100</a> for Vascular See <a href="#">Template ID 5200</a> for Adult Echo See <a href="#">Template ID 5220</a> for Ped Echo	ALWAYS	AUTO
Value Type	(0040,A040)	CS	CONTAINER, always first tag of SR	ALWAYS	AUTO

Attribute Name	Tag	VR	Value	Presence of Value	Source
Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>Code Value	(0008,0100)		125000 for OB-GYN 125100 for Vascular 125200 for Adult Echo 125195 for Ped Echo	ALWAYS	AUTO
>Coding Scheme Designator	(0008,0102)		DCM	ALWAYS	AUTO
>Code Meaning	(0008,0104)		“OB-GYN Procedure Report” “Vascular Ultrasound Procedure Report” “Adult Echocardiography Procedure Report” “Pediatric Cardiac Ultrasound Report”	ALWAYS	AUTO
Continuity of Content	(0040,A050)	CS	SEPARATE	ALWAYS	AUTO
Numeric Measurement Macro			See <a href="#">Template ID 5000</a> for OB-GYN See <a href="#">Template ID 5100</a> for Vascular See <a href="#">Template ID 5200</a> for Adult Echo See <a href="#">Template ID 5220</a> for Ped Echo	ALWAYS	AUTO
Code Macro			See <a href="#">Template ID 5000</a> for OB-GYN See <a href="#">Template ID 5100</a> for Vascular See <a href="#">Template ID 5200</a> for Adult Echo See <a href="#">Template ID 5220</a> for Ped Echo	ALWAYS	AUTO

**Table 87**  
**SOP COMMON MODULE OF CREATED COMPOSITE SR SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
SOP Class UID	(0008,0016)	UI	1.2.840.10008.5.1.4.1.1.88.33	ALWAYS	AUTO
SOP Instance UID	(0008,0018)	UI	Generated by device	ALWAYS	AUTO
Specific Character Set	(0008,0005)	CS	ISO_IR 100. See Section 6 for details.	ALWAYS	CONFIG

## 8.2 USED FIELDS IN RECEIVED IOD BY APPLICATION

The ClearVue 350/550/650/850 3.1 storage applications do not receive SOP Instances. The usage of attributes received via MWL is described in section 4.2.2.3.1.3 SOP Specific Conformance for Modality Worklist.

## 8.3 ATTRIBUTE MAPPING

Table 88 summarizes the relationships between attributes received via MWL, stored in acquired images and communicated via MPPS. The format and conventions used in Table 88 are the same as the corresponding table in DICOM Part 4, Annex M.6

**Table 88**  
**ATTRIBUTE MAPPING BETWEEN MODALITY WORKLIST, IMAGE AND MPPS**

Modality Worklist	Image IOD	MPPS IOD
Patient's Name	Patient's Name	Patient's Name
Patient ID	Patient ID	Patient ID
Patient's Birth Date	Patient's Birth Date	Patient's Birth Date
Patient's Sex	Patient's Sex	Patient's Sex
Patient's Weight	Patient's Weight	
Referring Physician's Name	Referring Physician's Name	
----	----	Scheduled Step Attributes Sequence
Study Instance UID	Study Instance UID	>Study Instance UID
Referenced Study Sequence	Referenced Study Sequence	>Referenced Study Sequence
Accession Number	Accession Number	>Accession Number
----	Request Attributes Sequence	----
Requested Procedure ID	>Requested Procedure ID	>Requested Procedure ID
Requested Procedure Description	>Requested Procedure Description	>Requested Procedure Description
Scheduled Procedure Step ID	>Scheduled Procedure Step ID	>Scheduled Procedure Step ID
Scheduled Procedure Step Description	>Scheduled Procedure Step Description > Study Description > Series Description > Performed Procedure Step Description	>Scheduled Procedure Step Description
Scheduled Protocol Code Sequence	>Scheduled Protocol Code Sequence	>Scheduled Protocol Code Sequence
----	Performed Protocol Code Sequence	Performed Protocol Code Sequence
----	Study ID – Requested Procedure ID from MWL, else generated	Study ID – Requested Procedure ID from MWL, else generated
----	Performed Procedure Step ID	Performed Procedure Step ID
----	Performed Procedure Step Start Date	Performed Procedure Step Start Date
----	Performed Procedure Step Start Time	Performed Procedure Step Start Time

Modality Worklist	Image IOD	MPPS IOD
----	Performed Procedure Step Description	Performed Procedure Step Description
Requested Procedure Code Sequence	Procedure Code Sequence	Procedure Code Sequence
----	Referenced Performed Procedure Step Sequence	Performed Series Sequence
----	>Referenced SOP Class UID	SOP Class UID
----	>Referenced SOP Instance UID	SOP Instance UID
----	Protocol Name	Protocol Name

#### 8.4 COERCED/MODIFIED FIELDS

The MWL AE will truncate attribute values received in the response to a MWL Query if the value length is longer than the maximum length permitted by the attribute's VR.

#### 8.5 CONTROLLED TERMINOLOGY

The Workflow AE is capable of supporting arbitrary coding schemes for Procedure and Protocol Codes. The contents of Requested Procedure Code Sequence (0032,1064) and Scheduled Protocol Code Sequence (0040,0008) supplied in Worklist Items will be mapped to Image IOD and MPPS attributes as described in Table 88.

Structured Reporting uses codes supplied by DCMR (DICOM Code Mapping Resource, PS 3-16), LOINC (Logical Observation Names and Codes), SRT (SNOMED – Systematized Nomenclature of Medicine) and 99PMSBLUS (Philips Private Codes for Ultrasound).

#### 8.6 GRayscale IMAGE CONSISTENCY

The high-resolution display monitor is calibrated according to the Grayscale Standard Display Function (GSDF).

#### 8.7 EXTENSIONS / SPECIALIZATIONS / PRIVATIZATIONS

##### 8.7.1 Standard Extended / Specialized / Private SOPs

The US or US Multiframe Image Storage SOP Classes are extended to create a Standard Extended SOP Class by addition of standard and private attributes to the created SOP Instances as documented in section 8.1.

Tag Number	Tag Name	Added to:
0028,0030	Pixel Spacing	Images with a single 2D region or dual 2D with same depth See details in Section 8.7.3
2050,0020	Presentation LUT Shape	Images when 'GSDF' output format is selected

##### 8.7.2 2D

The Pixel Spacing tag is added to the exported DICOM file when the user has configured this tag to be included and the image contains only one 2D calibration region and no Doppler or M-Mode calibration regions.

**Contain the Pixel Spacing tag:** 2D still, 2D loop, 2D color still, 2D color loop, MMode Preview Still, PW Preview Still, CW Preview still, Dual with same calibration on both images.

**Do NOT contain the Pixel Spacing tag:** MMode live trace, MMode frozen trace, PW live trace, PW Frozen trace, CW live trace, CW frozen trace, Reports and dual images with different calibration on each image.

This attribute is system generated, if used.

Attribute Name	Tag	Type	VR	Description	Value
Pixel Spacing	0028,0030	3	DS	Physical distance in the patient between the center of each pixel, specified by a numeric pair adjacent row spacing (delimiter) adjacent column spacing (in mm).	Adjacent row spacing \ Adjacent column spacing (in mm)

#### 8.7.4 PRIVATE TRANSFER SYNTAXES

There are no Private Transfer Syntaxes.

## APPENDIX A – Structured Reports

### A.1 STRUCTURED REPORTS

Note that all the concepts defined privately by Philips have the CSD value as '99PMSBLUS'.

Note that the average value is the average of all instances for the measurement for the study.

### A.2 OB – GYN STRUCTURED REPORT TEMPLATE

ClearVue 350/550/650/850 3.1 implements the OB-GYN Ultrasound Procedure Report Template (TID 5000) from the DICOM standard, part 16. This appendix describes the scope and manner that ClearVue 350/550/650/850 3.1 measurements appear in DICOM SR.

Measurements and calculations performed for Obstetric and Gynecology studies will lead to creation of "OB-GYN Ultrasound Procedure Report" structured report document. Measurements can be performed by pressing the 'Calc' key on the ClearVue 350/550/650/850 3.1 control panel and selecting an OB or GYN analysis package. Measurements and calculations available in the menu can be configured through the setup application. It is also possible to configure the measurement unit (Metric or U.S.).

All concepts with value type (VT) NUM will always have a 'MeasurementUnitCodeSequence' that specifies the unit of the measurement. The CSD for all units will be UCUM (Unified Code for Units) and CV and CM will be based on application configuration and will conform to UCUM standards.

#### A.2.1 Template specific conformance for TID 5000

The template for the root of the content tree for TID 5000 and its use in the ClearVue 350/550/650/850 3.1 context is described in the following table.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	EV (125000, DCM, "OB-GYN Ultrasound Procedure Report")	This is the root 'CONTAINER'
2	>	CONTAINS	INCLUDE	DTID (5001) Patient Characteristics	Refer to A.2.1.1 for ClearVue 350/550/650/850 3.1 usage of this.
3	>	CONTAINS	INCLUDE	DTID (5002) OB-GYN Procedure Summary Section	Refer to A.2.1.2 for ClearVue 350/550/650/850 3.1 usage of this.
4	>	CONTAINS	INCLUDE	DTID (5004) Fetal Biometry Ratio Section	Concepts in CID 12004 will be used, refer to A.2.1.3 for ClearVue 350/550/650/850 3.1 usage of this.
5	>	CONTAINS	INCLUDE	DTID (5005) Fetal Biometry Section	Concepts in CID 12005 will be used, refer to A.2.1.4 for ClearVue 350/550/650/850 3.1 usage of this.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
6	>	CONTAINS	INCLUDE	DTID (5006) Long Bones Section	Concepts in CID 12006 will be used, refer to A.2.1.5 for ClearVue 350/550/650/850 3.1 usage of this.
7	>	CONTAINS	INCLUDE	DTID (5007) Fetal Cranium Section	Concepts in CID 12007 will be used, refer to A.2.1.6 for ClearVue 350/550/650/850 3.1 usage of this.
8	>	CONTAINS	INCLUDE	DTID (5009) Biophysical Profile Section	Refer to A.2.1.7 for ClearVue 350/550/650/850 3.1 usage of this.
9	>	CONTAINS	INCLUDE	DTID (5011) Early Gestation Section	Concepts in CID 12009 will be used, refer to A.2.1.8 for ClearVue 350/550/650/850 3.1 usage of this.
10	>	CONTAINS	INCLUDE	DTID (5010) Amniotic Sac Section	Concepts in CID 12008 will be used, refer to A.2.1.9 for ClearVue 350/550/650/850 3.1 usage of this.
11	>	CONTAINS	INCLUDE	DTID (5015) Pelvis and Uterus Section	Concepts in CID 12011 will be used, refer to A.2.1.10 for ClearVue 350/550/650/850 3.1 usage of this.
12	>	CONTAINS	INCLUDE	DTID (5012) Ovaries Section	Refer to A.2.1.11 for ClearVue 350/550/650/850 3.1 usage of this.
13	>	CONTAINS	INCLUDE	DTID (5013) Follicles Section	This section is used with concept modifier Laterality = Left. Refer to A.2.1.12 for ClearVue 350/550/650/850 3.1 usage of this.
14	>	CONTAINS	INCLUDE	DTID (5013) Follicles Section	This section is used with concept modifier Laterality = Right. Refer to A.2.1.12 for ClearVue 350/550/650/850 3.1 usage of this.
15	>	CONTAINS	CONTAINER	EV (121070, DCM, "Findings")	This section (rows 15, 16, and 17) is used to include fetus vascular measurements. Refer to section A.2.1.13 for details. Measurements from DCID (12141), 'Fetal Vasculature' are used.
16	>>	HAS CONCEPT MOD	CODE	EV (G-C0E3, SRT, "Finding Site")	EV (T-F6800, SRT, "Embryonic Vascular Structure")
17	>>	CONTAINS	INCLUDE	DTID (5025) OB-GYN Fetal Vascular Measurement Group)	\$AnatomyGroup = DCID (12141) Fetal Vasculature). Refer to section A.2.1.13 for details of TID 5025.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
18	>	CONTAINS	CONTAINER	EV (121070, DCM, "Findings")	This section (rows 18, 19, and 20) is used to include pelvic vascular measurements. Refer to section A.2.1.14 for details. Measurements from DCID (12140), 'Fetal Vasculature' are used.
19	>>	HAS CONCEPT MOD	CODE	EV (G-C0E3, SRT, "Finding Site")	EV (T-D6007, SRT, "Pelvic Vascular Structure")
20	>>	CONTAINS	INCLUDE	DTID (5026) OB-GYN Pelvic Vascular Measurement Group)	\$AnatomyGroup = DCID (12140) Pelvic Vasculature Anatomical Location. Refer to section A.2.1.14 for details of TID 5026.

#### A.2.1.1 OB-GYN Patient Characteristics (TID 5001)

Use of the template TID 5001 in the context of ClearVue 350/550/650/850 3.1 is described in the following table.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	EV (121118, DCM, "Patient Characteristics")	
2	>	CONTAINS	TEXT	EV (121106, DCM, "Comment")	
3	>	CONTAINS	NUM	EV (8302-2, LN, "Patient Height")	Value is taken from PDE (Patient Data Entry) screen or from the MWL.
4	>	CONTAINS	NUM	EV (29463-7, LN, "Patient Weight")	Value is taken from PDE (Patient Data Entry) screen or from the MWL.
5	>	CONTAINS	NUM	EV (11996-6, LN, "Gravida")	Value is taken from PDE (Patient Data Entry) screen.
6	>	CONTAINS	NUM	EV (11977-6, LN, "Para")	Value is taken from PDE (Patient Data Entry) screen.
7	>	CONTAINS	NUM	EV (11612-9, LN, "Aborta")	Value is taken from PDE (Patient Data Entry) screen.
8	>	CONTAINS	NUM	EV (33065-4, LN, "Ectopic Pregnancies")	Value is taken from PDE (Patient Data Entry) screen.

#### A.2.1.2 OB-GYN Procedure Summary (TID 5002)

The following table describes the use of this template in the context of ClearVue 350/550/650/850 3.1.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	DT (121111, DCM, "Summary")	
2	>	CONTAINS	DATE	(11955-2, LN, "LMP")	Value is taken from PDE (Patient Data Entry) screen. -- Row 2, 3 and 4 are concepts from DCID 12003, "OB-GYN Dates"
3	>	CONTAINS	DATE	(11779-6, LN, "EDD from LMP")	Value automatically calculated by the ClearVue 350/550/650/850 3.1 system based on the value entered for LMP.
4	>	CONTAINS	DATE	(11781-2, LN, "EDD from average ultrasound age")	Value automatically calculated by the ClearVue 350/550/650/850 3.1 system based various measurements and on the LMP. If there is more than one fetus, the value used is the earliest calculated EDD amongst all fetuses.
5	>	CONTAINS	NUM	(11878-6, LN, "Number of Fetuses")	Value is taken from PDE (Patient Data Entry) screen. -- This value is actually inserted as invocation of TID 300 (Measurement) with concept(s) from DCID 12001, "OB-GYN summary" passed as parameters.
6	>	TEXT	CONTAINS	EV (121106, DCM, "Comment")	
7	>	CONTAINS	INCLUDE	"OB-GYN Fetus Summary" (BTID 5003)	Refer to section A.2.1.2.1 for details of ClearVue 350/550/650/850 3.1 usage of this. This template is included 1 per fetus.

#### A.2.1.2.1 OB-GYN Fetus Summary (TID 5003)

ClearVue 350/550/650/850 3.1 uses this template to insert measurements from DCID 12019. ClearVue 350/550/650/850 3.1 uses a private extension to DCID 12019 to define a new Fetus Summary measurement concept for 'Peak-to-Peak time interval over two beats'.

Following table shows the extension to Fetus Summary (CID 12019) used by ClearVue 350/550/650/850 3.1.

CSD	CV	CM
99PMSBLUS	C12019-01	Peak-to-Peak time interval over two beats

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	DT (125008, DCM, "Fetus Summary")	
2	>	HAS OBS CONTEXT	TEXT	EV (11951-1, LN, "Fetus ID")	<p>Value of "1", "2", "3" or "4" is used as identifier of the Fetus.</p> <p>-- This value is actually inserted as invocation of TID 1008 (Subject context - Fetus)</p> <p>-- This is present only if the study has more than one fetus.</p>
3	>	CONTAINS	TEXT	EV (121106, DCM, "Comment")	<p>This field contains all observations, findings (only the Finding text value preceded by the Finding Group Name) and the comments entered in the reporting screen on the ClearVue 350/550/650/850 3.1. In case of multiple fetuses, these observations are associated with the selected Fetus ID.</p> <p>For the Anatomy Visualized finding, a string 'Seen' will be displayed against the anatomy if the check box against the particular anatomy is checked in the reporting screen. A string 'Not Seen' will be displayed against the anatomy if the check box against the particular anatomy is not checked in the reporting screen.</p>
4	>	CONTAINS	NUM	(11888-5, LN, "Composite Ultrasound Age")	<p>This is a system-calculated value. This attribute is used to convey the "Average Ultrasound Age".</p> <p>-- This value is inserted as invocation of TID 300 (Measurement) with concepts from DCID 12019</p>

No	NL	REL WITH PARENT	VT	Concept Name	Comments
5	>	CONTAINS	NUM	(11885-1, LN, "Gestational Age by LMP")	This is a system-calculated value. -- This value is inserted as invocation of TID 300 (Measurement) with concepts from DCID 12019
6	>	CONTAINS	NUM	(11727-5, LN, "Estimated Weight")	This is a system-calculated value. -- This value is inserted as invocation of TID 300 (Measurement) with concepts from DCID 12019
7	>>	HAS CONCEPT MOD	CODE	Equation or Table using (121424, DCM, "Table of Values")	Concepts from CID 12014, OB Body Fetal Weight Equations and Tables will be used. Refer to section A.2.1.16 for concepts used in ClearVue 350/550/650/850 3.1.
8	>	CONTAINS	NUM	(99PMSBLUS, C12019-01, "Peak-to-Peak time interval over two beats")	This value is inserted as invocation of TID 300 (Measurement) with concepts from DCID 12019. This concept is an extension of DCID 12019.
9	>	CONTAINS	NUM	(LN, 11948-7, "Fetal Heart Rate")	Exported as "xxx {H.B.}/min (UCUM, Beats Per Minute) where xxx = number of beats

#### A.2.1.3 Fetal Biometry Ratio Section (TID 5004)

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	DT (125001, DCM, "Fetal Biometry Ratios")	
2	>	HAS OBS CONTEXT	TEXT	EV (11951-1,LN, "Fetus ID")	Value of "1", "2", "3" or "4" is used as identifier of the Fetus. -- This value is actually inserted as invocation of TID 1008 (Subject context - Fetus) -- This value is present only if more than one fetus exists.
3	>	CONTAINS	NUM	Measurements from CID 12004 (Fetal Biometry Ratios) are included.	These biometry measurements are added as part of invocation of Measurement (TID 300) template.

#### A.2.1.3.1 Fetal Biometry Ratios (CID 12004)

ClearVue 350/550/650/850 3.1 defines an extension of CID 12004 to include HrtC / TC ratio as part of this context group. Following table shows the concepts in CID 12004 (including the private extension for ClearVue 350/550/650/850 3.1) that are used in ClearVue 350/550/650/850 3.1.

CSD	CV	Code Meaning
LN	11947-9	HC/AC
LN	11871-1	FL/AC
LN	11872-9	FL/BPD
LN	11823-2	Cephalic Index
99PMSBLUS	C12004-01	HrtC/TC (Heart Circumference/Thoracic Circumference)

#### A.2.1.4 Fetal Biometry Section (TID 5005)

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	DT (125002, DCM, "Fetal Biometry")	
2	>	HAS OBS CONTEXT	TEXT	EV (11951-1,LN, "Fetus ID")	Will be present if more than one fetus.
3	>	CONTAINS	INCLUDE	Biometry Group (DTID 5008)	Measurements from DCID 12005 are used as 'Biometry type' to invoke this template one or more number of times. Refer to section A.2.1.6.1 for details of Biometry Group template usage.

#### A.2.1.4.1 Fetal Biometry Measurements (CID 12005)

ClearVue 350/550/650/850 3.1 defines a private extension to CID 12005 to include measurements available on ClearVue 350/550/650/850 3.1 but not (yet) defined in this context group. The following table shows the measurements from CID 12005 (including ClearVue 350/550/650/850 3.1 private extensions) that are used in ClearVue 350/550/650/850 3.1. All private extensions will use the coding scheme designator as 99PMSBLUS.

CSD	CV	Code Meaning
LN	11979-2	Abdominal Circumference

CSD	CV	Code Meaning
LN	11818-2	Anterior-Posterior Abdominal Diameter
LN	11819-0	Anterior-Posterior Trunk Diameter
LN	11820-8	Biparietal Diameter
LN	11965-1	Foot Length
LN	11984-2	Head Circumference
LN	11851-3	Occipital-Frontal Diameter
LN	11988-3	Thoracic Circumference
LN	11862-0	Transverse Abdominal Diameter
LN	11864-6	Transverse Thoracic Diameter
99PMSBLUS	C12005-01	Ear Length
99PMSBLUS	C12005-02	Fetal Trunk Cross Sectional Area
99PMSBLUS	C12005-03	Heart Circumference
99PMSBLUS	C12005-04	Length of Middle Phalanx of the Fifth Digit
99PMSBLUS	C12005-05	Renal Width
99PMSBLUS	C12005-06	Renal Length
99PMSBLUS	C12005-07	Anterior-Posterior Thoracic Diameter
99PMSBLUS	C12005-08	Transverse Trunk Diameter
99PMSBLUS	C12005-10	APTD*TTD

#### A.2.1.5 Fetal Long Bones Section (TID 5006)

Fetal Long Bones section is inserted in the SR Document in the same way as Fetal Biometry Section (Refer section A.2.1.4) using “DT (125003, DCM, “Fetal Long Bones”). \$Biometry Type used to invoke the template TID 5008 is taken from the context group Fetal Long Bones Measurement (CID 12006). All the measurements in CID 12006 are available in ClearVue 350/550/650/850 3.1 as described in the following table.

CSD	CV	Code Meaning
LN	11966-9	Humerus length
LN	11967-7	Radius length
LN	11969-3	Ulna length
LN	11968-5	Tibia length
LN	11964-4	Fibula length
LN	11962-8	Clavicle length
LN	11963-6	Femur Length

#### A.2.1.6 Fetal Cranium Section (TID 5007)

Fetal Cranium section is inserted in the SR Document in the same way as Fetal Biometry Section (Refer section A.2.1.4) using “DT (125004, DCM, “Fetal Cranium”). \$Biometry Type used to invoke the template TID 5008 is taken from the context group Fetal Cranium (CID 12007).

ClearVue 350/550/650/850 3.1 defines a private extension to CID 12007 to include cranial measurements available in ClearVue 350/550/650/850 3.1 but not (yet) defined in CID 12007. The following table shows the measurements from CID 12007 (including ClearVue 350/550/650/850 3.1 private extensions) that are used in ClearVue 350/550/650/850 3.1. All private extensions will use the coding scheme designator as 99PMSBLUS.

CSD	CV	Code Meaning
LN	12171-5	Lateral Ventricle width
LN	11860-4	Cisterna Magna Length
LN	12146-7	Nuchal Fold thickness
LN	33070-4	Inner Orbital Diameter
LN	11629-3	Outer Orbital Diameter
LN	11863-8	Trans Cerebellar Diameter
LN	33197-5	Anterior Horn Lateral ventricular width
LN	33196-7	Posterior Horn Lateral ventricular width
LN	12170-7	Width of Hemisphere
99PMSBLUS	C12007-01	Diameter of First Orbit
99PMSBLUS	C12007-02	Diameter of Second Orbit
99PMSBLUS	C12007-03	Ratio of Posterior Horn Lateral ventricular width/Hemisphere

#### A.2.1.6.1 Fetal Biometry Group (TID 5008)

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	DT(125005, DCM, “Biometry Group”)	
2	>	CONTAINS	NUM	Measurement of selected ‘Biometry Type’	This row and next two rows are inserted as part of TID 300 (Measurement) invocation. If multiple measurements are made of the same biometry type, these three rows will be repeated for each measurement instance.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
3	>>	INFERRRED FROM	IMAGE	Referenced Content Item Identifier	An ordered set of one or more integers that uniquely identify the Image in the 'Image Library' section of this SR document. This is the image from which the measurement is inferred.  This item will not be present, if the measurement does not refer to any image.
4	>>	HAS CONCEPT MOD	CODE	EV (121401, DCM, "Derivation")	If a user has performed more than one measurement then he / she can either use average (default) of these instances or he can specifically select one of the measured instances for using in calculations. If the selection is Average, then that average measurement instance will have a derivation modifier as (R-00317, SRT, "Mean").
5	>>	HAS PROPERTIES	CODE	EV (121404, DCM, "Selection Status")	This will have a value (121412, DCM, "Mean Value Chosen") if the Derivation is 'Mean'. In all other cases, this will have a value as (121410, DCM "User chosen value").
6	>	CONTAINS	NUM	EV (18185-9, LN, "Gestational Age")	This will be present if user has selected the corresponding gestation age calculation. For example, if the biometry type is BPD and user has selected GA (BPD) as one of the calculations (from the analysis setup application), this row will be present.  ClearVue 350/550/650/850 3.1 system automatically calculates the GA based on standard (or user defined) equations and tables.
7	>>	INFERRRED FROM	CODE	Equation or Table using (121424, DCM, "Table of Values")	Concepts from CID 12013, Gestation age equations and tables will be used. Refer to section A.2.1.15 for concepts used in ClearVue 350/550/650/850 3.1.

#### A.2.1.7 Fetal Biophysical Profile Section (TID5009)

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	DT (125006, DCM, "Biophysical Profile")	

2	>	HAS OBS CONTEXT	TEXT	EV (11951-1, LN, "Fetus ID")	Will be present if more than one fetus.
3	>	CONTAINS	NUM	EV (11631-9, LN, "Gross Body Movement")	ClearVue 350/550/650/850 3.1 uses the value as entered in the reporting screen.
4	>	CONTAINS	NUM	EV (11632-7, LN, "Fetal Breathing")	ClearVue 350/550/650/850 3.1 uses the value as entered in the reporting screen.
5	>	CONTAINS	NUM	EV (11635-0, LN, "Fetal Tone")	ClearVue 350/550/650/850 3.1 uses the value as entered in the reporting screen.
6	>	CONTAINS	NUM	EV (11630-1, LN, "Amniotic Fluid Volume")	ClearVue 350/550/650/850 3.1 uses the value as entered in the reporting screen.
7	>	CONTAINS	NUM	DT (11634-3, LN, "Biophysical Profile Sum Score")	ClearVue 350/550/650/850 3.1 automatically calculates the sum of all the scores.

#### A.2.1.8 Early Gestation Section (TID 5011)

Early Gestation section is inserted in the SR Document in the same way as Fetal Biometry Section (Refer section A.2.1.4) using "DT (125009, DCM, "Early Gestation")". \$Biometry Type used to invoke the template TID 5008 is taken from the context group Early Gestation Biometry Measurements (CID 12009).

CSD	CV	Code Meaning
LN	11957-8	Crown Rump Length
LN	11850-5	Gestational Sac Diameter
LN	33071-2	Spine Length
LN	11816-6	Yolk Sac length
99PMSBLUS	C12009-05	Endomyometrial Mantle

#### A.2.1.9 Amniotic Sac Section (TID 5010)

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	DT (121070, DCM, "Findings")	
2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3, SRT, "Finding Site")	DT (T-F1300, SRT, "Amniotic Sac")

3	>	CONTAINS	NUM	(11627-7, LN, "Amniotic Fluid Index")	This is inserted as part of the invocation of template TID 300 (Measurement)
4	>	CONTAINS	NUM	(11624-4, LN, "First Quadrant Diameter")	This is inserted as part of the invocation of template TID 300 (Measurement)
5	>	CONTAINS	NUM	(11626-9, LN, "Second Quadrant Diameter")	This is inserted as part of the invocation of template TID 300 (Measurement)
6	>	CONTAINS	NUM	(11625-1, LN, "Third Quadrant Diameter")	This is inserted as part of the invocation of template TID 300 (Measurement)
7	>	CONTAINS	NUM	(11623-6, LN, "Fourth Quadrant Diameter")	This is inserted as part of the invocation of template TID 300 (Measurement)
8	>>	HAS CONCEPT MOD	CODE	EV (121401, DCM, "Derivation")	This will have a value 'Mean' IFF average measurement instance is used in calculations.
9	>>	HAS PROPERTIES	CODE	EV (121404, DCM, "Selection Status")	This will have a value 'Mean Value Chosen' if the Derivation is 'Mean'. In all other cases, this will have a value, 'User Chosen Value'.
10	>>	INFERRRED FROM	IMAGE	Referenced Content Item Identifier	Refers to the image on which this measurement was done.

#### A.2.1.10 Pelvis and Uterus Section (TID 5015)

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	DT (125011, DCM, "Pelvis and Uterus")	
2	>	CONTAINS	CONTAINER	EV (T-83000, SRT, "Uterus")	DTID 5016 (LWH Volume Group) is included. Uterus volume, length and width measurements are inserted. Group Name is 'Uterus'
3	>>	CONTAINS	NUM	(33192-6, LN, "Uterus Volume")	This row is inserted as part of TID 300 (Measurement) invocation. ClearVue 350/550/650/850 3.1 automatically calculates the volume based on L, W and H measurements.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
4	>>	CONTAINS	NUM	(11842-2, LN, "Uterus Length")	This row is inserted as part of TID 300 (Measurement) invocation. -- Similar to rows 4, 5 and 6, the concepts for Uterus Height and Uterus Width are added too. These concepts are: (11859-6, LN, "Uterus Height") and (11865-3, LN, "Uterus Width")
5	>>>	HAS CONCEPT MOD	CODE	EV (121401, DCM, "Derivation")	This will have a value 'Mean' IFF the average measurement instance is used in calculations.
6	>>>	HAS PROPERTIES	CODE	EV (121404, DCM, "Selection Status")	This will have a value (121412, DCM, "Mean Value Chosen") if the Derivation is 'Mean'. In all other cases, this will have a value as (121410, DCM "User chosen value").
7	>>>	INFERRRED FROM	IMAGE	Referenced Content Item Identifier	Refers to the image on which this measurement was done.
8	>	CONTAINS	NUM	(11961-0, LN, "Cervix Length")	This measurement is from CID 12011, "Ultrasound Pelvic and Uterus". This is inserted as part of invocation of TID 300 (Measurement). Similar to other measurements, the concept modifier for 'Derivation', Selection Status and 'Referenced Content Item' would be present for this measurement.  Note:- Only Cervix Length and Endometrium Thickness from CID 12011 will be present in rows 7 and 8. All bladder related measurements from CID 12011 will be present under the group 'Bladder' as shown in the rows from 9.
9	>	CONTAINS	NUM	(12145-9, LN, "Endometrium Thickness")	This measurement is from CID 12011, "Ultrasound Pelvic and Uterus".
10	>	CONTAINS	CONTAINER	EV (T-74000, SRT, "Bladder")	DTID 5016 (LWH Volume Group) is included. Bladder volume, length and width measurements are inserted. Group Name is 'Bladder'

No	NL	REL WITH PARENT	VT	Concept Name	Comments
11	>>	CONTAINS	NUM	(C12011-04, 99PMSBLUS, "Bladder Volume")	This row is inserted as part of TID 300 (Measurement) invocation. ClearVue 350/550/650/850 3.1 automatically calculates the volume based on L, W and H measurements.
12	>>	CONTAINS	NUM	(C12011-01, 99PMSBLUS, "Bladder Length")	This row is inserted as part of TID 300 (Measurement) invocation. -- Similar to rows 11, 12 and 13, the concepts for Bladder Width and Bladder Height are added too. These concepts are: (C12011-02, 99PMSBLUS, "Bladder Width") and (C12011-03, 99PMSBLUS, "Bladder Height")
13	>>>	HAS CONCEPT MOD	CODE	EV (121401, DCM, "Derivation")	This will have a value 'Mean' IFF the average measurement instance is used in calculations.
14	>>>	HAS PROPERTIES	CODE	EV (121404, DCM, "Selection Status")	This will have a value (121412, DCM, "Mean Value Chosen") if the Derivation is 'Mean'. In all other cases, this will have a value as (121410, DCM "User chosen value").
15	>>>	INFERRRED FROM	IMAGE	Referenced Content Item Identifier	Refers to the image on which this measurement was done.
16	>	CONTAINS	CONTAINER	EV (T-74000, SRT, "Bladder")	DTID 5016 (LWH Volume Group) is included. Post Void Bladder volume, length and width measurements are inserted. Group Name is 'Bladder'
17	>>	CONTAINS	NUM	(C12011-08, 99PMSBLUS, "Post Void Bladder Volume")	This row is inserted as part of TID 300 (Measurement) invocation. ClearVue 350/550/650/850 3.1 automatically calculates the volume based on L, W and H measurements.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
18	>>	CONTAINS	NUM	(C12011-05, 99PMSBLUS, "Post Void Bladder Length")	This row is inserted as part of TID 300 (Measurement) invocation. -- Similar to rows 16, 17 and 18, the concepts for Post Void Bladder Width and Post Void Bladder Height are added too. These concepts are: (C12011-06, 99PMSBLUS, "Post Void Bladder Width") and (C12011-07, 99PMSBLUS, "Post Void Bladder Height")
19	>>>	HAS CONCEPT MOD	CODE	EV (121401, DCM, "Derivation")	This will have a value 'Mean' IFF the average measurement instance is used in calculations.
20	>>>	HAS PROPERTIES	CODE	EV (121404, DCM, "Selection Status")	This will have a value (121412, DCM, "Mean Value Chosen") if the Derivation is 'Mean'. In all other cases, this will have a value as (121410, DCM "User chosen value").
21	>>>	INFERRRED FROM	IMAGE	Referenced Content Item Identifier	Refers to the image on which this measurement was done.

#### A.2.1.10.1 CID 12011 Ultrasound Pelvis And Uterus

ClearVue 350/550/650/850 3.1 uses a private extension to CID 12011 to define new concepts for Bladder related measurements. Following table shows the details.

CSD	CV	CM
LN	11961-0	Cervix Length
LN	12145-9	Endometrium Thickness
99PMSBLUS	C12011-01	Bladder Length
99PMSBLUS	C12011-02	Bladder Width
99PMSBLUS	C12011-03	Bladder Height
99PMSBLUS	C12011-04	Bladder Volume
99PMSBLUS	C12011-05	Post Void Bladder Length
99PMSBLUS	C12011-06	Post Void Bladder Width
99PMSBLUS	C12011-07	Post Void Bladder Height
99PMSBLUS	C12011-08	Post Void Bladder Volume

A.2.1.11      **Ovaries Section (TID 5012)**

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	DT (121070, DCM, "Findings")	
2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3, SRT, "Finding Site")	DT (T-87000, SRT, "Ovary")
3	>	CONTAINS	CONTAINER	EV (T-87000, SRT, "Ovary")	DTID 5016 (LWH Volume Group) is included. Left ovary volume, length and width measurements are inserted. Group name is 'Ovary'.
4	>>	CONTAINS	NUM	EV (12164-0, LN, "Left Ovary Volume")	This row is inserted as part of TID 300 (Measurement) invocation. ClearVue 350/550/650/850 3.1 automatically calculates the volume based on L, W and H measurements.
5	>>	CONTAINS	NUM	EV (11840-6, LN, "Left Ovary Length")	This row is inserted as part of TID 300 (Measurement) invocation. -- Similar to rows 5, 6 and 7, the concepts for Ovary Height and Ovary Width are added too. These concepts are: EV (11857-0, LN, "Left Ovary Height") and EV (11829-9, LN, "Left Ovary Width")
6	>> >	HAS CONCEPT MOD	CODE	EV (121401, DCM, "Derivation")	This will have a value "Mean" IFF the average measurement instance is used in calculations.
7	>> >	HAS PROPERTIES	CODE	EV (121404, DCM, "Selection Status")	This will have a value (121412, DCM, "Mean Value Chosen") if the Derivation is 'Mean'. In all other cases, this will have a value as (121410, DCM "User chosen value").
8	>> >	INFERRRED FROM	IMAGE	Referenced Content Item Identifier	Refers to the image on which this measurement was done.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
					<p>Similarly DTID 5016 (LWH Volume Group) is included for Right ovary volume, length and width measurements. The related concepts codes are –</p> <p>\$GroupName = EV (T-87000, SRT, "Ovary")  \$Width = EV (11830-7, LN, "Right Ovary Width")  \$Length = EV (11841-4, LN, "Right Ovary Length")  \$Height = EV (11858-8, LN, "Right Ovary Height")  \$Volume= EV (12165-7, LN, "Right Ovary Volume")</p>

#### A.2.1.12      Follicles Section (TID 5013)

SR Document may contain two instances of the Follicles section. First instance is included for left ovarian follicles and the second instance is included for right ovarian follicle. Laterality concept modifier will be used accordingly. Measurements for up to 16 follicles may be included in this section.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	DT (121070, DCM, "Findings")	
2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3, SRT, "Finding Site")	DT (T-87600, SRT, "Ovarian Follicle")
3	>	HAS CONCEPT MOD	CODE	EV (G-C171, SRT, "Laterality")	EV (G-A101, SRT, "Left") OR EV (G-A100, SRT, "Right")
4	>	CONTAINS	NUM	EV (11879-4, LN, "Number of follicles in left ovary") OR EV (11880-2, LN, "Number of follicles in right ovary")	Number of follicles in the ovary.
5	>	CONTAINS	CONTAINER	EV (125007, DCM, "Measurement Group")	Template TID 5014 (Follicle Measurement Group) is included.
6	>>	HAS OBS CONTEXT	TEXT	EV (125010, DCM, "Identifier")	ClearVue 350/550/650/850 3.1 uses numbers "1", "2", "3"...up to "16" to identify the follicle. -- Row 6, 7 and 8 are added per follicle measurement.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
7	>>	CONTAINS	NUM	EV (G-D705, SRT, "Volume")	This is inserted as part of TID 300 invocation. ClearVue 350/550/650/850 3.1 automatically calculates the volume based on the follicle diameter.
8	>>	CONTAINS	NUM	(11793-7, LN, "Follicle diameter")	This is inserted as part of TID 300 invocation.

#### A.2.1.13 OB-GYN Fetus Vascular Ultrasound Measurement Group (TID 5025)

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	EV (T-F6800, SRT, "Embryonic Vascular Structure")	
2	>	HAS OBS CONTEXT	TEXT	EV (11951-1, LN, "Fetus ID")	Will be present if more than one fetus.
3	>	CONTAINS	NUM	Measurement of selected fetal vascular anatomic location.	Measurement types from CID 12119 (Vascular Ultrasound Property) and CID 12121 (Vascular Indices and Ratios) for the anatomical locations specified in CID 12141 (Fetal Vasculature Anatomic Locations) are used.

##### A.2.1.13.1 Fetal Vascular Measurements

ClearVue 350/550/650/850 3.1 uses a private extension to CID 12141 to define a new fetal vascular anatomical location for 'Ductus Venosus'. Also, the anatomical locations 'Umbilical Artery' and 'Uterine Artery' defined in CID 12140 ('Pelvic Vasculature Anatomic Location') have been included in CID 12141 as ClearVue 350/550/650/850 3.1 considers this as Fetal measurement rather than Pelvic measurement.

The following table shows the extension to Fetal Vasculature Anatomical Locations (CID 12141) used by ClearVue 350/550/650/850 3.1.

CSD	CV	CM
99PMSBLUS	C12141-01	Ductus Venosus
SRT	T-F1810	Umbilical Artery

SRT	T-46820	Uterine Artery*
-----	---------	-----------------

\* Uterine Artery for Fetal Vascular includes \$LATERALITY=(G-A101, SRT, "Left"); (G-A100, SRT, "Right")

The following table shows the fetal vascular measurements (and calculations) used in ClearVue 350/550/650/850 3.1 as part of TID 5025.

#### Fetal Vascular Measurements

Measurement	Measurement Type from CID 12119 and it's includes.	Vascular Anatomic Location from CID 12141
Diastolic Velocity (Ductus Venosus)	(LN, 11653-3, End Diastolic Velocity)	(99PMSBLUS, C12141-01, Ductus Venosus)
Systolic Velocity (Ductus Venosus)	(LN, 11726-7, Peak Systolic Velocity)	(99PMSBLUS, C12141-01, Ductus Venosus)
Minimum Diastolic Velocity (Ductus Venosus)	(LN, 11665-7, Minimum Diastolic Velocity)	(99PMSBLUS, C12141-01, Ductus Venosus)
Time Averaged Peak Velocity (Ductus Venosus)	(LN, 11692-1, Time Averaged Peak Velocity)	(99PMSBLUS, C12141-01, Ductus Venosus)
Time Averaged Mean Velocity <sup>1</sup> (Ductus Venosus)	(LN, 20352-1, Time Averaged Mean Velocity)	(99PMSBLUS, C12141-01, Ductus Venosus)
Acceleration Index (Ductus Venosus)	(LN, 20167-3, Acceleration Index)	(99PMSBLUS, C12141-01, Ductus Venosus)
Acceleration Time (Ductus Venosus)	(LN, 20168-1, Acceleration Time)	(99PMSBLUS, C12141-01, Ductus Venosus)
Velocity Time Integral (Ductus Venosus)	(LN, 20354-7, Velocity Time Integral)	(99PMSBLUS, C12141-01, Ductus Venosus)
Pulsatility Index (Ductus Venosus)	(LN, 12008-9, Pulsatility Index)	(99PMSBLUS, C12141-01, Ductus Venosus)
Resistivity Index (Ductus Venosus)	(LN, 12023-8, Resistivity Index)	(99PMSBLUS, C12141-01, Ductus Venosus)
Systolic to Diastolic Ratio (Ductus Venosus)	(LN, 12144-2, Systolic to Diastolic Velocity Ratio)	(99PMSBLUS, C12141-01, Ductus Venosus)
Diastolic to Systolic Velocity Ratio (Ductus Venosus)	(99PMSBLUS, C12121-01, Diastolic to Systolic Velocity Ratio)	(99PMSBLUS, C12141-01, Ductus Venosus)
Diastolic Velocity (Umbilical Artery)	(LN, 11653-3, End Diastolic Velocity)	(SRT, T-F1810, Umbilical Artery)
Systolic Velocity (Umbilical Artery)	(LN, 11726-7, Peak Systolic Velocity)	(SRT, T-F1810, Umbilical Artery)
Minimum Diastolic Velocity (Umbilical Artery)	(LN, 11665-7, Minimum Diastolic Velocity)	(SRT, T-F1810, Umbilical Artery)
Time Averaged Peak Velocity (Umbilical Artery)	(LN, 11692-1, Time Averaged Peak Velocity)	(SRT, T-F1810, Umbilical Artery)

<b>Measurement</b>	<b>Measurement Type from CID 12119 and it's includes.</b>	<b>Vascular Anatomic Location from CID 12141</b>
Time Averaged Mean Velocity <sup>1</sup> (Umbilical Artery)	(LN, 20352-1, Time Averaged Mean Velocity)	(SRT, T-F1810, Umbilical Artery)
Acceleration Index (Umbilical Artery)	(LN, 20167-3, Acceleration Index)	(SRT, T-F1810, Umbilical Artery)
Acceleration Time (Umbilical Artery)	(LN, 20168-1, Acceleration Time)	(SRT, T-F1810, Umbilical Artery)
Velocity Time Integral (Umbilical Artery)	(LN, 20354-7, Velocity Time Integral)	(SRT, T-F1810, Umbilical Artery)
Pulsatility Index (Umbilical Artery)	(LN, 12008-9, Pulsatility Index)	(SRT, T-F1810, Umbilical Artery)
Resistivity Index (Umbilical Artery)	(LN, 12023-8, Resistivity Index)	(SRT, T-F1810, Umbilical Artery)
Systolic to Diastolic Ratio (Umbilical Artery)	(LN, 12144-2, Systolic to Diastolic Velocity Ratio)	(SRT, T-F1810, Umbilical Artery)
Diastolic to Systolic Velocity Ratio (Umbilical Artery)	(99PMSBLUS, C12121-01, Diastolic to Systolic Velocity Ratio)	(SRT, T-F1810, Umbilical Artery)
Diastolic Velocity (Middle Cerebral Artery)	(LN, 11653-3, End Diastolic Velocity)	(SRT, T-45600, Middle Cerebral Artery)
Systolic Velocity (Middle Cerebral Artery)	(LN, 11726-7, Peak Systolic Velocity)	(SRT, T-45600, Middle Cerebral Artery)
Minimum Diastolic Velocity (Middle Cerebral Artery)	(LN, 11665-7, Minimum Diastolic Velocity)	(SRT, T-45600, Middle Cerebral Artery)
Time Averaged Peak Velocity (Middle Cerebral Artery)	(LN, 11692-1, Time Averaged Peak Velocity)	(SRT, T-45600, Middle Cerebral Artery)
Time Averaged Mean Velocity <sup>1</sup> (Middle Cerebral Artery)	(LN, 20352-1, Time Averaged Mean Velocity)	(SRT, T-45600, Middle Cerebral Artery)
Acceleration Index (Middle Cerebral Artery)	(LN, 20167-3, Acceleration Index)	(SRT, T-45600, Middle Cerebral Artery)
Acceleration Time (Middle Cerebral Artery)	(LN, 20168-1, Acceleration Time)	(SRT, T-45600, Middle Cerebral Artery)
Velocity Time Integral (Middle Cerebral Artery)	(LN, 20354-7, Velocity Time Integral)	(SRT, T-45600, Middle Cerebral Artery)
Pulsatility Index (Middle Cerebral Artery)	(LN, 12008-9, Pulsatility Index)	(SRT, T-45600, Middle Cerebral Artery)
Resistivity Index (Middle Cerebral Artery)	(LN, 12023-8, Resistivity Index)	(SRT, T-45600, Middle Cerebral Artery)
Systolic to Diastolic Ratio (Middle Cerebral Artery)	(LN, 12144-2, Systolic to Diastolic Velocity Ratio)	(SRT, T-45600, Middle Cerebral Artery)

<b>Measurement</b>	<b>Measurement Type from CID 12119 and it's includes.</b>	<b>Vascular Anatomic Location from CID 12141</b>
Diastolic to Systolic Velocity Ratio (Middle Cerebral Artery)	(99PMSBLUS, C12121-01, Diastolic to Systolic Velocity Ratio)	(SRT, T-45600, Middle Cerebral Artery)
Diastolic Velocity (Left Uterine Artery)	(LN, 11653-3, End Diastolic Velocity)	(SRT, T-46820, Uterine Artery) \$Laterality= Left
Systolic Velocity (Left Uterine Artery)	(LN, 11726-7, Peak Systolic Velocity)	(SRT, T-46820, Uterine Artery) \$Laterality= Left
Minimum Diastolic Velocity (Left Uterine Artery)	(LN, 11665-7, Minimum Diastolic Velocity)	(SRT, T-46820, Uterine Artery) \$Laterality= Left
Time Averaged Peak Velocity (Left Uterine Artery)	(LN, 11692-1, Time Averaged Peak Velocity)	(SRT, T-46820, Uterine Artery) \$Laterality= Left
Pulsatility Index (Left Uterine Artery)	(LN, 12008-9, Pulsatility Index)	(SRT, T-46820, Uterine Artery) \$Laterality= Left
Resistivity Index (Left Uterine Artery)	(LN, 12023-8, Resistivity Index)	(SRT, T-46820, Uterine Artery) \$Laterality= Left
Systolic to Diastolic Ratio (Left Uterine Artery)	(LN, 12144-2, Systolic to Diastolic Velocity Ratio)	(SRT, T-46820, Uterine Artery) \$Laterality= Left
Diastolic Velocity (Right Uterine Artery)	(LN, 11653-3, End Diastolic Velocity)	(SRT, T-46820, Uterine Artery) \$Laterality= Right
Systolic Velocity (Right Uterine Artery)	(LN, 11726-7, Peak Systolic Velocity)	(SRT, T-46820, Uterine Artery) \$Laterality= Right
Minimum Diastolic Velocity (Right Uterine Artery)	(LN, 11665-7, Minimum Diastolic Velocity)	(SRT, T-46820, Uterine Artery) \$Laterality= Right
Time Averaged Peak Velocity (Right Uterine Artery)	(LN, 11692-1, Time Averaged Peak Velocity)	(SRT, T-46820, Uterine Artery) \$Laterality= Right
Pulsatility Index (Right Uterine Artery)	(LN, 12008-9, Pulsatility Index)	(SRT, T-46820, Uterine Artery) \$Laterality= Right
Resistivity Index (Right Uterine Artery)	(LN, 12023-8, Resistivity Index)	(SRT, T-46820, Uterine Artery) \$Laterality= Right
Systolic to Diastolic Ratio (Right Uterine Artery)	(LN, 12144-2, Systolic to Diastolic Velocity Ratio)	(SRT, T-46820, Uterine Artery) \$Laterality= Right

<sup>1</sup> Available only on ClearVue 550 with High Q

**A.2.1.14 OB-GYN Pelvic Vascular Ultrasound Measurement Group (TID 5026)**

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	EV (T-D6007, SRT, "Pelvic Vascular Structure")	
2	>	HAS CONCEPT MOD	CODE	EV (G-C171, SRT "Laterality")	Laterality is used only if the measurement needs to be qualified with the laterality of the anatomy.
3	>	CONTAINS	NUM	Measurement of selected pelvic vascular anatomic location.	Measurement types from CID 12119 (Vascular Ultrasound Property) and CID 12121 (Vascular Indices and Ratios) for the anatomical locations specified in CID 12140 (Pelvic Vasculature Anatomic Locations) are used.

#### A.2.1.14.1 Pelvic Vascular Measurements

The following table shows the pelvic vascular measurements (and calculations) used in ClearVue 350/550/650/850 3.1 as part of TID 5026.

Measurement	Measurement Type from CID 12119 and it's includes.	Vascular Anatomic Location from CID 12140
Diastolic Velocity (Left Ovarian Artery)	(LN, 11653-3, End Diastolic Velocity)	(SRT, T-46980, Ovarian Artery) \$Laterality = Left
Systolic Velocity (Left Ovarian Artery)	(LN, 11726-7, Peak Systolic Velocity)	(SRT, T-46980, Ovarian Artery) \$Laterality = Left
Minimum Diastolic Velocity (Left Ovarian Artery)	(LN, 11665-7, Minimum Diastolic Velocity)	(SRT, T-46980, Ovarian Artery) \$Laterality = Left
Time Averaged Peak Velocity (Left Ovarian Artery)	(LN, 11692-1, Time Averaged Peak Velocity)	(SRT, T-46980, Ovarian Artery) \$Laterality = Left
Time Averaged Mean Velocity <sup>1</sup> (Left Ovarian Artery)	(LN, 20352-1, Time Averaged Mean Velocity)	(SRT, T-46980, Ovarian Artery) \$Laterality = Left
Acceleration Index (Left Ovarian Artery)	(LN, 20167-3, Acceleration Index)	(SRT, T-46980, Ovarian Artery) \$Laterality = Left
Acceleration Time (Left Ovarian Artery)	(LN, 20168-1, Acceleration Time)	(SRT, T-46980, Ovarian Artery) \$Laterality = Left
Velocity Time Integral (Left Ovarian Artery)	(LN, 20354-7, Velocity Time Integral)	(SRT, T-46980, Ovarian Artery) \$Laterality = Left
Pulsatility Index (Left Ovarian Artery)	(LN, 12008-9, Pulsatility Index)	(SRT, T-46980, Ovarian Artery) \$Laterality = Left
Resistivity Index (Left Ovarian Artery)	(LN, 12023-8, Resistivity Index)	(SRT, T-46980, Ovarian Artery) \$Laterality = Left
Systolic to Diastolic Ratio (Left Ovarian Artery)	(LN, 12144-2, Systolic to Diastolic Velocity Ratio)	(SRT, T-46980, Ovarian Artery) \$Laterality = Left
Diastolic to Systolic Ratio (Left Ovarian Artery)	(99PMSBLUS, C12121-01, Diastolic to Systolic Velocity Ratio)	(SRT, T-46980, Ovarian Artery) \$Laterality = Left
Diastolic Velocity (Right Ovarian Artery)	(LN, 11653-3, End Diastolic Velocity)	(SRT, T-46980, Ovarian Artery) \$Laterality = Right
Systolic Velocity (Right Ovarian Artery)	(LN, 11726-7, Peak Systolic Velocity)	(SRT, T-46980, Ovarian Artery) \$Laterality = Right
Minimum Diastolic Velocity (Right Ovarian Artery)	(LN, 11665-7, Minimum Diastolic Velocity)	(SRT, T-46980, Ovarian Artery) \$Laterality = Right
Time Averaged Peak Velocity (Right Ovarian Artery)	(LN, 11692-1, Time Averaged Peak Velocity)	(SRT, T-46980, Ovarian Artery) \$Laterality = Right
Time Averaged Mean Velocity <sup>1</sup> (Right Ovarian Artery)	(LN, 20352-1, Time Averaged Mean Velocity)	(SRT, T-46980, Ovarian Artery) \$Laterality = Right
Acceleration Index (Right Ovarian Artery)	(LN, 20167-3, Acceleration Index)	(SRT, T-46980, Ovarian Artery) \$Laterality = Right

<b>Measurement</b>	<b>Measurement Type from CID 12119 and it's includes.</b>	<b>Vascular Anatomic Location from CID 12140</b>
Acceleration Time (Right Ovarian Artery)	(LN, 20168-1, Acceleration Time)	(SRT, T-46980, Ovarian Artery) \$Laterality = Right
Velocity Time Integral (Right Ovarian Artery)	(LN, 20354-7, Velocity Time Integral)	(SRT, T-46980, Ovarian Artery) \$Laterality = Right
Pulsatility Index (Right Ovarian Artery)	(LN, 12008-9, Pulsatility Index)	(SRT, T-46980, Ovarian Artery) \$Laterality = Right
Resistivity Index (Right Ovarian Artery)	(LN, 12023-8, Resistivity Index)	(SRT, T-46980, Ovarian Artery) \$Laterality = Right
Systolic to Diastolic Ratio (Right Ovarian Artery)	(LN, 12144-2, Systolic to Diastolic Velocity Ratio)	(SRT, T-46980, Ovarian Artery) \$Laterality = Right
Diastolic to Systolic Ratio (Right Ovarian Artery)	(99PMSBLUS, C12121-01, Diastolic to Systolic Velocity Ratio)	(SRT, T-46980, Ovarian Artery) \$Laterality = Right
Diastolic Velocity (Uterine Artery)	(LN, 11653-3, End Diastolic Velocity)	(SRT, T-46820, Uterine Artery)
Systolic Velocity (Uterine Artery)	(LN, 11726-7, Peak Systolic Velocity)	(SRT, T-46820, Uterine Artery)
Minimum Diastolic Velocity (Uterine Artery)	(LN, 11665-7, Minimum Diastolic Velocity)	(SRT, T-46820, Uterine Artery)
Time Averaged Peak Velocity (Uterine Artery)	(LN, 11692-1, Time Averaged Peak Velocity)	(SRT, T-46820, Uterine Artery)
Time Averaged Mean Velocity <sup>1</sup> (Uterine Artery)	(LN, 20352-1, Time Averaged Mean Velocity)	(SRT, T-46820, Uterine Artery)
Acceleration Index (Uterine Artery)	(LN, 20167-3, Acceleration Index)	(SRT, T-46820, Uterine Artery)
Acceleration Time (Uterine Artery)	(LN, 20168-1, Acceleration Time)	(SRT, T-46820, Uterine Artery)
Velocity Time Integral (Uterine Artery)	(LN, 20354-7, Velocity Time Integral)	(SRT, T-46820, Uterine Artery)
Pulsatility Index (Uterine Artery)	(LN, 12008-9, Pulsatility Index)	(SRT, T-46820, Uterine Artery)
Resistivity Index (Uterine Artery)	(LN, 12023-8, Resistivity Index)	(SRT, T-46820, Uterine Artery)
Systolic to Diastolic Ratio (Uterine Artery)	(LN, 12144-2, Systolic to Diastolic Velocity Ratio)	(SRT, T-46820, Uterine Artery)
Diastolic to Systolic Ratio (Uterine Artery)	(99PMSBLUS, C12121-01, Diastolic to Systolic Velocity Ratio)	(SRT, T-46820, Uterine Artery)

<sup>1</sup> Available only on ClearVue 550 with High Q

**A.2.1.15 Gestation Age Equations & Tables (CID 12013)**

The following are the Gestation Age Equations and Tables supported by ClearVue 350/550/650/850 3.1:

CSD	CV	Code Meaning
LN	11885-1	Gestational Age by LMP
LN	11892-7	AC, Hadlock 1984
99PMSBLUS	C12013-30	AC, Hansmann 1986
LN	33076-1	AC, Shinozuka 1996
99PMSBLUS	C12013-01	AC, ASUM 2001
99PMSBLUS	C12013-02	BPD, ASUM 2001
LN	33086-0	BPD-oi, Chitty 1997
LN	33087-8	BPD-oo, Chitty 1997
LN	11902-4	BPD, Hadlock 1984
LN	33538-0	BPD, Hansmann 1986
LN	11905-7	BPD, Jeanty 1984
99PMSBLUS	C12013-31	BPD, Osaka 1988
LN	33084-5	BPD, Shinozuka 1996
99PMSBLUS	C12013-26	BPD, Tokyo 1989
99PMSBLUS	C12013-37	BPD by GA, Verburg 2008
LN	33088-6	Clavical length, Yarkoni 1985
99PMSBLUS	C12013-05	CRL, ASUM 2001
LN	33540-6	CRL, Hansmann 1986
LN	11910-7	CRL, Hadlock 1992
LN	11917-2	CRL, Jeanty 1984
99PMSBLUS	C12013-32	CRL, Osaka 1988
LN	33094-4	CRL, Rempen 1991
LN	11914-9	CRL, Robinson 1975
LN	33095-1	CRL, Shinozuka 1996
99PMSBLUS	C12013-27	CRL, Tokyo 1989
99PMSBLUS	C12013-36	CRL by GA, Verburg 2008
99PMSBLUS	C12013-06	FL, ASUM 2001
LN	33098-5	FL, Chitty 1997
LN	11920-6	FL, Hadlock 1984
LN	33541-4	FL, Hansmann 1986
LN	11923-0	FL, Jeanty 1984

<b>CSD</b>	<b>CV</b>	<b>Code Meaning</b>
99PMSBLUS	C12013-24	FL, Merz 1991
99PMSBLUS	C12013-33	FL, Osaka 1988
LN	33102-5	FL, Shinozuka 1996
99PMSBLUS	C12013-28	FL, Tokyo 1989
LN	33106-6	GS, Hansmann 1982
LN	11928-9	GS, Hellman 1969
LN	11929-7	GS, Rempen 1991
99PMSBLUS	C12013-29	GS, Tokyo 1989
LN	33107-4	GS, Nyberg 1992
99PMSBLUS	C12013-07	HC, ASUM 2001
LN	33110-8	HC measured, Chitty 1997
LN	33111-6	HC derived, Chitty 1997
LN	11932-1	HC, Hadlock 1984
LN	33543-0	HC, Hansmann 1986
99PMSBLUS	C12013-25	HC Merz, 1991
99PMSBLUS	C12013-09	Humerus, ASUM 2001
99PMSBLUS	C12013-34	Humerus Length, Osaka 1988
LN	11936-2	Humerus, Jeanty 1984
99PMSBLUS	C12013-11	OFD, ASUM 2001
LN	33120-7	OFD, Hansmann 1986
99PMSBLUS	C12013-12	OOD, Jeanty 1984
LN	33127-2	Spine Length, Tokyo, 1989
99PMSBLUS	C12013-41	TAD, Hansmann 1986
LN	11941-2	Tibia, Jeanty 1984
99PMSBLUS	C12013-15	TCD, Chitty 1997
LN	33134-8	TCD, Hill 1990
99PMSBLUS	C12013-35	Fetal Trunk Cross Sectional Area, Osaka 1988
LN	11944-6	Ulna, Jeanty 1984
99PMSBLUS	C12013-16	AC Merz 1991
99PMSBLUS	C12013-17	BPD Merz 1991
99PMSBLUS	C12013-18	Transverse Trunk Diameter Hansmann 1986
99PMSBLUS	C12013-19	CRL Robinson Fleming 1975

CSD	CV	Code Meaning
LN	33078-7	AxT, Shinozuka 1996
99PMSBLUS	C12013-22	CRL JSUM 2001
99PMSBLUS	C12013-23	TC Nimrod 1986

#### A.2.1.15.1 Gestational Age Equations and Tables Not Exported in DICOM SR

The following labels, equations or authors are not exported in Structured Reports for OB.

Label
GA (EFW) Shinozuka

#### A.2.1.16 OB Fetal Body Weight Equations & Tables

CSD	CV	Code Meaning
LN	11756-4	EFW by AC, Campbell 1975
LN	11738-2	EFW by AC, BPD, Hadlock 1984
LN	11735-8	EFW by AC, BPD, FL, Hadlock 1985
LN	11732-5	EFW by AC, BPD, FL, HC, Hadlock 1985
LN	11751-5	EFW by AC, FL, Hadlock 1985
LN	11746-5	EFW by AC, FL, HC, Hadlock 1985
LN	11739-0	EFW by AC and BPD, Shepard 1982
LN	33140-5	EFW by BPD, FTA, FL, Osaka 1990
99PMSBLUS	C12014-02	EFW by BPD, APAD, TAD, FL, Tokyo 1986
LN	33143-9	EFW3 by Shinozuka 1996
99PMSBLUS	C12014-01	EFW by AC, BPD and FL Shinozuka 2000

## A.3 VASCULAR ULTRASOUND STRUCTURED REPORT TEMPLATE

ClearVue 350/550/650/850 3.1 implements the Vascular Ultrasound Structured Report Template (TID 5100) from the DICOM standard, part 16. This appendix describes the scope and manner that ClearVue 350/550/650/850 3.1 measurements appear in DICOM SR.

Measurements and calculations performed for vascular studies will lead to creation of "Vascular Ultrasound Procedure Report" structured report documents. Measurements can be performed by pressing the 'Calc' key on ClearVue 350/550/650/850 3.1 control panel and selecting the vascular analysis package. Additional measurements may be made in the Abdominal analysis package. Measurements and calculations available in the menu can be configured through the setup application. It is also possible to configure the measurement unit (Metric or U.S.).

All concepts with value type (VT) NUM will always have a 'MeasurementUnitCodeSequence' that specifies the unit of the measurement. The CSD for all units will be UCUM (Unified Code for Units) and CV and CM will be based on application configuration and will conform to UCUM standards.

### A.3.1 Template specific conformance for TID 5100

The template for the root of the content tree for TID 5100 and its use in the ClearVue 350/550/650/850 3.1 context is described in the following table.

Note: Only the rows that apply to use by ClearVue 350/550/650/850 3.1 are included.

### A.3.2 TID 5100 Vascular Ultrasound Report

This is the template for the root the content tree for the vascular ultrasound procedure report.

No	NL	Rel with Parent	VT	Concept Name	Comments
1			CONTAINER	EV (125100, DCM, "Vascular Ultrasound Procedure Report")	This is the root 'CONTAINER'
2	>	CONTAINS	INCLUDE	DTID (5101) Vascular Patient Characteristics	See Section A.3.2 for the description of this.
3	>	CONTAINS	INCLUDE	DTID (5102) Vascular Procedure Summary Section	See Section A.3.3 for the description of this.
4	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-40501, SRT, "Blood Vessel of Head") \$SectionLaterality = EV (G-A101, SRT, "Left") \$Anatomy = DCID (12105) Intracranial Cerebral Vessels
5	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-40501, SRT, "Blood Vessel of Head") \$SectionLaterality = EV (G-A100, SRT, "Right") \$Anatomy = DCID (12105) Intracranial Cerebral Vessels
6	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-40501, SRT, "Blood Vessel of Head") \$SectionLaterality = EV (G-A103, SRT, "Unilateral") \$Anatomy = DCID (12106) Intracranial Cerebral Vessels (unilateral)
7	>	CONTAINS	INCLUDE	DTID (5103) Vascular	\$SectionScope = DT (T-45005, SRT, "Artery")

No	NL	Rel with Parent	VT	Concept Name	Comments
				Ultrasound Section	of neck") \$SectionLaterality = EV (G-A101, SRT, "Left") \$Anatomy = DCID (12104) Extracranial Arteries \$AnatomyRatio = DCID (12123) Carotid Ratios
8	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-45005, SRT, "Artery of neck") \$SectionLaterality = EV (G-A100, SRT, "Right") \$Anatomy = DCID (12104) Extracranial Arteries \$AnatomyRatio = DCID (12123) Carotid Ratios
9	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-47040, SRT, "Artery of Lower Extremity") \$SectionLaterality = EV (G-A101, SRT, "Left") \$Anatomy = DCID (12109) Lower Extremity Arteries
10	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-47040, SRT, "Artery of Lower Extremity") \$SectionLaterality = EV (G-A100, SRT, "Right") \$Anatomy = DCID (12109) Lower Extremity Arteries
11	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-49403, SRT, "Vein of Lower Extremity") \$SectionLaterality = EV (G-A101, SRT, "Left") \$Anatomy = DCID (12110) Lower Extremity Veins
12	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-49403, SRT, "Vein of Lower Extremity") \$SectionLaterality = EV (G-A100, SRT, "Right") \$Anatomy = DCID (12110) Lower Extremity Veins
13	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-47020, SRT, "Artery Of Upper Extremity") \$SectionLaterality = EV (G-A101, SRT, "Left") \$Anatomy = DCID (12107) Upper Extremity Arteries
14	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-47020, SRT, "Artery Of Upper Extremity") \$SectionLaterality = EV (G-A100, SRT, "Right") \$Anatomy = DCID (12107) Upper Extremity

No	NL	Rel with Parent	VT	Concept Name	Comments
					Arteries
15	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-49103, SRT, "Vein Of Upper Extremity") \$SectionLaterality = EV (G-A101, SRT, "Left") \$Anatomy = DCID (12108) Upper Extremity Veins
16	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-49103, SRT, "Vein Of Upper Extremity") \$SectionLaterality = EV (G-A100, SRT, "Right") \$Anatomy = DCID (12108) Upper Extremity Veins
17	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-71019, SRT, "Vascular Structure Of Kidney") \$SectionLaterality = EV (G-A101, SRT, "Left") \$Anatomy = DCID (12115) Renal Vessels \$AnatomyRatio = DCID (12124) Renal Ratios
18	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-71019, SRT, "Vascular Structure Of Kidney") \$SectionLaterality = EV (G-A100, SRT, "Right") \$Anatomy = DCID (12115) Renal Vessels \$AnatomyRatio = DCID (12124) Renal Ratios
19	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-46002, SRT, "Artery of Abdomen") \$SectionLaterality = EV (G-A101, SRT, "Left") \$Anatomy = DCID (12111) Abdominal Arteries (lateral)
20	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-46002, SRT, "Artery of Abdomen") \$SectionLaterality = EV (G-A100, SRT, "Right") \$Anatomy = DCID (12111) Abdominal Arteries (lateral)
21	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-46002, SRT, "Artery of Abdomen") \$SectionLaterality = EV (G-A103, SRT, "Unilateral") \$Anatomy = DCID (12112) Abdominal Arteries (unilateral)
22	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-487A0, SRT, "Vein of Abdomen") \$SectionLaterality = EV (G-A101, SRT, "Left") \$Anatomy = DCID (12113) Abdominal Veins

No	NL	Rel with Parent	VT	Concept Name	Comments
					(lateral)
23	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-487A0, SRT, "Vein of Abdomen") \$SectionLaterality = EV (G-A100, SRT, "Right") \$Anatomy = DCID (12113) Abdominal Veins (lateral)
24	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section	\$SectionScope = DT (T-487A0, SRT, " Vein of Abdomen") \$SectionLaterality = EV (G-A103, SRT, "Unilateral") \$Anatomy = DCID (12114) Abdominal Veins (unilateral)

### A.3.3 Vascular Patient Characteristics (TID 5101)

Use of the template TID 5101 in the context of ClearVue 350/550/650/850 3.1 is described in the following table.

No	NL	Rel with Parent	VT	Concept Name	Comments
1			CONTAINER	EV (121118, DCM, "Patient Characteristics")	
2	>	CONTAINS	NUM	EV (121033, DCM, "Subject Age")	Units = DCID (7456) Units of Measure for Age
3	>	CONTAINS	CODE	EV (121032, DCM, "Subject Sex")	DCID (7455) Sex
4	>	CONTAINS	NUM	(8277-6, LN, "Body Surface Area")	Derived from Patient Height and Weight
5	>	CONTAINS	NUM	(8302-2, LN, "Patient Height")	From Patient Data Entry
6	>	CONTAINS	NUM	(29463-7, LN, "Patient Weight")	From Patient Data Entry
7	>	CONTAINS	TEXT	(121029, DCM, "Subject Name")	From Patient Data Entry
8	>	CONTAINS	TEXT	(121030, DCM, "Subject ID")	From Patient Data Entry
9	>	CONTAINS	TEXT	(121031, DCM, "Subject Birth Date")	From Patient Data Entry
10	>	CONTAINS	TEXT	(T9910-04, 99PMSBLUS, "Reason for Study")	From Patient Data Entry
11	>	CONTAINS	TEXT	(T9910-112, 99PMSBLUS, "Alternate ID Number")	From Patient Data Entry
12	>	CONTAINS	TEXT	(T9910-111, 99PMSBLUS, "Accession Number")	From Patient Data Entry
13	>	CONTAINS	TEXT	(T9910-08, 99PMSBLUS, "Referring Physician")	From Patient Data Entry

No	NL	Rel with Parent	VT	Concept Name	Comments
14	>	CONTAINS	TEXT	(T9910-06, 99PMSBLUS, "Sonographer")	From Patient Data Entry
15	>	CONTAINS	TEXT	(T9910-07, 99PMSBLUS, "Study Description")	From Patient Data Entry
16	>	CONTAINS	TEXT	(T9910-10, 99PMSBLUS, "Patient History")	From Patient Data Entry
17	>	CONTAINS	TEXT	(T9910-09, 99PMSBLUS, "Exam Date")	From Patient Data Entry
18	>	CONTAINS	TEXT	(121106, DCM, "Comment")	From Patient Data Entry

#### A.3.4 Vascular Procedure Summary (TID 5102)

Use of the template TID 5002 in the context of ClearVue 350/550/650/850 3.1 is described in the following table.

No	NL	Rel with Parent	VT	Concept Name	Comments
1			CONTAINER	DT (121111, DCM, "Summary")	
2	>		TEXT	DCID (12101) Vascular Summary	

#### A.3.5 eDCS – Vascular Template Support

The following list represents the Electronic DICOM Conformance Statement (eDCS) format for the Structured Report output for the Vascular Ultrasound Procedure Report as supported on ClearVue 350/550/650/850 3.1.

This list is made up of ‘signatures’ that describe the group of codes used for each exported measurement and calculation result.

A ‘signature’ will contain the Label as displayed on the system user interface in the Calcs application and report pages, followed by the modifiers required by the DICOM SR Template and Structured Reporting SOP Class in order to include a given measurement or calculation value.

Some signatures will contain as few as two or as many as six modifiers.

In the table below, the following terms are used:

CSD	Coding Scheme Designator
CV	Code Value
CM	Code Meaning
Mod Type	Concept Modifier Type
Laterality	Describes laterality of vessel

#### “Mod Type” Field

Anatomy	The finding site as specified by the template
Concept	The code sequence as defined by the CSD
Section	The section as specified by the template
Segment	The name of the vessel segment

Units	Units of this measurement
Meas Type	Used only to indicate QLAB measurements

#### A.3.5.1 eDCS Table

ClearVue 350/550/650/850 3.1 Report Label	MOD Type	CSD	CV	CM	Laterality
ACA EDV	anatomy	SRT	T-45540	Anterior Cerebral Artery	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
ACA PI	anatomy	SRT	T-45540	Anterior Cerebral Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
ACA PSV	anatomy	SRT	T-45540	Anterior Cerebral Artery	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
ACA TAPV	anatomy	SRT	T-45540	Anterior Cerebral Artery	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
ACA TCD Mean	anatomy	SRT	T-45540	Anterior Cerebral Artery	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
ACA TCD PI	anatomy	SRT	T-45540	Anterior Cerebral Artery	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
ACoA EDV	anatomy	SRT	T-45530	Anterior Communicating Artery	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
ACoA PI	anatomy	SRT	T-45530	Anterior Communicating Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
ACoA PSV	anatomy	SRT	T-45530	Anterior Communicating Artery	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
ACoA TAPV	anatomy	SRT	T-45530	Anterior Communicating Artery	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
ACoA TCD Mean	anatomy	SRT	T-45530	Anterior Communicating Artery	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
ACoA TCD PI	anatomy	SRT	T-45530	Anterior Communicating Artery	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
AI	anatomy	99PMSBLUS	sup71_001	Antecube	bilateral
		SRT	T-45100	Common Carotid Artery	bilateral
			T-45170	Carotid Bulb	bilateral
			T-45200	External Carotid Artery	bilateral
			T-45300	Internal Carotid Artery	bilateral
			T-45700	Vertebral Artery	bilateral
			T-46010	Innominate Artery	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
			T-46100	Subclavian Artery	bilateral
			T-46710	Common Iliac Artery	bilateral
			T-46740	Internal Iliac Artery	bilateral
			T-46910	External Iliac Artery	bilateral
			T-47100	Axillary Artery	bilateral
			T-47160	Brachial Artery	bilateral
			T-47200	Ulnar Artery	bilateral
			T-47300	Radial Artery	bilateral
			T-47400	Common Femoral Artery	bilateral
			T-47403	Superficial Femoral Artery	bilateral
			T-47440	Profunda Femoris Artery	bilateral
			T-47500	Popliteal Artery	bilateral
			T-47600	Posterior Tibial Artery	bilateral
			T-47630	Peroneal Artery	bilateral
			T-47700	Anterior Tibial Artery	bilateral
			T-47741	Dorsalis Pedis Artery	bilateral
	concept	LN	20167-3	Acceleration Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
			T-47020	Artery Of Upper Extremity	bilateral
			T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
			G-A119	Distal	bilateral
			G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	bilateral
<b>Antecube PI</b>	anatomy	99PMSBLUS	sup71_001	Antecube	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Antecube RI</b>	anatomy	99PMSBLUS	sup71_001	Antecube	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Antecube S/D</b>	anatomy	99PMSBLUS	sup71_001	Antecube	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Ao % Area Reduction</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	SRT	G-0371	Percent Area Reduction	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	%	Percent	unilateral
<b>Ao % Diam Reduction</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	SRT	G-0372	Percent Diameter Reduction	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	%	Percent	unilateral
<b>Ao Area Resid</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	99PMSBLUS	C7471-01	Area 1 of Area Percent Reduction	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm <sup>2</sup>	Square Centimeter	unilateral
<b>Ao Area True</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	99PMSBLUS	C7471-02	Area 2 of Area Percent Reduction	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm <sup>2</sup>	Square Centimeter	unilateral
<b>Ao Diam Resid</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	99PMSBLUS	C7470-05	Diameter 1 of Diameter Reduction	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Ao Diam True</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	99PMSBLUS	C7470-06	Diameter 2 of Diameter Reduction	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Ao Dist Diam</b>	anatomy	SRT	T-42000	Aorta	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	SRT	G-0364	Vessel lumen diameter	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Ao Mid Diam</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	SRT	G-0364	Vessel lumen diameter	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Ao Prox Diam</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	SRT	G-0364	Vessel lumen diameter	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Aorta PSV</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>AT</b>	anatomy	99PMSBLUS	sup71_001	Antecube	bilateral
		SRT	T-45100	Common Carotid Artery	bilateral
			T-45170	Carotid Bulb	bilateral
			T-45200	External Carotid Artery	bilateral
			T-45300	Internal Carotid Artery	bilateral
			T-45700	Vertebral Artery	bilateral
			T-46010	Innominate Artery	bilateral
			T-46100	Subclavian Artery	bilateral
			T-46710	Common Iliac Artery	bilateral
			T-46740	Internal Iliac Artery	bilateral
			T-46910	External Iliac Artery	bilateral
			T-47100	Axillary Artery	bilateral
			T-47160	Brachial Artery	bilateral
			T-47200	Ulnar Artery	bilateral
			T-47300	Radial Artery	bilateral
			T-47400	Common Femoral Artery	bilateral
			T-47403	Superficial Femoral Artery	bilateral
			T-47440	Profunda Femoris Artery	bilateral
			T-47500	Popliteal Artery	bilateral
			T-47600	Posterior Tibial Artery	bilateral
			T-47630	Peroneal Artery	bilateral
			T-47700	Anterior Tibial Artery	bilateral
			T-47741	Dorsalis Pedis Artery	bilateral
	concept	LN	20168-1	Acceleration Time	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
			T-47020	Artery Of Upper Extremity	bilateral
			T-47040	Artery of Lower Extremity	bilateral
<b>Ax A PI</b>	segment	SRT	G-A118	Proximal	bilateral
			G-A119	Distal	bilateral
			G-A188	Mid-longitudinal	bilateral
	units	UCUM	sec	Seconds	bilateral
<b>Ax A RI</b>	anatomy	SRT	T-47100	Axillary Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Ax A S/D</b>	anatomy	SRT	T-47100	Axillary Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	units	UCUM	1	ratio	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
<b>Bifur ACA EDV</b>	anatomy	SRT	G-0369	Anterior-Posterior Cerebral Artery Bifurcation	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Bifur ACA PI</b>	anatomy	SRT	G-0369	Anterior-Posterior Cerebral Artery Bifurcation	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>Bifur ACA PSV</b>	anatomy	SRT	G-0369	Anterior-Posterior Cerebral Artery Bifurcation	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Bifur ACA TAPV</b>	anatomy	SRT	G-0369	Anterior-Posterior Cerebral Artery Bifurcation	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Bifur ACA TCD Mean</b>	anatomy	SRT	G-0369	Anterior-Posterior Cerebral Artery Bifurcation	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Bifur ACA TCD PI</b>	anatomy	SRT	G-0369	Anterior-Posterior Cerebral Artery Bifurcation	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>Bifur MCA EDV</b>	anatomy	SRT	G-0368	Anterior-Middle Cerebral Artery Bifurcation	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Bifur MCA PI</b>	anatomy	SRT	G-0368	Anterior-Middle Cerebral Artery Bifurcation	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>Bifur MCA PSV</b>	anatomy	SRT	G-0368	Anterior-Middle Cerebral Artery Bifurcation	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Bifur MCA TAPV</b>	anatomy	SRT	G-0368	Anterior-Middle Cerebral Artery Bifurcation	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Bifur MCA TCD Mean</b>	anatomy	SRT	G-0368	Anterior-Middle Cerebral Artery Bifurcation	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Bifur MCA TCD PI</b>	anatomy	SRT	G-0368	Anterior-Middle Cerebral Artery Bifurcation	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>Bladder Height</b>	anatomy	SNM3	T-74000	Bladder	unilateral
	concept	99PMSBLUS	C12011-03	Bladder Height	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Bladder Length</b>	anatomy	SNM3	T-74000	Bladder	unilateral
	concept	99PMSBLUS	C12011-01	Bladder Length	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	cm	Centimeter	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
<b>Bladder Vol</b>	anatomy	SNM3	T-74000	Bladder	unilateral
	concept	99PMSBLUS	C12011-04	Bladder Volume	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	cm3	Cubic Centimeter	unilateral
<b>Bladder Width</b>	anatomy	SNM3	T-74000	Bladder	unilateral
	concept	99PMSBLUS	C12011-02	Bladder Width	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Brachioceph A PI</b>	anatomy	SRT	T-46010	Innominata Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Brachioceph A RI</b>	anatomy	SRT	T-46010	Innominata Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Brachioceph A S/D</b>	anatomy	SRT	T-46010	Innominata Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Bulb IMT(Q)</b>	anatomy	SRT	T-45170	Carotid Bulb	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	MeasType	99PMSBLUS	C3627-01	QLAB IMT measurement	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Bulb PI</b>	anatomy	SRT	T-45170	Carotid Bulb	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	1	ratio	bilateral
<b>Bulb RI</b>	anatomy	SRT	T-45170	Carotid Bulb	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	1	ratio	bilateral
<b>Bulb S/D</b>	anatomy	SRT	T-45170	Carotid Bulb	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	1	ratio	bilateral
<b>Carotid Siphon EDV</b>	anatomy	SRT	T-45308	Carotid Siphon	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Carotid Siphon PI</b>	anatomy	SRT	T-45308	Carotid Siphon	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>Carotid Siphon PSV</b>	anatomy	SRT	T-45308	Carotid Siphon	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Carotid Siphon TAPV</b>	anatomy	SRT	T-45308	Carotid Siphon	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Carotid Siphon TCD Mean</b>	anatomy	SRT	T-45308	Carotid Siphon	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Carotid Siphon TCD PI</b>	anatomy	SRT	T-45308	Carotid Siphon	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral

ClearVue 350/550/650/850 3.1 Report Label	MOD Type	CSD	CV	CM	Laterality
<b>CBD Diam</b>	anatomy	SNM3	T-60610	Bileduct	unilateral
	concept	DCM	121206	Distance	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	mm	Millimeter	unilateral
<b>CCA % Area Reduction</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	SRT	G-0371	Percent Area Reduction	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	%	Percent	bilateral
<b>CCA % Diam Reduction</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	SRT	G-0372	Percent Diameter Reduction	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	%	Percent	bilateral
<b>CCA Area Resid</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	99PMSBLUS	C7471-01	Area 1 of Area Percent Reduction	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	cm2	Square Centimeter	bilateral
<b>CCA Area True</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	99PMSBLUS	C7471-02	Area 2 of Area Percent Reduction	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	cm2	Square Centimeter	bilateral
<b>CCA Diam Resid</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	99PMSBLUS	C7470-05	Diameter 1 of Diameter Reduction	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>CCA Diam True</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	99PMSBLUS	C7470-06	Diameter 2 of Diameter Reduction	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>CCA PSV</b>	anatomy	99PMSBLUS	C12104-02	ICA/CCA Ratio Denominator	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Celiac A AI</b>	anatomy	SRT	T-46400	Celiac Axis	unilateral
	concept	LN	20167-3	Acceleration Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	unilateral
<b>Celiac A AT</b>	anatomy	SRT	T-46400	Celiac Axis	unilateral
	concept	LN	20168-1	Acceleration Time	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	sec	Seconds	unilateral
<b>Celiac A EDV</b>	anatomy	SRT	T-46400	Celiac Axis	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Celiac A MDV</b>	anatomy	SRT	T-46400	Celiac Axis	unilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Celiac A PI</b>	anatomy	SRT	T-46400	Celiac Axis	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Celiac A PSV</b>	anatomy	SRT	T-46400	Celiac Axis	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Celiac A RI</b>	anatomy	SRT	T-46400	Celiac Axis	unilateral
	concept	LN	12023-8	Resistivity Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Celiac A S/D</b>	anatomy	SRT	T-46400	Celiac Axis	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Celiac A TAMV<sup>1</sup></b>	anatomy	SRT	T-46400	Celiac Axis	unilateral
	concept	LN	20352-1	Time averaged mean velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Celiac A TAPV</b>	anatomy	SRT	T-46400	Celiac Axis	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Celiac A VTI</b>	anatomy	SRT	T-46400	Celiac Axis	unilateral
	concept	LN	20354-7	Velocity Time Integral	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>CFA % Area Reduction</b>	anatomy	SRT	T-47400	Common Femoral Artery	bilateral
	concept	SRT	G-0371	Percent Area Reduction	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	%	Percent	bilateral
<b>CFA % Diam Reduction</b>	anatomy	SRT	T-47400	Common Femoral Artery	bilateral
	concept	SRT	G-0372	Percent Diameter Reduction	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	%	Percent	bilateral
<b>CFA Area Resid</b>	anatomy	SRT	T-47400	Common Femoral Artery	bilateral
	concept	99PMSBLUS	C7471-01	Area 1 of Area Percent Reduction	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	cm <sup>2</sup>	Square Centimeter	bilateral
<b>CFA Area True</b>	anatomy	SRT	T-47400	Common Femoral Artery	bilateral
	concept	99PMSBLUS	C7471-02	Area 2 of Area Percent Reduction	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	cm <sup>2</sup>	Square Centimeter	bilateral
<b>CFA Diam Resid</b>	anatomy	SRT	T-47400	Common Femoral Artery	bilateral
	concept	99PMSBLUS	C7470-05	Diameter 1 of Diameter Reduction	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>CFA Diam True</b>	anatomy	SRT	T-47400	Common Femoral Artery	bilateral
	concept	99PMSBLUS	C7470-06	Diameter 2 of Diameter Reduction	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>CFA PI</b>	anatomy	SRT	T-47400	Common Femoral Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>CFA RI</b>	anatomy	SRT	T-47400	Common Femoral Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>CFA S/D</b>	anatomy	SRT	T-47400	Common Femoral Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Com Hepatic A AI</b>	anatomy	SRT	T-46421	Common Hepatic Artery	unilateral
	concept	LN	20167-3	Acceleration Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	unilateral
<b>Com Hepatic A AT</b>	anatomy	SRT	T-46421	Common Hepatic Artery	unilateral
	concept	LN	20168-1	Acceleration Time	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	sec	Seconds	unilateral
<b>Com Hepatic A EDV</b>	anatomy	SRT	T-46421	Common Hepatic Artery	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Com Hepatic A MDV</b>	anatomy	SRT	T-46421	Common Hepatic Artery	unilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Com Hepatic A PI</b>	anatomy	SRT	T-46421	Common Hepatic Artery	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Com Hepatic A PSV</b>	anatomy	SRT	T-46421	Common Hepatic Artery	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Com Hepatic A RI</b>	anatomy	SRT	T-46421	Common Hepatic Artery	unilateral
	concept	LN	12023-8	Resistivity Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Com Hepatic A S/D</b>	anatomy	SRT	T-46421	Common Hepatic Artery	unilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Com Hepatic A TAMV</b>	anatomy	SRT	T-46421	Common Hepatic Artery	unilateral
	concept	LN	20352-1	Time averaged mean velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Com Hepatic A TAPV</b>	anatomy	SRT	T-46421	Common Hepatic Artery	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Com Hepatic A VTI</b>	anatomy	SRT	T-46421	Common Hepatic Artery	unilateral
	concept	LN	20354-7	Velocity Time Integral	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Com Iliac A PI</b>	anatomy	SRT	T-46710	Common Iliac Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Com Iliac A RI</b>	anatomy	SRT	T-46710	Common Iliac Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Com Iliac A S/D</b>	anatomy	SRT	T-46710	Common Iliac Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Ao AI</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	LN	20167-3	Acceleration Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	unilateral
<b>Dist Ao AT</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	LN	20168-1	Acceleration Time	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	sec	Seconds	unilateral
<b>Dist Ao EDV</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
<b>Dist Ao MDV</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Dist Ao PI</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Dist Ao PSV</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Dist Ao RI</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	LN	12023-8	Resistivity Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Dist Ao S/D</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Dist Ao TAMV</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	LN	20352-1	Time averaged mean velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Dist Ao TAPV</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Dist Ao VTI</b>	anatomy	SRT	T-42000	Aorta	unilateral
	concept	LN	20354-7	Velocity Time Integral	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Dist ATA PI</b>	anatomy	SRT	T-47700	Anterior Tibial Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist ATA RI</b>	anatomy	SRT	T-47700	Anterior Tibial Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist ATA S/D</b>	anatomy	SRT	T-47700	Anterior Tibial Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Basilar A EDV</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Dist Basilar A PI</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Dist Basilar A PSV</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Dist Basilar A TAPV</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Dist Basilar A TCD Mean</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Dist Basilar A TCD PI</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Dist Brach A PI</b>	anatomy	SRT	T-47160	Brachial Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Brach A RI</b>	anatomy	SRT	T-47160	Brachial Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Brach A S/D</b>	anatomy	SRT	T-47160	Brachial Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Bulb IMT</b>	anatomy	SRT	T-45170	Carotid Bulb	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Dist CCA IMT</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Dist CCA IMT(Q)</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	MeasType	99PMSBLUS	C3627-01	QLAB IMT measurement	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Dist CCA PI</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist CCA RI</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist CCA S/D</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist ICA EDV</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Dist ICA IMT</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Dist ICA IMT(Q)</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	MeasType	99PMSBLUS	C3627-01	QLAB IMT measurement	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Dist ICA PI</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist ICA PSV</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Dist ICA RI</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist ICA S/D</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist ICA TAPV</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Dist ICA TCD Mean</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Dist ICA TCD PI</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
<b>Dist M1 EDV</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Dist M1 PI</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist M1 PSV</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Dist M1 TAPV</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Dist M1 TCD Mean</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Dist M1 TCD PI</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Pero A PI</b>	anatomy	SRT	T-47630	Peroneal Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Pero A RI</b>	anatomy	SRT	T-47630	Peroneal Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Pero A S/D</b>	anatomy	SRT	T-47630	Peroneal Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Pop A PI</b>	anatomy	SRT	T-47500	Popliteal Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Pop A RI</b>	anatomy	SRT	T-47500	Popliteal Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Pop A S/D</b>	anatomy	SRT	T-47500	Popliteal Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist PTA PI</b>	anatomy	SRT	T-47600	Posterior Tibial Artery	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist PTA RI</b>	anatomy	SRT	T-47600	Posterior Tibial Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist PTA S/D</b>	anatomy	SRT	T-47600	Posterior Tibial Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Rad A PI</b>	anatomy	SRT	T-47300	Radial Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Rad A RI</b>	anatomy	SRT	T-47300	Radial Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Rad A S/D</b>	anatomy	SRT	T-47300	Radial Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Ren A AI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20167-3	Acceleration Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	bilateral
<b>Dist Ren A AT</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20168-1	Acceleration Time	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	sec	Seconds	bilateral
<b>Dist Ren A EDV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Dist Ren A MDV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Dist Ren A PI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Ren A PSV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Dist Ren A RI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Ren A S/D</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Ren A TAMV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20352-1	Time averaged mean velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Dist Ren A TAPV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Dist Ren A VTI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20354-7	Velocity Time Integral	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Dist SFA PI</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist SFA RI</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist SFA S/D</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist SMA AI</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	20167-3	Acceleration Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	unilateral
<b>Dist SMA AT</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	20168-1	Acceleration Time	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	sec	Seconds	unilateral
<b>Dist SMA EDV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Dist SMA MDV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Dist SMA PI</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Dist SMA PSV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Dist SMA RI</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	12023-8	Resistivity Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Dist SMA S/D</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Dist SMA TAMV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	20352-1	Time averaged mean velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Dist SMA TAPV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Dist SMA VTI</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	20354-7	Velocity Time Integral	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A119	Distal	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Dist Ulnar A PI</b>	anatomy	SRT	T-47200	Ulnar Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Ulnar A RI</b>	anatomy	SRT	T-47200	Ulnar Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dist Ulnar A S/D</b>	anatomy	SRT	T-47200	Ulnar Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A119	Distal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dor Pedis PI</b>	anatomy	SRT	T-47741	Dorsalis Pedis Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dor Pedis RI</b>	anatomy	SRT	T-47741	Dorsalis Pedis Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Dor Pedis S/D</b>	anatomy	SRT	T-47741	Dorsalis Pedis Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>EDV</b>	anatomy	99PMSBLUS	sup71_001	Antecube	bilateral
		SRT	T-45100	Common Carotid Artery	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
			T-45170	Carotid Bulb	bilateral
			T-45200	External Carotid Artery	bilateral
			T-45300	Internal Carotid Artery	bilateral
			T-45700	Vertebral Artery	bilateral
			T-46010	Innominate Artery	bilateral
			T-46100	Subclavian Artery	bilateral
			T-46710	Common Iliac Artery	bilateral
			T-46740	Internal Iliac Artery	bilateral
			T-46910	External Iliac Artery	bilateral
			T-47100	Axillary Artery	bilateral
			T-47160	Brachial Artery	bilateral
			T-47200	Ulnar Artery	bilateral
			T-47300	Radial Artery	bilateral
			T-47400	Common Femoral Artery	bilateral
			T-47403	Superficial Femoral Artery	bilateral
			T-47440	Profunda Femoris Artery	bilateral
			T-47500	Popliteal Artery	bilateral
			T-47600	Posterior Tibial Artery	bilateral
			T-47630	Peroneal Artery	bilateral
			T-47700	Anterior Tibial Artery	bilateral
			T-47741	Dorsalis Pedis Artery	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
			T-47020	Artery Of Upper Extremity	bilateral
			T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
			G-A119	Distal	bilateral
			G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ext Iliac A PI</b>	anatomy	SRT	T-46910	External Iliac Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Ext Iliac A RI</b>	anatomy	SRT	T-46910	External Iliac Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Ext Iliac A S/D</b>	anatomy	SRT	T-46910	External Iliac Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>GB Wall Diam</b>	anatomy	SNM3	T-63000	Gallbladder	unilateral
	concept	DCM	121206	Distance	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	mm	Millimeter	unilateral
<b>GDA AI</b>	anatomy	SRT	T-46440	Gastrooduodenal Artery	unilateral
	concept	LN	20167-3	Acceleration Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	unilateral
<b>GDA AT</b>	anatomy	SRT	T-46440	Gastrooduodenal Artery	unilateral
	concept	LN	20168-1	Acceleration Time	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	sec	Seconds	unilateral
<b>GDA EDV</b>	anatomy	SRT	T-46440	Gastrooduodenal Artery	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>GDA MDV</b>	anatomy	SRT	T-46440	Gastrooduodenal Artery	unilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
<b>GDA PI</b>	anatomy	SRT	T-46440	Gastroduodenal Artery	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>GDA PSV</b>	anatomy	SRT	T-46440	Gastroduodenal Artery	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>GDA RI</b>	anatomy	SRT	T-46440	Gastroduodenal Artery	unilateral
	concept	LN	12023-8	Resistivity Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>GDA S/D</b>	anatomy	SRT	T-46440	Gastroduodenal Artery	unilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>GDA TAMV</b>	anatomy	SRT	T-46440	Gastroduodenal Artery	unilateral
	concept	LN	20352-1	Time averaged mean velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>GDA TAPV</b>	anatomy	SRT	T-46440	Gastroduodenal Artery	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>GDA VTI</b>	anatomy	SRT	T-46440	Gastroduodenal Artery	unilateral
	concept	LN	20354-7	Velocity Time Integral	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Hilar A AI</b>	anatomy	SRT	G-035C	Hilar Artery	bilateral
	concept	LN	20167-3	Acceleration Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	bilateral
<b>Hilar A AT</b>	anatomy	SRT	G-035C	Hilar Artery	bilateral
	concept	LN	20168-1	Acceleration Time	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	sec	Seconds	bilateral
<b>Hilar A EDV</b>	anatomy	SRT	G-035C	Hilar Artery	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Hilar A MDV</b>	anatomy	SRT	G-035C	Hilar Artery	bilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Hilar A PI</b>	anatomy	SRT	G-035C	Hilar Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Hilar A PSV</b>	anatomy	SRT	G-035C	Hilar Artery	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Hilar A RI</b>	anatomy	SRT	G-035C	Hilar Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Hilar A S/D</b>	anatomy	SRT	G-035C	Hilar Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Hilar A TAMV'</b>	anatomy	SRT	G-035C	Hilar Artery	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	LN	20352-1	Time averaged mean velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Hilar A TAPV</b>	anatomy	SRT	G-035C	Hilar Artery	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Hilar A VTI</b>	anatomy	SRT	G-035C	Hilar Artery	bilateral
	concept	LN	20354-7	Velocity Time Integral	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>ICA</b>	anatomy	99PMSBLUS	C12105-02	MCA/Dist ICA Ratio Denominator	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>ICA % Area Reduction</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	SRT	G-0371	Percent Area Reduction	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	%	Percent	bilateral
<b>ICA % Diam Reduction</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	SRT	G-0372	Percent Diameter Reduction	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	%	Percent	bilateral
<b>ICA Area Resid</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	99PMSBLUS	C7471-01	Area 1 of Area Percent Reduction	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	cm <sup>2</sup>	Square Centimeter	bilateral
<b>ICA Area True</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	99PMSBLUS	C7471-02	Area 2 of Area Percent Reduction	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	cm <sup>2</sup>	Square Centimeter	bilateral
<b>ICA Diam Resid</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	99PMSBLUS	C7470-05	Diameter 1 of Diameter Reduction	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>ICA Diam True</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	99PMSBLUS	C7470-06	Diameter 2 of Diameter Reduction	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>ICA PSV</b>	anatomy	99PMSBLUS	C12104-01	ICA/CCA Ratio Numerator	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>ICA/CCA</b>	concept	LN	33868-1	ICA/CCA velocity ratio	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	1	ratio	bilateral
<b>IMA AI</b>	anatomy	SRT	T-46520	Inferior Mesenteric Artery	unilateral
	concept	LN	20167-3	Acceleration Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	unilateral
<b>IMA AT</b>	anatomy	SRT	T-46520	Inferior Mesenteric Artery	unilateral
	concept	LN	20168-1	Acceleration Time	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	sec	Seconds	unilateral
<b>IMA EDV</b>	anatomy	SRT	T-46520	Inferior Mesenteric Artery	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>IMA MDV</b>	anatomy	SRT	T-46520	Inferior Mesenteric Artery	unilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>IMA PI</b>	anatomy	SRT	T-46520	Inferior Mesenteric Artery	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>IMA PSV</b>	anatomy	SRT	T-46520	Inferior Mesenteric Artery	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>IMA RI</b>	anatomy	SRT	T-46520	Inferior Mesenteric Artery	unilateral
	concept	LN	12023-8	Resistivity Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>IMA S/D</b>	anatomy	SRT	T-46520	Inferior Mesenteric Artery	unilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>IMA TAMV</b>	anatomy	SRT	T-46520	Inferior Mesenteric Artery	unilateral
	concept	LN	20352-1	Time averaged mean velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>IMA TAPV</b>	anatomy	SRT	T-46520	Inferior Mesenteric Artery	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>IMA VTI</b>	anatomy	SRT	T-46520	Inferior Mesenteric Artery	unilateral
	concept	LN	20354-7	Velocity Time Integral	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Inf Arc AI</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	20167-3	Acceleration Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	bilateral
<b>Inf Arc AT</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	20168-1	Acceleration Time	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	sec	Seconds	bilateral
<b>Inf Arc EDV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Inf Arc MDV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Inf Arc PI</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Inf Arc PSV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Inf Arc RI</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A115	Inferior	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Inf Arc S/D</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Inf Arc TAMV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	20352-1	Time averaged mean velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Inf Arc TAPV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Inf Arc VTI</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	20354-7	Velocity Time Integral	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Inf Ren Ao AI</b>	anatomy	SRT	T-42520	Infra-renal Aorta	unilateral
	concept	LN	20167-3	Acceleration Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	unilateral
<b>Inf Ren Ao AT</b>	anatomy	SRT	T-42520	Infra-renal Aorta	unilateral
	concept	LN	20168-1	Acceleration Time	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	sec	Seconds	unilateral
<b>Inf Ren Ao EDV</b>	anatomy	SRT	T-42520	Infra-renal Aorta	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Inf Ren Ao MDV</b>	anatomy	SRT	T-42520	Infra-renal Aorta	unilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Inf Ren Ao PI</b>	anatomy	SRT	T-42520	Infra-renal Aorta	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Inf Ren Ao PSV</b>	anatomy	SRT	T-42520	Infra-renal Aorta	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Inf Ren Ao RI</b>	anatomy	SRT	T-42520	Infra-renal Aorta	unilateral
	concept	LN	12023-8	Resistivity Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Inf Ren Ao S/D</b>	anatomy	SRT	T-42520	Infra-renal Aorta	unilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Inf Ren Ao TAMV</b>	anatomy	SRT	T-42520	Infra-renal Aorta	unilateral
	concept	LN	20352-1	Time averaged mean velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Inf Ren Ao TAPV</b>	anatomy	SRT	T-42520	Infra-renal Aorta	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Inf Ren Ao VTI</b>	anatomy	SRT	T-42520	Infra-renal Aorta	unilateral
	concept	LN	20354-7	Velocity Time Integral	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Inf Seg AI</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	20167-3	Acceleration Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	bilateral
<b>Inf Seg AT</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	20168-1	Acceleration Time	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	sec	Seconds	bilateral
<b>Inf Seg EDV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Inf Seg MDV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Inf Seg PI</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Inf Seg PSV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Inf Seg RI</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Inf Seg S/D</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Inf Seg TAMV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	20352-1	Time averaged mean velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Inf Seg TAPV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Inf Seg VTI</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A115	Inferior	bilateral
	concept	LN	20354-7	Velocity Time Integral	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm	Centimeter	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
<b>Int Iliac A PI</b>	anatomy	SRT	T-46740	Internal Iliac Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Int Iliac A RI</b>	anatomy	SRT	T-46740	Internal Iliac Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>Int Iliac A S/D</b>	anatomy	SRT	T-46740	Internal Iliac Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	1	ratio	bilateral
<b>IVC Diameter</b>	anatomy	SRT	T-48710	Inferior Vena Cava	unilateral
	concept	LN	18006-7	Inferior Vena Cava Diameter	unilateral
	section	SRT	T-487A0	Vein of Abdomen	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Kidney Height</b>	anatomy	SNM3	T-71000	Kidney	bilateral
	concept	99PMSBLUS	C7470-01	Height	bilateral
	section	99PMSBLUS	T5100-01	Anatomic Structures	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Kidney Length</b>	anatomy	SNM3	T-71000	Kidney	bilateral
	concept	SRT	G-A22A	Length	bilateral
	section	99PMSBLUS	T5100-01	Anatomic Structures	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Kidney Vol</b>	anatomy	SNM3	T-71000	Kidney	bilateral
	concept	DCM	121221	Volume of ellipsoid	bilateral
	section	99PMSBLUS	T5100-01	Anatomic Structures	bilateral
	units	UCUM	cm3	Cubic Centimeter	bilateral
<b>Kidney Width</b>	anatomy	SNM3	T-71000	Kidney	bilateral
	concept	SNM3	G-A220	Width	bilateral
	section	99PMSBLUS	T5100-01	Anatomic Structures	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>L Hepatic A AI</b>	anatomy	SRT	T-46427	Left Branch of Hepatic Artery	unilateral
	concept	LN	20167-3	Acceleration Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	unilateral
<b>L Hepatic A AT</b>	anatomy	SRT	T-46427	Left Branch of Hepatic Artery	unilateral
	concept	LN	20168-1	Acceleration Time	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	sec	Seconds	unilateral
<b>L Hepatic A EDV</b>	anatomy	SRT	T-46427	Left Branch of Hepatic Artery	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>L Hepatic A MDV</b>	anatomy	SRT	T-46427	Left Branch of Hepatic Artery	unilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>L Hepatic A PI</b>	anatomy	SRT	T-46427	Left Branch of Hepatic Artery	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>L Hepatic A PSV</b>	anatomy	SRT	T-46427	Left Branch of Hepatic Artery	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>L Hepatic A RI</b>	anatomy	SRT	T-46427	Left Branch of Hepatic Artery	unilateral
	concept	LN	12023-8	Resistivity Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>L Hepatic A S/D</b>	anatomy	SRT	T-46427	Left Branch of Hepatic Artery	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>L Hepatic A TAMV</b>	anatomy	SRT	T-46427	Left Branch of Hepatic Artery	unilateral
	concept	LN	20352-1	Time averaged mean velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>L Hepatic A TAPV</b>	anatomy	SRT	T-46427	Left Branch of Hepatic Artery	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>L Hepatic A VTI</b>	anatomy	SRT	T-46427	Left Branch of Hepatic Artery	unilateral
	concept	LN	20354-7	Velocity Time Integral	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Liver Length</b>	anatomy	SNM3	T-62000	Liver	unilateral
	concept	SRT	G-A22A	Length	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>M2 EDV</b>	anatomy	SRT	R-10251	Middle Cerebral Artery M2 Segment	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>M2 PI</b>	anatomy	SRT	R-10251	Middle Cerebral Artery M2 Segment	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>M2 PSV</b>	anatomy	SRT	R-10251	Middle Cerebral Artery M2 Segment	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>M2 TAPV</b>	anatomy	SRT	R-10251	Middle Cerebral Artery M2 Segment	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>M2 TCD Mean</b>	anatomy	SRT	R-10251	Middle Cerebral Artery M2 Segment	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>M2 TCD PI</b>	anatomy	SRT	R-10251	Middle Cerebral Artery M2 Segment	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>MCA</b>	anatomy	99PMSBLUS	C12105-01	MCA/Dist ICA Ratio Numerator	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>MCA/ICA</b>	anatomy	99PMSBLUS	C12105-05	MCA/Dist ICA Ratio	bilateral
	concept	99PMSBLUS	C12105-03	MCA/Dist ICA Ratio	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>MDV</b>	anatomy	99PMSBLUS	sup71_001	Antecube	bilateral
		SRT	T-45100	Common Carotid Artery	bilateral
			T-45170	Carotid Bulb	bilateral
			T-45200	External Carotid Artery	bilateral
			T-45300	Internal Carotid Artery	bilateral
			T-45700	Vertebral Artery	bilateral
			T-46010	Innominate Artery	bilateral
			T-46100	Subclavian Artery	bilateral
			T-46710	Common Iliac Artery	bilateral
			T-46740	Internal Iliac Artery	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
			T-46910	External Iliac Artery	bilateral
			T-47100	Axillary Artery	bilateral
			T-47160	Brachial Artery	bilateral
			T-47200	Ulnar Artery	bilateral
			T-47300	Radial Artery	bilateral
			T-47400	Common Femoral Artery	bilateral
			T-47403	Superficial Femoral Artery	bilateral
			T-47440	Profunda Femoris Artery	bilateral
			T-47500	Popliteal Artery	bilateral
			T-47600	Posterior Tibial Artery	bilateral
			T-47630	Peroneal Artery	bilateral
			T-47700	Anterior Tibial Artery	bilateral
			T-47741	Dorsalis Pedis Artery	bilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
			T-47020	Artery Of Upper Extremity	bilateral
			T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
			G-A119	Distal	bilateral
			G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Arc AI</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	20167-3	Acceleration Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	bilateral
<b>Mid Arc AT</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	20168-1	Acceleration Time	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	sec	Seconds	bilateral
<b>Mid Arc EDV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Arc MDV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Arc PI</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Arc PSV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Arc RI</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Arc S/D</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
<b>Mid Arc TAMV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	20352-1	Time averaged mean velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Arc TAPV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Arc VTI</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	20354-7	Velocity Time Integral	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Mid ATA PI</b>	anatomy	SRT	T-47700	Anterior Tibial Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid ATA RI</b>	anatomy	SRT	T-47700	Anterior Tibial Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid ATA S/D</b>	anatomy	SRT	T-47700	Anterior Tibial Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Basilar A EDV</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Mid Basilar A PI</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Mid Basilar A PSV</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Mid Basilar A TAPV</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Mid Basilar A TCD Mean</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Mid Basilar A TCD PI</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Mid Bulb IMT</b>	anatomy	SRT	T-45170	Carotid Bulb	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Mid CCA IMT</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Mid CCA IMT(Q)</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	MeasType	99PMSBLUS	C3627-01	QLAB IMT measurement	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Mid CCA PI</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid CCA RI</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid CCA S/D</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid ECA PI</b>	anatomy	SRT	T-45200	External Carotid Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid ECA RI</b>	anatomy	SRT	T-45200	External Carotid Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid ECA S/D</b>	anatomy	SRT	T-45200	External Carotid Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid ICA IMT</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Mid ICA IMT(Q)</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	MeasType	99PMSBLUS	C3627-01	QLAB IMT measurement	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Mid ICA PI</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
<b>Mid ICA RI</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid ICA S/D</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid M1 EDV</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid M1 PI</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid M1 PSV</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid M1 TAPV</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid M1 TCD Mean</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid M1 TCD PI</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Pero A PI</b>	anatomy	SRT	T-47630	Peroneal Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Pero A RI</b>	anatomy	SRT	T-47630	Peroneal Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Pero A S/D</b>	anatomy	SRT	T-47630	Peroneal Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid PTA PI</b>	anatomy	SRT	T-47600	Posterior Tibial Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid PTA RI</b>	anatomy	SRT	T-47600	Posterior Tibial Artery	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid PTA S/D</b>	anatomy	SRT	T-47600	Posterior Tibial Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Rad A PI</b>	anatomy	SRT	T-47300	Radial Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Rad A RI</b>	anatomy	SRT	T-47300	Radial Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Rad A S/D</b>	anatomy	SRT	T-47300	Radial Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Ren A AI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20167-3	Acceleration Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	bilateral
<b>Mid Ren A AT</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20168-1	Acceleration Time	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	sec	Seconds	bilateral
<b>Mid Ren A EDV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Ren A MDV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Ren A PI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Ren A PSV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Ren A RI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Ren A S/D</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Ren A TAMV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20352-1	Time averaged mean velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Ren A TAPV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Ren A VTI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20354-7	Velocity Time Integral	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Mid SCL A PI</b>	anatomy	SRT	T-46100	Subclavian Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid SCL A RI</b>	anatomy	SRT	T-46100	Subclavian Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid SCL A S/D</b>	anatomy	SRT	T-46100	Subclavian Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Seg AI</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	20167-3	Acceleration Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	bilateral
<b>Mid Seg AT</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	20168-1	Acceleration Time	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	sec	Seconds	bilateral
<b>Mid Seg EDV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Seg MDV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Seg PI</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Seg PSV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Seg RI</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Seg S/D</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Seg TAMV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	20352-1	Time averaged mean velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Seg TAPV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Mid Seg VTI</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A109	Medial	bilateral
	concept	LN	20354-7	Velocity Time Integral	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Mid SFA PI</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid SFA RI</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid SFA S/D</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid SMA AI</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	20167-3	Acceleration Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	unilateral
<b>Mid SMA AT</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	20168-1	Acceleration Time	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	sec	Seconds	unilateral
<b>Mid SMA EDV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Mid SMA MDV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Mid SMA PI</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Mid SMA PSV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Mid SMA RI</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	12023-8	Resistivity Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Mid SMA S/D</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Mid SMA TAMV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	20352-1	Time averaged mean velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Mid SMA TAPV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Mid SMA VTI</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	20354-7	Velocity Time Integral	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A188	Mid-longitudinal	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Mid Ulnar A PI</b>	anatomy	SRT	T-47200	Ulnar Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Ulnar A RI</b>	anatomy	SRT	T-47200	Ulnar Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Mid Ulnar A S/D</b>	anatomy	SRT	T-47200	Ulnar Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A188	Mid-longitudinal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Ophthalmic A EDV</b>	anatomy	SRT	T-45400	Ophthalmic Artery	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ophthalmic A PI</b>	anatomy	SRT	T-45400	Ophthalmic Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>Ophthalmic A PSV</b>	anatomy	SRT	T-45400	Ophthalmic Artery	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ophthalmic A TAPV</b>	anatomy	SRT	T-45400	Ophthalmic Artery	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ophthalmic A TCD Mean</b>	anatomy	SRT	T-45400	Ophthalmic Artery	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ophthalmic A TCD PI</b>	anatomy	SRT	T-45400	Ophthalmic Artery	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>PCA P1 EDV</b>	anatomy	SRT	R-10253	Posterior Cerebral Artery P1 Segment	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>PCA P1 PI</b>	anatomy	SRT	R-10253	Posterior Cerebral Artery P1 Segment	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>PCA P1 PSV</b>	anatomy	SRT	R-10253	Posterior Cerebral Artery P1 Segment	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>PCA P1 TAPV</b>	anatomy	SRT	R-10253	Posterior Cerebral Artery P1 Segment	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>PCA P1 TCD Mean</b>	anatomy	SRT	R-10253	Posterior Cerebral Artery P1 Segment	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>PCA P1 TCD PI</b>	anatomy	SRT	R-10253	Posterior Cerebral Artery P1 Segment	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>PCA P2 EDV</b>	anatomy	SRT	R-10255	Posterior Cerebral Artery P2 Segment	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>PCA P2 PI</b>	anatomy	SRT	R-10255	Posterior Cerebral Artery P2 Segment	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>PCA P2 PSV</b>	anatomy	SRT	R-10255	Posterior Cerebral Artery P2 Segment	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>PCA P2 TAPV</b>	anatomy	SRT	R-10255	Posterior Cerebral Artery P2 Segment	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>PCA P2 TCD Mean</b>	anatomy	SRT	R-10255	Posterior Cerebral Artery P2 Segment	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>PCA P2 TCD PI</b>	anatomy	SRT	R-10255	Posterior Cerebral Artery P2 Segment	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	units	UCUM	1	ratio	bilateral
<b>PCoA EDV</b>	anatomy	SRT	T-45320	Posterior Communicating Artery	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>PCoA PI</b>	anatomy	SRT	T-45320	Posterior Communicating Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>PCoA PSV</b>	anatomy	SRT	T-45320	Posterior Communicating Artery	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>PCoA TAPV</b>	anatomy	SRT	T-45320	Posterior Communicating Artery	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>PCoA TCD Mean</b>	anatomy	SRT	T-45320	Posterior Communicating Artery	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>PCoA TCD PI</b>	anatomy	SRT	T-45320	Posterior Communicating Artery	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox ATA PI</b>	anatomy	SRT	T-47700	Anterior Tibial Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox ATA RI</b>	anatomy	SRT	T-47700	Anterior Tibial Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox ATA S/D</b>	anatomy	SRT	T-47700	Anterior Tibial Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Basilar A EDV</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Prox Basilar A PI</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Prox Basilar A PSV</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Prox Basilar A TAPV</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Prox Basilar A TCD Mean</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Prox Basilar A TCD PI</b>	anatomy	SRT	T-45800	Basilar Artery	unilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	unilateral
	section	SRT	T-40501	Blood Vessel of Head	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Prox Brach A PI</b>	anatomy	SRT	T-47160	Brachial Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Brach A RI</b>	anatomy	SRT	T-47160	Brachial Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Brach A S/D</b>	anatomy	SRT	T-47160	Brachial Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Bulb IMT</b>	anatomy	SRT	T-45170	Carotid Bulb	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Prox CCA IMT</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Prox CCA IMT(Q)</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	MeasType	99PMSBLUS	C3627-01	QLAB IMT measurement	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Prox CCA PI</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox CCA RI</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox CCA S/D</b>	anatomy	SRT	T-45100	Common Carotid Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox ECA PI</b>	anatomy	SRT	T-45200	External Carotid Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox ECA RI</b>	anatomy	SRT	T-45200	External Carotid Artery	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox ECA S/D</b>	anatomy	SRT	T-45200	External Carotid Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox ICA IMT</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Prox ICA IMT(Q)</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	99PMSBLUS	C12122-08	Mean Intima Media Thickness	bilateral
	MeasType	99PMSBLUS	C3627-01	QLAB IMT measurement	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Prox ICA PI</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox ICA RI</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox ICA S/D</b>	anatomy	SRT	T-45300	Internal Carotid Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox M1 EDV</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Prox M1 PI</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox M1 PSV</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Prox M1 TAPV</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Prox M1 TCD Mean</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Prox M1 TCD PI</b>	anatomy	SRT	R-1024F	Middle Cerebral Artery M1 Segment	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Pero A PI</b>	anatomy	SRT	T-47630	Peroneal Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Pero A RI</b>	anatomy	SRT	T-47630	Peroneal Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Pero A S/D</b>	anatomy	SRT	T-47630	Peroneal Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox PFA PI</b>	anatomy	SRT	T-47440	Profunda Femoris Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox PFA RI</b>	anatomy	SRT	T-47440	Profunda Femoris Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox PFA S/D</b>	anatomy	SRT	T-47440	Profunda Femoris Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Pop A PI</b>	anatomy	SRT	T-47500	Popliteal Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Pop A RI</b>	anatomy	SRT	T-47500	Popliteal Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Pop A S/D</b>	anatomy	SRT	T-47500	Popliteal Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox PTA PI</b>	anatomy	SRT	T-47600	Posterior Tibial Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox PTA RI</b>	anatomy	SRT	T-47600	Posterior Tibial Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox PTA S/D</b>	anatomy	SRT	T-47600	Posterior Tibial Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Rad A PI</b>	anatomy	SRT	T-47300	Radial Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Rad A RI</b>	anatomy	SRT	T-47300	Radial Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Rad A S/D</b>	anatomy	SRT	T-47300	Radial Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Ren A AI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20167-3	Acceleration Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	bilateral
<b>Prox Ren A AT</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20168-1	Acceleration Time	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	sec	Seconds	bilateral
<b>Prox Ren A EDV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Prox Ren A MDV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Prox Ren A PI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Ren A PSV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Prox Ren A RI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Ren A S/D</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Ren A TAMV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20352-1	Time averaged mean velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Prox Ren A TAPV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Prox Ren A VTI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20354-7	Velocity Time Integral	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Prox SCL A PI</b>	anatomy	SRT	T-46100	Subclavian Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox SCL A RI</b>	anatomy	SRT	T-46100	Subclavian Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox SCL A S/D</b>	anatomy	SRT	T-46100	Subclavian Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox SFA PI</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox SFA RI</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox SFA S/D</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox SMA AI</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	20167-3	Acceleration Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	unilateral
<b>Prox SMA AT</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	20168-1	Acceleration Time	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	sec	Seconds	unilateral
<b>Prox SMA EDV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Prox SMA MDV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A118	Proximal	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Prox SMA PI</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Prox SMA PSV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Prox SMA RI</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	12023-8	Resistivity Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Prox SMA S/D</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	1	ratio	unilateral
<b>Prox SMA TAMV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	20352-1	Time averaged mean velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Prox SMA TAPV</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Prox SMA VTI</b>	anatomy	SRT	T-46510	Superior Mesenteric Artery	unilateral
	concept	LN	20354-7	Velocity Time Integral	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	segment	SRT	G-A118	Proximal	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Prox Ulnar A PI</b>	anatomy	SRT	T-47200	Ulnar Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Ulnar A RI</b>	anatomy	SRT	T-47200	Ulnar Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>Prox Ulnar A S/D</b>	anatomy	SRT	T-47200	Ulnar Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-47020	Artery Of Upper Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
	units	UCUM	1	ratio	bilateral
<b>PSV</b>	anatomy	99PMSBLUS	sup71_001	Antecube	bilateral
		SRT	T-45100	Common Carotid Artery	bilateral
			T-45170	Carotid Bulb	bilateral
			T-45200	External Carotid Artery	bilateral
			T-45300	Internal Carotid Artery	bilateral
			T-45700	Vertebral Artery	bilateral
			T-46010	Innominate Artery	bilateral
			T-46100	Subclavian Artery	bilateral
			T-46710	Common Iliac Artery	bilateral
			T-46740	Internal Iliac Artery	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
			T-46910	External Iliac Artery	bilateral
			T-47100	Axillary Artery	bilateral
			T-47160	Brachial Artery	bilateral
			T-47200	Ulnar Artery	bilateral
			T-47300	Radial Artery	bilateral
			T-47400	Common Femoral Artery	bilateral
			T-47403	Superficial Femoral Artery	bilateral
			T-47440	Profunda Femoris Artery	bilateral
			T-47500	Popliteal Artery	bilateral
			T-47600	Posterior Tibial Artery	bilateral
			T-47630	Peroneal Artery	bilateral
			T-47700	Anterior Tibial Artery	bilateral
			T-47741	Dorsalis Pedis Artery	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
			T-47020	Artery Of Upper Extremity	bilateral
			T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
			G-A119	Distal	bilateral
			G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>PV Bladder Height</b>	anatomy	99PMSBLUS	C4-01	Post Void Bladder	unilateral
	concept	99PMSBLUS	C12011-07	Post Void Bladder Height	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>PV Bladder Length</b>	anatomy	99PMSBLUS	C4-01	Post Void Bladder	unilateral
	concept	99PMSBLUS	C12011-05	Post Void Bladder Length	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>PV Bladder Vol</b>	anatomy	99PMSBLUS	C4-01	Post Void Bladder	unilateral
	concept	99PMSBLUS	C12011-08	Post Void Bladder Volume	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	cm <sup>3</sup>	Cubic Centimeter	unilateral
<b>PV Bladder Width</b>	anatomy	99PMSBLUS	C4-01	Post Void Bladder	unilateral
	concept	99PMSBLUS	C12011-06	Post Void Bladder Width	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>R Hepatic A AI</b>	anatomy	SRT	T-46423	Right Branch of Hepatic Artery	unilateral
	concept	LN	20167-3	Acceleration Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	unilateral
<b>R Hepatic A AT</b>	anatomy	SRT	T-46423	Right Branch of Hepatic Artery	unilateral
	concept	LN	20168-1	Acceleration Time	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	sec	Seconds	unilateral
<b>R Hepatic A EDV</b>	anatomy	SRT	T-46423	Right Branch of Hepatic Artery	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>R Hepatic A MDV</b>	anatomy	SRT	T-46423	Right Branch of Hepatic Artery	unilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>R Hepatic A PI</b>	anatomy	SRT	T-46423	Right Branch of Hepatic Artery	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>R Hepatic A PSV</b>	anatomy	SRT	T-46423	Right Branch of Hepatic Artery	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral

ClearVue 350/550/650/850 3.1 Report Label	MOD Type	CSD	CV	CM	Laterality
<b>R Hepatic A RI</b>	anatomy	SRT	T-46423	Right Branch of Hepatic Artery	unilateral
	concept	LN	12023-8	Resistivity Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>R Hepatic A S/D</b>	anatomy	SRT	T-46423	Right Branch of Hepatic Artery	unilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>R Hepatic A TAMV</b>	anatomy	SRT	T-46423	Right Branch of Hepatic Artery	unilateral
	concept	LN	20352-1	Time averaged mean velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>R Hepatic A TAPV</b>	anatomy	SRT	T-46423	Right Branch of Hepatic Artery	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>R Hepatic A VTI</b>	anatomy	SRT	T-46423	Right Branch of Hepatic Artery	unilateral
	concept	LN	20354-7	Velocity Time Integral	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>RAR</b>	concept	LN	33869-9	Renal Artery/Aorta velocity ratio	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Ren A Org AI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20167-3	Acceleration Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-036A	Origin of vessel	bilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	bilateral
<b>Ren A Org AT</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20168-1	Acceleration Time	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-036A	Origin of vessel	bilateral
	units	UCUM	sec	Seconds	bilateral
<b>Ren A Org EDV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-036A	Origin of vessel	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ren A Org MDV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-036A	Origin of vessel	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ren A Org PI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-036A	Origin of vessel	bilateral
	units	UCUM	1	ratio	bilateral
<b>Ren A Org PSV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-036A	Origin of vessel	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ren A Org RI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-036A	Origin of vessel	bilateral
	units	UCUM	1	ratio	bilateral
<b>Ren A Org S/D</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	segment	SRT	G-036A	Origin of vessel	bilateral
	units	UCUM	1	ratio	bilateral
<b>Ren A Org TAMV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20352-1	Time averaged mean velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-036A	Origin of vessel	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ren A Org TAPV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-036A	Origin of vessel	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ren A Org VTI</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	20354-7	Velocity Time Integral	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	segment	SRT	G-036A	Origin of vessel	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Ren V AI</b>	anatomy	SRT	T-48740	Renal Vein	bilateral
	concept	LN	20167-3	Acceleration Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	bilateral
<b>Ren V AT</b>	anatomy	SRT	T-48740	Renal Vein	bilateral
	concept	LN	20168-1	Acceleration Time	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	sec	Seconds	bilateral
<b>Ren V EDV</b>	anatomy	SRT	T-48740	Renal Vein	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ren V MDV</b>	anatomy	SRT	T-48740	Renal Vein	bilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ren V PI</b>	anatomy	SRT	T-48740	Renal Vein	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Ren V PSV</b>	anatomy	SRT	T-48740	Renal Vein	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ren V RI</b>	anatomy	SRT	T-48740	Renal Vein	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Ren V S/D</b>	anatomy	SRT	T-48740	Renal Vein	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Ren V TAMV</b>	anatomy	SRT	T-48740	Renal Vein	bilateral
	concept	LN	20352-1	Time averaged mean velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ren V TAPV</b>	anatomy	SRT	T-48740	Renal Vein	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Ren V VTI</b>	anatomy	SRT	T-48740	Renal Vein	bilateral
	concept	LN	20354-7	Velocity Time Integral	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm	Centimeter	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
<b>Renal A PSV</b>	anatomy	SRT	T-46600	Renal Artery	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>SFA % Area Reduction</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	SRT	G-0371	Percent Area Reduction	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	%	Percent	bilateral
<b>SFA % Diam Reduction</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	SRT	G-0372	Percent Diameter Reduction	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	%	Percent	bilateral
<b>SFA Area Resid</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	99PMSBLUS	C7471-01	Area 1 of Area Percent Reduction	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	cm2	Square Centimeter	bilateral
<b>SFA Area True</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	99PMSBLUS	C7471-02	Area 2 of Area Percent Reduction	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	cm2	Square Centimeter	bilateral
<b>SFA Diam Resid</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	99PMSBLUS	C7470-05	Diameter 1 of Diameter Reduction	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>SFA Diam True</b>	anatomy	SRT	T-47403	Superficial Femoral Artery	bilateral
	concept	99PMSBLUS	C7470-06	Diameter 2 of Diameter Reduction	bilateral
	section	SRT	T-47040	Artery of Lower Extremity	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Spleen Height</b>	anatomy	SNM3	T-C3000	Spleen	unilateral
	concept	99PMSBLUS	C7470-01	Height	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Spleen Length</b>	anatomy	SNM3	T-C3000	Spleen	unilateral
	concept	SRT	G-A22A	Length	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Spleen Vol</b>	anatomy	SNM3	T-C3000	Spleen	unilateral
	concept	DCM	121221	Volume of ellipsoid	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	cm3	Cubic Centimeter	unilateral
<b>Spleen Width</b>	anatomy	SNM3	T-C3000	Spleen	unilateral
	concept	SNM3	G-A220	Width	unilateral
	section	99PMSBLUS	T5100-02	Anatomic Structures (unilateral)	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Splenic A AI</b>	anatomy	SRT	T-46460	Splenic Artery	unilateral
	concept	LN	20167-3	Acceleration Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	unilateral
<b>Splenic A AT</b>	anatomy	SRT	T-46460	Splenic Artery	unilateral
	concept	LN	20168-1	Acceleration Time	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	sec	Seconds	unilateral
<b>Splenic A EDV</b>	anatomy	SRT	T-46460	Splenic Artery	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Splenic A MDV</b>	anatomy	SRT	T-46460	Splenic Artery	unilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Splenic A PI</b>	anatomy	SRT	T-46460	Splenic Artery	unilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Splenic A PSV</b>	anatomy	SRT	T-46460	Splenic Artery	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Splenic A RI</b>	anatomy	SRT	T-46460	Splenic Artery	unilateral
	concept	LN	12023-8	Resistivity Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Splenic A S/D</b>	anatomy	SRT	T-46460	Splenic Artery	unilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Splenic A TAMV</b>	anatomy	SRT	T-46460	Splenic Artery	unilateral
	concept	LN	20352-1	Time averaged mean velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Splenic A TAPV</b>	anatomy	SRT	T-46460	Splenic Artery	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Splenic A VTI</b>	anatomy	SRT	T-46460	Splenic Artery	unilateral
	concept	LN	20354-7	Velocity Time Integral	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Sup Arc AI</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	20167-3	Acceleration Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	bilateral
<b>Sup Arc AT</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	20168-1	Acceleration Time	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	sec	Seconds	bilateral
<b>Sup Arc EDV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Sup Arc MDV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Sup Arc PI</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Sup Arc PSV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Sup Arc RI</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	units	UCUM	1	ratio	bilateral
<b>Sup Arc S/D</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Sup Arc TAMV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	20352-1	Time averaged mean velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Sup Arc TAPV</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Sup Arc VTI</b>	anatomy	SRT	T-4668A	Arcuate Artery of the Kidney	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	20354-7	Velocity Time Integral	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>Sup Ren Ao AI</b>	anatomy	SRT	T-42510	Supra-renal Aorta	unilateral
	concept	LN	20167-3	Acceleration Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	unilateral
<b>Sup Ren Ao AT</b>	anatomy	SRT	T-42510	Supra-renal Aorta	unilateral
	concept	LN	20168-1	Acceleration Time	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	sec	Seconds	unilateral
<b>Sup Ren Ao EDV</b>	anatomy	SRT	T-42510	Supra-renal Aorta	unilateral
	concept	LN	11653-3	End Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Sup Ren Ao MDV</b>	anatomy	SRT	T-42510	Supra-renal Aorta	unilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Sup Ren Ao PI</b>	anatomy	SRT	T-42510	Supra-renal Aorta	unilateral
	concept	LN	12008-9	Pulsatility Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Sup Ren Ao PSV</b>	anatomy	SRT	T-42510	Supra-renal Aorta	unilateral
	concept	LN	11726-7	Peak Systolic Velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Sup Ren Ao RI</b>	anatomy	SRT	T-42510	Supra-renal Aorta	unilateral
	concept	LN	12023-8	Resistivity Index	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Sup Ren Ao S/D</b>	anatomy	SRT	T-42510	Supra-renal Aorta	unilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	1	ratio	unilateral
<b>Sup Ren Ao TAMV</b>	anatomy	SRT	T-42510	Supra-renal Aorta	unilateral
	concept	LN	20352-1	Time averaged mean velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral
<b>Sup Ren Ao TAPV</b>	anatomy	SRT	T-42510	Supra-renal Aorta	unilateral
	concept	LN	11692-1	Time averaged peak velocity	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm/s	Centimeter Per Second	unilateral

ClearVue 350/550/650/850 3.1 Report Label	MOD Type	CSD	CV	CM	Laterality
<b>Sup Ren Ao VTI</b>	anatomy	SRT	T-42510	Supra-renal Aorta	unilateral
	concept	LN	20354-7	Velocity Time Integral	unilateral
	section	SRT	T-46002	Artery of Abdomen	unilateral
	units	UCUM	cm	Centimeter	unilateral
<b>Sup Seg AI</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	20167-3	Acceleration Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square	bilateral
<b>Sup Seg AT</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	20168-1	Acceleration Time	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	sec	Seconds	bilateral
<b>Sup Seg EDV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Sup Seg MDV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	11665-7	Minimum Diastolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Sup Seg PI</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Sup Seg PSV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Sup Seg RI</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Sup Seg S/D</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	1	ratio	bilateral
<b>Sup Seg TAMV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	20352-1	Time averaged mean velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Sup Seg TAPV</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Sup Seg VTI</b>	anatomy	SRT	T-46659	Segmental Artery	bilateral
	branch	SRT	G-A116	Superior	bilateral
	concept	LN	20354-7	Velocity Time Integral	bilateral
	section	SRT	T-71019	Vascular Structure Of Kidney	bilateral
	units	UCUM	cm	Centimeter	bilateral
<b>TAMV</b>	anatomy	99PMSBLUS	sup71_001	Antecube	bilateral
		SRT	T-45100	Common Carotid Artery	bilateral

ClearVue 350/550/650/850 3.1 Report Label	MOD Type	CSD	CV	CM	Laterality
			T-45170	Carotid Bulb	bilateral
			T-45200	External Carotid Artery	bilateral
			T-45300	Internal Carotid Artery	bilateral
			T-45700	Vertebral Artery	bilateral
			T-46010	Innominate Artery	bilateral
			T-46100	Subclavian Artery	bilateral
			T-46710	Common Iliac Artery	bilateral
			T-46740	Internal Iliac Artery	bilateral
			T-46910	External Iliac Artery	bilateral
			T-47100	Axillary Artery	bilateral
			T-47160	Brachial Artery	bilateral
			T-47200	Ulnar Artery	bilateral
			T-47300	Radial Artery	bilateral
			T-47400	Common Femoral Artery	bilateral
			T-47403	Superficial Femoral Artery	bilateral
			T-47440	Profunda Femoris Artery	bilateral
			T-47500	Popliteal Artery	bilateral
			T-47600	Posterior Tibial Artery	bilateral
			T-47630	Peroneal Artery	bilateral
			T-47700	Anterior Tibial Artery	bilateral
			T-47741	Dorsalis Pedis Artery	bilateral
	concept	LN	20352-1	Time averaged mean velocity	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
			T-47020	Artery Of Upper Extremity	bilateral
			T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
			G-A119	Distal	bilateral
			G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
TAPV	anatomy	99PMSBLUS	sup71_001	Antecube	bilateral
		SRT	T-45100	Common Carotid Artery	bilateral
			T-45170	Carotid Bulb	bilateral
			T-45200	External Carotid Artery	bilateral
			T-45300	Internal Carotid Artery	bilateral
			T-45700	Vertebral Artery	bilateral
			T-46010	Innominate Artery	bilateral
			T-46100	Subclavian Artery	bilateral
			T-46710	Common Iliac Artery	bilateral
			T-46740	Internal Iliac Artery	bilateral
			T-46910	External Iliac Artery	bilateral
			T-47100	Axillary Artery	bilateral
			T-47160	Brachial Artery	bilateral
			T-47200	Ulnar Artery	bilateral
			T-47300	Radial Artery	bilateral
			T-47400	Common Femoral Artery	bilateral
			T-47403	Superficial Femoral Artery	bilateral
			T-47440	Profunda Femoris Artery	bilateral
			T-47500	Popliteal Artery	bilateral
			T-47600	Posterior Tibial Artery	bilateral
			T-47630	Peroneal Artery	bilateral
			T-47700	Anterior Tibial Artery	bilateral
			T-47741	Dorsalis Pedis Artery	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
			T-47020	Artery Of Upper Extremity	bilateral
			T-47040	Artery of Lower Extremity	bilateral
	segment	SRT	G-A118	Proximal	bilateral
			G-A119	Distal	bilateral
			G-A188	Mid-longitudinal	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Term ICA EDV</b>		anatomy	SRT	R-102BD	Terminal internal carotid artery
bilateral					

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Term ICA PI</b>	anatomy	SRT	R-102BD	Terminal internal carotid artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>Term ICA PSV</b>	anatomy	SRT	R-102BD	Terminal internal carotid artery	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Term ICA TAPV</b>	anatomy	SRT	R-102BD	Terminal internal carotid artery	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Term ICA TCD Mean</b>	anatomy	SRT	R-102BD	Terminal internal carotid artery	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Term ICA TCD PI</b>	anatomy	SRT	R-102BD	Terminal internal carotid artery	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>Vertebral A EDV</b>	anatomy	99PMSBLUS	C12105-04	Vertebral Artery in TCD	bilateral
	concept	LN	11653-3	End Diastolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Vertebral A PI</b>	anatomy	99PMSBLUS	C12105-04	Vertebral Artery in TCD	bilateral
		SRT	T-45700	Vertebral Artery	bilateral
	concept	LN	12008-9	Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
			T-45005	Artery of neck	bilateral
	units	UCUM	1	ratio	bilateral
<b>Vertebral A PSV</b>	anatomy	99PMSBLUS	C12105-04	Vertebral Artery in TCD	bilateral
	concept	LN	11726-7	Peak Systolic Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Vertebral A RI</b>	anatomy	SRT	T-45700	Vertebral Artery	bilateral
	concept	LN	12023-8	Resistivity Index	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	1	ratio	bilateral
<b>Vertebral A S/D</b>	anatomy	SRT	T-45700	Vertebral Artery	bilateral
	concept	LN	12144-2	Systolic to Diastolic Velocity Ratio	bilateral
	section	SRT	T-45005	Artery of neck	bilateral
	units	UCUM	1	ratio	bilateral
<b>Vertebral A TAPV</b>	anatomy	99PMSBLUS	C12105-04	Vertebral Artery in TCD	bilateral
	concept	LN	11692-1	Time averaged peak velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Vertebral A TCD Mean</b>	anatomy	99PMSBLUS	C12105-04	Vertebral Artery in TCD	bilateral
	concept	99PMSBLUS	C12221-03	TCD Mean Velocity	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	cm/s	Centimeter Per Second	bilateral
<b>Vertebral A TCD PI</b>	anatomy	99PMSBLUS	C12105-04	Vertebral Artery in TCD	bilateral
	concept	99PMSBLUS	C12221-04	TCD Pulsatility Index	bilateral
	section	SRT	T-40501	Blood Vessel of Head	bilateral
	units	UCUM	1	ratio	bilateral
<b>VTI</b>	anatomy	99PMSBLUS	sup71_001	Antecube	bilateral
		SRT	T-45100	Common Carotid Artery	bilateral
			T-45170	Carotid Bulb	bilateral
			T-45200	External Carotid Artery	bilateral

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>	<b>Laterality</b>
			T-45300	Internal Carotid Artery	bilateral
			T-45700	Vertebral Artery	bilateral
			T-46010	Innominate Artery	bilateral
			T-46100	Subclavian Artery	bilateral
			T-46710	Common Iliac Artery	bilateral
			T-46740	Internal Iliac Artery	bilateral
			T-46910	External Iliac Artery	bilateral
			T-47100	Axillary Artery	bilateral
			T-47160	Brachial Artery	bilateral
			T-47200	Ulnar Artery	bilateral
			T-47300	Radial Artery	bilateral
			T-47400	Common Femoral Artery	bilateral
			T-47403	Superficial Femoral Artery	bilateral
			T-47440	Profunda Femoris Artery	bilateral
			T-47500	Popliteal Artery	bilateral
			T-47600	Posterior Tibial Artery	bilateral
			T-47630	Peroneal Artery	bilateral
			T-47700	Anterior Tibial Artery	bilateral
			T-47741	Dorsalis Pedis Artery	bilateral
concept	LN	20354-7		Velocity Time Integral	bilateral
section	SRT	T-45005		Artery of neck	bilateral
		T-47020		Artery Of Upper Extremity	bilateral
		T-47040		Artery of Lower Extremity	bilateral
segment	SRT	G-A118		Proximal	bilateral
		G-A119		Distal	bilateral
		G-A188		Mid-longitudinal	bilateral
units	UCUM	cm		Centimeter	bilateral

<sup>1</sup> Available only on ClearVue 550 with High Q

## A.4 ADULT ECHOCARDIOGRAPHY STRUCTURED REPORT TEMPLATE

ClearVue 350/550/650/850 3.1 implements the Adult Echocardiography Template (TID 5200) from the DICOM standard, part 16. This appendix describes the scope and manner that ClearVue 350/550/650/850 3.1 measurements appear in DICOM SR.

Measurements and calculations performed for cardiac studies will lead to creation of “Adult Echocardiography Procedure Report” structured report documents. Measurements can be performed by pressing the ‘Calc’ key on ClearVue 350/550/650/850 3.1 control panel and selecting the Cardiac (Adult Echo) analysis package. Measurements and calculations available in the menu can be configured through the setup application. It is also possible to configure the measurement unit (Metric or U.S.).

All concepts with value type (VT) NUM will always have a ‘MeasurementUnitCodeSequence’ that specifies the unit of the measurement. The CSD for all units will be UCUM (Unified Code for Units) and CV and CM will be based on application configuration and will conform to UCUM standards.

### A.4.1 Template specific conformance for TID 5200

The template for the root of the content tree for TID 5200 and its use in the ClearVue 350/550/650/850 3.1 context is described in the following table.

Note: Only the rows that apply to use by ClearVue 350/550/650/850 3.1 are included.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	EV (125200, DCM, “Adult Echocardiography Procedure Report”)	This is the root ‘CONTAINER’
2	>	CONTAINS	INCLUDE	DTID (5201) Echocardiography Patient Characteristics	Refer to A.4.2 for ClearVue 350/550/650/850 3.1 usage of this.
3	>	CONTAINS	INCLUDE	DTID (T5200-03) Echo Procedure Summary Section	Refer to A.4.3 for ClearVue 350/550/650/850 3.1 usage of this.
4	>	CONTAINS	INCLUDE	DTID (5202) Echo Section	Concepts in CID 12200 will be used with \$SectionSubject = EV (T-32600, SRT, “Left Ventricle”).
5	>	CONTAINS	INCLUDE	DTID (5202) Echo Section	Concepts in CID 12204 will be used with \$SectionSubject = EV (T-32500, SRT, “Right Ventricle”).
6	>	CONTAINS	INCLUDE	DTID (5202) Echo Section	Concepts in CID 12205 will be used with \$SectionSubject = EV (T-32300, SRT, “Left Atrium”).
7	>	CONTAINS	INCLUDE	DTID (5202) Echo Section	Concepts in CID 12206 will be used with \$SectionSubject = EV (T-32200, SRT, “Right Atrium”).
8	>	CONTAINS	INCLUDE	DTID (5202) Echo Section	Concepts in CID 12211 will be used with \$SectionSubject = EV (T-35400, SRT, “Aortic Valve”).

No	NL	REL WITH PARENT	VT	Concept Name	Comments
9	>	CONTAINS	INCLUDE	DTID (5202) Echo Section	Concepts in CID 12207 will be used with \$SectionSubject = EV (T-35300, SRT, "Mitral Valve").
10	>	CONTAINS	INCLUDE	DTID (5202) Echo Section	Concepts in CID 12209 will be used with \$SectionSubject = EV (T-35200, SRT, "Pulmonic Valve").
11	>	CONTAINS	INCLUDE	DTID (5202) Echo Section	Concepts in CID 12208 will be used with \$SectionSubject = EV (T-35100, SRT, "Tricuspid Valve").
12	>	CONTAINS	INCLUDE	DTID (5202) Echo Section	Concepts in CID 12212 will be used with \$SectionSubject = EV (T-42000, SRT, "Aorta".
13	>	CONTAINS	INCLUDE	DTID (5202) Echo Section	Concepts in CID 12210 will be used with \$SectionSubject = EV (T-44000, SRT, "Pulmonary artery").
14	>	CONTAINS	INCLUDE	DTID (5202) Echo Section	Concepts in CID 12215 will be used with \$SectionSubject = EV (T-48600, SRT, "Vena Cava").
15	>	CONTAINS	INCLUDE	DTID (5202) Echo Section	Concepts in CID 12214 will be used with \$SectionSubject = EV (T-48581, SRT, "Pulmonary Venous Structure").
16	>	CONTAINS	INCLUDE	DTID (5202) Echo Section	Concepts in CID 12217 will be used with \$SectionSubject = EV (P5-30031, SRT, "Cardiac Shunt Study").
17	>	CONTAINS	INCLUDE	DTID (T-48720) Hepatic Veins Section	Concepts in CID 12216 will be used with \$SectionSubject = EV (T-48720, SRT, "Hepatic Veins"). Refer to A.4.7 for more details.

#### A.4.2 Echocardiography Patient Characteristics (TID 5201)

Use of the template TID 5201 in the context of ClearVue 350/550/650/850 3.1 is described in the following table.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	EV (121118, DCM, "Patient Characteristics")	
2	>	CONTAINS	NUM	EV (121033, DCM, "Subject Age")	Units = DCID (7456
3	>	CONTAINS	CODE	EV (121032, DCM, "Subject Sex")	Value is taken from PDE (Patient Data Entry) screen or from the MWL and the corresponding Concepts are taken from the DCID 7455.

4	>	CONTAINS	NUM	EV (F-008EC, SRT, "Systolic Blood Pressure")	Value is taken from PDE (Patient Data Entry) screen.
5	>	CONTAINS	NUM	EV (F-008ED, SRT, "Diastolic Blood Pressure")	Value is taken from PDE (Patient Data Entry) screen.
6	>	CONTAINS	NUM	EV (8277-6, LN, "Body Surface Area")	Value automatically calculated by the ClearVue 350/550/650/850 3.1 system based on the Height and Weight values entered on PDE (Patient Data Entry) screen.

#### A.4.3 Echo Procedure Summary Section (TID 5200-03)

This is a privately defined template to put all the observations, findings and comments entered for the cardiac study in the reporting screen. The following table describes the use of this template in the context of ClearVue 350/550/650/850 3.1.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	DT (121111, DCM, "Summary")	
2	>	CONTAINS	TEXT	EV (121106, DCM, "Comment")	This field contains all observations, findings and the comments entered in the reporting screen on the ClearVue 350/550/650/850 3.1. The format of the finding entry is "<FindingGroupName>space<FindingText>", where FindingGroupName is the Anatomy name and FindingText is the text description of the finding.

#### A.4.4 Echo Section (TID 5202)

This template is invoked multiple times by passing different section subjects as 'Finding Site' value. Use of the template TID 5202 in the context of ClearVue 350/550/650/850 3.1 is described in the following table.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	EV(121070, DCM, "Findings")	
2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3, SRT, "Finding Site")	Value passed in the parameter \$SectionSubject is given here.
3	>	CONTAINS	CONTAINER	DT (125007, DCM, "Measurement Group")	

4	>>	HAS CONCEPT MOD	CODE	EV(G-0373, SRT, "Image Mode")	The value is taken from BCID 12224.
5	>	CONTAINS	INCLUDE	DTID (5203) Echo Measurement	This template is invoked multiple times for all the measurements done on the \$SectionSubject. Refer to section A.4.5 for details of ClearVue 350/550/650/850 3.1 usage of this.

#### A.4.5 Echo Measurement (TID 5203)

Use of the template TID 5203 in the context of ClearVue 350/550/650/850 3.1 is described in the following table.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			INCLUDE	DTID (300) Measurement	
2	>>	HAS CONCEPT MOD	CODE	EV (G-C036, SRT, "Measurement Method")	This row is used only if the measurement or calculation this template is invoked with mandates it. Otherwise this row is not used. The values are taken from the BCID 12227.
3	>>	INFERRRED FROM	SCOORD	Spatial Coordinate Macro	This gives information on measurements coordinates on the referenced image. Coordinate information is given in the form of Graphic Data and Graphic Type.
4	>>>	SELECTED FROM	IMAGE	Image Reference Macro	It refers to the single frame image on which this measurement is done. SOP Class UID and SOP Instance UID of the corresponding image will be present.
5	>>	INFERRRED FROM	NUM	Referenced Content Item Identifier	This row is used only if the measurement or calculation this template is invoked with is of type MOD Volume measurements. In this case, reference to those twenty Left Ventricle MOD Diam entries, based on which this volume measurement is calculated is given here.
6	>>	HAS CONCEPT MOD	CODE	EV (121401, DCM, "Derivation")	If a user has performed more than one measurement then he / she can either use average (default) of these instances or he can specifically select one of the measured instance for using in calculations. If the selection is Average, then that average measurement instance will have a derivation modifier as (R-00317, SRT, "Mean").

No	NL	REL WITH PARENT	VT	Concept Name	Comments
7	>>	HAS PROPERTIES	CODE	EV (121404, DCM, "Selection Status")	This will have a value 'Mean Value Chosen' if the Derivation is 'Mean'. In all other cases, this will have a value, 'User Chosen Value'.
8	>	HAS CONCEPT MOD	CODE	EV (G-C048, SRT, "Flow Direction")	This row is used only if the measurement or calculation this template is invoked with mandates it. Otherwise this row is not used. The values are taken from the BCID 12221.
9	>	HAS CONCEPT MOD	CODE	EV (R-4089A, SRT, "Cardiac Cycle Point")	IFF \$Measurement = (99PMSBLUS, C12201-01, "Left Ventricle MOD Diam"). The values are taken from DCID 12233.
10	>	HAS CONCEPT MOD	CODE	EV (G-0373, SRT, "Image Mode")	This row is used only if the measurement or calculation this template is invoked with mandates it. Otherwise this row is not used. The values are taken from the BCID 12224.
11	>	HAS CONCEPT MOD	CODE	EV (111031, DCM, "Image View")	This row is used only if the measurement or calculation this template is invoked with mandates it. Otherwise this row is not used. The values are taken from the BCID 12226.
12	>	HAS CONCEPT MOD	TEXT	EV (99PMSBLUS, T5203-01, "Simpson's Disk Number") = value	IFF \$Measurement = (99PMSBLUS, C12201-01, "Left Ventricle MOD Diam"). The 'value' will be in the range, 1-20.

#### A.4.6 Hepatic Veins (T-48720)

This template is used for measurements of the Hepatic Veins. Use of the template T-48720 in the context of ClearVue 350/550/650/850 3.1 is described in the following table.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	EV (121070, DCM, "Findings")	
2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3, SRT, "Finding Site")	Value passed in the parameter \$SectionSubject is given here.
3	>	CONTAINS	CONTAINER	DT (125007, DCM, "Measurement Group")	
4	>>	HAS PROPERTIES	CODE	EV (121404, DCM, "Selection Status")	This will have a value 'Mean Value Chosen' if the Derivation is 'Mean'. In all other cases, this will have a value, 'User Chosen Value'.
5	>>	CONTAINS	CODE	EV (29471-0, LN, "Hepatic Vein Systolic Peak Velocity")	This value is taken from CID 12216.

6	>>	CONTAINS	CODE	EV (29474-4, LN, "Hepatic Vein Atrial Contraction Reversal Peak Velocity")	This value is taken from CID 12216.
7	>>	CONTAINS	CODE	EV (C12216-01, 99PMSBLUS, "Hepatic Vein A-Wave Duration")	This value is an extension to CID 12216.
8	>>	CONTAINS	CODE	EV (29472-8, LN, "Hepatic Vein Diastolic Peak Velocity")	This value is taken from CID 12216.
9	>>	CONTAINS	CODE	EV (29473-6, LN "Hepatic Vein Systolic to Diastolic Ratio")	This value is taken from CID 12216.

#### A.4.7 eDCS – Adult Echocardiography Template Support

The following list represents the Electronic DICOM Conformance Statement (eDCS) format for the Structured Report output for the Adult Echocardiography Procedure Report as supported on ClearVue 350/550/650/850 3.1.

This list is made up of ‘signatures’ that describe the group of codes used for each exported measurement and calculation result.

A ‘signature’ will contain the Label as displayed on the system user interface in the Calcs application and report pages, followed by the modifiers required by the DICOM SR Template and Structured Reporting SOP Class in order to include a given measurement or calculation value.

Some signatures will contain as few as two or as many as six modifiers.

In the table below, the following terms are used:

CSD	Coding Scheme Designator
CV	Code Value
CM	Code Meaning
Mod Type	Concept Modifier Type

“Mod Type” Field

App	Application or SR Template this measurement or calculation applies to
Site	The finding site as specified by the template
Concept	The code sequence as defined by the CSD
Mode	The imaging mode used for this value
Direction	Regurgitant or Antegrade flow
Method	Measurement or Calculation method used
Target	Location
View	Cardiac Imaging View

Following this list is a list of measurements that will not be exported.

##### A.4.7.1 eDCS Table

ClearVue 350/550/650/850 3.1 Report Label	MOD Type	CSD	CV	CM
A Wave Amp	concept	LN	59100-8	A Wave Amp
	mode	SRT	G-0394	M mode
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	cm	Centimeter
AI Acc Time	concept	LN	20168-1	Acceleration Time
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	sec	Seconds
AI Acc Time Slope	concept	LN	20167-3	Acceleration Slope
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
AI Alias Vel	concept	LN	59130-5	Alias Velocity
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	units	UCUM	cm/s	Centimeter Per Second
<b>AI Dec Slope</b>	concept	LN	20216-8	Deceleration Slope
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
<b>AI Dec Slope Time</b>	concept	LN	20217-6	Deceleration Time
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	sec	Seconds
<b>AI End Dias Vel</b>	concept	LN	11653-3	End Diastolic Velocity
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>AI ERO</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	direction	SRT	G-0367	Regurgitant Flow
	method	DCM	125216	Proximal Isovelocity Surface Area
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>AI Flow Rate</b>	concept	LN	34141-2	Peak Instantaneous Flow Rate
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	ml/sec	ml/sec
<b>AI Fraction</b>	concept	SRT	G-0390	Regurgitant Fraction
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	%	Percent
<b>AI Max PG</b>	concept	LN	20247-3	Peak Gradient
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>AI Mean PG</b>	concept	LN	20256-4	Mean Gradient
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>AI P1/2t</b>	concept	LN	20280-4	Pressure Half-Time
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	msec	Millisecond
<b>AI Radius</b>	concept	LN	59102-4	Flow Radius
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm	Centimeter
<b>AI Vmax</b>	concept	LN	20351-3	Peak Velocity

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>AI Vmean</b>	concept	LN	20352-1	Time Averaged Mean Velocity
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>AI Volume</b>	concept	LN	33878-0	Volume Flow
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	ml	Milliliter
<b>AI VTI</b>	concept	LN	20354-7	Velocity Time Integral
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm	Centimeter
<b>Ao Arch Diam</b>	concept	LN	18011-7	Aortic Arch Diameter
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-42000	Aorta
	units	UCUM	cm	Centimeter
<b>Ao Isthmus Diam</b>	concept	LN	18014-1	Aortic Isthmus Diameter
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-42000	Aorta
	units	UCUM	cm	Centimeter
<b>AoR Diam (2D)</b>	concept	LN	18015-8	Aortic Root Diameter
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-42000	Aorta
	units	UCUM	cm	Centimeter
<b>AoR Diam (MM)</b>	concept	LN	18015-8	Aortic Root Diameter
	mode	SRT	G-0394	M mode
	site	SNM3	T-42000	Aorta
	units	UCUM	cm	Centimeter
<b>Asc Ao Diam</b>	concept	LN	18012-5	Ascending Aortic Diameter
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-42000	Aorta
	units	UCUM	cm	Centimeter
<b>AV Acc Time</b>	concept	LN	20168-1	Acceleration Time
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	sec	Seconds
<b>AV Acc Time Slope</b>	concept	LN	20167-3	Acceleration Slope
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
<b>AV Area</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	method	DCM	125220	Planimetry
	mode	SRT	G-03A2	2D mode
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>AV Cusp Sep</b>	concept	LN	17996-0	Aortic Valve Cusp Separation
	mode	SRT	G-0394	M mode
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm	Centimeter
<b>AV Dec Time</b>	concept	LN	20217-6	Deceleration Time
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	sec	Seconds
<b>AV Max PG</b>	concept	LN	20247-3	Peak Gradient
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>AV Mean PG</b>	concept	LN	20256-4	Mean Gradient
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>AV R-R</b>	concept	LN	8867-4	Heart rate
	site	SRT	T-35400	Aortic Valve
	units	UCUM	{H.B}/min	Beats Per Minute
<b>AV Vmax</b>	concept	LN	20351-3	Peak Velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>AV Vmean</b>	concept	LN	20352-1	Time Averaged Mean Velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>AV VTI</b>	concept	LN	20354-7	Velocity Time Integral
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm	Centimeter
<b>AVA (Vmax)</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	method	DCM	125214	Continuity Equation by Peak Velocity
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>AVA (VTI)</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	method	DCM	125215	Continuity Equation by Velocity Time Integral
	site	SRT	T-35400	Aortic Valve

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	units	UCUM	cm2	Square Centimeter
<b>B-C Slope</b>	concept	99PMSBLU S	C12209-03	B-C Slope
	mode	SRT	G-0394	M mode
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>CI (2D-Cubed)</b>	concept	SRT	F-32110	Cardiac Index
	method	DCM	125206	Cube Method
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min/m2	l/min/m2
<b>CI (2D-Teich)</b>	concept	SRT	F-32110	Cardiac Index
	method	DCM	125209	Teichholz
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min/m2	l/min/m2
<b>CI (A/L)</b>	concept	SRT	F-32110	Cardiac Index
	method	DCM	125226	Single Plane Ellipse
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min/m2	l/min/m2
<b>CI (MM-Cubed)</b>	concept	SRT	F-32110	Cardiac Index
	method	DCM	125206	Cube Method
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min/m2	l/min/m2
<b>CI (MM-Teich)</b>	concept	SRT	F-32110	Cardiac Index
	method	DCM	125209	Teichholz
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min/m2	l/min/m2
<b>CI(MOD-bp)</b>	concept	SRT	F-32110	Cardiac Index
	method	DCM	125207	Method of Disks, Biplane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min/m2	l/min/m2
<b>CI(MOD-sp2)</b>	concept	SRT	F-32110	Cardiac Index
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min/m2	l/min/m2
	view	SRT	G-A19B	Apical two chamber
<b>CI(MOD-sp4)</b>	concept	SRT	F-32110	Cardiac Index

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min/m <sup>2</sup>	l/min/m <sup>2</sup>
	view	SRT	G-A19C	Apical four chamber
<b>CO (2D-Cubed)</b>	concept	SRT	F-32100	Cardiac Output
	method	DCM	125206	Cube Method
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min	Litre Per Minute
<b>CO (2D-Teich)</b>	concept	SRT	F-32100	Cardiac Output
	method	DCM	125209	Teichholz
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min	Litre Per Minute
<b>CO (A/L)</b>	concept	SRT	F-32100	Cardiac Output
	method	DCM	125226	Single Plane Ellipse
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min	Litre Per Minute
<b>CO (LVOT)</b>	concept	SRT	F-32100	Cardiac Output
	site	SNM3	T-32600	Left Ventricle
	target	SNM3	T-32650	Left Ventricle Outflow Tract
	units	UCUM	l/min	Litre Per Minute
<b>CO (MM-Cubed)</b>	concept	SRT	F-32100	Cardiac Output
	method	DCM	125206	Cube Method
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min	Litre Per Minute
<b>CO (MM-Teich)</b>	concept	SRT	F-32100	Cardiac Output
	method	DCM	125209	Teichholz
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min	Litre Per Minute
<b>CO (MV)</b>	concept	SRT	F-32100	Cardiac Output
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	l/min	Litre Per Minute
<b>CO (RVOT)</b>	concept	SRT	F-32100	Cardiac Output
	site	SRT	T-32500	Right Ventricle
	target	SNM3	T-32550	Right Ventricle Outflow Tract
	units	UCUM	l/min	Litre Per Minute
<b>CO (TV)</b>	concept	SRT	F-32100	Cardiac Output
	site	SRT	T-35100	Tricuspid Valve

ClearVue 350/550/650/850 3.1 Report Label	MOD Type	CSD	CV	CM
	units	UCUM	l/min	Litre Per Minute
<b>CO(MOD-bp)</b>	concept	SRT	F-32100	Cardiac Output
	method	DCM	125207	Method of Disks, Biplane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min	Litre Per Minute
<b>CO(MOD-sp2)</b>	concept	SRT	F-32100	Cardiac Output
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min	Litre Per Minute
	view	SRT	G-A19B	Apical two chamber
<b>CO(MOD-sp4)</b>	concept	SRT	F-32100	Cardiac Output
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	l/min	Litre Per Minute
	view	SRT	G-A19C	Apical four chamber
<b>Desc Ao Diam</b>	concept	LN	18013-3	Descending Aortic Diameter
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-42000	Aorta
	units	UCUM	cm	Centimeter
<b>E/Lat E`</b>	concept	SRT	G-037B	Ratio of MV Peak Velocity to LV Peak Tissue Velocity E-Wave
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0392	Lateral Mitral Annulus
	units	UCUM	1	no units
<b>E/Med E`</b>	concept	SRT	G-037B	Ratio of MV Peak Velocity to LV Peak Tissue Velocity E-Wave
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0391	Medial Mitral Annulus
	units	UCUM	1	no units
<b>E`/A` Lateral</b>	concept	LN	59129-7	Left Ventricle E to A Tissue Velocity Ratio
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0392	Lateral Mitral Annulus
	units	UCUM	1	no units
<b>E`/A` Medial</b>	concept	LN	59129-7	Left Ventricle E to A Tissue Velocity Ratio
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0391	Medial Mitral Annulus
	units	UCUM	1	no units
<b>EDV (2D-Cubed)</b>	concept	LN	18026-5	Left Ventricular End Diastolic Volume
	method	DCM	125206	Cube Method

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>EDV (2D-Teich)</b>	concept	LN	18026-5	Left Ventricular End Diastolic Volume
	method	DCM	125209	Teichholz
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>EDV (A/L)</b>	concept	LN	18026-5	Left Ventricular End Diastolic Volume
	method	DCM	125226	Single Plane Ellipse
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>EDV (MM-Cubed)</b>	concept	LN	18026-5	Left Ventricular End Diastolic Volume
	method	DCM	125206	Cube Method
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>EDV (MM-Teich)</b>	concept	LN	18026-5	Left Ventricular End Diastolic Volume
	method	DCM	125209	Teichholz
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>EDV(MOD-bp)</b>	concept	LN	18026-5	Left Ventricular End Diastolic Volume
	method	DCM	125207	Method of Disks, Biplane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>EDV(MOD-sp2)</b>	concept	LN	18026-5	Left Ventricular End Diastolic Volume
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm3	Cubic Centimeter
	view	SRT	G-A19B	Apical two chamber
<b>EDV(MOD-sp4)</b>	concept	LN	18026-5	Left Ventricular End Diastolic Volume
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm3	Cubic Centimeter
	view	SRT	G-A19C	Apical four chamber
<b>EF (2D-Cubed)</b>	concept	LN	18043-0	Left Ventricular Ejection Fraction
	method	DCM	125206	Cube Method
	mode	SRT	G-03A2	2D mode

ClearVue 350/550/650/850 3.1 Report Label	MOD Type	CSD	CV	CM
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>EF (2D-Teich)</b>	concept	LN	18043-0	Left Ventricular Ejection Fraction
	method	DCM	125209	Teichholz
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>EF (A/L)</b>	concept	LN	18043-0	Left Ventricular Ejection Fraction
	method	DCM	125226	Single Plane Ellipse
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>EF (Dumesnil)</b>	concept	99PMSBLU S	C3467-04	Left Ventricular Ejection Fraction by Dumesnil 1995
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>EF (MM-Cubed)</b>	concept	LN	18043-0	Left Ventricular Ejection Fraction
	method	DCM	125206	Cube Method
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>EF (MM-Teich)</b>	concept	LN	18043-0	Left Ventricular Ejection Fraction
	method	DCM	125209	Teichholz
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>EF(MOD-bp)</b>	concept	LN	18043-0	Left Ventricular Ejection Fraction
	method	DCM	125207	Method of Disks, Biplane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>EF(MOD-sp2)</b>	concept	LN	18043-0	Left Ventricular Ejection Fraction
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
	view	SRT	G-A19B	Apical two chamber
<b>EF(MOD-sp4)</b>	concept	LN	18043-0	Left Ventricular Ejection Fraction
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
	view	SRT	G-A19C	Apical four chamber

ClearVue 350/550/650/850 3.1 Report Label	MOD Type	CSD	CV	CM
<b>ESV (2D-Cubed)</b>	concept	LN	18148-7	Left Ventricular End Systolic Volume
	method	DCM	125206	Cube Method
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>ESV (2D-Teich)</b>	concept	LN	18148-7	Left Ventricular End Systolic Volume
	method	DCM	125209	Teichholz
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>ESV (A/L)</b>	concept	LN	18148-7	Left Ventricular End Systolic Volume
	method	DCM	125226	Single Plane Ellipse
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>ESV (MM-Cubed)</b>	concept	LN	18148-7	Left Ventricular End Systolic Volume
	method	DCM	125206	Cube Method
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>ESV (MM-Teich)</b>	concept	LN	18148-7	Left Ventricular End Systolic Volume
	method	DCM	125209	Teichholz
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>ESV(MOD-bp)</b>	concept	LN	18148-7	Left Ventricular End Systolic Volume
	method	DCM	125207	Method of Disks, Biplane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>ESV(MOD-sp2)</b>	concept	LN	18148-7	Left Ventricular End Systolic Volume
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm3	Cubic Centimeter
	view	SRT	G-A19B	Apical two chamber
<b>ESV(MOD-sp4)</b>	concept	LN	18148-7	Left Ventricular End Systolic Volume
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm3	Cubic Centimeter
	view	SRT	G-A19C	Apical four chamber
<b>FS (2D-Cubed)</b>	concept	LN	18051-3	Left Ventricular Fractional Shortening

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	method	DCM	125206	Cube Method
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>FS (2D-Teich)</b>	concept	LN	18051-3	Left Ventricular Fractional Shortening
	method	DCM	125209	Teichholz
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>FS (MM-Cubed)</b>	concept	LN	18051-3	Left Ventricular Fractional Shortening
	method	DCM	125206	Cube Method
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>FS (MM-Teich)</b>	concept	LN	18051-3	Left Ventricular Fractional Shortening
	method	DCM	125209	Teichholz
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>Hep. A Revs Dur Time</b>	concept	99PMSBLU S	C12216-01	Hepatic Vein A-Wave Duration
	site	SRT	T-48720	Hepatic Veins
	units	UCUM	sec	Seconds
<b>Hep. A Revs Vel</b>	concept	LN	29474-4	Hepatic Vein Atrial Contraction Reversal Peak Velocity
	site	SRT	T-48720	Hepatic Veins
	units	UCUM	cm/s	Centimeter Per Second
<b>Hepatic Dias Vel</b>	concept	LN	29472-8	Hepatic Vein Diastolic Peak Velocity
	site	SRT	T-48720	Hepatic Veins
	units	UCUM	cm/s	Centimeter Per Second
<b>Hepatic S/D</b>	concept	LN	29473-6	Hepatic Vein Systolic to Diastolic Ratio
	site	SRT	T-48720	Hepatic Veins
	units	UCUM	1	no units
<b>Hepatic Sys Vel</b>	concept	LN	29471-0	Hepatic Vein Systolic Peak Velocity
	site	SRT	T-48720	Hepatic Veins
	units	UCUM	cm/s	Centimeter Per Second
<b>HR LV</b>	concept	LN	8867-4	Heart rate
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	{H.B.}/min	Beats Per Minute
<b>HR LV</b>	concept	LN	8867-4	Heart rate
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	{H.B.}/min	Beats Per Minute

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
<b>IVC Diameter</b>	concept	LN	18006-7	Inferior Vena Cava Diameter
	mode	SRT	G-03A2	2D mode
	site	SRT	T-48600	Vena Cava
	units	UCUM	cm	Centimeter
<b>IVCT Time</b>	concept	SRT	G-037E	Left Ventricular Isovolumic Contraction Time
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	sec	Seconds
<b>IVRT Time</b>	concept	LN	18071-1	Left Ventricular Isovolumic Relaxation Time
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	sec	Seconds
<b>IVS % (2D)</b>	concept	LN	18054-7	Interventricular Septum % Thickening
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>IVS % (MM)</b>	concept	LN	18054-7	Interventricular Septum % Thickening
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>IVS/LVPW (2D)</b>	concept	LN	18155-2	Interventricular Septum to Posterior Wall Thickness Ratio
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	1	no units
<b>IVS/LVPW (MM)</b>	concept	LN	18155-2	Interventricular Septum to Posterior Wall Thickness Ratio
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	1	no units
<b>IVSd (2D)</b>	concept	LN	18154-5	Interventricular Septum Diastolic Thickness
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>IVSd (MM)</b>	concept	LN	18154-5	Interventricular Septum Diastolic Thickness
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>IVSs (2D)</b>	concept	LN	18158-6	Interventricular Septum Systolic Thickness
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>IVSs (MM)</b>	concept	LN	18158-6	Interventricular Septum Systolic Thickness
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>LA Dimen (2D)</b>	concept	LN	29469-4	Left Atrium Antero-posterior Systolic Dimension

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	mode	SRT	G-03A2	2D mode
	site	SRT	T-32300	Left Atrium
	units	UCUM	cm	Centimeter
<b>LA Dimen (MM)</b>	concept	LN	29469-4	Left Atrium Antero-posterior Systolic Dimension
	mode	SRT	G-0394	M mode
	site	SRT	T-32300	Left Atrium
	units	UCUM	cm	Centimeter
<b>LA/Ao (2D)</b>	concept	LN	17985-3	Left Atrium to Aortic Root Ratio
	mode	SRT	G-03A2	2D mode
	site	SRT	T-32300	Left Atrium
	units	UCUM	1	no units
<b>LA/Ao (MM)</b>	concept	LN	17985-3	Left Atrium to Aortic Root Ratio
	mode	SRT	G-0394	M mode
	site	SRT	T-32300	Left Atrium
	units	UCUM	1	no units
<b>Lat A` Area VTI</b>	concept	LN	59125-5	LV VTI A wave US
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0392	Lateral Mitral Annulus
	units	UCUM	cm	Centimeter
<b>Lat A` Vel</b>	concept	SRT	G-037C	LV Peak Diastolic Tissue Velocity During Atrial Systole
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0392	Lateral Mitral Annulus
	units	UCUM	cm/s	Centimeter Per Second
<b>Lat Acc Time</b>	concept	LN	20168-1	Acceleration Time
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0392	Lateral Mitral Annulus
	units	UCUM	sec	Seconds
<b>Lat Dec Time</b>	concept	LN	20217-6	Deceleration Time
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0392	Lateral Mitral Annulus
	units	UCUM	sec	Seconds
<b>Lat E` Area VTI</b>	concept	LN	59124-8	LV VTI E wave US
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0392	Lateral Mitral Annulus
	units	UCUM	cm	Centimeter
<b>Lat E` Vel</b>	concept	SRT	G-037A	Left Ventricular Peak Early Diastolic Tissue Velocity
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	target	SRT	G-0392	Lateral Mitral Annulus
	units	UCUM	cm/s	Centimeter Per Second
<b>Lat IVCT Time</b>	concept	SRT	G-037E	Left Ventricular Isovolumic Contraction Time
	mode	99PMSBLU S	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0392	Lateral Mitral Annulus
	units	UCUM	sec	Seconds
<b>Lat IVRT Time</b>	concept	LN	18071-1	Left Ventricular Isovolumic Relaxation Time
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0392	Lateral Mitral Annulus
	units	UCUM	sec	Seconds
<b>Lat S Vel</b>	concept	SRT	G-037D	Left Ventricular Peak Systolic Tissue Velocity
	mode	99PMSBLU S	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0392	Lateral Mitral Annulus
	units	UCUM	cm/s	Centimeter Per Second
<b>Late Dias Slope</b>	concept	99PMSBLU S	C12209-01	Late Diastolic Slope
	mode	SRT	G-0394	M mode
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>LPA Diam</b>	concept	LN	18019-0	Left Pulmonary Artery Diameter
	mode	SRT	G-03A2	2D mode
	site	SRT	T-44000	Pulmonary artery
	units	UCUM	cm	Centimeter
<b>LV Dp/dt</b>	concept	LN	18035-6	Mitral Regurgitation dP/dt derived from Mitral Reg velocity
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	mm[Hg]/s	mmHg/s
<b>LV EDA</b>	concept	SRT	G-0375	Left Ventricular Diastolic Area
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>LV ESA</b>	concept	SRT	G-0374	Left Ventricular Systolic Area
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>LV ET Time</b>	concept	LN	20222-6	Ejection Time
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	sec	Seconds
<b>LV FAC</b>	concept	SRT	G-0376	Left Ventricular Fractional Area Change

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	mode	SRT	G-03A2	2D mode
	site	SRT	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>LV Mass (A/L)</b>	concept	LN	18087-7	Left Ventricle Mass
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	g	Gram
<b>LV Mass (Cubed)</b>	concept	LN	18087-7	Left Ventricle Mass
	method	DCM	125206	Cube Method
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	g	Gram
<b>LV Mass Index (A/L)</b>	concept	99PMSBLU S	C12203-01	Left Ventricle Mass Index
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	g/m <sup>2</sup>	g/m <sup>2</sup>
<b>LV Mass Index(Cubed)</b>	concept	99PMSBLU S	C12203-01	Left Ventricle Mass Index
	method	DCM	125206	Cube Method
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	g/m <sup>2</sup>	g/m <sup>2</sup>
<b>LV PEP Time</b>	concept	LN	59085-1	Pre-Ejection Period
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	sec	Seconds
<b>LV PEP/ET</b>	concept	99PMSBLU S	C12203-04	PEP/ET
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	1	no units
<b>LV R-R</b>	concept	LN	8867-4	Heart rate
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	{H.B.}/min	Beats Per Minute
<b>LVAd (A/L)</b>	concept	SRT	G-0375	Left Ventricular Diastolic Area
	method	DCM	125226	Single Plane Ellipse
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>LVAd ap2</b>	concept	SRT	G-0375	Left Ventricular Diastolic Area
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm <sup>2</sup>	Square Centimeter

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	view	SRT	G-A19B	Apical two chamber
<b>LVAd ap4</b>	concept	SRT	G-0375	Left Ventricular Diastolic Area
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm <sup>2</sup>	Square Centimeter
	view	SRT	G-A19C	Apical four chamber
<b>LVAd Sax Endo Area</b>	concept	SRT	G-0375	Left Ventricular Diastolic Area
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm <sup>2</sup>	Square Centimeter
	view	SRT	G-039B	Parasternal short axis at the Papillary Muscle level
<b>LVAd Sax Epi Area</b>	concept	SRT	G-0379	Left Ventricle Epicardial Diastolic Area, psax pap view
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm <sup>2</sup>	Square Centimeter
	view	SRT	G-039B	Parasternal short axis at the Papillary Muscle level
<b>LVAs (A/L)</b>	concept	SRT	G-0374	Left Ventricular Systolic Area
	method	DCM	125226	Single Plane Ellipse
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>LVAs ap2</b>	concept	SRT	G-0374	Left Ventricular Systolic Area
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm <sup>2</sup>	Square Centimeter
	view	SRT	G-A19B	Apical two chamber
<b>LVAs ap4</b>	concept	SRT	G-0374	Left Ventricular Systolic Area
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm <sup>2</sup>	Square Centimeter
	view	SRT	G-A19C	Apical four chamber
<b>LVIDd (2D)</b>	concept	LN	29436-3	Left Ventricle Internal End Diastolic Dimension
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>LVIDd (MM)</b>	concept	LN	29436-3	Left Ventricle Internal End Diastolic Dimension
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>LVIDs (2D)</b>	concept	LN	29438-9	Left Ventricle Internal Systolic Dimension

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>LVIDs (MM)</b>	concept	LN	29438-9	Left Ventricle Internal Systolic Dimension
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>LVLd (A/L)</b>	concept	LN	18077-8	Left Ventricle diastolic major axis
	method	DCM	125226	Single Plane Ellipse
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>LVLd Apical</b>	concept	LN	18077-8	Left Ventricle diastolic major axis
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>LVLs (A/L)</b>	concept	LN	18076-0	Left Ventricle systolic major axis
	method	DCM	125226	Single Plane Ellipse
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>LVOT Acc Time</b>	concept	LN	20168-1	Acceleration Time
	site	SNM3	T-32600	Left Ventricle
	target	SNM3	T-32650	Left Ventricle Outflow Tract
	units	UCUM	sec	Seconds
<b>LVOT Acc Time Slope</b>	concept	LN	20167-3	Acceleration Slope
	site	SNM3	T-32600	Left Ventricle
	target	SNM3	T-32650	Left Ventricle Outflow Tract
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
<b>LVOT Area</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	target	SNM3	T-32650	Left Ventricle Outflow Tract
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>LVOT Diam</b>	concept	SRT	G-038F	Cardiovascular Orifice Diameter
	site	SNM3	T-32600	Left Ventricle
	target	SNM3	T-32650	Left Ventricle Outflow Tract
	units	UCUM	cm	Centimeter
<b>LVOT Max PG</b>	concept	LN	20247-3	Peak Gradient
	site	SNM3	T-32600	Left Ventricle
	target	SNM3	T-32650	Left Ventricle Outflow Tract
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>LVOT Mean PG</b>	concept	LN	20256-4	Mean Gradient

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	site	SNM3	T-32600	Left Ventricle
	target	SNM3	T-32650	Left Ventricle Outflow Tract
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>LVOT Vmax</b>	concept	LN	20351-3	Peak Velocity
	site	SNM3	T-32600	Left Ventricle
	target	SNM3	T-32650	Left Ventricle Outflow Tract
	units	UCUM	cm/s	Centimeter Per Second
<b>LVOT Vmean</b>	concept	LN	20352-1	Time Averaged Mean Velocity
	site	SNM3	T-32600	Left Ventricle
	target	SNM3	T-32650	Left Ventricle Outflow Tract
	units	UCUM	cm/s	Centimeter Per Second
<b>LVOT VTI</b>	concept	LN	20354-7	Velocity Time Integral
	site	SNM3	T-32600	Left Ventricle
	target	SNM3	T-32650	Left Ventricle Outflow Tract
	units	UCUM	cm	Centimeter
<b>LVPW % (2D)</b>	concept	LN	18053-9	Left Ventricle Posterior Wall % Thickening
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>LVPW % (MM)</b>	concept	LN	18053-9	Left Ventricle Posterior Wall % Thickening
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	%	Percent
<b>LVPWd (2D)</b>	concept	LN	18152-9	Left Ventricle Posterior Wall Diastolic Thickness
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>LVPWd (MM)</b>	concept	LN	18152-9	Left Ventricle Posterior Wall Diastolic Thickness
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>LVPWs (2D)</b>	concept	LN	18156-0	Left Ventricle Posterior Wall Systolic Thickness
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>LVPWs (MM)</b>	concept	LN	18156-0	Left Ventricle Posterior Wall Systolic Thickness
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	cm	Centimeter
<b>Med A' Area VTI</b>	concept	LN	59125-5	LV VTI A wave US
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0391	Medial Mitral Annulus

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	units	UCUM	cm	Centimeter
<b>Med A` Vel</b>	concept	SRT	G-037C	LV Peak Diastolic Tissue Velocity During Atrial Systole
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0391	Medial Mitral Annulus
	units	UCUM	cm/s	Centimeter Per Second
<b>Med Acc Time</b>	concept	LN	20168-1	Acceleration Time
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0391	Medial Mitral Annulus
	units	UCUM	sec	Seconds
<b>Med Dec Time</b>	concept	LN	20217-6	Deceleration Time
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0391	Medial Mitral Annulus
	units	UCUM	sec	Seconds
<b>Med E` Area VTI</b>	concept	LN	59124-8	Area under LV E Tissue Velocity
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0391	Medial Mitral Annulus
	units	UCUM	cm	Centimeter
<b>Med E` Vel</b>	concept	SRT	G-037A	Left Ventricular Peak Early Diastolic Tissue Velocity
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0391	Medial Mitral Annulus
	units	UCUM	cm/s	Centimeter Per Second
<b>Med IVCT Time</b>	concept	SRT	G-037E	Left Ventricular Isovolumic Contraction Time
	mode	99PMSBLU S	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0391	Medial Mitral Annulus
	units	UCUM	sec	Seconds
<b>Med IVRT Time</b>	concept	LN	18071-1	Left Ventricular Isovolumic Relaxation Time
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0391	Medial Mitral Annulus
	units	UCUM	sec	Seconds
<b>Med S Vel</b>	concept	SRT	G-037D	Left Ventricular Peak Systolic Tissue Velocity
	mode	99PMSBLU S	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0391	Medial Mitral Annulus
	units	UCUM	cm/s	Centimeter Per Second
<b>MPA Diam</b>	concept	LN	18020-8	Main Pulmonary Artery Diameter

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	mode	SRT	G-03A2	2D mode
	site	SRT	T-44000	Pulmonary artery
	units	UCUM	cm	Centimeter
<b>MR Alias Vel</b>	concept	LN	59130-5	Alias Velocity
	direction	SRT	G-0367	Regurgitant Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>MR ERO</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	direction	SRT	G-0367	Regurgitant Flow
	method	DCM	125216	Proximal Isovelocity Surface Area
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>MR Flow Rate</b>	concept	LN	34141-2	Peak Instantaneous Flow Rate
	direction	SRT	G-0367	Regurgitant Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	ml/sec	ml/sec
<b>MR Fraction</b>	concept	SRT	G-0390	Regurgitant Fraction
	direction	SRT	G-0367	Regurgitant Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	%	Percent
<b>MR Max PG</b>	concept	LN	20247-3	Peak Gradient
	direction	SRT	G-0367	Regurgitant Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>MR Mean PG</b>	concept	LN	20256-4	Mean Gradient
	direction	SRT	G-0367	Regurgitant Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>MR Radius</b>	concept	LN	59102-4	Flow Radius
	direction	SRT	G-0367	Regurgitant Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm	Centimeter
<b>MR Vmax</b>	concept	LN	20351-3	Peak Velocity
	direction	SRT	G-0367	Regurgitant Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>MR Vmean</b>	concept	LN	20352-1	Time Averaged Mean Velocity
	direction	SRT	G-0367	Regurgitant Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>MR Volume</b>	concept	LN	33878-0	Volume Flow
	direction	SRT	G-0367	Regurgitant Flow
	method	DCM	125216	Proximal Isovelocity Surface Area

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	ml	Milliliter
<b>MR VTI</b>	concept	LN	20354-7	Velocity Time Integral
	direction	SRT	G-0367	Regurgitant Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm	Centimeter
<b>MV A Dur Time</b>	concept	SRT	G-0385	Mitral Valve A-Wave Duration
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	sec	Seconds
<b>MV A-C Interval Time</b>	concept	99PMSBLU S	C12207-04	Mitral Valve A-C Interval
	mode	SRT	G-0394	M mode
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	sec	Seconds
<b>MV Acc Time</b>	concept	LN	20168-1	Acceleration Time
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	sec	Seconds
<b>MV Acc Time Slope</b>	concept	LN	20167-3	Acceleration Slope
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
<b>MV Alias Vel</b>	concept	LN	59130-5	Alias Velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>MV Area (Planim)</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	method	DCM	125220	Planimetry
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>MV D-E Exc Dist</b>	concept	99PMSBLU S	C12207-01	Mitral Valve D-E Excursion
	mode	SRT	G-0394	M mode
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm	Centimeter
<b>MV D-E Slope</b>	concept	99PMSBLU S	C12207-02	Mitral Valve D-E Slope
	mode	SRT	G-0394	M mode
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>MV Dec Slope</b>	concept	LN	20216-8	Deceleration Slope
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	units	UCUM	cm/s2	Centimeter Per Second Square
<b>MV Dec Time</b>	concept	LN	20217-6	Deceleration Time
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	sec	Seconds
<b>MV Diam</b>	concept	SRT	G-038F	Cardiovascular Orifice Diameter
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm	Centimeter
<b>MV E/A</b>	concept	LN	18038-0	Mitral Valve E to A Ratio
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	1	no units
<b>MV E-E Sep</b>	concept	99PMSBLU S	C12207-03	Mitral Valve E-E Separation
	mode	SRT	G-0394	M mode
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm	Centimeter
<b>MV E-F Slope</b>	concept	LN	18040-6	Mitral Valve E-F Slope by M-Mode
	mode	SRT	G-0394	M mode
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>MV EPSS</b>	concept	LN	18036-4	Mitral Valve EPSS, E wave
	mode	SRT	G-0394	M mode
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm	Centimeter
<b>MV Max PG</b>	concept	LN	20247-3	Peak Gradient
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>MV Mean PG</b>	concept	LN	20256-4	Mean Gradient
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>MV P1/2t</b>	concept	LN	20280-4	Pressure Half-Time
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	msec	Millisecond
<b>MV P1/2t Vmax</b>	concept	99PMSBLU S	C12222-03	Pressure Half-Time Peak velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>MV Peak A Vel</b>	concept	LN	17978-8	Mitral Valve A-Wave Peak Velocity
	direction	SRT	R-42047	Antegrade Flow

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>MV Peak E Vel</b>	concept	LN	18037-2	Mitral Valve E-Wave Peak Velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>MV Radius</b>	concept	LN	59102-4	Flow Radius
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm	Centimeter
<b>MV R-R</b>	concept	LN	8867-4	Heart rate
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	{H.B.}/min	Beats Per Minute
<b>MV Vmax</b>	concept	LN	20351-3	Peak Velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>MV Vmean</b>	concept	LN	20352-1	Time Averaged Mean Velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>MV VTI</b>	concept	LN	20354-7	Velocity Time Integral
	direction	SRT	R-42047	Antegrade Flow
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm	Centimeter
<b>MVA (P1/2t)</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	method	DCM	125210	Area by Pressure Half-Time
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>MVA (PISA)</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	method	DCM	125216	Proximal Isovelocity Surface Area
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>MVA (VTI)</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	method	DCM	125215	Continuity Equation by Velocity Time Integral
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>PI End Dias PG</b>	concept	LN	20247-3	Peak Gradient
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>PI End Dias Vel</b>	concept	LN	11653-3	End Diastolic Velocity
	direction	SRT	G-0367	Regurgitant Flow

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>PISA (AI)</b>	concept	99PMSBLU S	C12211-01	Aortic Valve Flow Area
	direction	SRT	G-0367	Regurgitant Flow
	method	DCM	125216	Proximal Isovelocity Surface Area
	site	SRT	T-35400	Aortic Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>PISA (MR)</b>	concept	99PMSBLU S	C12207-06	Mitral Valve Flow Area
	direction	SRT	G-0367	Regurgitant Flow
	method	DCM	125216	Proximal Isovelocity Surface Area
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>PISA (TR)</b>	concept	99PMSBLU S	C12208-05	Tricuspid Valve Flow Area
	direction	SRT	G-0367	Regurgitant Flow
	method	DCM	125216	Proximal Isovelocity Surface Area
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>Pulm A Revs Dur Time</b>	concept	SRT	G-038B	Pulmonary Vein A-Wave Duration
	site	SRT	T-48581	Pulmonary Venous Structure
	units	UCUM	sec	Seconds
<b>Pulm A Revs Vel</b>	concept	LN	29453-8	Pulmonary Vein Atrial Contraction Reversal Peak Velocity
	site	SRT	T-48581	Pulmonary Venous Structure
	units	UCUM	cm/s	Centimeter Per Second
<b>Pulm Dias Vel</b>	concept	LN	29451-2	Pulmonary Vein Diastolic Peak Velocity
	site	SRT	T-48581	Pulmonary Venous Structure
	units	UCUM	cm/s	Centimeter Per Second
<b>Pulm S/D</b>	concept	LN	29452-0	Pulmonary Vein Systolic to Diastolic Ratio
	site	SRT	T-48581	Pulmonary Venous Structure
	units	UCUM	1	no units
<b>Pulm Sys Vel</b>	concept	LN	29450-4	Pulmonary Vein Systolic Peak Velocity
	site	SRT	T-48581	Pulmonary Venous Structure
	units	UCUM	cm/s	Centimeter Per Second
<b>PV Acc Time</b>	concept	LN	20168-1	Acceleration Time
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	sec	Seconds
<b>PV Acc Time Slope</b>	concept	LN	20167-3	Acceleration Slope
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
<b>PV Max PG</b>	concept	LN	20247-3	Peak Gradient

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>PV Mean PG</b>	concept	LN	20256-4	Mean Gradient
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>PV R-R</b>	concept	LN	8867-4	Heart rate
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	{H.B.}/min	Beats Per Minute
<b>PV Vmax</b>	concept	LN	20351-3	Peak Velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>PV Vmean</b>	concept	LN	20352-1	Time Averaged Mean Velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>PV VTI</b>	concept	LN	20354-7	Velocity Time Integral
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	cm	Centimeter
<b>PVA (Vmax)</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	method	DCM	125214	Continuity Equation by Peak Velocity
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>PVA (VTI)</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	method	DCM	125215	Continuity Equation by Velocity Time Integral
	site	SRT	T-35200	Pulmonic Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>Qp/Qs</b>	concept	LN	29462-9	Pulmonary-to-Systemic Shunt Flow Ratio
	site	SRT	P5-30031	Cardiac Shunt Study
	units	UCUM	1	no units
<b>R to AV Closure</b>	concept	99PMSBLU S	C12211-07	R Wave to Aortic Valve Closure Time
	site	SRT	T-35400	Aortic Valve
	units	UCUM	msec	Millisecond
<b>R to AV Open</b>	concept	99PMSBLU S	C12211-06	R Wave to Aortic Valve Opening Time
	site	SRT	T-35400	Aortic Valve
	units	UCUM	msec	Millisecond
<b>R to MV Closure</b>	concept	99PMSBLU S	C12207-42	R Wave to Mitral Valve Closure Time
	site	SNM3	T-35300	Mitral Valve

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	units	UCUM	msec	Millisecond
<b>R to MV Open</b>	concept	99PMSBLU S	C12207-41	R Wave to Mitral Valve Opening Time
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	msec	Millisecond
<b>RA Pressure</b>	concept	LN	18070-3	Right Atrium Systolic Pressure
	site	SRT	T-32200	Right Atrium
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>RPA Diam</b>	concept	LN	18021-6	Right Pulmonary Artery Diameter
	mode	SRT	G-03A2	2D mode
	site	SRT	T-44000	Pulmonary artery
	units	UCUM	cm	Centimeter
<b>RV EDA</b>	concept	99PMSBLU S	C12204-01	Right Ventricular Diastolic Area
	mode	SRT	G-03A2	2D mode
	site	SRT	T-32500	Right Ventricle
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>RV ET Time</b>	concept	LN	20222-6	Ejection Time
	mode	SRT	G-0394	M mode
	site	SRT	T-32500	Right Ventricle
	units	UCUM	sec	Seconds
<b>RV/LV</b>	concept	99PMSBLU S	C12204-04	Right and Left Ventricular End Diastolic Diameter Ratio
	mode	SRT	G-03A2	2D mode
	site	SRT	T-32500	Right Ventricle
	units	UCUM	1	no units
<b>RV ESA</b>	concept	99PMSBLU S	C12204-02	Right Ventricular Systolic Area
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32500	Right Ventricle
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>RV FAC</b>	concept	99PMSBLU S	C12204-03	Right Ventricular Fractional Area Change
	mode	SRT	G-03A2	2D mode
	site	SRT	T-32500	Right Ventricle
	units	UCUM	%	Percent
<b>RV PEP Time</b>	concept	LN	59085-1	Pre-Ejection Period
	mode	SRT	G-0394	M mode
	site	SRT	T-32500	Right Ventricle
	units	UCUM	sec	Seconds
<b>RV PEP/ET</b>	concept	99PMSBLU S	C12203-04	PEP/ET
	site	SRT	T-32500	Right Ventricle
	units	UCUM	1	no units
<b>RVAWd (2D)</b>	concept	LN	18153-7	Right Ventricular Anterior Wall Diastolic Thickness
	mode	SRT	G-03A2	2D mode

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	site	SRT	T-32500	Right Ventricle
	units	UCUM	cm	Centimeter
<b>RVAWd (MM)</b>	concept	LN	18153-7	Right Ventricular Anterior Wall Diastolic Thickness
	mode	SRT	G-0394	M mode
	site	SRT	T-32500	Right Ventricle
	units	UCUM	cm	Centimeter
<b>RVIDd (2D)</b>	concept	LN	20304-2	Right Ventricular Internal Diastolic Dimension
	mode	SRT	G-03A2	2D mode
	site	SRT	T-32500	Right Ventricle
	units	UCUM	cm	Centimeter
<b>RVIDd (MM)</b>	concept	LN	20304-2	Right Ventricular Internal Diastolic Dimension
	mode	SRT	G-0394	M mode
	site	SRT	T-32500	Right Ventricle
	units	UCUM	cm	Centimeter
<b>RVOT Area</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	mode	SRT	G-03A2	2D mode
	site	SRT	T-32500	Right Ventricle
	target	SNM3	T-32550	Right Ventricle Outflow Tract
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>RVOT Diam</b>	concept	SRT	G-038F	Cardiovascular Orifice Diameter
	mode	SRT	G-03A2	2D mode
	site	SRT	T-32500	Right Ventricle
	target	SNM3	T-32550	Right Ventricle Outflow Tract
	units	UCUM	cm	Centimeter
<b>RVOT Max PG</b>	concept	LN	20247-3	Peak Gradient
	site	SRT	T-32500	Right Ventricle
	target	SNM3	T-32550	Right Ventricle Outflow Tract
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>RVOT Mean PG</b>	concept	LN	20256-4	Mean Gradient
	site	SRT	T-32500	Right Ventricle
	target	SNM3	T-32550	Right Ventricle Outflow Tract
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>RVOT Vmax</b>	concept	LN	20351-3	Peak Velocity
	site	SRT	T-32500	Right Ventricle
	target	SNM3	T-32550	Right Ventricle Outflow Tract
	units	UCUM	cm/s	Centimeter Per Second
<b>RVOT Vmean</b>	concept	LN	20352-1	Time Averaged Mean Velocity
	site	SRT	T-32500	Right Ventricle
	target	SNM3	T-32550	Right Ventricle Outflow Tract
	units	UCUM	cm/s	Centimeter Per Second
<b>RVOT VTI</b>	concept	LN	20354-7	Velocity Time Integral
	site	SRT	T-32500	Right Ventricle
	target	SNM3	T-32550	Right Ventricle Outflow Tract

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	units	UCUM	cm	Centimeter
<b>RVSP</b>	concept	SRT	G-0380	Right Ventricular Peak Systolic Pressure
	site	SRT	T-32500	Right Ventricle
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>SI (2D-Cubed)</b>	concept	SRT	F-00078	Stroke Index
	method	DCM	125206	Cube Method
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml/m2	ml/m2
<b>SI (2D-Teich)</b>	concept	SRT	F-00078	Stroke Index
	method	DCM	125209	Teichholz
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml/m2	ml/m2
<b>SI (A/L)</b>	concept	SRT	F-00078	Stroke Index
	method	DCM	125226	Single Plane Ellipse
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml/m2	ml/m2
<b>SI (MM-Cubed)</b>	concept	SRT	F-00078	Stroke Index
	method	DCM	125206	Cube Method
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml/m2	ml/m2
<b>SI (MM-Teich)</b>	concept	SRT	F-00078	Stroke Index
	method	DCM	125209	Teichholz
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml/m2	ml/m2
<b>SI(MOD-bp)</b>	concept	SRT	F-00078	Stroke Index
	method	DCM	125207	Method of Disks, Biplane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml/m2	ml/m2
<b>SI(MOD-sp2)</b>	concept	SRT	F-00078	Stroke Index
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml/m2	ml/m2
	view	SRT	G-A19B	Apical two chamber
<b>SI(MOD-sp4)</b>	concept	SRT	F-00078	Stroke Index
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml/m2	ml/m2
	view	SRT	G-A19C	Apical four chamber
<b>SV (2D-Cubed)</b>	concept	SRT	F-32120	Stroke Volume
	method	DCM	125206	Cube Method
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>SV (2D-Teich)</b>	concept	SRT	F-32120	Stroke Volume
	method	DCM	125209	Teichholz
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>SV (A/L)</b>	concept	SRT	F-32120	Stroke Volume
	method	DCM	125226	Single Plane Ellipse
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>SV (LVOT)</b>	concept	SRT	F-32120	Stroke Volume
	site	SNM3	T-32600	Left Ventricle
	target	SNM3	T-32650	Left Ventricle Outflow Tract
	units	UCUM	ml	Milliliter
<b>SV (MM-Cubed)</b>	concept	SRT	F-32120	Stroke Volume
	method	DCM	125206	Cube Method
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>SV (MM-Teich)</b>	concept	SRT	F-32120	Stroke Volume
	method	DCM	125209	Teichholz
	mode	SRT	G-0394	M mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>SV (MV)</b>	concept	SRT	F-32120	Stroke Volume
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	ml	Milliliter
<b>SV (RVOT)</b>	concept	SRT	F-32120	Stroke Volume
	site	SRT	T-32500	Right Ventricle
	target	SNM3	T-32550	Right Ventricle Outflow Tract
	units	UCUM	ml	Milliliter
<b>SV (TV)</b>	concept	SRT	F-32120	Stroke Volume
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	ml	Milliliter
<b>SV(MOD-bp)</b>	concept	SRT	F-32120	Stroke Volume

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	method	DCM	125207	Method of Disks, Biplane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
<b>SV(MOD-sp2)</b>	concept	SRT	F-32120	Stroke Volume
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
	view	SRT	G-A19B	Apical two chamber
<b>SV(MOD-sp4)</b>	concept	SRT	F-32120	Stroke Volume
	method	DCM	125208	Method of Disks, Single Plane
	mode	SRT	G-03A2	2D mode
	site	SNM3	T-32600	Left Ventricle
	units	UCUM	ml	Milliliter
	view	SRT	G-A19C	Apical four chamber
<b>Tei Index</b>	concept	99PMSBLU S	C12207-05	Tei Index
	site	SNM3	T-35300	Mitral Valve
	units	UCUM	1	no units
<b>Time to Lat E`</b>	concept	LN	59096-8	Time to Left Ventricle E Tissue Velocity
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0392	Lateral Mitral Annulus
	units	UCUM	sec	Seconds
<b>Time to Lat S</b>	concept	LN	59095-0	Time to Left Ventricle S Tissue Velocity
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0392	Lateral Mitral Annulus
	units	UCUM	sec	Seconds
<b>Time to Med E`</b>	concept	LN	59096-8	Time to Left Ventricle E Tissue Velocity
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0391	Medial Mitral Annulus
	units	UCUM	sec	Seconds
<b>Time to Med S</b>	concept	LN	59095-0	Time to Left Ventricle S Tissue Velocity
	mode	SRT	P5-B0128	Tissue Doppler Imaging
	site	SNM3	T-32600	Left Ventricle
	target	SRT	G-0391	Medial Mitral Annulus
	units	UCUM	sec	Seconds
<b>TR Alias Vel</b>	concept	LN	59130-5	Alias Velocity
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35100	Tricuspid Valve

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	units	UCUM	cm/s	Centimeter Per Second
<b>TR ERO</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	direction	SRT	G-0367	Regurgitant Flow
	method	DCM	125216	Proximal Isovelocity Surface Area
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>TR Flow Rate</b>	concept	LN	34141-2	Peak Instantaneous Flow Rate
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	ml/sec	ml/sec
<b>TR Fraction</b>	concept	SRT	G-0390	Regurgitant Fraction
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	%	Percent
<b>TR Max PG</b>	concept	LN	20247-3	Peak Gradient
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>TR Mean PG</b>	concept	LN	20256-4	Mean Gradient
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>TR Radius</b>	concept	LN	59102-4	Flow Radius
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm	Centimeter
<b>TR Vmax</b>	concept	LN	20351-3	Peak Velocity
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>TR Vmean</b>	concept	LN	20352-1	Time Averaged Mean Velocity
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>TR Volume</b>	concept	LN	33878-0	Volume Flow
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	ml	Milliliter
<b>TR VTI</b>	concept	LN	20354-7	Velocity Time Integral
	direction	SRT	G-0367	Regurgitant Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm	Centimeter
<b>TV A-C Interval Time</b>	concept	99PMSBLU	C12208-04	Tricuspid Valve A-C Interval

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
		S		
	mode	SRT	G-0394	M mode
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	sec	Seconds
<b>TV Acc Time</b>	concept	LN	20168-1	Acceleration Time
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	sec	Seconds
<b>TV Acc Time Slope</b>	concept	LN	20167-3	Acceleration Slope
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
<b>TV Alias Vel</b>	concept	LN	59130-5	Alias Velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>TV Area</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	mode	SRT	G-03A2	2D mode
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter
<b>TV D-E Exc Dist</b>	concept	99PMSBLU S	C12208-01	Tricuspid Valve D-E Excursion
	mode	SRT	G-0394	M mode
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm	Centimeter
<b>TV D-E Slope</b>	concept	99PMSBLU S	C12208-02	Tricuspid Valve D-E Slope
	mode	SRT	G-0394	M mode
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>TV Diam</b>	concept	SRT	G-038F	Cardiovascular Orifice Diameter
	mode	SRT	G-03A2	2D mode
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm	Centimeter
<b>TV E/A</b>	concept	LN	18039-8	Tricuspid Valve E to A Ratio
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	1	no units
<b>TV E-F Slope</b>	concept	99PMSBLU S	C12208-03	Tricuspid Valve E-F Slope
	mode	SRT	G-0394	M mode
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>TV Max PG</b>	concept	LN	20247-3	Peak Gradient
	direction	SRT	R-42047	Antegrade Flow

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>MOD Type</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>TV Mean PG</b>	concept	LN	20256-4	Mean Gradient
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	mm[Hg]	Millimeters Of Mercury
<b>TV Peak A Vel</b>	concept	LN	18030-7	Tricuspid Valve A Wave Peak Velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>TV Peak E Vel</b>	concept	LN	18031-5	Tricuspid Valve E Wave Peak Velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>TV Radius</b>	concept	LN	59102-4	Flow Radius
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm	Centimeter
<b>TV R-R</b>	concept	LN	8867-4	Heart rate
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	{H.B.}/min	Beats Per Minute
<b>TV Vmax</b>	concept	LN	20351-3	Peak Velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>TV Vmean</b>	concept	LN	20352-1	Time Averaged Mean Velocity
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm/s	Centimeter Per Second
<b>TV VTI</b>	concept	LN	20354-7	Velocity Time Integral
	direction	SRT	R-42047	Antegrade Flow
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm	Centimeter
<b>TVA (PISA)</b>	concept	SRT	G-038E	Cardiovascular Orifice Area
	method	DCM	125216	Proximal Isovelocity Surface Area
	site	SRT	T-35100	Tricuspid Valve
	units	UCUM	cm <sup>2</sup>	Square Centimeter

#### A.4.8 Cardiac (Adult Echo) Meas/Calcs NOT exported in Dicom

The following labels are not exported in DICOM Structured Reports for Adult Echo.

ClearVue 350/550/650/850 3.1 Label
AI AT Max PG
AI AT Vmax
AI DS Max PG
AI DS P1/2t
AI DS Vmax
AI End Dias PG
AI P1/2t Max PG
AI P1/2t Slope
AI P1/2t Time
AI P1/2t Vmax
Ao Arch Area
Ao Isthmus Area
AoR Area
Asc Ao Area
AV Area Circ
AV AT Max PG
AV AT Vmax
AV DT Max PG
AV DT P1/2t
AV DT Slope
AV DT Vmax
B-C Slope Dist
B-C Time
Desc Ao Area
Hep. A Revs Dur Max PG
Hep. A Revs Dur P1/2t
Hep. A Revs Dur Slope
Hep. A Revs Dur Vmax
Hep. A Revs PG
Hepatic Dias PG
Hepatic Sys PG
IVCT P1/2t
IVCT Slope
IVCT Slope Max PG
IVCT Slope Vmax
IVRT P1/2t
IVRT Slope
IVRT Slope Max PG
IVRT Slope Vmax
LA Area
Lat A` Area Vmax
Lat A` Area Vmean
Lat AT Slope

ClearVue 350/550/650/850 3.1 Label
Lat AT Vmax
Lat DT P1/2t
Lat DT Slope
Lat DT Vmax
Lat E` Area Vmax
Lat E` Area Vmean
Lat IVCT P1/2t
Lat IVCT Slope
Lat IVCT Vmax
Lat IVRT P1/2t
Lat IVRT Slope
Lat IVRT Vmax
Late Dias Slope Dist
Late Dias Time
LPA Area
LV ET Dist
LV ET Slope
LV PEP Dist
LV PEP Slope
LVAd Sax Endo Circ
LVAd Sax Epi Circ
LVLd Apical Area
LVOT Area
LVOT AT Max PG
LVOT AT Vmax
Med A` Area Vmax
Med A` Area Vmean
Med AT Slope
Med AT Vmax
Med DT P1/2t
Med DT Slope
Med DT Vmax
Med E` Area Vmax
Med E` Area Vmean
Med IVCT P1/2t
Med IVCT Slope
Med IVCT Vmax
Med IVRT P1/2t
Med IVRT Slope
Med IVRT Vmax
MPA Area
MV A Dur MaxPG
MV A Dur P1/2t

ClearVue 350/550/650/850 3.1 Label
MV A Dur Slope
MV A Dur Vmax
MV A-C Int Dist
MV A-C Int Slope
MV Area
MV Area
MV Area (Planim) Circ
MV AT MaxPG
MV AT Vmax
MV D-E Dist
MV D-E Exc Time
MV D-E Time
MV DS MaxPG
MV DS P1/2t
MV DS Vmax
MV DT MaxPG
MV DT P1/2t
MV DT Slope
MV DT Vmax
MV E-F Dist
MV E-F Time
MV P1/2t MaxPG
MV P1/2t Slope
MV P1/2t Time
MV Peak A PG
MV Peak E PG
Pulm A Revs Dur Max PG
Pulm A Revs Dur P1/2t
Pulm A Revs Dur Slope
Pulm A Revs Dur Vmax
Pulm A Revs PG
Pulm Dias PG
Pulm Sys PG
PV AT Max PG
PV AT Vmax
RPA Area
RV ET Dist
RV ET Slope
RV PEP Dist
RV PEP Slope
RVOT Area
TV A-C Int Dist
TV A-C Int Slope

<b>ClearVue 350/550/650/850 3.1</b>
<b>Label</b>
TV Area
TV AT Max PG
TV AT Vmax
TV D-E Dist

<b>ClearVue 350/550/650/850 3.1</b>
<b>Label</b>
TV D-E Exc Time
TV D-E Time
TV E-F Dist
TV E-F Time

<b>ClearVue 350/550/650/850 3.1</b>
<b>Label</b>
TV Peak A PG
TV Peak E PG

#### A.4.9 Units Codes

ClearVue 350/550/650/850 3.1 make use of the following codes for Units associated with the exported measurements.

CSD	CV	CM
UCUM	%	Percent
UCUM	{H.B}/min	Beats Per Minute
UCUM[1.4]	cm	Centimeter
UCUM[1.4]	cm/s	Centimeter Per Second
UCUM[1.4]	cm/s2	Centimeter Per Second Square
UCUM[1.4]	cm2	Square Centimeter
UCUM	cm3	Cubic Centimeter
UCUM[1.4}	g	Gram
UCUM[1.4}	g/m2	g/m2
UCUM[1.4]	l/min	Litre Per Minute
UCUM	l/min/m2	l/min/m2
UCUM[1.4]	ml	Milliliter
UCUM	ml/m2	ml/m2
UCUM[1.4]	mm[Hg]	Millimeters Of Mercury
UCUM	mm[Hg]/s	mmHg/s
UCUM[1.4]	msec	Millisecond
UCUM	sec	Seconds

## A.5 PEDIATRIC ECHOCARDIOGRAPHY STRUCTURED REPORT TEMPLATE

ClearVue 350/550/650/850 3.1 implements the Pediatric Echocardiography Template (TID 5220) from the DICOM standard, part 16. This appendix describes the scope and manner that ClearVue 350/550/650/850 3.1 measurements appear in DICOM SR.

Measurements and calculations performed for Cardiac→Ped Echo studies will lead to creation of “Pediatric Cardiac Procedure Report” structured report documents. Measurements can be performed by pressing the ‘Calc’ key on ClearVue 350/550/650/850 3.1 control panel and selecting the Cardiac (Ped Echo) analysis package. Measurements and calculations available in the menu can be configured through the setup application. It is also possible to configure the measurement unit (Metric or U.S.).

All concepts with value type (VT) NUM will always have a ‘MeasurementUnitCodeSequence’ that specifies the unit of the measurement. The CSD for all units will be UCUM (Unified Code for Units) and CV and CM will be based on application configuration and will conform to UCUM standards.

### A.5.1 Template specific conformance for TID 5220

This template forms the top of a content tree that allows an ultrasound application to describe the results of a Cardiac Ultrasound imaging procedure.

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	DCID (12245) Cardiac Ultrasound Report Titles	
2	>	HAS CONCEPT MOD	INCLUDE	DTID (1204) Language of Content Item and Descendants	
3	>	HAS OBS CONTEXT	INCLUDE	DTID (1001) Observation Context	
4	>	CONTAINS	CONTAINER	EV (121109, DCM, “Indications for Procedure”)	
5	>>	CONTAINS	CODE	EV (121071, DCM, “Finding”)	
6	>>	CONTAINS	TEXT	EV (121071, DCM, “Finding”)	
7	>	CONTAINS	INCLUDE	DTID (3802) Cardiovascular Patient History	
8	>	CONTAINS	INCLUDE	DTID (3602) Cardiovascular Patient Characteristics	
9	>	CONTAINS	INCLUDE	DTID (5225) Cardiac Ultrasound Fetal Characteristics	
10	>	CONTAINS	INCLUDE	DTID (5226) Cardiac Ultrasound Summary Section	
11	>	CONTAINS	INCLUDE	DTID (5227) Cardiac Ultrasound Fetal Summary Section	

No	NL	REL WITH PARENT	VT	Concept Name	Comments
12	>	CONTAINS	CONTAINER	(111028, DCM, "Image Library")	
13	>>	CONTAINS	IMAGE	No purpose of reference	
14	>	CONTAINS	INCLUDE	DTID (5221) Cardiac Ultrasound Pediatric Measurement Section	
15	>	CONTAINS	INCLUDE	TID (5228) Cardiac Ultrasound Fetal Measurement Section	

#### A.5.1.1 Cardiovascular Patient Characteristics (TID 3606)

Contents of the following table may be present in the report if entered in Patient Data Entry

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	EV (121118, DCM, "Patient Characteristics")	
2	>	CONTAINS	NUM	(121033, DCM, "Subject Age")	From Patient Data Entry
3	>	CONTAINS	CODE	(121032, DCM, "Subject Sex")	From Patient Data Entry
4	>	CONTAINS	NUM	(8302-2, LN, "Patient Height")	From Patient Data Entry
5	>	CONTAINS	NUM	(29463-7, LN, "Patient Weight")	From Patient Data Entry
6	>	CONTAINS	NUM	(8277-6, LN, "Body Surface Area")	From Patient Data Entry
7	>>	Inferred From	CODE	(8278-4, LN, "Body Surface Area Formula")	
8	>	CONTAINS	NUM	(F-008EC, SRT, "Systolic Blood Pressure")	From Patient Data Entry
9	>	CONTAINS	NUM	(F-008ED, SRT, "Diastolic Blood Pressure")	From Patient Data Entry
10	>	CONTAINS	TEXT	(121029, DCM, "Subject Name")	From Patient Data Entry
11	>	CONTAINS	TEXT	(121030, DCM, "Subject ID")	From Patient Data Entry
12	>	CONTAINS	TEXT	(121031, DCM, "Subject Birth Date")	From Patient Data Entry
13	>	CONTAINS	TEXT	(T9910-04, 99PMSBLUS, "Reason for Study")	From Patient Data Entry
14	>	CONTAINS	TEXT	(T9910-112, 99PMSBLUS, "Alternate ID Number")	From Patient Data Entry

15	>	CONTAINS	TEXT	(121022, DCM, "Accession Number")	From Patient Data Entry
16	>	CONTAINS	TEXT	(T9910-08, 99PMSBLUS, "Referring Physician")	From Patient Data Entry
17	>	CONTAINS	TEXT	(121093, DCM, "Sonographer")	From Patient Data Entry
18	>	CONTAINS	TEXT	(T9910-07, 99PMSBLUS, "Study Description")	From Patient Data Entry
19	>	CONTAINS	TEXT	(T9910-10, 99PMSBLUS, "Patient History")	From Patient Data Entry
20	>	CONTAINS	TEXT	(T9910-09, 99PMSBLUS, "Exam date")	From Patient Data Entry
21	>	CONTAINS	TEXT	(T9910-182, 99PMSBLUS, "Surgeries Type")	From Patient Data Entry
22	>	CONTAINS	TEXT	(D3-30000, SRT, "Arrhythmia")	From Patient Data Entry
23	>	CONTAINS	TEXT	(T9910-176, 99PMSBLUS, "Arrhythmia Type")	From Patient Data Entry
24	>	CONTAINS	TEXT	(R-00302, SRT, "Murmur")	From Patient Data Entry
25	>	CONTAINS	TEXT	(T9910-178, 99PMSBLUS, "Murmur Type")	From Patient Data Entry
26	>	CONTAINS	TEXT	(F-37000, SRT, "Chest Pain")	From Patient Data Entry
27	>	CONTAINS	TEXT	(D3-10008, SRT, "Cardiomegaly")	From Patient Data Entry
28	>	CONTAINS	TEXT	(M-04100, SRT, "Cyanosis")	From Patient Data Entry
29	>	CONTAINS	TEXT	(D4-31B16, SRT, "Dextrocardia")	From Patient Data Entry
30	>	CONTAINS	TEXT	(F-201B3, SRT, "Dyspnea")	From Patient Data Entry
31	>	CONTAINS	TEXT	(F-0A44A, SRT, "Fever")	From Patient Data Entry
32	>	CONTAINS	TEXT	(F-24210, SRT, "Hemoptysis")	From Patient Data Entry
33	>	CONTAINS	TEXT	(D3-02000, SRT, "Hypertension")	From Patient Data Entry
34	>	CONTAINS	TEXT	(G-0586, SRT, "Insulin dependent mother (IDM)")	From Patient Data Entry
35	>	CONTAINS	TEXT	(D4-31B24, SRT, "Mesocardia")	From Patient Data Entry
36	>	CONTAINS	TEXT	(A-11100, SRT, "Cardiac Pacemaker")	From Patient Data Entry
37	>	CONTAINS	TEXT	(D3-00006, SRT, "Syncope")	From Patient Data Entry
38	>	CONTAINS	TEXT	(D4-31220, SRT, "Atrial Septal Defect")	From Patient Data Entry

39	>	CONTAINS	TEXT	(D4-31159, SRT, "Ventricular Septal Defect (VSD)")	From Patient Data Entry
40	>	CONTAINS	TEXT	(D4-32012, SRT, "Patent Ductus Arteriosus")	From Patient Data Entry
41	>	CONTAINS	TEXT	(D4-32014, SRT, "Coarctation of aorta")	From Patient Data Entry
42	>	CONTAINS	TEXT	(D4-31110, SRT, "Tetralogy of Fallot")	From Patient Data Entry
43	>	CONTAINS	TEXT	(D3-29021, SRT, "Aortic Stenosis")	From Patient Data Entry
44	>	CONTAINS	TEXT	(D3-29051, SRT, "Pulmonic valve stenosis")	From Patient Data Entry
45	>	CONTAINS	TEXT	(D4-33622, SRT, "Partial anomalous pulmonary venous connection")	From Patient Data Entry
46	>	CONTAINS	TEXT	(D4-31303, SRT, "Common atrioventricular canal")	From Patient Data Entry
47	>	CONTAINS	TEXT	(D4-31310, SRT, "Atrial septal defect with endocardial cushion defect, partial")	From Patient Data Entry
48	>	CONTAINS	TEXT	(D4-31010, SRT, "Complete transposition of great vessels")	From Patient Data Entry
49	>	CONTAINS	TEXT	(D3-83001, SRT, "Interrupted Aortic Arch")	From Patient Data Entry
50	>	CONTAINS	TEXT	(T9910-180, 99PMSBLUS, "Cardiomyopathy Type")	From Patient Data Entry
51	>	CONTAINS	TEXT	(T9910-181, 99PMSBLUS, "Infections Type")	From Patient Data Entry
52	>	CONTAINS	TEXT	(D3-29011, SRT, "Mitral stenosis")	From Patient Data Entry
53	>	CONTAINS	TEXT	(D3-29012, SRT, "Mitral regurgitation")	From Patient Data Entry
54	>	CONTAINS	TEXT	(D3-29022, SRT, "Aortic regurgitation")	From Patient Data Entry
55	>	CONTAINS	TEXT	(T9910-187, 99PMSBLUS, "AV Stenosis (acquired) (AS)")	From Patient Data Entry
56	>	CONTAINS	TEXT	(D3-29013, SRT, "Mitral valve prolapse")	From Patient Data Entry
57	>	CONTAINS	TEXT	(F-0331B, SRT, "HIV Positive")	From Patient Data Entry
58	>	CONTAINS	TEXT	(D3-81660, SRT, "Acute febrile mucocutaneous lymph node syndrome")	From Patient Data Entry
59	>	CONTAINS	TEXT	(D3-17100, SRT, "Rheumatic Fever")	From Patient Data Entry

#### A.5.1.2 Cardiac Ultrasound Pediatric Echo Measurement Section (TID 5221)

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	\$SectionSubject=DCID (12282) Cardiac Ultrasound Venous Return Systemic Finding Sites \$MeasType = DCID (12264) Cardiac Ultrasound Venous Return Systemic Measurements
2			INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	\$SectionSubject=DCID (12283) Cardiac Ultrasound Venous Return Pulmonary Finding Sites \$MeasType = DCID (12263) Cardiac Ultrasound Venous Return Pulmonary Measurements
3			INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	\$SectionSubject=DCID (12284) Cardiac Ultrasound Atria and Atrial Septum Finding Sites \$MeasType = DCID (12265) Cardiac Ultrasound Atria and Atrial Septum Measurements
4			INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	\$SectionSubject=DCID (12285) Cardiac Ultrasound Atrioventricular Valves Finding Sites \$MeasType = DCID (12268) Cardiac Ultrasound Atrioventricular Valves Measurements
5			INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	\$SectionSubject=DCID (12286) Cardiac Ultrasound Interventricular Septum Finding Sites \$MeasType = DCID (12269) Cardiac Ultrasound Interventricular Septum Measurements
6			INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	\$SectionSubject=DCID (12287) Cardiac Ultrasound Ventricles Finding Sites \$MeasType = DCID (12259) Cardiac Ultrasound Ventricles Measurements
7			INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	\$SectionSubject=DCID (12288) Cardiac Ultrasound Outflow Tracts Finding Sites \$MeasType = DCID (12271) Cardiac Ultrasound Outflow Tracts Measurements
8			INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	\$SectionSubject=DCID (12289) Cardiac Ultrasound Semilunar Valves, Annulus and Sinuses Finding Sites \$MeasType = DCID (12272) Cardiac Ultrasound Semilunar Valves, Annulus and Sinuses Measurements
9			INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	\$SectionSubject=DCID (12290) Cardiac Ultrasound Pulmonary Arteries Finding Sites \$MeasType = DCID (12260) Cardiac Ultrasound Pulmonary Artery

10			INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	\$SectionSubject=DCID (12291) Cardiac Ultrasound Aorta Finding Sites \$MeasType = DCID (12274) Cardiac Ultrasound Aorta Measurements
11			INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	\$SectionSubject=DCID (12292) Cardiac Ultrasound Coronary Arteries Finding Sites \$MeasType = DCID (12275) Cardiac Ultrasound Coronary Arteries Measurements
12			INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	\$SectionSubject=DCID (12293) Cardiac Ultrasound Aorta Pulmonary Connections Finding Sites \$MeasType = DCID (12276) Cardiac Ultrasound Aorta Pulmonary Connections Measurements
13			INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	\$SectionSubject=DCID (12294) Cardiac Ultrasound Pericardium and Pleura Finding Sites \$MeasType = DCID (12277) Cardiac Ultrasound Pericardium and Pleura Measurements

#### A.5.1.3 Pediatric, Fetal and Congenital Cardiac Ultrasound Section (TID 5222)

This is a generic section heading Template for any of the anatomical headings. Measurements within a section heading appear as groups (by image mode or acquisition protocol).

No	NL	REL WITH PARENT	VT	Concept Name	Comments
1			CONTAINER	EV (121070, DCM, "Findings")	
2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3, SRT, "Finding Site")	\$SectionSubject
3	>>	HAS CONCEPT MOD	CODE	EV (P1-32006, SRT, "Heart valve replacement - prosthesis")	
4	>	CONTAINS	CONTAINER	DT (125007, DCM, "Measurement Group")	
5	>>	HAS CONCEPT MOD	CODE	EV (G-0373, SRT, "Image Mode" )	BCID (12224) Ultrasound Image Modes
6	>>	HAS CONCEPT MOD	TEXT	DT (125203, DCM, "Acquisition Protocol")	
7	>>	CONTAINS	INCLUDE	DTID (5223) Pediatric, Fetal and Congenital Cardiac Ultrasound Measurement	\$Measurement = \$MeasType \$Method=CID (12227) Echocardiography Measurement Method

#### A 5.1.4 Pediatric, Fetal and Congenital Cardiac Ultrasound Measurement (TID 5223)

This Template provides for the post-coordination of a measurement with a variety of concept modifiers and acquisition context observations. When invoked from TID 5222, the measurement concept is implicitly post-coordinated with the concept modifiers of the Measurement Group (TID 5222 Rows 5 and 6), and with the Finding Site of the report section (TID 5222 Row 2). The finding site may be further specified within this Template by the Target Site and Target Site Modifiers (CID 12280 and CID 12281).

The implicit finding site inherited from TID 5222 can be made explicit by using the same finding site concept in the Target Site (the measurement concept modifier), rather than a term from CID 12280. This explicit post-coordination allows the use of one of the modifiers of CID 12281 to that finding site, as the Target Site Modifier requires an explicit Target Site in the measurement structure (TID 300 Rows 5 and 7). In fact, any child concept of the finding site in the SNOMED hierarchy may be used as the measurement Target Site.

The finding or target site may be identified by a concept from the SNOMED “clinical finding” or “morphological anomaly” hierarchies (e.g., D4-31220 “Atrial Septal Defect”, or M-36700 “Effusion”), rather than the “anatomical structure” hierarchy. In this case, the meaning is inferred as “the anatomic location of the clinical finding or morphological anomaly, within the constraints of other implicit or explicit post-coordinated finding site concepts.”

No	NL	Rel with Parent	VT	Concept Name	Comments
1			INCLUDE	DTID (300) Measurement	\$Measurement = \$Measurement \$Method = \$Method \$TargetSite = BCID (12280) Cardiac Ultrasound Target Sites \$TargetSiteMod = BCID (12281) Cardiac Ultrasound Target Site Modifiers \$Derivation=DCID (3838) Diameter Derivation
2	>	HAS CONCEPT MOD	CODE	EV (121425, DCM, “Index”)	DCID (3455) Index Methods
3	>	HAS CONCEPT MOD	CODE	EV (G-C048, SRT, “Flow Direction”)	BCID (12221) Flow Direction
4	>	HAS CONCEPT MOD	CODE	EV (R-40899, SRT, “Respiratory Cycle Point”)	DCID (12234) Respiration State
5	>	HAS CONCEPT MOD	CODE	EV (R-4089A, SRT, “Cardiac Cycle Point”)	DCID (12233) Cardiac Phase
6	>	HAS ACQ CONTEXT	CODE	EV (G-0373, SRT, “Image Mode”)	DCID (12224) Ultrasound Image Modes
7	>	HAS ACQ CONTEXT	CODE	EV (111031, DCM, “Image View”)	BCID (12226) Echocardiography Image View

#### A 5.1.5 Cardiac Ultrasound Fetal Characteristics (TID 5225)

Contains a list of Fetus Specific characteristics

No	NL	Rel with Parent	VT	Concept Name	Comments
1			CONTAINER	EV (125015, DCM, “Fetus Characteristics”)	
2	>	HAS OBS CONTEXT	INCLUDE	DTID (1008) Subject Context, Fetus	
3	>	CONTAINS	NUM	EV (18185-9, LN, “Gestational Age”)	
4	>	CONTAINS	DATE	EV (11778-8, LN, “EDD”)	
5	>	CONTAINS	NUM	EV (8867-4, LN, “Heart Rate”)	

#### A5.1.6 Cardiac Ultrasound Summary Section (TID 5226)

Comments and observations of the procedure of immediate clinical interest

No	NL	Rel with Parent	VT	Concept Name	Comments
1			CONTAINER	EV (121111, DCM, "Summary")	
2	>	CONTAINS	CODE	EV (121071, DCM, "Finding")	
3	>	CONTAINS	TEXT	EV (121071, DCM, "Finding")	
4	>	CONTAINS	CODE	EV (P0-009C3, SRT "Surgical Procedure")	

#### A5.1.7 Cardiac Ultrasound FetalSummary Section (TID 5227)

Comments and observations of the procedure of immediate clinical interest

No	NL	Rel with Parent	VT	Concept Name	Comments
1			CONTAINER	DT (125008, DCM, "Fetus Summary")	
2	>	HAS OBS CONTEXT	INCLUDE	DTID (1008) Subject Context, Fetus	
3	>	CONTAINS	CODE	EV (121071, DCM, "Finding")	
4	>	CONTAINS	TEXT	EV (121071, DCM, "Finding")	
5	>	CONTAINS	CODE	EV (P0-009C3, SRT "Surgical Procedure")	

#### A 5.1.8 Cardiac Ultrasound Fetal Measurement Section (TID 5228)

No	NL	Rel with Parent	VT	Concept Name	Comments
1			CONTAINER	EV (125016, DCM, "Fetal Measurements")	
2	>	HAS OBS CONTEXT	INCLUDE	DTID (1008) Subject Context, Fetus	
3	>	CONTAINS	INCLUDE	DTID (300) Measurement	
4	>	CONTAINS	INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	
5	>	CONTAINS	INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	
6	>	CONTAINS	INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	
7	>	CONTAINS	INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	
8	>	CONTAINS	INCLUDE	DTID (5222) Pediatric, Fetal and Congenital Cardiac Ultrasound Section	

#### A 5.2 eDCS – Pediatric Echocardiography Template Support

The following list represents the Electronic DICOM Conformance Statement (eDCS) format for the Structured Report output for the Pediatric Echocardiography Procedure Report as supported on ClearVue 350/550/650 3.1.

This list is made up of 'signatures' that describe the group of codes used for each exported measurement and calculation result.

A 'signature' will contain the Label as displayed on the system user interface in the Calcs application and report pages, followed by the modifiers required by the DICOM SR Template and Structured Reporting SOP Class in order to include a given measurement or calculation value.

Some signatures will contain as few as two or as many as six modifiers.

In the table below, the following terms are used:

CSD	Coding Scheme Designator
CV	Code Value
CM	Code Meaning

#### A 5.2.1 eDCS Table

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
<b>A Wave Amp</b>	LN	59100-8	A-Wave Amplitude
	SRT	T-35200	Pulmonic Valve
	SRT	G-0394	M mode
	UCUM	cm	Centimeter
<b>AI Accel Slope</b>	LN	20167-3	Acceleration Slope
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
<b>AI Accel Time</b>	LN	20168-1	Acceleration Time
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	sec	Seconds
<b>AI Alias Vel</b>	LN	59130-5	Alias velocity
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm/s	Centimeter Per Second
<b>AI Decel Slope</b>	LN	20216-8	Deceleration Slope
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
<b>AI Decel Time</b>	LN	20217-6	Deceleration Time
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	sec	Seconds
<b>AI End Dias Vel</b>	LN	11653-3	End Diastolic Velocity

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	SRT	F-32011	End Diastole
	UCUM	cm/s	Centimeter Per Second
<b>AI ERO</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35400	Aortic Valve
	DCM	125216	Proximal Isovelocity Surface Area
	SRT	G-0367	Regurgitant Flow
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>AI Flow Rate</b>	LN	34141-2	Peak Instantaneous Flow Rate
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	ml/sec	ml/sec
<b>AI Fraction</b>	SRT	G-0390	Regurgitant Fraction
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	%	Percent
<b>AI Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>AI Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>AI P1/2t</b>	LN	20280-4	Pressure Half-Time
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	msec	Millisecond
<b>AI Radius</b>	LN	59102-4	Flow Radius
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm	Centimeter
<b>AI Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm/s	Centimeter Per Second
<b>AI Vmean</b>	LN	11692-1	Time Averaged Peak Velocity

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm/s	Centimeter Per Second
<b>AI Volume</b>	LN	33878-0	Volume Flow
	SRT	T-35400	Aortic Valve
	DCM	125216	Proximal Isovelocity Surface Area
	SRT	G-0367	Regurgitant Flow
	UCUM	ml	Milliliter
<b>AI VTI</b>	LN	20354-7	Velocity Time Integral
	SRT	T-35400	Aortic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm	Centimeter
<b>Ao Arch Diam</b>	SRT	M-02550	Diameter
	SRT	T-42300	Aortic arch
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>Ao Arch Dist Diam</b>	SRT	M-02550	Diameter
	SRT	T-42300	Aortic arch
	SRT	G-03A2	2D mode
	SRT	G-A119	Distal
	UCUM	cm	Centimeter
<b>Ao Isthmus Diam</b>	SRT	M-02550	Diameter
	SRT	T-42310	Aortic isthmus
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>Ao Sinus Diam</b>	SRT	M-02550	Diameter
	SRT	T-42200	Structure Sinus of Valsalva
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>Ao ST Jx Diam</b>	SRT	M-02550	Diameter
	SRT	T-42102	Aortic sinotubular junction
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>AoR Area</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-42110	Root of Aorta
	SRT	G-03A2	2D mode
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>AoR Diam (2D)</b>	SRT	M-02550	Diameter

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	T-42110	Root of Aorta
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>AoR Diam (MM)</b>	SRT	M-02550	Diameter
	SRT	T-42110	Root of Aorta
	SRT	G-0394	M mode
	UCUM	cm	Centimeter
<b>AS Max PG</b>	LN	59106-5	Stenosis Peak Gradient
	SRT	T-35400	Aortic Valve
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>AS Vmax</b>	LN	59107-3	Stenosis Peak Velocity
	SRT	T-35400	Aortic Valve
	UCUM	cm/s	Centimeter Per Second
<b>Asc Ao Diam</b>	SRT	M-02550	Diameter
	SRT	T-42100	Ascending aorta
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>Asc Ao Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-42100	Ascending aorta
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>Asc Ao Max PG (full)</b>	LN	20247-3	Peak Gradient
	SRT	T-42100	Ascending aorta
	DCM	125217	Full Bernoulli
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>Asc Ao Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-42100	Ascending aorta
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>Asc Ao Mean PG (full)</b>	LN	20256-4	Mean Gradient
	SRT	T-42100	Ascending aorta
	DCM	125217	Full Bernoulli
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>Asc Ao Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-42100	Ascending aorta
	UCUM	cm/s	Centimeter Per Second
<b>ASD Diam</b>	SRT	M-02550	Diameter
	SRT	D4-31220	Atrial Septal Defect
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
<b>ASD Major</b>	SRT	G-A193	Major Axis
	SRT	D4-31220	Atrial Septal Defect
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>ASD Max PG</b>	LN	20247-3	Peak Gradient
	SRT	D4-31220	Atrial Septal Defect
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>ASD Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	D4-31220	Atrial Septal Defect
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>ASD Minor</b>	SRT	G-A194	Minor Axis
	SRT	D4-31220	Atrial Septal Defect
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>ASD Vmax</b>	LN	20351-3	Peak Velocity
	SRT	D4-31220	Atrial Septal Defect
	UCUM	cm/s	Centimeter Per Second
<b>ASD Vmean</b>	LN	11692-1	Time Averaged Peak Velocity
	SRT	D4-31220	Atrial Septal Defect
	UCUM	cm/s	Centimeter Per Second
<b>ASD VTI</b>	LN	20354-7	Velocity Time Integral
	SRT	D4-31220	Atrial Septal Defect
	UCUM	cm	Centimeter
<b>AV Accel Slope</b>	LN	20167-3	Acceleration Slope
	SRT	T-35400	Aortic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
<b>AV Accel Time</b>	LN	20168-1	Acceleration Time
	SRT	T-35400	Aortic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	sec	Seconds
<b>AV Annul Diam</b>	SRT	M-02550	Diameter
	SRT	T-35400	Aortic Valve
	SRT	G-03A2	2D mode
	SRT	T-3500E	Cardiac valve annulus
	UCUM	cm	Centimeter
<b>AV Area</b>	SRT	G-A166	Area
	SRT	T-35400	Aortic Valve

<b>ClearVue 350/550/650/850 3.1</b>			
<b>Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	G-03A2	2D mode
	UCUM	cm2	Square Centimeter
<b>AV Cusp Sep</b>	LN	17996-0	Aortic Valve Cusp Separation
	SRT	T-35400	Aortic Valve
	SRT	G-0394	M mode
	UCUM	cm	Centimeter
<b>AV Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-35400	Aortic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>AV Max PG (full)</b>	LN	20247-3	Peak Gradient
	SRT	T-35400	Aortic Valve
	DCM	125217	Full Bernoulli
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>AV Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-35400	Aortic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>AV Mean PG (full)</b>	LN	20256-4	Mean Gradient
	SRT	T-35400	Aortic Valve
	DCM	125217	Full Bernoulli
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>AV R-R (DOP)</b>	LN	8867-4	Heart Rate
	SRT	T-35400	Aortic Valve
	UCUM	sec	Seconds
<b>AV R-R (MM)</b>	LN	8867-4	Heart Rate
	SRT	T-35400	Aortic Valve
	SRT	G-0394	M mode
	UCUM	sec	Seconds
<b>AV Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-35400	Aortic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s	Centimeter Per Second
<b>AV Vmean</b>	LN	11692-1	Time Averaged Peak Velocity
	SRT	T-35400	Aortic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s	Centimeter Per Second
<b>AV VTI</b>	LN	20354-7	Velocity Time Integral

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	T-35400	Aortic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm	Centimeter
<b>AVA (Vmax)</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35400	Aortic Valve
	DCM	125214	Continuity Equation by Peak Velocity
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>AVA (VTI)</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35400	Aortic Valve
	DCM	125215	Continuity Equation by Velocity Time Integral
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>AV-HR (DOP)</b>	LN	8867-4	Heart Rate
	SRT	T-35400	Aortic Valve
	UCUM	{H.B.}/min	Beats Per Minute
<b>AV-HR (MM)</b>	LN	8867-4	Heart Rate
	SRT	T-35400	Aortic Valve
	SRT	G-0394	M mode
	UCUM	{H.B.}/min	Beats Per Minute
<b>B-C Slope</b>	LN	59126-3	B-C Slope
	SRT	T-35200	Pulmonic Valve
	SRT	G-0394	M mode
	UCUM	cm/s	Centimeter Per Second
<b>CI (2D-Cubed)</b>	SRT	F-32110	Cardiac Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125206	Cube Method
	UCUM	l/min/m <sup>2</sup>	l/min/m <sup>2</sup>
<b>CI (2D-Teich)</b>	SRT	F-32110	Cardiac Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125209	Teichholz
	UCUM	l/min/m <sup>2</sup>	l/min/m <sup>2</sup>
<b>CI (A/L)</b>	SRT	F-32110	Cardiac Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125226	Single Plane Ellipse
	UCUM	l/min/m <sup>2</sup>	l/min/m <sup>2</sup>
<b>CI (A2C)</b>	SRT	F-32110	Cardiac Index

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125208	Method of Disks, Single Plane
	UCUM	l/min/m <sup>2</sup>	l/min/m <sup>2</sup>
<b>CI (A2C-A/L)</b>	SRT	F-32110	Cardiac Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125226	Single Plane Ellipse
	UCUM	l/min/m <sup>2</sup>	l/min/m <sup>2</sup>
<b>CI (A4C)</b>	SRT	F-32110	Cardiac Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125208	Method of Disks, Single Plane
	UCUM	l/min/m <sup>2</sup>	l/min/m <sup>2</sup>
<b>CI (A4C-A/L)</b>	SRT	F-32110	Cardiac Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125226	Single Plane Ellipse
	UCUM	l/min/m <sup>2</sup>	l/min/m <sup>2</sup>
<b>CI (BP)</b>	SRT	F-32110	Cardiac Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125207	Method of Disks, Biplane
	UCUM	l/min/m <sup>2</sup>	l/min/m <sup>2</sup>
<b>CI (MM-Cubed)</b>	SRT	F-32110	Cardiac Index
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125206	Cube Method
	UCUM	l/min/m <sup>2</sup>	l/min/m <sup>2</sup>
<b>CI (MM-Teich)</b>	SRT	F-32110	Cardiac Index
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125209	Teichholz
	UCUM	l/min/m <sup>2</sup>	l/min/m <sup>2</sup>

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
<b>CO (2D-Cubed)</b>	SRT	F-32100	Cardiac Output
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125206	Cube Method
	UCUM	l/min	Litre Per Minute
<b>CO (2D-Teich)</b>	SRT	F-32100	Cardiac Output
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125209	Teichholz
	UCUM	l/min	Litre Per Minute
<b>CO (A/L)</b>	SRT	F-32100	Cardiac Output
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125226	Single Plane Ellipse
	UCUM	l/min	Litre Per Minute
<b>CO (A2C)</b>	SRT	F-32100	Cardiac Output
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125208	Method of Disks, Single Plane
	UCUM	l/min	Litre Per Minute
<b>CO (A2C-A/L)</b>	SRT	F-32100	Cardiac Output
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125226	Single Plane Ellipse
	UCUM	l/min	Litre Per Minute
<b>CO (A4C)</b>	SRT	F-32100	Cardiac Output
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125208	Method of Disks, Single Plane
	UCUM	l/min	Litre Per Minute
<b>CO (A4C-A/L)</b>	SRT	F-32100	Cardiac Output
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125226	Single Plane Ellipse

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	UCUM	l/min	Litre Per Minute
<b>CO (BP)</b>	SRT	F-32100	Cardiac Output
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125207	Method of Disks, Biplane
	UCUM	l/min	Litre Per Minute
<b>CO (LVOT)</b>	SRT	F-32100	Cardiac Output
	SRT	T-32600	Left Ventricle
	SRT	T-32650	Left Ventricle Outflow Tract
	UCUM	l/min	Litre Per Minute
<b>CO (MM-Cubed)</b>	SRT	F-32100	Cardiac Output
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125206	Cube Method
	UCUM	l/min	Litre Per Minute
<b>CO (MM-Teich)</b>	SRT	F-32100	Cardiac Output
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125209	Teichholz
	UCUM	l/min	Litre Per Minute
<b>CO (MV)</b>	SRT	F-32100	Cardiac Output
	SRT	T-35300	Mitral Valve
	UCUM	l/min	Litre Per Minute
<b>CO (PV)</b>	SRT	F-32100	Cardiac Output
	SRT	T-35200	Pulmonic Valve
	UCUM	l/min	Litre Per Minute
<b>CO (RVOT)</b>	SRT	F-32100	Cardiac Output
	SRT	T-32500	Right Ventricle
	SRT	T-32550	Right Ventricle Outflow Tract
	UCUM	l/min	Litre Per Minute
<b>CO (TV)</b>	SRT	F-32100	Cardiac Output
	SRT	T-35100	Tricuspid Valve
	UCUM	l/min	Litre Per Minute
<b>Coarctation Diam</b>	SRT	M-02550	Diameter
	SRT	D4-32014	Coarctation of aorta
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>Cx Diam</b>	SRT	M-02550	Diameter

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	T-43120	Circumflex Coronary Artery
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>Desc Ao Diam</b>	SRT	M-02550	Diameter
	SRT	T-42070	Thoracic aorta
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>Desc Ao Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-42070	Thoracic aorta
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>Desc Ao Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-42070	Thoracic aorta
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>Desc Ao Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-42070	Thoracic aorta
	UCUM	cm/s	Centimeter Per Second
<b>Dsc Ao Max PG (full)</b>	LN	20247-3	Peak Gradient
	SRT	T-42070	Thoracic aorta
	DCM	125217	Full Bernoulli
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>Dsc Ao Mean PG (full)</b>	LN	20256-4	Mean Gradient
	SRT	T-42070	Thoracic aorta
	DCM	125217	Full Bernoulli
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>E/E` Lateral</b>	SRT	G-037B	Ratio of MV Peak Velocity to LV Peak Tissue Velocity E-Wave
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0392	Lateral Mitral Annulus
	UCUM	1	no units
<b>E/E` Medial</b>	SRT	G-037B	Ratio of MV Peak Velocity to LV Peak Tissue Velocity E-Wave
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0391	Medial Mitral Annulus
	UCUM	1	no units
<b>E`/A` Lateral</b>	LN	59129-7	Left Ventricle E to A Tissue Velocity Ratio
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0392	Lateral Mitral Annulus

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	UCUM	1	no units
<b>E`/A` Medial</b>	LN	59129-7	Left Ventricle E to A Tissue Velocity Ratio
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0391	Medial Mitral Annulus
	UCUM	1	no units
<b>EDV (2D-Cubed)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125206	Cube Method
	SRT	F-32011	End Diastole
	UCUM	ml	Milliliter
<b>EDV (2D-Teich)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125209	Teichholz
	SRT	F-32011	End Diastole
	UCUM	ml	Milliliter
<b>EDV (A/L)</b>	LN	18026-5	Left Ventricular End Diastolic Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125226	Single Plane Ellipse
	UCUM	ml	Milliliter
<b>EDV (A2C)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125208	Method of Disks, Single Plane
	SRT	F-32011	End Diastole
	UCUM	ml	Millileter
<b>EDV (A2C-A/L)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125226	Single Plane Ellipse
	SRT	F-32011	End Diastole
	UCUM	ml	Milliliter
<b>EDV (A4C)</b>	SRT	G-D705	Volume

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125208	Method of Disks, Single Plane
	SRT	F-32011	End Diastole
	UCUM	ml	Millileter
<b>EDV (A4C-A/L)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125226	Single Plane Ellipse
	SRT	F-32011	End Diastole
	UCUM	ml	Milliliter
<b>EDV (BP)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125207	Method of Disks, Biplane
	SRT	F-32011	End Diastole
	UCUM	ml	Milliliter
<b>EDV (MM-Cubed)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125206	Cube Method
	SRT	F-32011	End Diastole
	UCUM	ml	Milliliter
<b>EDV (MM-Teich)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125209	Teichholz
	SRT	F-32011	End Diastole
	UCUM	ml	Milliliter
<b>EF (2D-Cubed)</b>	SRT	F-32070	Cardiac ejection fraction
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125206	Cube Method
	UCUM	%	Percent
<b>EF (2D-Teich)</b>	SRT	F-32070	Cardiac ejection fraction
	SRT	T-32600	Left Ventricle

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	G-03A2	2D mode
	DCM	125209	Teichholz
	UCUM	%	Percent
<b>EF (A/L)</b>	SRT	F-32070	Cardiac ejection fraction
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125226	Single Plane Ellipse
	UCUM	%	Percent
<b>EF (A2C)</b>	SRT	F-32070	Cardiac ejection fraction
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125208	Method of Disks, Single Plane
	UCUM	%	Percent
<b>EF (A2C-A/L)</b>	SRT	F-32070	Cardiac ejection fraction
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125226	Single Plane Ellipse
	UCUM	%	Percent
<b>EF (A4C)</b>	SRT	F-32070	Cardiac ejection fraction
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125208	Method of Disks, Single Plane
	UCUM	%	Percent
<b>EF (A4C-A/L)</b>	SRT	F-32070	Cardiac ejection fraction
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125226	Single Plane Ellipse
	UCUM	%	Percent
<b>EF (BP)</b>	SRT	F-32070	Cardiac ejection fraction
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125207	Method of Disks, Biplane
	UCUM	%	Percent
<b>EF (MM-Cubed)</b>	SRT	F-32070	Cardiac ejection fraction

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125206	Cube Method
	UCUM	%	Percent
<b>EF (MM-Teich)</b>	SRT	F-32070	Cardiac ejection fraction
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125209	Teichholz
	UCUM	%	Percent
<b>ESV (2D-Cubed)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125206	Cube Method
	SRT	R-FAB5B	End Systole
	UCUM	ml	Milliliter
<b>ESV (2D-Teich)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125209	Teichholz
	SRT	R-FAB5B	End Systole
	UCUM	ml	Milliliter
<b>ESV (A/L)</b>	LN	18148-7	Left Ventricular End Systolic Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125226	Single Plane Ellipse
	UCUM	ml	Milliliter
<b>ESV (A2C)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125208	Method of Disks, Single Plane
	SRT	R-FAB5B	End systole
	UCUM	ml	Millileter
<b>ESV (A2C-A/L)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125226	Single Plane Ellipse

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	R-FAB5B	End Systole
	UCUM	ml	Milliliter
<b>ESV (A4C)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125208	Method of Disks, Single Plane
	SRT	R-FAB5B	End systole
	UCUM	ml	Milliliter
<b>ESV (A4C-A/L)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125226	Single Plane Ellipse
	SRT	R-FAB5B	End Systole
	UCUM	ml	Milliliter
<b>ESV (BP)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125207	Method of Disks, Biplane
	SRT	R-FAB5B	End Systole
	UCUM	ml	Milliliter
<b>ESV (MM-Cubed)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125206	Cube Method
	SRT	R-FAB5B	End Systole
	UCUM	ml	Milliliter
<b>ESV (MM-Teich)</b>	SRT	G-D705	Volume
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125209	Teichholz
	SRT	R-FAB5B	End Systole
	UCUM	ml	Milliliter
<b>Hepatic A Dur</b>	LN	59105-7	A-Wave Duration
	SRT	T-48720	Hepatic Vein
	UCUM	sec	Seconds
<b>Hepatic A Vel</b>	LN	59079-4	Peak Reversal Velocity during Atrial Contraction

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	T-48720	Hepatic Vein
	UCUM	cm/s	Centimeter Per Second
<b>Hepatic Dias Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48720	Hepatic Vein
	SRT	F-32011	End Diastole
	UCUM	cm/s	Centimeter Per Second
<b>Hepatic S/D</b>	LN	12144-2	Systolic to Diastolic Velocity Ratio
	SRT	T-48720	Hepatic Vein
	UCUM	1	no units
<b>Hepatic Sys Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48720	Hepatic Vein
	SRT	R-FAB5B	End Systole
	UCUM	cm/s	Centimeter Per Second
<b>HR LV (2D)</b>	LN	8867-4	Heart Rate
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	UCUM	{H.B.}/min	Beats Per Minute
<b>HR LV (MM)</b>	LN	8867-4	Heart Rate
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	UCUM	{H.B.}/min	Beats Per Minute
<b>IVC A Dur</b>	LN	59105-7	A-Wave Duration
	SRT	T-48710	Inferior vena cava
	UCUM	sec	Seconds
<b>IVC A Vel</b>	LN	59079-4	Peak Reversal Velocity during Atrial Contraction
	SRT	T-48710	Inferior vena cava
	UCUM	cm/s	Centimeter Per Second
<b>IVC Diam</b>	SRT	M-02550	Diameter
	SRT	T-48710	Inferior vena cava
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>IVC Dias Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48710	Inferior vena cava
	SRT	F-32011	End Diastole
	UCUM	cm/s	Centimeter Per Second
<b>IVC S/D</b>	LN	12144-2	Systolic to Diastolic Velocity Ratio
	SRT	T-48710	Inferior vena cava
	UCUM	1	no units

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
<b>IVC Sys Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48710	Inferior vena cava
	SRT	R-FAB5B	End Systole
	UCUM	cm/s	Centimeter Per Second
<b>IVCT</b>	LN	59084-4	Isovolumic Contraction Time
	SRT	T-32600	Left Ventricle
	UCUM	sec	Seconds
<b>IVRT</b>	LN	59083-6	Isovolumic Relaxation Time
	SRT	T-32600	Left Ventricle
	UCUM	sec	Seconds
<b>IVS % (2D)</b>	LN	59092-7	% Thickening
	SRT	T-32410	Interventricular septum
	SRT	G-03A2	2D mode
	UCUM	%	Percent
<b>IVS % (MM)</b>	LN	59092-7	% Thickening
	SRT	T-32410	Interventricular septum
	SRT	G-0394	M mode
	UCUM	%	Percent
<b>IVS/LVPW (2D)</b>	LN	18155-2	Interventricular Septum to Posterior Wall Thickness Ratio
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	UCUM	1	no units
<b>IVS/LVPW (MM)</b>	LN	18155-2	Interventricular Septum to Posterior Wall Thickness Ratio
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	UCUM	1	no units
<b>IVSd (2D)</b>	LN	59089-3	ROI Thickness by US
	SRT	T-32410	Interventricular septum
	SRT	G-03A2	2D mode
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>IVSd (MM)</b>	LN	59089-3	ROI Thickness by US
	SRT	T-32410	Interventricular septum
	SRT	G-0394	M mode
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>IVSs (2D)</b>	LN	59089-3	ROI Thickness by US
	SRT	T-32410	Interventricular septum

<b>ClearVue 350/550/650/850 3.1</b>			
<b>Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	G-03A2	2D mode
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>IVSs (MM)</b>	LN	59089-3	ROI Thickness by US
	SRT	T-32410	Interventricular septum
	SRT	G-0394	M mode
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>LA Dimen (2D)</b>	LN	29469-4	Left Atrium Antero-posterior Systolic Dimension
	SRT	T-32300	Left Atrium
	SRT	G-03A2	2D mode
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>LA Dimen (MM)</b>	LN	29469-4	Left Atrium Antero-posterior Systolic Dimension
	SRT	T-32300	Left Atrium
	SRT	G-0394	M mode
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>LA ESV (BP)</b>	SRT	G-0383	Left Atrium Systolic Volume
	SRT	T-32300	Left Atrium
	SRT	G-03A2	2D mode
	DCM	125207	Method of Disks, Biplane
	UCUM	ml	Milliliter
<b>LA ESV/BSA (A2C)</b>	99PMSBLUS	C12205-03	Left Atrium Systolic Volume Index
	SRT	T-32300	Left Atrium
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125208	Method of Disks, Single Plane
	LN	8277-6	Body Surface Area
	UCUM	ml/m <sup>2</sup>	ml/m <sup>2</sup>
<b>LA ESV/BSA (A4C)</b>	99PMSBLUS	C12205-03	Left Atrium Systolic Volume Index
	SRT	T-32300	Left Atrium
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125208	Method of Disks, Single Plane
	LN	8277-6	Body Surface Area
	UCUM	ml/m <sup>2</sup>	ml/m <sup>2</sup>
<b>LA ESV/BSA (BP)</b>	99PMSBLUS	C12205-03	Left Atrium Systolic Volume Index

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	T-32300	Left Atrium
	SRT	G-03A2	2D mode
	DCM	125207	Method of Disks, Biplane
	LN	8277-6	Body Surface Area
	UCUM	ml/m2	ml/m2
<b>LA/Ao (2D)</b>	LN	17985-3	Left Atrium to Aortic Root Ratio
	SRT	T-32300	Left Atrium
	SRT	G-03A2	2D mode
	UCUM	1	no units
<b>LA/Ao (MM)</b>	LN	17985-3	Left Atrium to Aortic Root Ratio
	SRT	T-32300	Left Atrium
	SRT	G-0394	M mode
	UCUM	1	no units
<b>LAD Diam</b>	SRT	M-02550	Diameter
	SRT	T-43110	Anterior Descending Branch of Left Coronary Artery
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>LAED Major-A4C</b>	SRT	G-A193	Major Axis
	SRT	T-32300	Left Atrium
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LAED Minor-A4C</b>	SRT	G-A194	Minor Axis
	SRT	T-32300	Left Atrium
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LAES Major-A4C</b>	SRT	G-A193	Major Axis
	SRT	T-32300	Left Atrium
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>LAES Minor-A4C</b>	SRT	G-A194	Minor Axis
	SRT	T-32300	Left Atrium
	SRT	G-03A2	2D mode

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	G-A19C	Apical four chamber
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>Lat A` Area</b>	LN	59125-5	LV VTI A wave US
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0392	Lateral Mitral Annulus
	UCUM	cm	Centimeter
<b>Lat A` Vel</b>	LN	59133-9	Peak Tissue Velocity
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0392	Lateral Mitral Annulus
	SRT	F-32030	Atrial Systole
	UCUM	cm/s	Centimeter Per Second
<b>Lat Accel Time</b>	LN	20168-1	Acceleration Time
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0392	Lateral Mitral Annulus
	UCUM	sec	Seconds
<b>Lat Decel Time</b>	LN	20217-6	Deceleration Time
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0392	Lateral Mitral Annulus
	UCUM	sec	Seconds
<b>Lat E` Area</b>	LN	59124-8	LV VTI E wave US
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0392	Lateral Mitral Annulus
	UCUM	cm	Centimeter
<b>Lat E` Vel</b>	LN	59133-9	Peak Tissue Velocity
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0392	Lateral Mitral Annulus
	SRT	R-40B1B	Early Diastole
	UCUM	cm/s	Centimeter Per Second
<b>Lat IVCT</b>	LN	59084-4	Isovolumic Contraction Time
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	G-0392	Lateral Mitral Annulus
	UCUM	sec	Seconds
<b>Lat IVRT</b>	LN	59083-6	Isovolumic Relaxation Time
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0392	Lateral Mitral Annulus
	UCUM	sec	Seconds
<b>Lat S Vel</b>	LN	59133-9	Peak Tissue Velocity
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0392	Lateral Mitral Annulus
	SRT	R-FAB5B	End Systole
	UCUM	cm/s	Centimeter Per Second
<b>Late Dias Slope</b>	LN	20216-8	Deceleration Slope
	SRT	T-35200	Pulmonic Valve
	SRT	G-0394	M mode
	SRT	F-32011	End Diastole
	UCUM	cm/s	Centimeter Per Second
<b>Left Main</b>	SRT	M-02550	Diameter
	SRT	T-43107	Left Main Coronary Artery
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>LL PulmV A Dur</b>	LN	59105-7	A-Wave Duration
	SRT	T-48581	Pulmonary Vein
	SRT	T-48540	Left Inferior Pulmonary Vein
	UCUM	sec	Seconds
<b>LL PulmV A Vel</b>	LN	59079-4	Peak Reversal Velocity during Atrial Contraction
	SRT	T-48581	Pulmonary Vein
	SRT	T-48540	Left Inferior Pulmonary Vein
	UCUM	cm/s	Centimeter Per Second
<b>LL PulmV Diam</b>	SRT	M-02550	Diameter
	SRT	T-48581	Pulmonary Vein
	SRT	G-03A2	2D mode
	SRT	T-48540	Left Inferior Pulmonary Vein
	UCUM	cm	Centimeter
<b>LL PulmV Dias Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48581	Pulmonary Vein
	SRT	T-48540	Left Inferior Pulmonary Vein

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	F-32011	End Diastole
	UCUM	cm/s	Centimeter Per Second
<b>LL PulmV S/D</b>	LN	12144-2	Systolic to Diastolic Velocity Ratio
	SRT	T-48581	Pulmonary Vein
	SRT	T-48540	Left Inferior Pulmonary Vein
	UCUM	1	no units
<b>LL PulmV Sys Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48581	Pulmonary Vein
	SRT	T-48540	Left Inferior Pulmonary Vein
	SRT	R-FAB5B	End Systole
	UCUM	cm/s	Centimeter Per Second
<b>LPA Diam</b>	SRT	M-02550	Diameter
	SRT	T-44000	Pulmonary artery
	SRT	G-03A2	2D mode
	SRT	T-44400	Left pulmonary artery
	UCUM	cm	Centimeter
<b>LPA Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-44000	Pulmonary artery
	SRT	T-44400	Left pulmonary artery
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>LPA Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-44000	Pulmonary artery
	SRT	T-44400	Left pulmonary artery
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>LPA Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-44000	Pulmonary artery
	SRT	T-44400	Left pulmonary artery
	UCUM	cm/s	Centimeter Per Second
<b>LU PulmV A Dur</b>	LN	59105-7	A-Wave Duration
	SRT	T-48581	Pulmonary Vein
	SRT	T-48530	Left Superior Pulmonary Vein
	UCUM	sec	Seconds
<b>LU PulmV A Vel</b>	LN	59079-4	Peak Reversal Velocity during Atrial Contraction
	SRT	T-48581	Pulmonary Vein
	SRT	T-48530	Left Superior Pulmonary Vein
	UCUM	cm/s	Centimeter Per Second
<b>LU PulmV Diam</b>	SRT	M-02550	Diameter
	SRT	T-48581	Pulmonary Vein

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	G-03A2	2D mode
	SRT	T-48530	Left Superior Pulmonary Vein
	UCUM	cm	Centimeter
<b>LU PulmV Dias Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48581	Pulmonary Vein
	SRT	T-48530	Left Superior Pulmonary Vein
	SRT	F-32011	End Diastole
	UCUM	cm/s	Centimeter Per Second
<b>LU PulmV S/D</b>	LN	12144-2	Systolic to Diastolic Velocity Ratio
	SRT	T-48581	Pulmonary Vein
	SRT	T-48530	Left Superior Pulmonary Vein
	UCUM	1	no units
<b>LU PulmV Sys Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48581	Pulmonary Vein
	SRT	T-48530	Left Superior Pulmonary Vein
	SRT	R-FAB5B	End Systole
	UCUM	cm/s	Centimeter Per Second
<b>LV Dp/dt</b>	LN	18035-6	Mitral Regurgitation dP/dt derived from Mitral Reg velocity
	SNM3	T-35300	Mitral Valve
	UCUM	mm[Hg]/s	mmHg/s
<b>LV ET (DOP)</b>	LN	20222-6	Ejection Time
	SRT	T-32600	Left Ventricle
	UCUM	sec	Seconds
<b>LV ET (MM)</b>	LN	20222-6	Ejection Time
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	UCUM	sec	Seconds
<b>LV FS (2D)</b>	LN	59132-1	Fractional Shortening
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	UCUM	%	Percent
<b>LV FS (MM)</b>	LN	59132-1	Fractional Shortening
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	UCUM	%	Percent
<b>LV Mass (A/L)</b>	DCM	125270	Left Ventricle Mass by Area Length
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	UCUM	g	Gram
<b>LV Mass (Cubed)</b>	LN	18087-7	Left Ventricle Mass
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125206	Cube Method
	UCUM	g	Gram
<b>LV Mass Index (A/L)</b>	99PMSBLUS	C12203-01	Left Ventricle Mass Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	LN	8277-6	Body Surface Area
	UCUM	g/m <sup>2</sup>	g/m <sup>2</sup>
<b>LV Mass Index(Cubed)</b>	99PMSBLUS	C12203-01	Left Ventricle Mass Index
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125206	Cube Method
	LN	8277-6	Body Surface Area
	UCUM	g/m <sup>2</sup>	g/m <sup>2</sup>
<b>LV MPI</b>	LN	59099-2	Myocardial Performance Index (Tei)
	SRT	T-32600	Left Ventricle
	UCUM	1	no units
<b>LV PEP</b>	LN	59085-1	Pre-Ejection Period
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	UCUM	sec	Seconds
<b>LV PEP/ET</b>	LN	59088-5	Pre-Ejection Period/Ejection Time Ratio
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	UCUM	1	no units
<b>LV PEPc</b>	LN	59087-7	Heart Rate-Corrected Pre-Ejection Period
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	UCUM	msec	Millisecond
<b>LV R-R (2D)</b>	LN	8867-4	Heart Rate
	SRT	T-32600	Left Ventricle
	UCUM	sec	Seconds
<b>LV R-R (MM)</b>	LN	8867-4	Heart Rate
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	UCUM	sec	Seconds
<b>LVAd (A/L)</b>	SRT	G-A166	Area
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125226	Single Plane Ellipse
	SRT	F-32011	End Diastole
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>LVAd (A2C-A/L)</b>	SRT	G-0375	Left Ventricular Diastolic Area
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125208	Method of Disks, Single Plane
	SRT	F-32011	End Diastole
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>LVAd (A4C-A/L)</b>	SRT	G-0375	Left Ventricular Diastolic Area
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125208	Method of Disks, Single Plane
	SRT	F-32011	End Diastole
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>LVAd Sax Endo Area</b>	LN	59094-3	Endocardial Area
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-039B	Parasternal short axis at the Papillary Muscle level
	SRT	F-32011	End Diastole
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>LVAd Sax Endo Circ</b>	99PMSBLUS	59094-3-1	Endocardial Circumference
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-039B	Parasternal short axis at the Papillary Muscle level
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVAd Sax Epi Area</b>	LN	59093-5	Epicardial Area
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-039B	Parasternal short axis at the Papillary Muscle level
	SRT	F-32011	End Diastole

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	UCUM	cm2	Square Centimeter
<b>LVAd Sax Epi Circ</b>	99PMSBLUS	59093-5-1	Epicardial Circumference
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-039B	Parasternal short axis at the Papillary Muscle level
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVAs (A/L)</b>	SRT	G-A166	Area
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125226	Single Plane Ellipse
	SRT	R-FAB5B	End Systole
	UCUM	cm2	Square Centimeter
<b>LVAs (A2C-A/L)</b>	SRT	G-0374	Left Ventricular Systolic Area
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125208	Method of Disks, Single Plane
	SRT	R-FAB5B	End systole
	UCUM	cm2	Square Centimeter
<b>LVAs (A4C-A/L)</b>	SRT	G-0374	Left Ventricular Systolic Area
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125208	Method of Disks, Single Plane
	SRT	R-FAB5B	End systole
	UCUM	cm2	Square Centimeter
<b>LVDP (AI)</b>	99PMSBLUS	C12212-02	Left Ventricle Diastolic Pressure with Aortic Insufficiency
	SRT	T-35400	Aortic Valve
	SRT	F-32011	End Diastole
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>LVED Major-A4C</b>	SRT	G-A193	Major Axis
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVED Minor-A4C</b>	SRT	G-A194	Minor Axis

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVED SAX CH</b>	DCM	121206	Distance
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-0399	Parasternal short axis at the level of the mitral chords
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVED SAX PM</b>	DCM	121206	Distance
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-039B	Parasternal short axis at the Papillary Muscle level
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVES Major-A4C</b>	SRT	G-A193	Major Axis
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>LVES Minor-A4C</b>	SRT	G-A194	Minor Axis
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>LVES SAX CH</b>	DCM	121206	Distance
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-0399	Parasternal short axis at the level of the mitral chords
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>LVES SAX PM</b>	DCM	121206	Distance
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	G-039B	Parasternal short axis at the Papillary Muscle level
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>LVETc</b>	LN	59086-9	Heart Rate-Corrected Ejection Time
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	UCUM	sec	Seconds
<b>LVIDd (2D)</b>	LN	59090-1	ROI Internal Dimension by US
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVIDd (MM)</b>	LN	59090-1	ROI Internal Dimension by US
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVIDs (2D)</b>	LN	59090-1	ROI Internal Dimension by US
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>LVIDs (MM)</b>	LN	59090-1	ROI Internal Dimension by US
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>LVLd (A/L)</b>	SRT	G-A193	Major Axis
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125226	Single Plane Ellipse
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVLd (A2C-A/L)</b>	LN	18077-8	Left Ventricle diastolic major axis
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125208	Method of Disks, Single Plane

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVLd (A2C-A/L)</b>	LN	18077-8	Left Ventricle diastolic major axis
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125208	Method of Disks, Single Plane
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVLd (A4C-A/L)</b>	LN	18077-8	Left Ventricle diastolic major axis
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125208	Method of Disks, Single Plane
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVLd Apical</b>	SRT	G-A193	Major Axis
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVLs (A/L)</b>	SRT	G-A193	Major Axis
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125226	Single Plane Ellipse
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>LVLs (A2C-A/L)</b>	LN	18076-0	Left Ventricle systolic major axis
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125208	Method of Disks, Single Plane
	SRT	R-FAB5B	End systole
	UCUM	cm	Centimeter
<b>LVLs (A2C-A/L)</b>	LN	18076-0	Left Ventricle systolic major axis
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	DCM	125208	Method of Disks, Single Plane
	SRT	R-FAB5B	End systole
	UCUM	cm	Centimeter
<b>LVLs (A4C-A/L)</b>	LN	18076-0	Left Ventricle systolic major axis
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125208	Method of Disks, Single Plane
	SRT	R-FAB5B	End systole
	UCUM	cm	Centimeter
<b>LVOT Accel Slope</b>	LN	20167-3	Acceleration Slope
	SRT	T-32600	Left Ventricle
	SRT	T-32650	Left Ventricle Outflow Tract
	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
<b>LVOT Accel Time</b>	LN	20168-1	Acceleration Time
	SRT	T-32600	Left Ventricle
	SRT	T-32650	Left Ventricle Outflow Tract
	UCUM	sec	Seconds
<b>LVOT Area</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-32600	Left Ventricle
	SRT	T-32650	Left Ventricle Outflow Tract
	UCUM	cm <sup>2</sup>	Square Centimeter
	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	T-32650	Left Ventricle Outflow Tract
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>LVOT Diam</b>	SRT	G-038F	Cardiovascular Orifice Diameter
	SRT	T-32600	Left Ventricle
	SRT	T-32650	Left Ventricle Outflow Tract
	UCUM	cm	Centimeter
<b>LVOT Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-32600	Left Ventricle
	SRT	T-32650	Left Ventricle Outflow Tract
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>LVOT Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-32600	Left Ventricle
	SRT	T-32650	Left Ventricle Outflow Tract

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>LVOT Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-32600	Left Ventricle
	SRT	T-32650	Left Ventricle Outflow Tract
	UCUM	cm/s	Centimeter Per Second
<b>LVOT Vmean</b>	LN	11692-1	Time Averaged Peak Velocity
	SRT	T-32600	Left Ventricle
	SRT	T-32650	Left Ventricle Outflow Tract
	UCUM	cm/s	Centimeter Per Second
<b>LVOT VTI</b>	LN	20354-7	Velocity Time Integral
	SRT	T-32600	Left Ventricle
	SRT	T-32650	Left Ventricle Outflow Tract
	UCUM	cm	Centimeter
<b>LVPW % (2D)</b>	LN	59092-7	% Thickening
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	99PMSBLUS	C12243-01	Left Ventricle Posterior Wall
	UCUM	%	Percent
<b>LVPW % (MM)</b>	LN	59092-7	% Thickening
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	99PMSBLUS	C12243-01	Left Ventricle Posterior Wall
	UCUM	%	Percent
<b>LVPWd (2D)</b>	LN	59089-3	ROI Thickness by US
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	R-42175	Posterior Wall
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVPWd (MM)</b>	LN	59089-3	ROI Thickness by US
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	SRT	R-42175	Posterior Wall
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>LVPWs (2D)</b>	LN	59089-3	ROI Thickness by US
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	R-42175	Posterior Wall
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>LVPWs (MM)</b>	LN	59089-3	ROI Thickness by US
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	SRT	R-42175	Posterior Wall
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>LVSP (AS)</b>	99PMSBLUS	C12212-01	Left Ventricle Systolic Pressure with Aortic Stenosis
	SRT	T-35400	Aortic Valve
	SRT	R-FAB5B	End Systole
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>Mean VCF</b>	LN	59117-2	Mean Velocity of Circumferential Fiber Shortening (Mean VcFv)
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	99PMSBLUS	circ/s	circ/s
<b>Mean VCFC</b>	LN	59118-0	HR-Corrected Mean Velocity of Circumferential Fiber Shortening
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	99PMSBLUS	circ/s	circ/s
<b>Med A` Area</b>	LN	59125-5	LV VTI A wave US
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0391	Medial Mitral Annulus
	UCUM	cm	Centimeter
<b>Med A` Vel</b>	LN	59133-9	Peak Tissue Velocity
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0391	Medial Mitral Annulus
	SRT	F-32030	Atrial Systole
	UCUM	cm/s	Centimeter Per Second
<b>Med Accel Time</b>	LN	20168-1	Acceleration Time
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0391	Medial Mitral Annulus
	UCUM	sec	Seconds
<b>Med Decel Time</b>	LN	20217-6	Deceleration Time

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0391	Medial Mitral Annulus
	UCUM	sec	Seconds
<b>Med E` Area</b>	LN	59124-8	LV VTI E wave US
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0391	Medial Mitral Annulus
	UCUM	cm	Centimeter
<b>Med E` Vel</b>	LN	59133-9	Peak Tissue Velocity
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0391	Medial Mitral Annulus
	SRT	R-40B1B	Early Diastole
	UCUM	cm/s	Centimeter Per Second
<b>Med IVCT</b>	LN	59084-4	Isovolumic Contraction Time
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0391	Medial Mitral Annulus
	UCUM	sec	Seconds
<b>Med IVRT</b>	LN	59083-6	Isovolumic Relaxation Time
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0391	Medial Mitral Annulus
	UCUM	sec	Seconds
<b>Med S Vel</b>	LN	59133-9	Peak Tissue Velocity
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0391	Medial Mitral Annulus
	SRT	R-FAB5B	End Systole
	UCUM	cm/s	Centimeter Per Second
<b>MPA Area</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-44100	Pulmonary Trunk
	SRT	G-03A2	2D mode
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>MPA Diam</b>	SRT	M-02550	Diameter
	SRT	T-44000	Pulmonary artery
	SRT	G-03A2	2D mode

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	UCUM	cm	Centimeter
<b>MPA Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-44100	Pulmonary Trunk
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>MPA Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-44100	Pulmonary Trunk
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>MPA Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-44100	Pulmonary Trunk
	UCUM	cm/s	Centimeter Per Second
<b>MR Alias Vel</b>	LN	59130-5	Alias velocity
	SRT	T-35300	Mitral Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm/s	Centimeter Per Second
<b>MR ERO</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35300	Mitral Valve
	DCM	125216	Proximal Isovelocity Surface Area
	SRT	G-0367	Regurgitant Flow
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>MR Flow Rate</b>	LN	34141-2	Peak Instantaneous Flow Rate
	SRT	T-35300	Mitral Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	ml/sec	ml/sec
<b>MR Fraction</b>	SRT	G-0390	Regurgitant Fraction
	SRT	T-35300	Mitral Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	%	Percent
<b>MR Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-35300	Mitral Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>MR Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-35300	Mitral Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>MR Radius</b>	LN	59102-4	Flow Radius
	SRT	T-35300	Mitral Valve
	SRT	G-03A2	2D mode

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	G-0367	Regurgitant Flow
	UCUM	cm	Centimeter
<b>MR Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-35300	Mitral Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm/s	Centimeter Per Second
<b>MR Vmean</b>	LN	11692-1	Time Averaged Peak Velocity
	SRT	T-35300	Mitral Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm/s	Centimeter Per Second
<b>MR Volume</b>	LN	33878-0	Volume Flow
	SRT	T-35300	Mitral Valve
	DCM	125216	Proximal Isovelocity Surface Area
	SRT	G-0367	Regurgitant Flow
	UCUM	ml	Milliliter
<b>MR VTI</b>	LN	20354-7	Velocity Time Integral
	SRT	T-35300	Mitral Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm	Centimeter
<b>MV A Dur</b>	LN	59105-7	A-Wave Duration
	SRT	T-35300	Mitral Valve
	UCUM	sec	Seconds
<b>MV A-C Interval</b>	LN	59103-2	A-C Interval
	SRT	T-35300	Mitral Valve
	SRT	G-0394	M mode
	UCUM	sec	Seconds
<b>MV Acc Slope</b>	LN	20167-3	Acceleration Slope
	SRT	T-35300	Mitral Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
<b>MV Acc Time</b>	LN	20168-1	Acceleration Time
	SRT	T-35300	Mitral Valve
	SRT	R-42047	Antegrade Flow
	UCUM	sec	Seconds
<b>MV Alias Vel</b>	LN	59130-5	Alias velocity
	SRT	T-35300	Mitral Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s	Centimeter Per Second

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
<b>MV Annul Area</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35300	Mitral Valve
	SRT	G-03A2	2D mode
	SRT	T-3500E	Cardiac valve annulus
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>MV Annul Diam</b>	SRT	M-02550	Diameter
	SRT	T-35300	Mitral Valve
	SRT	G-03A2	2D mode
	SRT	T-3500E	Cardiac valve annulus
	UCUM	cm	Centimeter
<b>MV Area</b>	SRT	G-A166	Area
	SRT	T-35300	Mitral Valve
	SRT	G-03A2	2D mode
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>MV Area (Ellipse)</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35300	Mitral Valve
	SRT	G-03A2	2D mode
	DCM	125211	Biplane Ellipse
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>MV Area (Planim)</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35300	Mitral Valve
	SRT	G-03A2	2D mode
	DCM	125220	Planimetry
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>MV Closure to Opening</b>	LN	59082-8	Closure to Opening Time
	SRT	T-35300	Mitral Valve
	UCUM	sec	Seconds
<b>MV D-E Exc Dist</b>	LN	59091-9	D-E Excursion
	SRT	T-35300	Mitral Valve
	SRT	G-0394	M mode
	UCUM	cm	Centimeter
<b>MV D-E Slope</b>	LN	59127-1	D-E Slope
	SRT	T-35300	Mitral Valve
	SRT	G-0394	M mode
	UCUM	cm/s	Centimeter Per Second
<b>MV Decel Slope</b>	LN	20216-8	Deceleration Slope
	SRT	T-35300	Mitral Valve
	SRT	R-42047	Antegrade Flow

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	UCUM	cm/s2	Centimeter Per Second Square
<b>MV Decel Time</b>	LN	20217-6	Deceleration Time
	SRT	T-35300	Mitral Valve
	SRT	R-42047	Antegrade Flow
	UCUM	sec	Seconds
<b>MV DFP</b>	SRT	R-0032C	Mitral Diastolic Filling Period (DFPm)
	SRT	T-35300	Mitral Valve
	UCUM	sec	Seconds
<b>MV Diam</b>	SRT	G-038F	Cardiovascular Orifice Diameter
	SRT	T-35300	Mitral Valve
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>MV E/A</b>	LN	59104-0	Peak E wave/Peak A wave by US
	SRT	T-35300	Mitral Valve
	SRT	P5-B0128	Tissue Doppler Imaging
	UCUM	1	no units
<b>MV E-E Sep</b>	LN	59098-4	Mitral Valve E-septal Separation
	SRT	T-35300	Mitral Valve
	SRT	G-0394	M mode
	UCUM	cm	Centimeter
<b>MV E-F Slope</b>	LN	59128-9	E-F Slope
	SRT	T-35300	Mitral Valve
	SRT	G-0394	M mode
	UCUM	cm/s	Centimeter Per Second
<b>MV EPSS</b>	LN	18036-4	Mitral Valve EPSS, E wave
	SRT	T-35300	Mitral Valve
	SRT	G-0394	M mode
	UCUM	cm	Centimeter
<b>MV Major</b>	SRT	G-A193	Major Axis
	SRT	T-35300	Mitral Valve
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>MV Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-35300	Mitral Valve
	SRT	R-42047	Antegrade Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>MV Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-35300	Mitral Valve

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	R-42047	Antegrade Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>MV Minor</b>	SRT	G-A194	Minor Axis
	SRT	T-35300	Mitral Valve
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>MV P1/2t</b>	LN	20280-4	Pressure Half-Time
	SRT	T-35300	Mitral Valve
	UCUM	msec	Millisecond
<b>MV Peak A Vel</b>	LN	59081-0	A-Wave Peak Velocity
	SRT	T-35300	Mitral Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s	Centimeter Per Second
<b>MV Peak E Vel</b>	LN	59080-2	E-Wave Peak Velocity
	SRT	T-35300	Mitral Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s	Centimeter Per Second
<b>MV Radius</b>	LN	59102-4	Flow Radius
	SRT	T-35300	Mitral Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm	Centimeter
<b>MV R-R (DOP)</b>	LN	8867-4	Heart Rate
	SRT	T-35300	Mitral Valve
	UCUM	sec	Seconds
<b>MV Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-35300	Mitral Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s	Centimeter Per Second
<b>MV Vmean</b>	LN	11692-1	Time Averaged Peak Velocity
	SRT	T-35300	Mitral Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s	Centimeter Per Second
<b>MV VTI</b>	LN	20354-7	Velocity Time Integral
	SRT	T-35300	Mitral Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm	Centimeter
<b>MVA (P<sup>1/2</sup>t)</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35300	Mitral Valve

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	DCM	125210	Area by Pressure Half-Time
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>MVA (PISA)</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35300	Mitral Valve
	DCM	125216	Proximal Isovelocity Surface Area
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>MVA (VTI)</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35300	Mitral Valve
	DCM	125215	Continuity Equation by Velocity Time Integral
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>MV-HR (DOP)</b>	LN	8867-4	Heart Rate
	SRT	T-35300	Mitral Valve
	UCUM	{H.B.}/min	Beats Per Minute
<b>PA Acc Time</b>	LN	20168-1	Acceleration Time
	SRT	T-44100	Pulmonary Trunk
	UCUM	sec	Seconds
<b>PAP (AT)</b>	LN	59101-6	Pulmonary Artery Pressure using Accel Time
	SRT	T-35200	Pulmonic Valve
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>PDA Diam</b>	SRT	M-02550	Diameter
	SRT	D4-32012	Patent Ductus Arteriosus
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>PDA Dias Vel</b>	LN	20351-3	Peak Velocity
	SRT	D4-32012	Patent Ductus Arteriosus
	SRT	F-32011	End Diastole
	UCUM	cm/s	Centimeter Per Second
<b>PDA Sys Vel</b>	LN	20351-3	Peak Velocity
	SRT	D4-32012	Patent Ductus Arteriosus
	SRT	R-FAB5B	End Systole
	UCUM	cm/s	Centimeter Per Second
<b>PDC Diam</b>	SRT	M-02550	Diameter
	SRT	T-D0878	Posterior Descending Coronary Artery
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>PI Decel Slope</b>	LN	20216-8	Deceleration Slope
	SRT	T-35200	Pulmonic Valve
	SRT	G-0367	Regurgitant Flow

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
<b>PI Decel Time</b>	LN	20217-6	Deceleration Time
	SRT	T-35200	Pulmonic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	sec	Seconds
<b>PI End Dias Vel</b>	LN	11653-3	End Diastolic Velocity
	SRT	T-35200	Pulmonic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm/s	Centimeter Per Second
<b>PI P1/2t</b>	LN	20280-4	Pressure Half-Time
	SRT	T-35200	Pulmonic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	msec	Millisecond
<b>PI P1/2t Vmax</b>	99PMSBLUS	C12222-03	Pressure Half-Time Peak velocity
	SRT	T-35200	Pulmonic Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm/s	Centimeter Per Second
<b>PISA (AI)</b>	LN	20226-7	Flow Area
	SRT	T-35400	Aortic Valve
	DCM	125216	Proximal Isovelocity Surface Area
	SRT	G-0367	Regurgitant Flow
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>PISA (MR)</b>	LN	20226-7	Flow Area
	SRT	T-35300	Mitral Valve
	DCM	125216	Proximal Isovelocity Surface Area
	SRT	G-0367	Regurgitant Flow
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>PISA (TR)</b>	LN	20226-7	Flow Area
	SRT	T-35100	Tricuspid Valve
	DCM	125216	Proximal Isovelocity Surface Area
	SRT	G-0367	Regurgitant Flow
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>Pulm V S/D</b>	LN	12144-2	Systolic to Diastolic Velocity Ratio
	SRT	T-48581	Pulmonary Vein
	UCUM	1	no units
<b>PulmV A Dur</b>	LN	59105-7	A-Wave Duration
	SRT	T-48581	Pulmonary Vein
	UCUM	sec	Seconds

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
<b>PulmV A Vel</b>	LN	59079-4	Peak Reversal Velocity during Atrial Contraction
	SRT	T-48581	Pulmonary Vein
	UCUM	cm/s	Centimeter Per Second
<b>PulmV Dias Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48581	Pulmonary Vein
	SRT	F-32011	End Diastole
	UCUM	cm/s	Centimeter Per Second
<b>PulmV Sys Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48581	Pulmonary Vein
	SRT	R-FAB5B	End Systole
	UCUM	cm/s	Centimeter Per Second
<b>PV Acc Slope</b>	LN	20167-3	Acceleration Slope
	SRT	T-35200	Pulmonic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
<b>PV Acc Time</b>	LN	20168-1	Acceleration Time
	SRT	T-35200	Pulmonic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	sec	Seconds
<b>PV Annul Diam</b>	SRT	M-02550	Diameter
	SRT	T-35200	Pulmonic Valve
	SRT	G-03A2	2D mode
	SRT	T-3500E	Cardiac valve annulus
	UCUM	cm	Centimeter
<b>PV Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-35200	Pulmonic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>PV Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-35200	Pulmonic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>PV R-R (DOP)</b>	LN	8867-4	Heart Rate
	SRT	T-35200	Pulmonic Valve
	UCUM	sec	Seconds
<b>PV R-R (MM)</b>	LN	8867-4	Heart Rate
	SRT	T-35200	Pulmonic Valve
	SRT	G-0394	M mode

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	UCUM	sec	Seconds
<b>PV Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-35200	Pulmonic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s	Centimeter Per Second
<b>PV Vmean</b>	LN	11692-1	Time Averaged Peak Velocity
	SRT	T-35200	Pulmonic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s	Centimeter Per Second
<b>PV VTI</b>	LN	20354-7	Velocity Time Integral
	SRT	T-35200	Pulmonic Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm	Centimeter
<b>PVA (Vmax)</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35200	Pulmonic Valve
	DCM	125214	Continuity Equation by Peak Velocity
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>PVA (VTI)</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35200	Pulmonic Valve
	DCM	125215	Continuity Equation by Velocity Time Integral
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>PV-HR (DOP)</b>	LN	8867-4	Heart Rate
	SRT	T-35200	Pulmonic Valve
	UCUM	{H.B.}/min	Beats Per Minute
<b>PV-HR (MM)</b>	LN	8867-4	Heart Rate
	SRT	T-35200	Pulmonic Valve
	SRT	G-0394	M mode
	UCUM	{H.B.}/min	Beats Per Minute
<b>Qp/Qs</b>	LN	29462-9	Pulmonary-to-Systemic Shunt Flow Ratio
	SRT	P5-30031	Cardiac Shunt Study
	UCUM	1	no units
<b>R to AV Closure</b>	99PMSBLUS	C12211-07	R Wave to Aortic Valve Closure Time
	SRT	T-35400	Aortic Valve
	UCUM	msec	Millisecond
<b>R to AV Open</b>	99PMSBLUS	C12211-06	R Wave to Aortic Valve Opening Time
	SRT	T-35400	Aortic Valve
	UCUM	msec	Millisecond
<b>R to MV Closure</b>	99PMSBLUS	C12207-42	R Wave to Mitral Valve Closure Time

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	T-35300	Mitral Valve
	UCUM	msec	Millisecond
<b>R to MV Open</b>	99PMSBLUS	C12207-41	R Wave to Mitral Valve Opening Time
	SRT	T-35300	Mitral Valve
	UCUM	msec	Millisecond
<b>RA Dimen (2D)</b>	LN	59090-1	ROI Internal Dimension by US
	SRT	T-32200	Right Atrium
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>RA Dimen (MM)</b>	LN	59090-1	ROI Internal Dimension by US
	SRT	T-32200	Right Atrium
	SRT	G-0394	M mode
	UCUM	cm	Centimeter
<b>RA Pressure</b>	LN	18070-3	Right Atrium Systolic Pressure
	SRT	T-32200	Right Atrium
	SRT	R-FAB5B	End Systole
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>RAED Major-A4C</b>	SRT	G-A193	Major Axis
	SRT	T-32200	Right Atrium
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>RAED Minor-A4C</b>	SRT	G-A194	Minor Axis
	SRT	T-32200	Right Atrium
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>RAES Major-A4C</b>	SRT	G-A193	Major Axis
	SRT	T-32200	Right Atrium
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>RAES Minor-A4C</b>	SRT	G-A194	Minor Axis
	SRT	T-32200	Right Atrium
	SRT	G-03A2	2D mode

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	G-A19C	Apical four chamber
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>RCA Diam</b>	SRT	M-02550	Diameter
	SRT	T-43203	Right Coronary Artery
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>RL PulmV A Dur</b>	LN	59105-7	A-Wave Duration
	SRT	T-48581	Pulmonary Vein
	SRT	T-48520	Right Inferior Pulmonary Vein
	UCUM	sec	Seconds
<b>RL PulmV A Vel</b>	LN	59079-4	Peak Reversal Velocity during Atrial Contraction
	SRT	T-48581	Pulmonary Vein
	SRT	T-48520	Right Inferior Pulmonary Vein
	UCUM	cm/s	Centimeter Per Second
<b>RL PulmV Diam</b>	SRT	M-02550	Diameter
	SRT	T-48581	Pulmonary Vein
	SRT	G-03A2	2D mode
	SRT	T-48520	Right Inferior Pulmonary Vein
	UCUM	cm	Centimeter
<b>RL PulmV Dias Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48581	Pulmonary Vein
	SRT	T-48520	Right Inferior Pulmonary Vein
	SRT	F-32011	End Diastole
	UCUM	cm/s	Centimeter Per Second
<b>RL PulmV S/D</b>	LN	12144-2	Systolic to Diastolic Velocity Ratio
	SRT	T-48581	Pulmonary Vein
	SRT	T-48520	Right Inferior Pulmonary Vein
	UCUM	1	no units
<b>RL PulmV Sys Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48581	Pulmonary Vein
	SRT	T-48520	Right Inferior Pulmonary Vein
	SRT	R-FAB5B	End Systole
	UCUM	cm/s	Centimeter Per Second
<b>RPA Diam</b>	SRT	M-02550	Diameter
	SRT	T-44000	Pulmonary artery
	SRT	G-03A2	2D mode
	SRT	T-44200	Right pulmonary artery

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	UCUM	cm	Centimeter
<b>RPA Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-44000	Pulmonary artery
	SRT	T-44200	Right pulmonary artery
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>RPA Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-44000	Pulmonary artery
	SRT	T-44200	Right pulmonary artery
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>RPA Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-44000	Pulmonary artery
	SRT	T-44200	Right pulmonary artery
	UCUM	cm/s	Centimeter Per Second
<b>RU PulmV A Dur</b>	LN	59105-7	A-Wave Duration
	SRT	T-48581	Pulmonary Vein
	SRT	T-48510	Right Superior Pulmonary Vein
	UCUM	sec	Seconds
<b>RU PulmV A Vel</b>	LN	59079-4	Peak Reversal Velocity during Atrial Contraction
	SRT	T-48581	Pulmonary Vein
	SRT	T-48510	Right Superior Pulmonary Vein
	UCUM	cm/s	Centimeter Per Second
<b>RU PulmV Diam</b>	SRT	M-02550	Diameter
	SRT	T-48581	Pulmonary Vein
	SRT	G-03A2	2D mode
	SRT	T-48510	Right Superior Pulmonary Vein
	UCUM	cm	Centimeter
<b>RU PulmV Dias Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48581	Pulmonary Vein
	SRT	T-48510	Right Superior Pulmonary Vein
	SRT	F-32011	End Diastole
	UCUM	cm/s	Centimeter Per Second
<b>RU PulmV S/D</b>	LN	12144-2	Systolic to Diastolic Velocity Ratio
	SRT	T-48581	Pulmonary Vein
	SRT	T-48510	Right Superior Pulmonary Vein
	UCUM	1	no units
<b>RU PulmV Sys Vel</b>	LN	20351-3	Peak Velocity
	SRT	T-48581	Pulmonary Vein
	SRT	T-48510	Right Superior Pulmonary Vein

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	R-FAB5B	End Systole
	UCUM	cm/s	Centimeter Per Second
<b>RV ET (DOP)</b>	LN	20222-6	Ejection Time
	SRT	T-32500	Right Ventricle
	UCUM	sec	Seconds
<b>RV ET (MM)</b>	LN	20222-6	Ejection Time
	SRT	T-32500	Right Ventricle
	SRT	G-0394	M mode
	UCUM	sec	Seconds
<b>RV MPI</b>	LN	59099-2	Myocardial Performance Index (Tei)
	SRT	T-32500	Right Ventricle
	UCUM	1	no units
<b>RV PEP</b>	LN	59085-1	Pre-Ejection Period
	SRT	T-32500	Right Ventricle
	SRT	G-0394	M mode
	UCUM	sec	Seconds
<b>RV PEP/ET</b>	LN	59088-5	Pre-Ejection Period/Ejection Time Ratio
	SRT	T-32500	Right Ventricle
	SRT	G-0394	M mode
	UCUM	1	no units
<b>RV PEPc</b>	LN	59087-7	Heart Rate-Corrected Pre-Ejection Period
	SRT	T-32500	Right Ventricle
	SRT	G-0394	M mode
	UCUM	msec	Millisecond
<b>RVAWd (2D)</b>	LN	59089-3	ROI Thickness by US
	SRT	T-32500	Right Ventricle
	SRT	G-03A2	2D mode
	SRT	R-4210B	Anterior Wall
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>RVAWd (MM)</b>	LN	59089-3	ROI Thickness by US
	SRT	T-32500	Right Ventricle
	SRT	G-0394	M mode
	SRT	R-4210B	Anterior Wall
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>RVED Major-A4C</b>	SRT	G-A193	Major Axis
	SRT	T-32500	Right Ventricle

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>RVED Minor-A4C</b>	SRT	G-A194	Minor Axis
	SRT	T-32500	Right Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>RVES Major-A4C</b>	SRT	G-A193	Major Axis
	SRT	T-32500	Right Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>RVES Minor-A4C</b>	SRT	G-A194	Minor Axis
	SRT	T-32500	Right Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	SRT	R-FAB5B	End Systole
	UCUM	cm	Centimeter
<b>RVIDd (2D)</b>	LN	59090-1	ROI Internal Dimension by US
	SRT	T-32500	Right Ventricle
	SRT	G-03A2	2D mode
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>RVIDd (MM)</b>	LN	59090-1	ROI Internal Dimension by US
	SRT	T-32500	Right Ventricle
	SRT	G-0394	M mode
	SRT	F-32011	End Diastole
	UCUM	cm	Centimeter
<b>RVOT Acc Slope</b>	LN	20167-3	Acceleration Slope
	SRT	T-32500	Right Ventricle
	SRT	T-32550	Right Ventricle Outflow Tract
	UCUM	cm/s <sup>2</sup>	Centimeter Per Second Square
<b>RVOT Acc Time</b>	LN	20168-1	Acceleration Time
	SRT	T-32500	Right Ventricle

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	T-32550	Right Ventricle Outflow Tract
	UCUM	sec	Seconds
<b>RVOT Area</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-32500	Right Ventricle
	SRT	G-03A2	2D mode
	SRT	T-32550	Right Ventricle Outflow Tract
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>RVOT Diam</b>	SRT	G-038F	Cardiovascular Orifice Diameter
	SRT	T-32500	Right Ventricle
	SRT	G-03A2	2D mode
	SRT	T-32550	Right Ventricle Outflow Tract
	UCUM	cm	Centimeter
<b>RVOT Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-32500	Right Ventricle
	SRT	T-32550	Right Ventricle Outflow Tract
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>RVOT Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-32500	Right Ventricle
	SRT	T-32550	Right Ventricle Outflow Tract
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>RVOT Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-32500	Right Ventricle
	SRT	T-32550	Right Ventricle Outflow Tract
	UCUM	cm/s	Centimeter Per Second
<b>RVOT Vmean</b>	LN	11692-1	Time Averaged Peak Velocity
	SRT	T-32500	Right Ventricle
	SRT	T-32550	Right Ventricle Outflow Tract
	UCUM	cm/s	Centimeter Per Second
<b>RVOT VTI</b>	LN	20354-7	Velocity Time Integral
	SRT	T-32500	Right Ventricle
	SRT	T-32550	Right Ventricle Outflow Tract
	UCUM	cm	Centimeter
<b>RVSP</b>	SRT	G-0380	Right Ventricular Peak Systolic Pressure
	SRT	T-32500	Right Ventricle
	SRT	R-FAB5B	End Systole
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>RVSP (VSD)</b>	SRT	F-31000	Blood Pressure
	SRT	D4-31150	Ventricular Septal Defect

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	R-FAB5B	End Systole
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>SI (2D-Cubed)</b>	SRT	F-00078	Stroke Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125206	Cube Method
	UCUM	ml/m2	ml/m2
<b>SI (2D-Teich)</b>	SRT	F-00078	Stroke Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125209	Teichholz
	UCUM	ml/m2	ml/m2
<b>SI (A/L)</b>	SRT	F-00078	Stroke Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125226	Single Plane Ellipse
	UCUM	ml/m2	ml/m2
<b>SI (A2C)</b>	SRT	F-00078	Stroke Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125208	Method of Disks, Single Plane
	UCUM	ml/m2	ml/m2
<b>SI (A2C-A/L)</b>	SRT	F-00078	Stroke Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125226	Single Plane Ellipse
	UCUM	ml/m2	ml/m2
<b>SI (A4C)</b>	SRT	F-00078	Stroke Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125208	Method of Disks, Single Plane
	UCUM	ml/m2	ml/m2
<b>SI (A4C-A/L)</b>	SRT	F-00078	Stroke Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	G-A19C	Apical four chamber
	DCM	125226	Single Plane Ellipse
	UCUM	ml/m2	ml/m2
<b>SI (BP)</b>	SRT	F-00078	Stroke Index
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125207	Method of Disks, Biplane
	UCUM	ml/m2	ml/m2
<b>SI (MM-Cubed)</b>	SRT	F-00078	Stroke Index
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125206	Cube Method
	UCUM	ml/m2	ml/m2
<b>SI (MM-Teich)</b>	SRT	F-00078	Stroke Index
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125209	Teichholz
	UCUM	ml/m2	ml/m2
<b>SV (2D-Cubed)</b>	SRT	F-32120	Stroke Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125206	Cube Method
	UCUM	ml	Milliliter
<b>SV (2D-Teich)</b>	SRT	F-32120	Stroke Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125209	Teichholz
	UCUM	ml	Milliliter
<b>SV (A/L)</b>	SRT	F-32120	Stroke Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125226	Single Plane Ellipse
	UCUM	ml	Milliliter
<b>SV (A2C)</b>	SRT	F-32120	Stroke Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125208	Method of Disks, Single Plane

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	UCUM	ml	Milliliter
<b>SV (A2C-A/L)</b>	SRT	F-32120	Stroke Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19B	Apical two chamber
	DCM	125226	Single Plane Ellipse
	UCUM	ml	Milliliter
<b>SV (A4C)</b>	SRT	F-32120	Stroke Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125208	Method of Disks, Single Plane
	UCUM	ml	Milliliter
<b>SV (A4C-A/L)</b>	SRT	F-32120	Stroke Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	SRT	G-A19C	Apical four chamber
	DCM	125226	Single Plane Ellipse
	UCUM	ml	Milliliter
<b>SV (BP)</b>	SRT	F-32120	Stroke Volume
	SRT	T-32600	Left Ventricle
	SRT	G-03A2	2D mode
	DCM	125207	Method of Disks, Biplane
	UCUM	ml	Milliliter
<b>SV (LVOT)</b>	SRT	F-32120	Stroke Volume
	SRT	T-32600	Left Ventricle
	SRT	T-32650	Left Ventricle Outflow Tract
	UCUM	ml	Milliliter
<b>SV (MM-Cubed)</b>	SRT	F-32120	Stroke Volume
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125206	Cube Method
	UCUM	ml	Milliliter
<b>SV (MM-Teich)</b>	SRT	F-32120	Stroke Volume
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	DCM	125209	Teichholz
	UCUM	ml	Milliliter

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
<b>SV (MV)</b>	SRT	F-32120	Stroke Volume
	SRT	T-35300	Mitral Valve
	UCUM	ml	Milliliter
<b>SV (PV)</b>	SRT	F-32120	Stroke Volume
	SRT	T-35200	Pulmonic Valve
	UCUM	ml	Milliliter
<b>SV (RVOT)</b>	SRT	F-32120	Stroke Volume
	SRT	T-32500	Right Ventricle
	SRT	T-32550	Right Ventricle Outflow Tract
	UCUM	ml	Milliliter
<b>SV (TV)</b>	SRT	F-32120	Stroke Volume
	SRT	T-35100	Tricuspid Valve
	UCUM	ml	Milliliter
<b>SVC A Dur</b>	LN	59105-7	A-Wave Duration
	SRT	M-2460D	Right Superior vena cava
	UCUM	sec	Seconds
<b>SVC A Vel</b>	LN	59079-4	Peak Reversal Velocity during Atrial Contraction
	SRT	M-2460D	Right Superior vena cava
	UCUM	cm/s	Centimeter Per Second
<b>SVC Diam</b>	SRT	M-02550	Diameter
	SRT	M-2460D	Right Superior vena cava
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>SVC Dias Vel</b>	LN	20351-3	Peak Velocity
	SRT	M-2460D	Right Superior vena cava
	SRT	F-32011	End Diastole
	UCUM	cm/s	Centimeter Per Second
<b>SVC S/D</b>	LN	12144-2	Systolic to Diastolic Velocity Ratio
	SRT	M-2460D	Right Superior vena cava
	UCUM	1	no units
<b>SVC Sys Vel</b>	LN	20351-3	Peak Velocity
	SRT	M-2460D	Right Superior vena cava
	SRT	R-FAB5B	End Systole
	UCUM	cm/s	Centimeter Per Second
<b>Tei Index</b>	LN	59099-2	Myocardial Performance Index (Tei)
	SRT	T-35300	Mitral Valve
	UCUM	1	no units
<b>Time to Lat E`</b>	LN	59096-8	Time to Left Ventricle E Tissue Velocity

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0392	Lateral Mitral Annulus
	UCUM	sec	Seconds
<b>Time to Lat S</b>	LN	59095-0	Time to Left Ventricle S Tissue Velocity
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0392	Lateral Mitral Annulus
	UCUM	sec	Seconds
<b>Time to Med E`</b>	LN	59096-8	Time to Left Ventricle E Tissue Velocity
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0391	Medial Mitral Annulus
	UCUM	sec	Seconds
<b>Time to Med S</b>	LN	59095-0	Time to Left Ventricle S Tissue Velocity
	SRT	T-32600	Left Ventricle
	SRT	P5-B0128	Tissue Doppler Imaging
	SRT	G-0391	Medial Mitral Annulus
	UCUM	sec	Seconds
<b>TR Alias Vel</b>	LN	59130-5	Alias velocity
	SRT	T-35100	Tricuspid Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm/s	Centimeter Per Second
<b>TR ERO</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35100	Tricuspid Valve
	DCM	125216	Proximal Isovelocity Surface Area
	SRT	G-0367	Regurgitant Flow
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>TR Flow Rate</b>	LN	34141-2	Peak Instantaneous Flow Rate
	SRT	T-35100	Tricuspid Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	ml/sec	ml/sec
<b>TR Fraction</b>	SRT	G-0390	Regurgitant Fraction
	SRT	T-35100	Tricuspid Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	%	Percent
<b>TR Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-35100	Tricuspid Valve

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	G-0367	Regurgitant Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>TR Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-35100	Tricuspid Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>TR Radius</b>	LN	59102-4	Flow Radius
	SRT	T-35100	Tricuspid Valve
	SRT	G-03A2	2D mode
	SRT	G-0367	Regurgitant Flow
	UCUM	cm	Centimeter
<b>TR Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-35100	Tricuspid Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm/s	Centimeter Per Second
<b>TR Vmean</b>	LN	11692-1	Time Averaged Peak Velocity
	SRT	T-35100	Tricuspid Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm/s	Centimeter Per Second
<b>TR Volume</b>	LN	33878-0	Volume Flow
	SRT	T-35100	Tricuspid Valve
	DCM	125216	Proximal Isovelocity Surface Area
	SRT	G-0367	Regurgitant Flow
	UCUM	ml	Milliliter
<b>TR VTI</b>	LN	20354-7	Velocity Time Integral
	SRT	T-35100	Tricuspid Valve
	SRT	G-0367	Regurgitant Flow
	UCUM	cm	Centimeter
<b>TV A Dur</b>	LN	59105-7	A-Wave Duration
	SRT	T-35100	Tricuspid Valve
	UCUM	sec	Seconds
<b>TV A-C Interval</b>	LN	59103-2	A-C Interval
	SRT	T-35100	Tricuspid Valve
	SRT	G-0394	M mode
	UCUM	sec	Seconds
<b>TV Acc Slope</b>	LN	20167-3	Acceleration Slope
	SRT	T-35100	Tricuspid Valve
	SRT	R-42047	Antegrade Flow

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	UCUM	cm/s2	Centimeter Per Second Square
<b>TV Acc Time</b>	LN	20168-1	Acceleration Time
	SRT	T-35100	Tricuspid Valve
	SRT	R-42047	Antegrade Flow
	UCUM	sec	Seconds
<b>TV Alias Vel</b>	LN	59130-5	Alias velocity
	SRT	R-42047	Antegrade Flow
	SRT	T-35100	Tricuspid Valve
	UCUM	cm/s	Centimeter Per Second
<b>TV Annul Area</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35100	Tricuspid Valve
	SRT	G-03A2	2D mode
	SRT	T-3500E	Cardiac valve annulus
	UCUM	cm2	Square Centimeter
<b>TV Annul Diam</b>	SRT	M-02550	Diameter
	SRT	T-35100	Tricuspid Valve
	SRT	G-03A2	2D mode
	SRT	T-3500E	Cardiac valve annulus
	UCUM	cm	Centimeter
<b>TV Area</b>	SRT	G-A166	Area
	SRT	T-35100	Tricuspid Valve
	SRT	G-03A2	2D mode
	UCUM	cm2	Square Centimeter
<b>TV Closure to Opening</b>	LN	59082-8	Closure to Opening Time
	SRT	T-35100	Tricuspid Valve
	UCUM	sec	Seconds
<b>TV D-E Exc Dist</b>	LN	59091-9	D-E Excursion
	SRT	T-35100	Tricuspid Valve
	SRT	G-0394	M mode
	UCUM	cm	Centimeter
<b>TV D-E Slope</b>	LN	59127-1	D-E Slope
	SRT	T-35100	Tricuspid Valve
	SRT	G-0394	M mode
	UCUM	cm/s	Centimeter Per Second
<b>TV Decel Slope</b>	LN	20216-8	Deceleration Slope
	SRT	T-35100	Tricuspid Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s2	Centimeter Per Second Square

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
<b>TV Decel Time</b>	LN	20217-6	Deceleration Time
	SRT	T-35100	Tricuspid Valve
	SRT	R-42047	Antegrade Flow
	UCUM	sec	Seconds
<b>TV DFP</b>	SRT	R-003A9	Tricuspid Diastolic Filling Period (DFPt)
	SRT	T-35100	Tricuspid Valve
	UCUM	sec	Seconds
<b>TV Diam</b>	SRT	G-038F	Cardiovascular Orifice Diameter
	SRT	T-35100	Tricuspid Valve
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>TV E/A</b>	LN	59104-0	Peak E wave/Peak A wave by US
	SRT	T-35100	Tricuspid Valve
	UCUM	1	no units
<b>TV E-F Slope</b>	LN	59128-9	E-F Slope
	SRT	T-35100	Tricuspid Valve
	SRT	G-0394	M mode
	UCUM	cm/s	Centimeter Per Second
<b>TV Max PG</b>	LN	20247-3	Peak Gradient
	SRT	T-35100	Tricuspid Valve
	SRT	R-42047	Antegrade Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>TV Mean PG</b>	LN	20256-4	Mean Gradient
	SRT	T-35100	Tricuspid Valve
	SRT	R-42047	Antegrade Flow
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>TV P1/2t</b>	LN	20280-4	Pressure Half-Time
	SRT	T-35100	Tricuspid Valve
	UCUM	msec	Millisecond
<b>TV P1/2t Vmax</b>	99PMSBLUS	C12222-03	Pressure Half-Time Peak velocity
	SRT	T-35100	Tricuspid Valve
	UCUM	cm/s	Centimeter Per Second
<b>TV Peak A Vel</b>	LN	59081-0	A-Wave Peak Velocity
	SRT	T-35100	Tricuspid Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s	Centimeter Per Second
<b>TV Peak E Vel</b>	LN	59080-2	E-Wave Peak Velocity
	SRT	T-35100	Tricuspid Valve

<b>ClearVue 350/550/650/850 3.1 Report Label</b>	<b>CSD</b>	<b>CV</b>	<b>CM</b>
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s	Centimeter Per Second
<b>TV Radius</b>	LN	59102-4	Flow Radius
	SRT	T-35100	Tricuspid Valve
	SRT	G-03A2	2D mode
	SRT	R-42047	Antegrade Flow
	UCUM	cm	Centimeter
<b>TV R-R (DOP)</b>	LN	8867-4	Heart Rate
	SRT	T-35100	Tricuspid Valve
	UCUM	sec	Seconds
<b>TV Vmax</b>	LN	20351-3	Peak Velocity
	SRT	T-35100	Tricuspid Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s	Centimeter Per Second
<b>TV Vmean</b>	LN	11692-1	Time Averaged Peak Velocity
	SRT	T-35100	Tricuspid Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm/s	Centimeter Per Second
<b>TV VTI</b>	LN	20354-7	Velocity Time Integral
	SRT	T-35100	Tricuspid Valve
	SRT	R-42047	Antegrade Flow
	UCUM	cm	Centimeter
<b>TVA (PISA)</b>	SRT	G-038E	Cardiovascular Orifice Area
	SRT	T-35100	Tricuspid Valve
	DCM	125216	Proximal Isovelocity Surface Area
	UCUM	cm <sup>2</sup>	Square Centimeter
<b>TV-HR (DOP)</b>	LN	8867-4	Heart Rate
	SRT	T-35100	Tricuspid Valve
	UCUM	{H.B.}/min	Beats Per Minute
<b>VSD Diam</b>	SRT	M-02550	Diameter
	SRT	D4-31150	Ventricular Septal Defect
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>VSD Major</b>	SRT	G-A193	Major Axis
	SRT	D4-31150	Ventricular Septal Defect
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>VSD Max PG</b>	LN	20247-3	Peak Gradient

ClearVue 350/550/650/850 3.1 Report Label	CSD	CV	CM
	SRT	D4-31150	Ventricular Septal Defect
	UCUM	mm[Hg]	Millimeters Of Mercury
<b>VSD Minor</b>	SRT	G-A194	Minor Axis
	SRT	D4-31150	Ventricular Septal Defect
	SRT	G-03A2	2D mode
	UCUM	cm	Centimeter
<b>VSD Vmax</b>	LN	20351-3	Peak Velocity
	SRT	D4-31150	Ventricular Septal Defect
	UCUM	cm/s	Centimeter Per Second
<b>Wall Stress</b>	LN	59097-6	Left Ventricle Meridional Wall Stress
	SRT	T-32600	Left Ventricle
	SRT	G-0394	M mode
	UCUM	kg/m2	kg/m2

#### A.5.3 Pediatric Echo Meas/Calcs NOT exported in Dicom

The following labels are not exported in DICOM Structured Reports for Pediatric Echo

ClearVue 350/550/650/850 3.1 Label
Ped AI End Dias PG
Ped AI PHalfT-DopSlope
Ped AI PHalfT-DopTime
Ped AI PHalfT-MaxPG
Ped AI PHalfT-Vmax
Ped B-C Slope-Dist
Ped B-C Slope-MMTime
Dist L PulmA Diam
Ped Dist L PulmA MaxPG
Ped Dist L PulmA Vmax
Dist R PulmA Diam
Ped Dist R PulmA MaxPG
Ped Dist R PulmA Vmax
m_p_IVC_ARevsVel_PG
m_p_IVC_DiasVel_PG
m_p_IVC_SysVel_PG
Ped Late Dias Slope-Dist
Ped Late Dias Slope-MMTime
Ped LV LdApical Area
Ped MV DE Exc MMTime

Ped MV DE Dist
Ped MV DE MMTime
MV PHalfT-DopSlope
MV PHalfT-DopTime
Ped PDA DiasVel PG
Ped PI End Dias PG
Ped PI PHalfT-DopSlope
Ped PI PHalfT-DopTime
Ped PI PHalfT-MaxPG
Hep. A Revs Vel-PG
m_p_SVC_DiasVel_PG
m_p_SVC_SysVel_PG
Ped TV D-E Exc-MMTime
Ped TV DE Distance
Ped TV DE MMTime
m_p_TV_PeakAVel_PG
m_p_TV_PeakEVel_PG
Ped TV PHalfT-DopSlope
Ped TV PHalfT-DopTime
Ped TV PHalfT-MaxPG

## APPENDIX B – BULK PRIVATE TAGS

### B.1 BULK PRIVATE TAGS

The private tags listed below are intended to provide awareness of large data sets of private data from ClearVue 350/550/650/850 3.1 datasets

Attribute Name	DICOM Tag	VR	Description
Private Data	200D,300E	OB	Bulk data
Private Data	200D,300B	OB	Bulk data
Private Data	200D,3CF3	OB	Bulk data

## APPENDIX C – Generic Angle Measurements

### C.1 GENERIC ANGLE MEASUREMENTS

ClearVue 350/550/650/850 3.1 uses a private tag to include all generic angle measurements except *Lung Angle* available on ClearVue 350/550/650/850 3.1 datasets as part of TID 5000/TID 5100 Template. All private extensions will use the coding scheme designator as 99PMSBLUS.

The following angle measurements are currently supported.

- Liver vasculature (Abdomen Gen) - Used to measure angles between vasculature such as portal veins and hepatic veins for planning for surgical shunts and planning for procedures such as biopsies.
- Lung angle measurement (Abdomen Gen) - Used to measure angles between the costal and diaphragmatic parietal pleura as they meet at the costodiaphragmatic line of pleura reflection.
- Frontomaxillary facial angle (OB, first trimester) – Used to measure on a midline sagittal view by creating a line along the maxilla and a second line along the axis of the frontal bone.
- Inferior facial angle (OB, first and second trimester) - Used to measure on a midline sagittal view by creating a line orthogonal to the vertical part of the forehead at the level of the nasal bones and a second line joining the tip of the mentum and anterior border of the more protruding lip.
- Iliac angle (OB, second trimester) - Used to measure in axial view at level of iliac wings. Create one line from vertebral body to left iliac wing, second line from vertebral body to right iliac wing.
- Heart axis (OB, second trimester) - Used to measure on Axial view at level of 4 chamber view.
- Head Angle (OB) – Used to measure the head descent angle during labor.

CSD	CV	Code Meaning
99PMSBLUS	C12221-05	Liver Vasc Angle
SRT	T-28000	Lung Angle
99PMSBLUS	C12005-11	Frontomaxillary Facial Angle
99PMSBLUS	C12005-13	Inferior Facial Angle
99PMSBLUS	C12005-15	Iliac Angle
99PMSBLUS	C12005-17	Heart Axis Angle
99PMSBLUS	C12019-06	Head Angle

\*\*\*\*\* End of Document \*\*\*\*\*