


# DICOM Conformance Statement

## Azurion R3.1

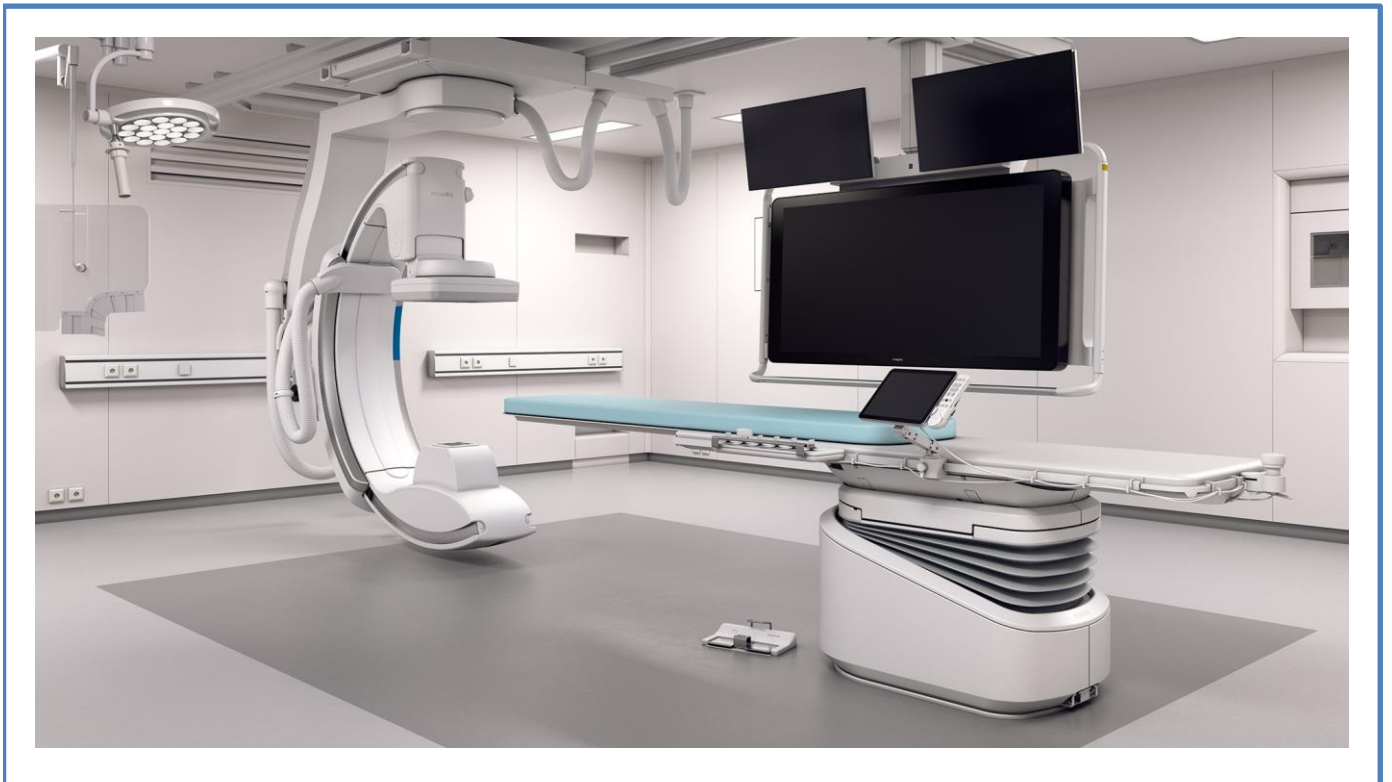

*- This page is left intentionally empty -*

## 1. DICOM Conformance Statement Overview

Azurion R3.1 system is an interventional X-ray system that is used to perform:

- Image guidance during diagnostic, interventional and minimally invasive surgery procedures for the following clinical application areas: vascular, non-vascular, cardiovascular and neuro procedures
- Cardiac imaging applications including diagnostics, interventional and minimally invasive surgery procedures

It provides the following DICOM data exchange features:

- Query the MWL SCP for a Modality Worklist (MWL)
- Update the Modality Performed Procedure Step (MPPS).
- Transfer of DICOM Images and Grayscale Presentation States.
- Query/Retrieve a Workstation or PACS for a list of entries representing Series information of DICOM Images
- Send Storage Commitment to the PACS (for the safe keeping of the previously transmitted images) and handling the Storage Commitment notifications received from the PACS.
- Print Images on DICOM Printers
- Transfer of X-Ray Radiation Dose Structured Reports to the PACS or Workstation.

The system is verified as DIN 6862-2 compliant.

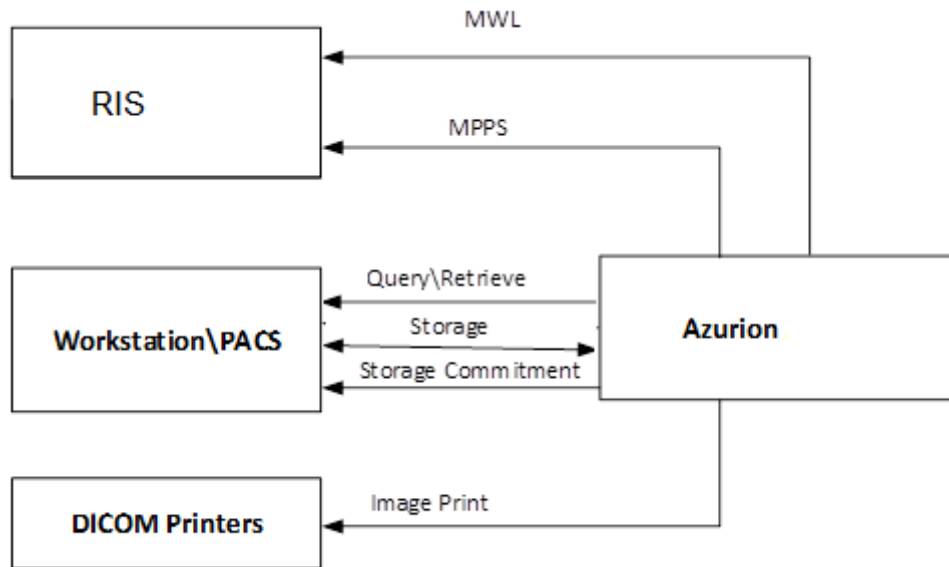


Figure 1: Data Flow of Azurion in a DICOM Network

Table 1: Network Services

SOP Class		User of Service (SCU)	Provider of Service (SCP)	Display
Name	UID			
<b>Other</b>				
Verification SOP Class	1.2.840.10008.1.1	Yes	Yes	N/A
<b>Print Management</b>				
Basic Grayscale Print Management Meta SOP Class	1.2.840.10008.5.1.1.9	Yes	No	N/A

SOP Class		User of Service (SCU)	Provider of Service (SCP)	Display
Name	UID			
>Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Yes	No	N/A
>Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Yes	No	N/A
>Basic Grayscale Image Box SOP Class	1.2.840.10008.5.1.1.4	Yes	No	N/A
>Printer SOP Class	1.2.840.10008.5.1.1.16	Yes	No	N/A
Basic Color Print Management Meta SOP Class	1.2.840.10008.5.1.1.18	Yes	No	N/A
>Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Yes	No	N/A
>Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Yes	No	N/A
>Basic Color Image Box SOP Class	1.2.840.10008.5.1.1.4.1	Yes	No	N/A
>Printer SOP Class	1.2.840.10008.5.1.1.16	Yes	No	N/A
<b>Query/Retrieve</b>				
Patient Root QR Information Model - FIND SOP Class	1.2.840.10008.5.1.4.1.2.1.1	Yes	No	N/A
Study Root QR Information Model - FIND SOP Class	1.2.840.10008.5.1.4.1.2.2.1	Yes	Yes	N/A
Patient Root QR Information Model - MOVE SOP Class	1.2.840.10008.5.1.4.1.2.1.2	Yes	Yes	N/A
Study Root QR Information Model - MOVE SOP Class	1.2.840.10008.5.1.4.1.2.2.2	Yes	Yes	N/A
<b>Transfer</b>				
Secondary Capture Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.7	Yes	Yes	N/A
Grayscale Softcopy Presentation State Storage SOP Class	1.2.840.10008.5.1.4.1.1.11.1	Yes	Yes	N/A
X-Ray Angiographic Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.12.1	Yes	Yes	N/A
X-Ray Radiation Dose Structured Report SOP Class	1.2.840.10008.5.1.4.1.1.88.67	Yes	Yes	N/A
<b>Workflow Management</b>				
Modality Worklist Information Model - FIND SOP Class	1.2.840.10008.5.1.4.31	Yes	No	N/A
Modality Performed Procedure Step SOP Class	1.2.840.10008.3.1.2.3.3	Yes	No	N/A
Storage Commitment Push Model SOP Class	1.2.840.10008.1.20.1	Yes	No	N/A

A table of Supported Media Storage Application Profiles (with roles) is provided.

**Table 2: Media Services**

Media Storage Application Profile	File-set Creator (FSC)	File-set Updater (FSU)	File-set Reader (FSR)
<b>Compact Disk-Recordable</b>			
General Purpose CD-R Interchange	Yes	No	Yes
<b>DVD-RAM</b>			
General Purpose Interchange on DVD-RAM Media	Yes	No	Yes
<b>USB</b>			
General Purpose USB Media	Yes	No	Yes

**2. Contents**

**1. DICOM CONFORMANCE STATEMENT OVERVIEW .....2**

**2. CONTENTS .....4**

**3. INTRODUCTION.....7**

**3.1. REVISION HISTORY .....7**

**3.2. AUDIENCE .....7**

**3.3. REMARKS .....7**

**3.4. DEFINITIONS, TERMS AND ABBREVIATIONS.....8**

**3.5. REFERENCES .....9**

**4. NETWORKING .....10**

**4.1. IMPLEMENTATION MODEL .....10**

4.1.1. Application Data Flow.....10

4.1.2. Functional Definition of AE's .....11

4.1.2.1. Functional Definition of Azurion R3.1.....11

4.1.3. Sequencing of Real World Activities.....12

**4.2. AE SPECIFICATIONS.....14**

4.2.1. AE Specification of Azurion R3.1.....14

4.2.1.1. SOP Classes .....14

4.2.1.2. Association Policies.....15

4.2.1.2.1. General .....15

4.2.1.2.2. Number of Associations.....15

4.2.1.2.3. Asynchronous Nature .....15

4.2.1.2.4. Implementation Identifying Information.....16

4.2.1.2.5. Communication Failure Handling .....16

4.2.1.3. Association Initiation Policy.....16

4.2.1.3.1. (Real-World) Activity – Verification as SCU .....17

4.2.1.3.2. (Real-World) Activity – Modality Worklist as SCU .....18

4.2.1.3.3. (Real-World) Activity – Modality Performed Procedure Step as SCU .....24

4.2.1.3.4. (Real-World) Activity – Image Export .....34

4.2.1.3.5. (Real-World) Activity – Storage Commitment Push Model AS SCU .....37

4.2.1.3.6. (Real-World) Activity – FIND as SCU .....39

4.2.1.3.7. (Real-World) Activity – MOVE as SCU.....45

4.2.1.4. Association Acceptance Policy.....58

4.2.1.4.1. (Real-World) Activity – Verification as SCP.....59

4.2.1.4.2. (Real-World) Activity – Image Import.....60

**4.3. NETWORK INTERFACES .....61**

4.3.1. Physical Network Interfaces .....61

4.3.2. Additional Protocols .....62

4.3.2.1. Basic Application-Level Confidentiality Profile .....62

4.3.3. IPv4 and IPv6 Support.....62

- 4.4. CONFIGURATION .....62**
- 4.4.1. AE Title/Presentation Address Mapping ..... 62
- 4.4.1.1. Local AE Titles .....62
- 4.4.1.2. Remote AE Title/Presentation Address Mapping.....62
- 4.4.2. Parameters .....62
- 5. MEDIA INTERCHANGE .....64**
- 5.1. IMPLEMENTATION MODEL .....64**
- 5.1.1. Application Data Flow Diagram .....64
- 5.1.2. Functional Definitions of AE's ..... 64
- 5.1.3. Sequencing of Real World Activities .....64
- 5.2. AE SPECIFICATIONS.....64**
- 5.2.1. Media - Specification .....64
- 5.2.1.1. DICOM File Meta Information for the Media .....65
- 5.2.1.2. Real-World Activities ..... 65
- 5.2.1.2.1. RWA - Read File-set .....65
- 5.2.1.2.2. RWA - Create File-set.....65
- 5.2.1.2.3. RWA - Update File-set.....66
- 5.3. AUGMENTED AND PRIVATE APPLICATION PROFILES.....66**
- 5.4. MEDIA CONFIGURATION.....66**
- 6. SUPPORT OF CHARACTER SETS .....67**
- 7. SECURITY .....68**
- 7.1. INTRODUCTION .....68**
- 7.2. DICOM SECURITY PROFILE SUPPORT .....68**
- 7.2.1. Secure Use and User Identity Profiles .....68
- 7.2.1.1. DICOM Security Profiles Details.....68
- 7.2.1.2. Audit Trail Messages.....68
- 7.2.2. Security Transport Connection Profiles .....69
- 7.2.3. Media Storage Security Profiles.....71
- 7.2.4. Attribute Confidentiality Profiles.....71
- 7.2.5. Digital Signature Profiles .....72
- 7.2.6. Basic Network Address Management Profiles .....72
- 7.2.7. Application Configuration Management Profiles .....72
- 7.2.8. Time Synchronization Profiles .....72
- 7.3. ASSOCIATION LEVEL SECURITY .....73**
- 7.4. APPLICATION LEVEL SECURITY.....73**
- 8. ANNEXES .....74**
- 8.1. IOD CONTENTS .....74**
- 8.1.1. Created SOP Instance .....74
- 8.1.1.1. List of created SOP Classes .....74
- 8.1.1.1.1. Secondary Capture Image Storage SOP Class.....75
- 8.1.1.1.2. Grayscale Softcopy Presentation State Storage SOP Class.....79

- 8.1.1.1.3. X-Ray Angiographic Image Storage SOP Class .....85
- 8.1.1.1.4. X-Ray Radiation Dose SR.....95
- 8.1.2. Attribute Mapping .....100
- 8.1.3. Coerced/Modified fields.....100
- 8.2. DATA DICTIONARY OF PRIVATE ATTRIBUTES ..... 100**
- 8.3. CODED TERMINOLOGY AND TEMPLATES ..... 100**
- 8.3.1. Context Groups.....100
- 8.3.2. Template Specifications.....100
- 8.3.2.1. TID 10001 Projection X-Ray Radiation Dose .....101
- 8.3.2.2. TID 10002 Accumulated X-Ray Dose.....102
- 8.3.2.3. TID 10003 Irradiation Event X-Ray Data .....103
- 8.3.2.4. TID 10003B Irradiation Event X-Ray Source Data (for Fluoroscopy Irradiation Event type)105
- 8.3.2.5. TID 10003B Irradiation Event X-Ray Source Data (for Stationary Acquisition Irradiation Event type).....107
- 8.3.2.6. TID 10003C Irradiation Event X-Ray Mechanical Data.....108
- 8.3.2.7. TID 10004 Accumulated Projection X-Ray Dose (for Fluoroscopy Irradiation Event type)109
- 8.3.2.8. TID 10004 Accumulated Projection X-Ray Dose (for Stationary Acquisition Irradiation Event type).....109
- 8.3.2.9. TID 10007 Accumulated Total Projection Radiography Dose .....109
- 8.3.2.10. TID 1002 Observer Context .....110
- 8.3.2.11. TID 1004 Device Observer Identifying Attributes .....110
- 8.3.3. Private code definitions .....111
- 8.4. GRAYSCALE IMAGE CONSISTENCY ..... 111**
- 8.5. STANDARD EXTENDED/SPECIALIZED/PRIVATE SOP CLASSES ..... 111**
- 8.6. PRIVATE TRANSFER SYNTAXES ..... 111**

### 3. Introduction

The introduction specifies product and relevant disclaimers as well as any general information that the vendor feels is appropriate.

#### 3.1. Revision History

The revision history provides dates and differences of the different releases.

**Table 3: Revision History**

Document Version	Date of Issue	Description of change
01	10-July-2024	Initial Version of Azurion R3.1

#### 3.2. Audience

This Conformance Statement is intended for:

- (Potential) customers
- System integrators of medical equipment
- Marketing staff interested in system functionality
- Software designers implementing DICOM interfaces

It is assumed that the reader is familiar with the DICOM standard.

#### 3.3. Remarks

The DICOM Conformance Statement is contained in chapter 4 through 8 and follows the contents and structuring requirements of DICOM PS 3.2.

This DICOM Conformance Statement by itself does not guarantee successful interoperability of Philips equipment with non-Philips equipment. The user (or user's agent) should be aware of the following issues:

- **Interoperability**  
 Interoperability refers to the ability of application functions, distributed over two or more systems, to work successfully together. The integration of medical devices into an IT environment may require application functions that are not specified within the scope of DICOM. Consequently, using only the information provided by this Conformance Statement does not guarantee interoperability of Philips equipment with non-Philips equipment.  
 It is the user's responsibility to analyze thoroughly the application requirements and to specify a solution that integrates Philips equipment with non-Philips equipment.
- **Validation**  
 Philips equipment has been carefully tested to ensure that the actual implementation of the DICOM interface corresponds with this Conformance Statement.  
 Where Philips equipment is linked to non-Philips equipment, the first step is to compare the relevant Conformance Statements. If the Conformance Statements indicate that successful information exchange should be possible, additional validation tests will be necessary to ensure the functionality, performance, accuracy and stability of image and image related data. It is the responsibility of the user (or user's agent) to specify the appropriate test suite and to carry out the additional validation tests.



- **New versions of the DICOM Standard**

The DICOM Standard will evolve in future to meet the user's growing requirements and to incorporate new features and technologies. Philips is actively involved in this evolution and plans to adapt its equipment to future versions of the DICOM Standard. In order to do so, Philips reserves the right to make changes to its products or to discontinue its delivery. The user should ensure that any non-Philips provider linking to Philips equipment also adapts to future versions of the DICOM Standard. If not, the incorporation of DICOM enhancements into Philips equipment may lead to loss of connectivity (in case of networking) and incompatibility (in case of media).

### 3.4. Definitions, Terms and Abbreviations

**Table 4: Definitions, Terms and Abbreviations**

Abbreviation/Term	Explanation
AE	Application Entity
ANSI	American National Standard Institute
AP	Application Profile
CD	Compact Disc
CD-R	CD-Recordable
CD-M	CD-Medical
DICOM	Digital Imaging and Communications in Medicine
DIMSE	DICOM Message Service Element
DIMSE-C	DIMSE-Composite
DIMSE-N	DIMSE-Normalized
DIN	Deutsches Institut für Normung E.V.
DVD	Digital Versatile Disc
EBE	DICOM Explicit VR Big Endian
ELE	DICOM Explicit VR Little Endian
FSC	File-set Creator
FSR	File-set Reader
FSU	File-set Updater
GSPS	Grayscale Softcopy Presentation State
GUI	Graphic User Interface
HIS	Hospital Information System
ILE	DICOM Implicit VR Little Endian
IOD	Information Object Definition
MOD	Magneto-Optical Disk
MPPS	Modality Performed Procedure Step
NEMA	National Electrical Manufacturers Association
PDU	Protocol Data Unit
RIS	Radiology Information System
RWA	Real-World Activity
SC	Secondary Capture
SCM	Study Component Management
SCP	Service Class Provider

Abbreviation/Term	Explanation
SCU	Service Class User
SOP	Service Object Pair
TCP/IP	Transmission Control Protocol/Internet Protocol
UID	Unique Identifier
WLM	Worklist Management
XA	X-Ray Angiographic

**3.5. References**

[DICOM] Digital Imaging and Communications in Medicine, Parts 1 - 22 (NEMA PS 3.1- PS 3.22),  
 National Electrical Manufacturers Association  
 1300 North 17th Street  
 Suite 900  
 Arlington, Virginia 22209  
 Internet: <https://www.dicomstandard.org/>

## 4. Networking

This section contains the networking related services (vs. the media related ones).

### 4.1. Implementation model

The implementation model consists of three sections:

- The application data flow diagram, specifying the relationship between the Application Entities and the "external world" or Real-World Activities,
- A functional description of each Application Entity, and
- The sequencing constraints among them.

#### 4.1.1. Application Data Flow

Azurion R3.1 has a single Application Entity in its implementation, namely Azurion R3.1 Application Entity. Figure 2 shows the relationship between the Local and Remote Real World Activities.

- After RWA Verify Application Level Communication, the Azurion R3.1 as SCU uses the remote Request Verification SCP functionality to verify communication.
- After RWA Modality Worklist, the Azurion R3.1 as SCU uses the remote Modality Worklist Information Model SCP functionality to query for Modality Worklist.
- After RWA Create and Set Modality Performed Procedure Step, the Azurion R3.1 as SCU uses the remote Modality Performed Procedure Step SOP Class functionality to Report Modality Performed Procedure Step.
- After RWA Transfer Images + Presentation States + X-Ray Dose Structured Report, the Azurion R3.1 as SCU uses the remote SCP Storage Service Class functionality to store local Images-Ray Dose Structured Report and presentation states in a remote database.
- The Azurion R3.1 as SCP Storage Service class accepts images + presentation states from the remote SCU.
- After RWA Storage Commitment, the Azurion R3.1 as SCU uses the remote SCP Storage Commitment Service Class functionality to commit remote images and presentation states.
- After RWA Print Images, the Azurion R3.1 as SCU uses the remote SCP Print Management Service Class functionality to print the images.
- After RWA Query Retrieve, the Azurion R3.1 as SCU uses the remote SCP Query Retrieve Images Service Class functionality to Query Retrieve.

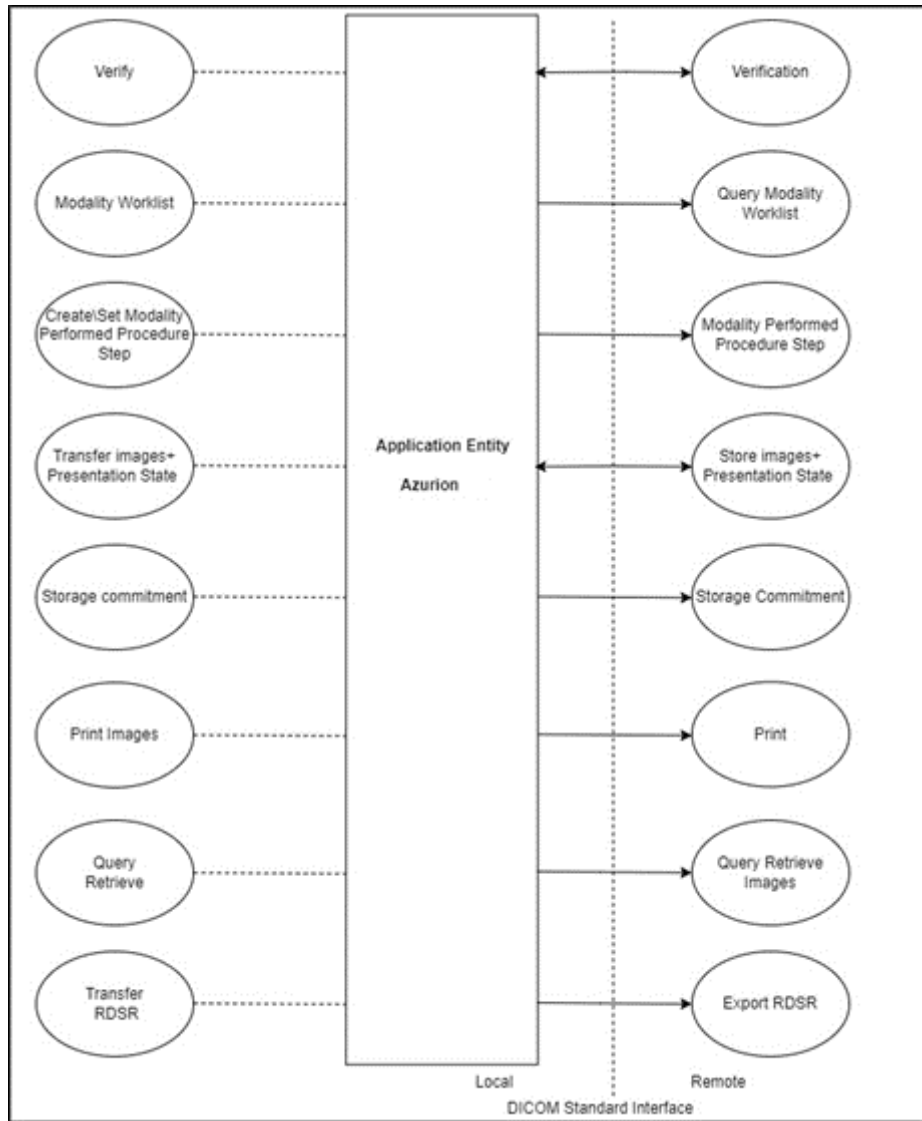


Figure 2: Functional Overview

4.1.2. Functional Definition of AE’s

This section contains a functional definition for each individual local Application Entity.

4.1.2.1. Functional Definition of Azurion R3.1

Verification Service Class

The Azurion R3.1 can perform (only to pre-configured systems) the Verification service as SCU, the Azurion R3.1 shall request an Association. When the association is accepted by the remote system, the Azurion R3.1 shall send the Verification request, receive the Verification response, and request for releasing the association.

The Azurion R3.1 can also perform the verification service as SCP, it shall accept association when the association is requested by the remote system.

### Storage Service Class

The Azurion R3.1 can perform (only to pre-configured systems) the Storage service as SCU (RWA Transfer Images + Presentation States and Structured Report), triggered by the operator or by an event in the system, e.g. closing of an examination, acquisition of images. The Azurion R3.1 shall request an association with the selected remote SCP for all applicable Storage SOP classes. When the association is accepted, the Azurion R3.1 shall send the Storage requests (including data from local database), receive the Storage responses and act accordingly, and finally request for releasing the association. The Azurion R3.1 can also perform (only to pre-configured systems) the Storage service as SCP (RWA accept Images + Presentation States). The Azurion R3.1 shall receive an association with the selected remote SCU for all applicable Storage SOP classes, accept the association and receives the Storage requests responses and act accordingly.

### Print Management Service Class

The Azurion R3.1 can perform the Print service as SCU (RWA Print Images), triggered by the operator. For each printed sheet, the Azurion R3.1 shall request an association with the selected remote SCP (i.e., a Print Server) for all applicable SOP classes of the applicable Print Management Meta SOP class. When the association is accepted, the Azurion R3.1 shall send the Print requests including data from local database (the N-GET RQ message to get the printer status, the N-CREATE-RQ message to create the Film Session and the Film Box, the N-SET-RQ message to set the Image Box on the printer, finally, the N-ACTION-RQ message to give printer the command to print), receive the Print responses and act accordingly, and finally request for releasing the association. The Azurion R3.1 can perform the Print service as SCU (RWA Get Printer Status), triggered by the operator in the service mode. The Azurion R3.1 shall request an association with the selected remote SCP (Print Server) for the Printer SOP class. When the association is accepted, the Azurion R3.1 shall send the N-GET request, receive the responses from the Print Server and act accordingly, and finally request for releasing the association.

### Basic Worklist Management Service Class

The Azurion R3.1 can perform (only to the pre-configured MWL SCP) the Basic Worklist Management service as SCU (RWA Request Modality Worklist), triggered by the operator. The Azurion R3.1 shall request an association. When the association is accepted, the Azurion R3.1 shall send the Worklist request, receive the Worklist responses, and request for releasing the association.

### Study Management Service Class

The Azurion R3.1 can perform (only to the pre-configured MWL SCP) the Study Management service as SCU (RWA Create and Set Modality Performed Procedure Step), triggered by the start of an examination (triggered by the first x-ray exposure) for acquisition or closing. The Azurion R3.1 shall request an association. When the association is accepted, the Azurion R3.1 shall send Create and Set requests, receive the responses, and request for releasing the association.

### Query Retrieve Service Class

The Azurion R3.1 can perform the Query Retrieve service as SCU. The Azurion R3.1 shall request an association. When the association is accepted, the Azurion R3.1 shall send a Query/Retrieve request, receive the responses, and request for releasing the association.

#### 4.1.3. Sequencing of Real World Activities

The following sequence of Real World activities are supported by Azurion R3.1:

- The clinical user queries the MWL SCP for a (specific) Worklist representing the list of Scheduled Procedure Steps (with demographic information). Based on that query entered at Azurion R3.1, it sends

the C-FIND-RQ message with the query criteria. The automatic broad query with configured query criteria shall be triggered whenever user selects scheduled patients page or all patients page.

- The clinical user starts the examination. As a result, Azurion R3.1 notifies the MWL SCP of the start of a new Procedure Step, i.e. it sends the MPPS N-CREATE-RQ message with the “IN PROGRESS” status of the examination.
- The clinical user acquires images with a certain procedure. As a result, if background image transfer is configured, Azurion R3.1 sends automatically the acquired images (and corresponding presentation states) to the PACS and/or the Workstation, i.e., it sends the C-STORE-RQ messages containing the image (and presentation state) information.
- The clinical user completes the examination. As a result, if auto-transfer is configured, Azurion R3.1 sends images (and corresponding presentation states) and dose report to the PACS and/or Workstation (background image transfer), i.e., it sends the C-STORE-RQ messages containing the image (and presentation state) and dose report information.
- When all images (and presentation states), which were to be automatically transferred to the PACS, have been transferred and storage-commit configured, the Azurion R3.1 asks the PACS to take responsibility for the images (and presentation states) that it has stored that originate from the examination, i.e., it sends the N-ACTION-RQ message containing the request for storage commit.
- Azurion R3.1 notifies the MWL SCP of the completion of a Procedure Step, i.e., it sends the N-SET-RQ message with the “COMPLETED” status of the examination. Additionally, to the basic flow of activities, the clinical user may also perform the following steps:
  - The clinical user manually transfers images to the PACS and/or Workstation. As a result, Azurion R3.1 sends the C-STORE-RQ messages containing the image information.
  - The clinical user manually prints selected images. As a result, Azurion R3.1 sends the N-GET-RQ message to get the printer status, the N-CREATE-RQ message to create the Film Session and the Film Box, the N-SET-RQ message to set the Image Box on the printer. Finally, it sends the N-ACTION-RQ message to give printer the command to print.

Figure 3 presents normal scheduled workflow. Other workflow situations (e.g., unscheduled procedure steps) will have other sequencing constraints. For example, printing could equally take place after the acquired images have been stored or after the examination have been closed or could be omitted completely. Query for images could take place before images have been acquired or could be omitted completely.

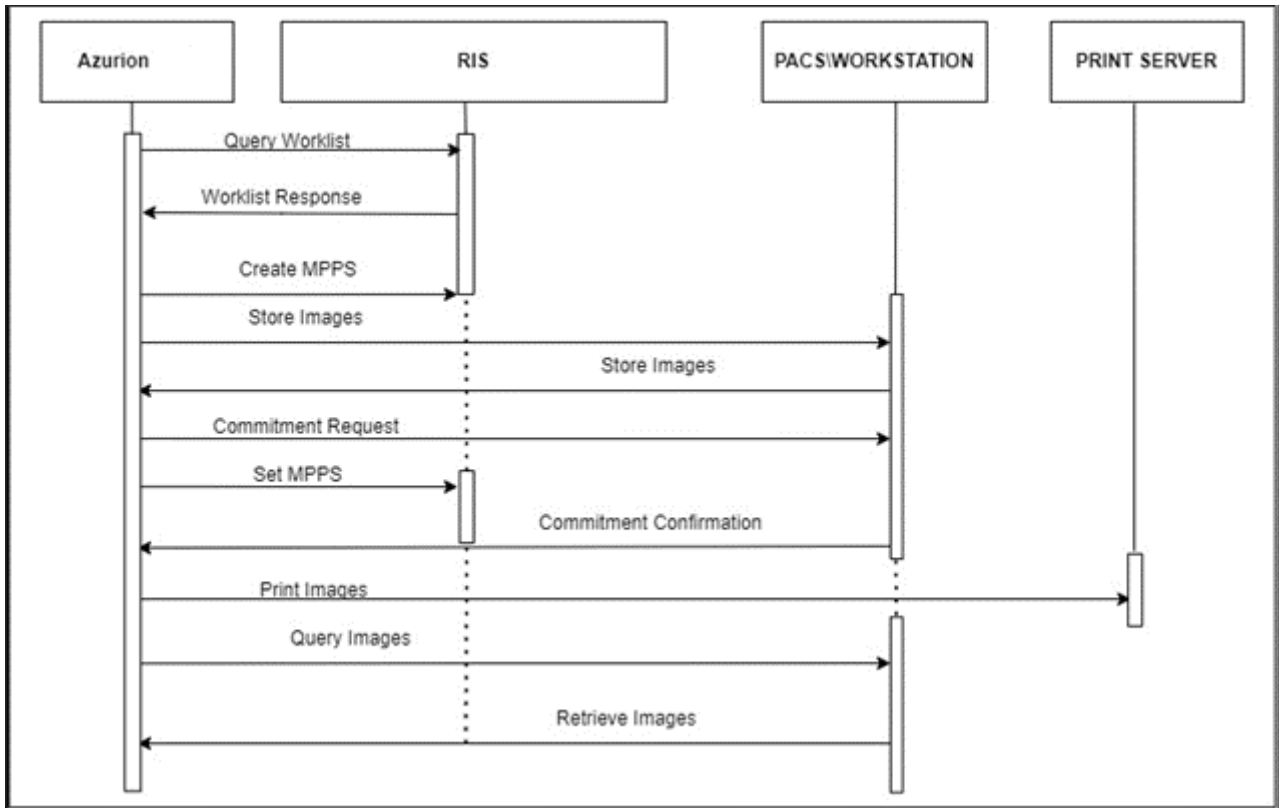


Figure 3: Azurion Sequence Diagram

4.2. AE Specifications

This section in the DICOM Conformance Statement is a set of Application Entity specifications. There are as many of these subsections as there are different AEs in the implementation.

4.2.1. AE Specification of Azurion R3.1

Detail of this specific Application Entity is specified in this section.

4.2.1.1. SOP Classes

This Application Entity provides Standard Conformance to the following SOP Classes.

Table 5: SOP Classes for Azurion R3.1

SOP Class Name	SOP Class UID	SCU	SCP
Verification SOP Class	1.2.840.10008.1.1	Yes	Yes
Storage Commitment Push Model SOP Class	1.2.840.10008.1.20.1	Yes	No
Modality Performed Procedure Step SOP Class	1.2.840.10008.3.1.2.3.3	Yes	No
Basic Grayscale Print Management Meta SOP Class	1.2.840.10008.5.1.1.9	Yes	No
>Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Yes	No
>Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Yes	No
>Basic Grayscale Image Box SOP Class	1.2.840.10008.5.1.1.4	Yes	No
>Printer SOP Class	1.2.840.10008.5.1.1.16	Yes	No

SOP Class Name	SOP Class UID	SCU	SCP
Basic Color Print Management Meta SOP Class	1.2.840.10008.5.1.1.18	Yes	No
>Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Yes	No
>Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Yes	No
>Basic Color Image Box SOP Class	1.2.840.10008.5.1.1.4.1	Yes	No
>Printer SOP Class	1.2.840.10008.5.1.1.16	Yes	No
Secondary Capture Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.7	Yes	Yes
Grayscale Softcopy Presentation State Storage SOP Class	1.2.840.10008.5.1.4.1.1.11.1	Yes	Yes
X-Ray Angiographic Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.12.1	Yes	Yes
X-Ray Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.67	Yes	No
Modality Worklist Information Model - FIND SOP Class	1.2.840.10008.5.1.4.31	Yes	No
Patient Root QR Information Model – FIND SOP Class	1.2.840.10008.5.1.4.1.2.1.1	Yes	No
Study Root QR Information Model - FIND SOP Class	1.2.840.10008.5.1.4.1.2.2.1	Yes	Yes
Patient Root QR Information Model – MOVE SOP Class	1.2.840.10008.5.1.4.1.2.1.2	Yes	No
Study Root QR Information Model - MOVE SOP Class	1.2.840.10008.5.1.4.1.2.2.2	Yes	Yes

**Note:** Any SOP specific behavior is documented later in the conformance statement in the applicable SOP specific conformance section.

#### 4.2.1.2. Association Policies

Each AE specification contains a description of the general association establishment and acceptance policies of the AE.

##### 4.2.1.2.1. General

The DICOM standard application context is specified below.

**Table 6: DICOM Application Context**

Description	Value
Application Context Name	1.2.840.10008.3.1.1.1

##### 4.2.1.2.2. Number of Associations

The number of simultaneous associations that an Application Entity may support as an Initiator or Acceptor is specified here.

**Table 7: Number of associations as an Association Initiator for this AE**

Description	Value
Maximum number of simultaneous associations	1

##### 4.2.1.2.3. Asynchronous Nature

The Azurion R3.1 does not support asynchronous operations except for storage commitment. After the storage commitment N-ACTION request is transmitted, storage commitment notification may be handled on another association.



**4.2.1.2.4. Implementation Identifying Information**

The value supplied for Implementation Class UID and version name are documented here.

**Table 8: DICOM Implementation Class and Version for Azurion R3.1**

Implementation Class UID	1.3.46.670589.7.29.3.1.1
Implementation Version Name	Azurion

**4.2.1.2.5. Communication Failure Handling**

The behavior of the AE during communication failure is summarized in the below table.

**Table 9: Communication Failure Behavior**

Exception	Behavior
ARTIM Timeout	The association is released, and the command is marked failed. The reason is logged and reported to the user.
Association aborted	The ABORT is handled by failing the job and the command is marked failed. The reason is logged and reported to the user.

**4.2.1.3. Association Initiation Policy**

The Application Entity will respond to a received Association rejection as shown in the below table.

**Table 10: Association Rejection response**

Result	Source	Reason/Diagnosis	Behavior
1 - rejected-permanent	1 - DICOM UL service-user	1 - no-reason-given	Log entry.
		2 - application-context-name-not supported	Log entry.
		3 - calling-AE-title-not-recognized	Log entry.
		7 - called-AE-title-not-recognized	Log entry.
	2 - DICOM UL service-provider (ACSE related function)	1 - no-reason-given	Log entry.
		2 - protocol-version-not-supported	Log entry.
3 - DICOM UL service-provider (Presentation related function)	1 - temporary-congestion	Log entry.	
	2 - local-limit-exceeded	Log entry.	
2 – rejected - transient	1 - DICOM UL service-user	1 - no-reason-given	Log entry.
		2 - application-context-name-not-supported	Log entry.
		3 - calling-AE-title-not-recognized	Log entry.
		7 - called-AE-title-not-recognized	Log entry.
	2 - DICOM UL service-provider (ACSE related function)	1 - no-reason-given	Log entry.
		2 - protocol-version-not-supported	Log entry.
	3 - DICOM UL service-provider (Presentation related function)	1 - temporary-congestion	Log entry.
		2 - local-limit-exceeded	Log entry.

The behavior of the AE on receiving an Association abort is summarized in the below table.

Table 11: Association Abort Handling

Source	Reason/Diagnosis	Behavior
0 - DICOM UL service-user (initiated abort)	0 - reason-not-specified	Log entry.
2 - DICOM UL service-provider (initiated abort)	0 - reason-not-specified	Log entry.
	1 - unrecognized-PDU	Log entry.
	2 - unexpected-PDU	Log entry.
	4 - unrecognized-PDU-parameter	Log entry.
	5 - unexpected-PDU-parameter	Log entry.
	6 - invalid-PDU-parameter-value	Log entry.

4.2.1.3.1. (Real-World) Activity – Verification as SCU

4.2.1.3.1.1. Description and Sequencing of Activities

For each Verify Application Level Communication request, an association towards the remote system is established and a C-ECHO request is transmitted. Once the response is received, the association is closed.

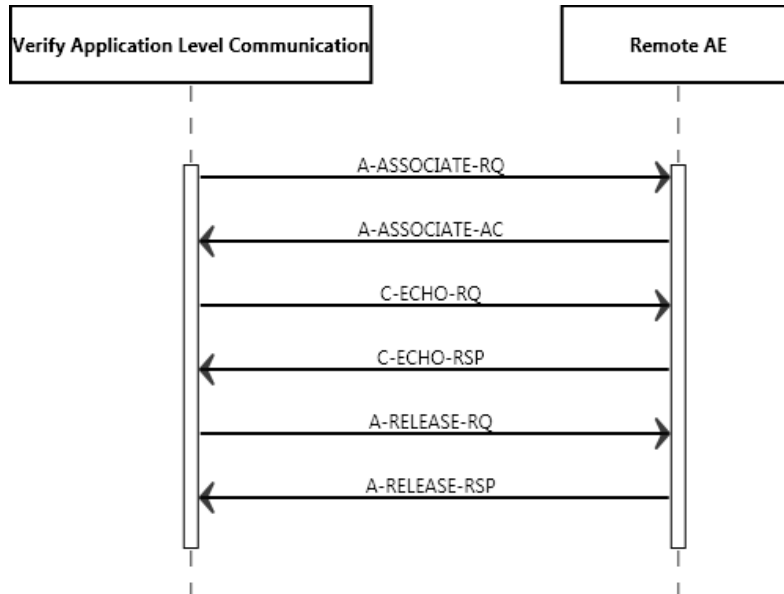


Figure 4: Sequencing of RWA Verify Application Level Communication

4.2.1.3.1.2. Proposed Presentation Contexts

Each time an association is initiated, the Azurion R3.1 proposes one presentation contexts to be used on that association. The presentation context proposed by the Azurion R3.1 for Verify Application Level Communication is defined in Table below.

**Table 12: Proposed Presentation Contexts for (Real-World) Activity – Verification As SCU**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Verification SOP Class	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

**4.2.1.3.1.3. SOP Specific Conformance for Verification SOP Class**

**4.2.1.3.1.3.1. Dataset Specific Conformance for Verification SOP Class C-ECHO-SCU**

The behavior of the Azurion R3.1 for status codes in a Verification response is summarized in next table.

**Table 13: Verification C-ECHO Response Status Handling Behavior**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Confirmation	The SCP has successfully responded to the verification request.

The behavior of the Azurion R3.1 during communication failure is summarized in next table

**Table 14: Verification Communication Failure Behavior**

Exception	Behavior
Timeout	Association is closed. The reason is logged and reported to the user.
Association aborted	The reason is logged, and failure is reported to the user.
Association rejected	The reason is logged, and failure is reported to the user.

**4.2.1.3.2. (Real-World) Activity – Modality Worklist as SCU**

**4.2.1.3.2.1. Description and Sequencing of Activities**

For each Broad or Specific Worklist request, the Azurion R3.1 opens an association towards the Basic Worklist Management SCP and sends a C-FIND request. After retrieval of all responses containing matching Worklist items, the association is closed (see Figure 5). All returned Worklist items are displayed to the operator who can select an item from the Worklist and perform an examination.

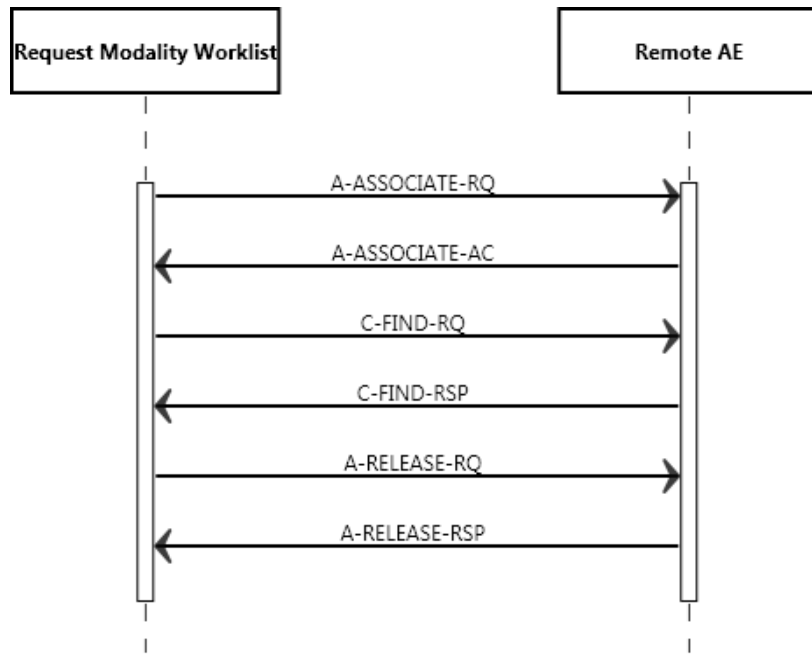


Figure 5: Sequencing of RWA Request Modality Worklist

The clinical user may cancel the query to the MWL SCP. As a result, Azurion R3.1 sends a C-FIND Cancel Request to the MWL SCP.

4.2.1.3.2.2. Proposed Presentation Contexts

The presentation contexts are defined in the next table.

Table 15: Proposed Presentation Contexts for (Real-World) Activity – Modality Worklist As SCU

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Modality Worklist Information Model – FIND SOP Class	1.2.840.10008.5.1.4.31	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

4.2.1.3.2.3. SOP Specific Conformance for Modality Worklist Information Model - FIND SOP Class

Two kinds of queries can be done with the Azurion R3.1: a broad query and a specific query. A broad query for the Worklist is initiated by the operator without filling in any search criteria (the search criteria are based on system configuration). The Matching Keys are presented in Table 16.

A specific Worklist request is initiated by the operator after filling in search criteria in the Graphical User Interface. At least one key should be specified. No verification of query results in relation to the original query criteria is done. The Matching Keys are presented in Table 17.

A received Worklist entry is validated. The entry will be discarded, and an error will be reported when a type-one or type-two attribute is missing, or when the translation of a type-one attribute fails (this includes individual attributes within a sub-sequence).

**Table 16: Broad Query Presentation Contexts for (Real-World) Activity Modality Worklist as SCU**

Attribute Name	Tag	Matching Key
Scheduled Station AE Title	(0040,0001)	Single value matching
Scheduled Procedure Step Start Date	(0040,0002)	Universal matching or range matching
Scheduled Procedure Step Start Time	(0040,0003)	Universal matching or range matching
Modality	(0008,0060)	Single value matching and Universal matching

**Table 17: Matching Table MWL Information Model – Specific Query**

Attribute Name	Tag	Matching Key
Scheduled Station AE Title	(0040,0001)	Universal matching or single value matching
Scheduled Procedure Step Start Date	(0040,0002)	Universal matching or range matching
Modality	(0008,0060)	Universal matching or single value matching
Patient’s Name	(0010,0010)	Universal matching or single value matching or wild card matching
Patient ID	(0010,0020)	Universal matching or single value matching
Accession Number	(0008,0050)	Universal matching or single value matching
Requested Procedure ID	(0040,1001)	Universal matching or single value matching

**4.2.1.3.2.3.1. Dataset Specific Conformance for Modality Worklist Information Model - FIND SOP Class C-FIND-SCU**

This section specifies the Modality Worklist Request Attributes.

For each attribute in the following information is supplied:

Attribute Name: Attributes supported to build a Modality Worklist Request Identifier.

Tag: DICOM tag for this attribute.

VR: DICOM VR for this attribute.

M: Matching Keys for (automatic) Worklist Update.

R: Return Keys. An “X” will indicate that this attribute as Return Key with zero length for Universal Matching.

Q: Interactive Query Key. An “X” will indicate that this attribute as matching key can be used.

D: Displayed Keys. An “X” indicates that this Worklist attribute is displayed to the user during a patient registration dialog.

IOD: An “X” indicates that this Worklist attribute is included into all object Instances created during performance of the related Procedure Step.

Types of matching supported:

- Single Value Matching
- List of UID Matching
- Wild Card Matching
- Range Matching
- Sequence Matching
- Universal Matching

Table 18: C-FIND-RQ Dataset Specification

Modality Worklist Information Model – FIND SOP Class									
Attribute Name	Tag	VR	M	R	Q	D	IOD	Type of Matching	Comment
<b>Scheduled Procedure Step</b>									
Scheduled Procedure Step Sequence	0040,0100	SQ		X				NA	
>Modality	0008,0060	CS	X	X	X	X	X	Single Value, Universal, Wild Card	
>Requested Contrast Agent	0032,1070	LO	X	X				Universal	
>Scheduled Station AE Title	0040,0001	AE	X	X	X	X		Single Value, Universal, Wild Card	
>Scheduled Procedure Step Start Date	0040,0002	DA	X	X	X	X		Single Value, Universal, Wild Card, range	
>Scheduled Procedure Step Start Time	0040,0003	TM	X	X		X		Single Value, Range, Universal	
>Scheduled Performing Physician’s Name	0040,0006	PN	X	X	X	X		Single Value, Universal, Wild Card	
>Scheduled Procedure Step Description	0040,0007	LO	X					Universal	
>Scheduled Protocol Code Sequence	0040,0008	SQ	X					Universal	
>>Code Value	0008,0100	SH	X					Universal	
>>Coding Scheme Designator	0008,0102	SH	X					Universal	
>>Coding Scheme Version	0008,0103	SH	X					Universal	
>>Code Meaning	0008,0104	LO	X					Universal	
>>Protocol Context Sequence	0040,0440	SQ	X					Universal	
>>>Measurement Units Code Sequence	0040,08EA	SQ	X					Universal	
>>>>Code Value	0008,0100	SH	X					Universal	
>>>>Coding Scheme Designator	0008,0102	SH	X					Universal	
>>>>Coding Scheme Version	0008,0103	SH	X					Universal	
>>>>Code Meaning	0008,0104	LO	X					Universal	
>>>Value Type	0040,A040	CS	X					Universal	
>>>Concept Name Code Sequence	0040,A043	SQ	X					Universal	
>>>>Code Value	0008,0100	SH	X					Universal	
>>>>Coding Scheme Designator	0008,0102	SH	X					Universal	
>>>>Coding Scheme Version	0008,0103	SH	X					Universal	
>>>>Code Meaning	0008,0104	LO	X					Universal	
>>>DateTime	0040,A120	DT	X					Universal	

Modality Worklist Information Model – FIND SOP Class									
Attribute Name	Tag	VR	M	R	Q	D	IOD	Type of Matching	Comment
>>>Person Name	0040,A123	PN	X					Universal	
>>>Text Value	0040,A160	UT	X					Universal	
>>>Concept Code Sequence	0040,A168	SQ	X					Universal	
>>>>Code Value	0008,0100	SH	X					Universal	
>>>>Coding Scheme Designator	0008,0102	SH	X					Universal	
>>>>Coding Scheme Version	0008,0103	SH	X					Universal	
>>>>Code Meaning	0008,0104	LO	X					Universal	
>>>Numeric Value	0040,A30A	DS	X					Universal	
>Scheduled Procedure Step ID	0040,0009	SH	X					Universal	
>Scheduled Station Name	0040,0010	SH	X					Universal	
>Scheduled Procedure Step Location	0040,0011	SH	X					Universal	
>Pre-Medication	0040,0012	LO	X					Universal	
>Scheduled Procedure Step Status	0040,0020	CS	X					Universal	
Requested Procedure									
Study Instance UID	0020,000D	UI	X	X				Universal	
Requested Procedure Code Sequence	0032,1064	SQ	X					Universal	
>Code Value	0008,0100	SH	X					Universal	
>Coding Scheme Designator	0008,0102	SH	X					Universal	
>Coding Scheme Version	0008,0103	SH	X					Universal	
>Code Meaning	0008,0104	LO	X					Universal	
Requested Procedure ID	0040,1001	SH	X		X	X		Single Value, Universal, Wild Card	
Patient Transport Arrangements	0040,1004	LO	X					Universal	
Imaging Service Request									
Accession Number	0008,0050	SH	X		X	X	X	Single Value, Universal, Wild Card	
Referring Physician's Name	0008,0090	PN	X	X			X	Universal	
Requesting Physician	0032,1032	PN	X					Universal	
Visit Relationship									
Referenced Patient Sequence	0008,1120	SQ						NA	
>Referenced SOP Class UID	0008,1150	UI	X					Universal	
>Referenced SOP Instance UID	0008,1155	UI	X					Universal	
Patient Identification									
Patient's Name	0010,0010	PN	X	X	X	X	X	Single Value, Universal	

Modality Worklist Information Model – FIND SOP Class									
Attribute Name	Tag	VR	M	R	Q	D	IOD	Type of Matching	Comment
Patient ID	0010,0020	LO	X	X	X	X	X	Single Value, Universal	
Patient Demographic									
Patients Birth Date	0010,0030	DA	X	X			X	Single, Universal, Range, Wild Card	
Patient's Sex	0010,0040	CS	X	X			X	Single Value, Universal	
Patient's Weight	0010,1030	DS	X	X			X	Universal	
Patient Medical									
Medical Alerts	0010,2000	LO	X					Universal	
Allergies	0010,2110	LO	X					Universal	
Pregnancy Status	0010,21C0	US	X	X				Universal	
Patient State	0038,0500	LO	X	X				Universal	
SOP Common Module									
Specific Character Set	0008,0005	CS		X					

The behavior of the Azurion R3.1 for status codes in C-FIND response is summarized in Table below.

**Table 19: Modality Worklist C-FIND Response Status Handling Behavior**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Matching is complete - No final Identifier is supplied.	The result is reported to the user and is logged.
Refused	A700	Out of Resources	Stops with processing the C-FIND Response(s) from the SCP. Responses displayed to the user.
Failed	A900	Identifier Does Not Match SOP Class	Stops with processing the C-FIND Response(s) from the SCP. The reason is logged, and the failure is reported to the user. Responses displayed to the user.
	C001	Unable to process	Stops with processing the C-FIND Response(s) from the SCP. The reason is logged, and the failure is reported to the user. No responses displayed to the user.
Cancel	FE00	Matching terminated due to Cancel Match request	Stops with processing the C-FIND Response(s) from the SCP. No responses displayed to the user.
Pending	FF00	Matches are continuing – Current. Match is supported in the same manner as supplied and any Optional Keys were Required Keys.	Continues with processing of the C-FIND
	FF01	Matches are continuing – Warning that one or more Optional Keys were not supported for existence for this Identifier.	Continues with processing of the C-FIND



Service Status	Error Code	Further Meaning	Behavior
*	Any other status code	*	The association is aborted using A-ABORT. The reason is logged, and the failure is reported to the user. No responses displayed to the user.

The behavior of the Azurion R3.1 during communication failure is summarized in Table 20

**Table 20: Modality Worklist Communication Failure Behavior**

Exception	Behavior
Timeout	The query is marked as failed. The reason is logged and reported to the user. The Azurion R3.1 stops processing the C-FIND Response(s) from the SCP.
Association Aborted	If the association is aborted using A-ABORT, the query is marked as failed. The reason is logged, and failure is reported to the user. Stops with processing the C-FIND Response(s) from the SCP.
Association Rejected	The query is marked as failed. The reason is logged, and failure is reported to the user. No C-FIND request performed.

### 4.2.1.3.3. (Real-World) Activity – Modality Performed Procedure Step as SCU

#### 4.2.1.3.3.1. Description and Sequencing of Activities

For each MPPS Job, a new association towards the Modality Performed Procedure Step is established and closed when the MPPS Job has been transmitted. There are three kinds of MPPS Jobs:

- *MPPS Create Job.* Only an N-CREATE request with status “IN PROGRESS” is transmitted. Once the response is received, the association is closed. The MPPS Create Job is submitted when:
  - A Worklist examination is selected for acquisition.
  - A local examination is selected for acquisition and the system is configured to be connected to an IHE compatible MWL SCP.
  - An already Completed Worklist examination or an already Completed, local examination, is re-selected for acquisition (IHE Append Use Case).
- *MPPS Set Job.* Only an N-SET request is transmitted. The status field will respectively be set to “DISCONTINUED” or “COMPLETED”. Once the response is received, the association is closed. The MPPS Set Job is submitted when:
  - An examination is discontinued/deleted/restored to solve patient mixing or closed and the MPPS Create Job is already handled (transmitted).
- *MPPS Create & Set Job.* Over the same association both the N-CREATE request and the N-SET request corresponding to the same examination are transmitted. The MPPS Create & Set Job is submitted when:
  - An examination is discontinued/deleted/restored to solve patient mixing and the MPPS Create Job is not already handled (not transmitted). In such a case the MPPS Create & Set Job replaces the MPPS Create Job.

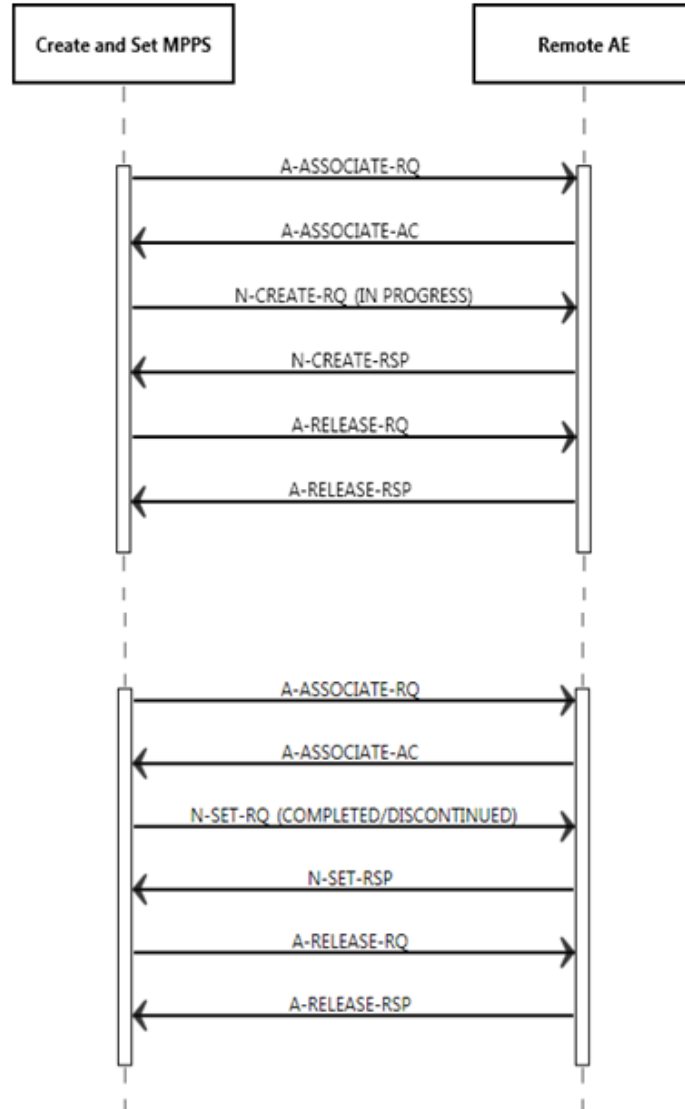


Figure 6: Sequencing of RWA separate MPPS Create and separate MPPS Set Job

MPPS Create and MPPS Set in same association can be established when a procedure is reopened for review and performed some snapshots and export them and then close the study.

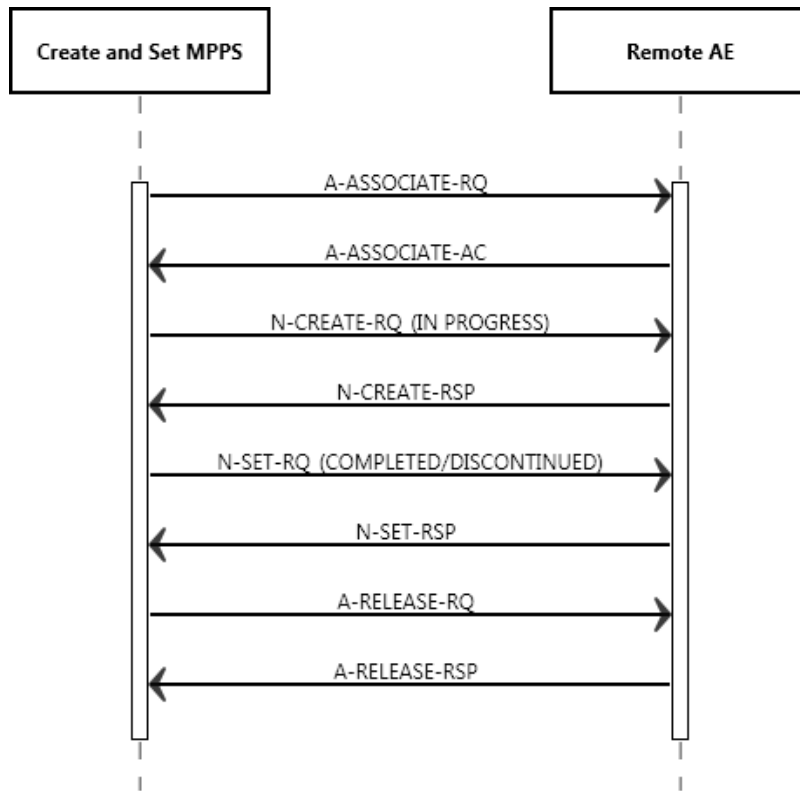


Figure 7: Sequencing of RWA MPPS Create and Set Job

4.2.1.3.3.2. Proposed Presentation Contexts

Each time an association is initiated, the Azurion R3.1 proposes one presentation context to be used on that association. The presentation context proposed by the Azurion R3.1 for Create and Set Modality Performed Procedure Step is defined in table below.

The implementation chooses Explicit VR Little Endian transfer syntax in case multiple transfer syntaxes are accepted in the association acceptance. All details regarding the specific conformance, including response behavior to all status codes, both from an application level and communication errors are provided in table 23.

Table 21: Proposed Presentation Contexts for (Real-World) Activity – MPPS as SCU

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Modality Performed Procedure Step SOP Class	1.2.840.10008.3.1.2.3.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

4.2.1.3.3.3. SOP Specific Conformance for Modality Performed Procedure Step SOP Class

The set of attributes within an N-CREATE and N-SET messages is fixed, and it does not depend on configuration settings. In an N-CREATE message, all possible attributes and attribute sequences used in the N-SET are

forecasted by defining the attributes and settings their values to NULL. When an N-SET message is transmitted, it may occur that a forecasted attribute isn't actually used. Table 22 up till Table 24 indicate whether or not an attribute and attribute value is sent during N-CREATE.

Table 24 up till Table 26 indicate whether or not an attribute and attribute value is sent during MPPS N-SET.

**4.2.1.3.3.3.1. Dataset Specific Conformance for Modality Performed Procedure Step SOP Class N-CREATE-SCU**

**Table 22: N-CREATE-RQ Dataset Specification**

Modality Performed Procedure Step SOP Class				
Attribute Name	Tag	VR	Value	Comment
<b>SOP Common Module</b>				
Specific Character Set	0008,0005	CS		
<b>Performed Procedure Step Relationship Module</b>				
Referenced Patient Sequence	0008,1120	SQ		
>Referenced SOP Class UID	0008,1150	UI		
>Referenced SOP Instance UID	0008,1155	UI		
Patient's Name	0010,0010	PN		
Patient ID	0010,0020	LO		
Patient's Birth Date	0010,0030	DA		
Patient's Sex	0010,0040	CS		
Scheduled Step Attributes Sequence	0040,0270	SQ		
>Accession Number	0008,0050	SH		Empty in case of an unscheduled exam
>Referenced Study Sequence	0008,1110	SQ		Empty in case of an unscheduled exam
>>Referenced SOP Class UID	0008,1150	UI		
>>Referenced SOP Instance UID	0008,1155	UI		
>Study Instance UID	0020,000D	UI		
>Requested Procedure description	0032,1060	LO		Empty in case of an unscheduled exam
>Scheduled Procedure Step description	0040,0007	LO		Empty in case of an unscheduled exam
>Scheduled Protocol Code Sequence	0040,0008	SQ		
>>Code Value	0008,0100	SH		
>>Coding Scheme Designator	0008,0102	SH		
>>Coding Meaning	0008,0104	LO		
>Scheduled Procedure Step ID	0040,0009	SH		Empty in case of an unscheduled exam
>Requested Procedure ID	0040,1001	SH		Empty in case of an unscheduled exam
<b>Performed Procedure Step Information Module</b>				
Procedure Code Sequence	0008,1032	SQ		
>Code Value	0008,0100	SH		
>Coding Scheme Designator	0008,0102	SH		
>Coding Meaning	0008,0104	LO		
>Context Group Extension Flag	0008,010B	CS		
>Context Identifier	0008,010F	CS		
>Context UID	0008,0117	UI		

Modality Performed Procedure Step SOP Class				
Attribute Name	Tag	VR	Value	Comment
Performed Station AE Title	0040,0241	AE		AE Title as configured by the MWL SCP/CIS unit.
Performed Station Name	0040,0242	SH		
Performed Location	0040,0243	SH		Always Empty
Performed Procedure Step Start Date	0040,0244	DA		
Performed Procedure Step Start Time	0040,0245	TM		
Performed Procedure Step End Date	0040,0250	DA		
Performed Procedure Step End Time	0040,0251	TM		
Performed Procedure Step Status	0040,0252	CS		
Performed Procedure Step ID	0040,0253	SH		
Performed Procedure Step Description	0040,0254	LO		
Performed Procedure Type Description	0040,0255	LO		
Image Acquisition Results Module				
Modality	0008,0060	CS		Applied Value(s): XA
Study ID	0020,0010	SH		If no Study ID is known, the Accession Number will be used as value.
Performed Protocol Code Sequence	0040,0260	SQ		
>Code Value	0008,0100	SH		
>Coding Scheme Designator	0008,0102	SH		
>Coding Scheme Version	0008,0103	LO		
>Code Meaning	0008,0104	LO		
>Context Group Extension Flag	0008,010B	CS		
>Context Identifier	0008,010F	CS		
>Context UID	0008,0117	UI		
>Protocol Context Sequence	0040,0440	SQ		
>>Content Item Modifier Sequence	0040,0441	SQ		
>>>Value Type	0040,A040	CS		
>>>Concept Name Code Sequence	0040,A043	SQ		
>>>>Code Value	0008,0100	SH		
>>>>Coding Scheme Designator	0008,0102	SH		
>>>>Code Meaning	0008,0104	LO		
>>>>Context Group Extension Flag	0008,010B	CS		
>>>>Context Identifier	0008,010F	CS		
>>>>Context UID	0008,0117	UI		
>>Value Type	0040,A040	CS		
>>Concept Name Code Sequence	0040,A043	SQ		
>>>Code Value	0008,0100	SH		
>>>Coding Scheme Designator	0008,0102	SH		
>>>Code Meaning	0008,0104	LO		
>>>Context Group Extension Flag	0008,010B	CS		
>>>Context Identifier	0008,010F	CS		

Modality Performed Procedure Step SOP Class				
Attribute Name	Tag	VR	Value	Comment
>>>Context UID	0008,0117	UI		
Performed Series Sequence	0040,0340	SQ		Sequence will be empty when there are no images to report
>Retrieve AE Title	0008,0054	AE		
>Series Description	0008,103E	LO		
>Performing Physician's Name	0008,1050	PN		
>Operators' Name	0008,1070	PN		
>Operator Identification Sequence	0008,1072	SQ		
>>Institution Address	0008,0081	ST		
>>Person Identification Code Sequence	0040,1101	SQ		
>>>Code Value	0008,0100	SH		
>>>Coding Scheme Designator	0008,0102	SH		
>>>Code Meaning	0008,0104	LO		
>>>Context Group Extension Flag	0008,010B	CS		
>>>Context Identifier	0008,010F	CS		
>>>Context UID	0008,0117	UI		
>>Person's Address	0040,1102	ST		
>>Person's Telephone Numbers	0040,1103	LO		
>Referenced Image Sequence	0008,1140	SQ		
>>Referenced SOP Class UID	0008,1150	UI		
>>Referenced SOP Instance UID	0008,1155	UI		
>>Container Identifier	0040,0512	LO		
>>Specimen Description Sequence	0040,0560	SQ		
>>>Specimen Identifier	0040,0551	LO		
>>>Specimen UID	0040,0554	UI		
>Protocol Name	0018,1030	LO		
>Series Instance UID	0020,000E	UI		
>Referenced Non-Image Composite SOP Instance Sequence	0040,0220	SQ		
>>Referenced SOP Class UID	0008,1150	UI		
>>Referenced SOP Instance UID	0008,1155	UI		
Radiation Dose Module				
Image and Fluoroscopy Area Dose Product	0018,115E	DS		
Total Time of Fluoroscopy	0040,0300	US		
Total Number of Exposures	0040,0301	US		
Entrance Dose	0040,0302	US		
Exposure Dose Sequence	0040,030E	SQ		See Table 25 for content items set through N-SET
Entrance Dose in mGy	0040,8302	DS		

Modality Performed Procedure Step SOP Class				
Attribute Name	Tag	VR	Value	Comment
Billing And Material Management Codes				
Film Consumption Sequence	0040,0321	SQ		Always Empty
>Medium Type	2000,0030	CS		
>Film Size ID	2010,0050	CS		
>Number of Films	2100,0170	IS		

The behavior of the Azurion R3.1 for status codes in an MPPS N-CREATE response and NSET response is presented in Table 23 and Table 24 respectively. In case of the retransmission attempt each message stored in the persistent queue is sent over a separate association.

**Table 23: MPPS N-CREATE Response Status Handling Behavior**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Successful operation.	Association will be released. The notify status of the related examination is Updated (set to in progress). The examination status is not changed (e.g., still in progress).
Failure	0213	Resource Limitation	The message contents are made persistent and the message is added to the persistent queue and waits for the next retransmission attempt. The examination status is observed as “Failed”
	0118	No Such SOP Class	The examination status is updated as failed. The reason for error is logged.
	0110	Processing Failure	The examination status is updated as failed. The reason for error is logged.
*	Any other status code	*	Association will be released. If the response status is reported during initial transmission the message contents is made persistent and the message is added to the Persistent queue. If this response status is the result of the retransmission attempt related examination is updated to the state as if the transmission Succeeded. This means that the notify status of the related examination is updated (set to in progress) The examination status is not changed (e.g., still in progress). The response status is logged as a warning.

**Table 24: MPPS Communication Failure Behavior (N-SET, N-CREATE) Exception Behavior**

Exception	Behavior
Timeout	The Association is aborted using A-ABORT. The reason is logged and reported to the user. The message content is made persistent, and the message is added to the persistent queue and waits for the next retransmission attempt. The examination status is set to CLOSED.

Exception	Behavior
Association aborted	The command is marked as failed. The reason is logged and reported to the user. The message content is made persistent, and the message is added to the persistent queue and waits for the next retransmission attempt. The examination status is set to CLOSED.
Association rejected	The command is marked as failed. The reason is logged and reported to the user. The message content is made persistent, and the message is added to the persistent queue and waits for the next retransmission attempt. The examination status is set to CLOSED.

#### 4.2.1.3.3.3.2. Dataset Specific Conformance for Modality Performed Procedure Step SOP Class N-SET-SCU

Table 25: N-SET-RQ Dataset Specification

Modality Performed Procedure Step SOP Class				
Attribute Name	Tag	VR	Value	Comment
<b>SOP Common Module</b>				
Specific Character Set	0008,0005	CS		
<b>Performed Procedure Step Information Module</b>				
Procedure Code Sequence	0008,1032	SQ		
>Code Value	0008,0100	SH		
>Coding Scheme Designator	0008,0102	SH		
>Code Meaning	0008,0104	LO		
>Context Group Extension Flag	0008,010B	CS		
>Context Identifier	0008,010F	CS		
>Context UID	0008,0117	UI		
Performed Procedure Step End Date	0040,0250	DA		
Performed Procedure Step End Time	0040,0251	TM		
Performed Procedure Step Status	0040,0252	CS		Applied Values: COMPLETED or DISCONTINUED
Performed Procedure Step Description	0040,0254	LO		May be Empty by configuration
Performed Procedure Type Description	0040,0255	LO		
<b>Image Acquisition Results Module</b>				
Performed Protocol Code Sequence	0040,0260	SQ		Sequence remains empty
>Code Value	0008,0100	SH		
>Coding Scheme Designator	0008,0102	SH		
>Code Meaning	0008,0104	LO		
>Context Group Extension Flag	0008,010B	CS		
>Context Identifier	0008,010F	CS		
>Context UID	0008,0117	UI		
>Protocol Context Sequence	0040,0440	SQ		May be empty when no images to be reported
>>Content Item Modifier Sequence	0040,0441	SQ		
>>>Value Type	0040,A040	CS		
>>>Concept Name Code Sequence	0040,A043	SQ		



Modality Performed Procedure Step SOP Class				
Attribute Name	Tag	VR	Value	Comment
>>>>Code Value	0008,0100	SH		
>>>>Coding Scheme Designator	0008,0102	SH		
>>>>Code Meaning	0008,0104	LO		
>>>>Context Group Extension Flag	0008,010B	CS		
>>>>Context Identifier	0008,010F	CS		
>>>>Context UID	0008,0117	UI		
>>Value Type	0040,A040	CS		
>>Concept Name Code Sequence	0040,A043	SQ		
>>>Code Value	0008,0100	SH		
>>>Coding Scheme Designator	0008,0102	SH		
>>>Code Meaning	0008,0104	LO		
>>>Context Group Extension Flag	0008,010B	CS		
>>>Context Identifier	0008,010F	CS		
>>>Context UID	0008,0117	UI		
Performed Series Sequence	0040,0340	SQ		
>Retrieve AE Title	0008,0054	AE		
>Series Description	0008,103E	LO		
>Series Description Code Sequence	0008,103F	SQ		
>>Code Value	0008,0100	SH		
>>Coding Scheme Designator	0008,0102	SH		
>>Code Meaning	0008,0104	LO		
>>Context Group Extension Flag	0008,010B	CS		
>>Context Identifier	0008,010F	CS		
>>Context UID	0008,0117	UI		
>Performing Physician's Name	0008,1050	PN		
>Performing Physician Identification Sequence	0008,1052	SQ		
>>Institution Address	0008,0081	ST		
>>Person Identification Code Sequence	0040,1101	SQ		
>>>Code Value	0008,0100	SH		
>>>Coding Scheme Designator	0008,0102	SH		
>>>Code Meaning	0008,0104	LO		
>>>Context Group Extension Flag	0008,010B	CS		
>>>Context Identifier	0008,010F	CS		
>>>Context UID	0008,0117	UI		
>>Person's Address	0040,1102	ST		
>>Person's Telephone Numbers	0040,1103	LO		
>Operators' Name	0008,1070	PN		
>Operator Identification Sequence	0008,1072	SQ		
>>Institution Address	0008,0081	ST		

Modality Performed Procedure Step SOP Class				
Attribute Name	Tag	VR	Value	Comment
>>Person Identification Code Sequence	0040,1101	SQ		
>>>Code Value	0008,0100	SH		
>>>Coding Scheme Designator	0008,0102	SH		
>>>Code Meaning	0008,0104	LO		
>>>Context Group Extension Flag	0008,010B	CS		
>>>Context Identifier	0008,010F	CS		
>>>Context UID	0008,0117	UI		
>>Person's Address	0040,1102	ST		
>>Person's Telephone Numbers	0040,1103	LO		
>Referenced Image Sequence	0008,1140	SQ		
>>Referenced SOP Class UID	0008,1150	UI		
>>Referenced SOP Instance UID	0008,1155	UI		
>>Container Identifier	0040,0512	LO		
>>Specimen Description Sequence	0040,0560	SQ		
>>>Specimen Identifier	0040,0551	LO		
>>>Specimen UID	0040,0554	UI		
>Protocol Name	0018,1030	LO		
>Series Instance UID	0020,000E	UI		
>Referenced Non-Image Composite SOP Instance Sequence	0040,0220	SQ		Refers to DICOM Object that were transferred to the PACS.
>>Referenced SOP Class UID	0008,1150	UI		
>>Referenced SOP Instance UID	0008,1155	UI		
>Archive Requested	0040,A494	CS		
Radiation Dose Module				
Image and Fluoroscopy Area Dose Product	0018,115E	DS		
Total Time of Fluoroscopy	0040,0300	US		
Total Number of Exposures	0040,0301	US		
Entrance Dose	0040,0302	US		
Entrance Dose in mGy	0040,8302	DS		
Exposure Dose Sequence	0040,030E	SQ		
>KVP	0018,0060	DS		
>Exposure Time	0018,1150	IS		
>Radiation Mode	0018,115A	CS	PULSED	
>Filter Type	0018,1160	SH		
>Filter Material	0018,7050	CS		
>X-Ray Tube Current In uA	0018,8151	DS		
>Comments on Radiation Dose	0040,0310	ST		
Billing And Material Management Codes				
Film Consumption Sequence	0040,0321	SQ		Always Empty
>Medium Type	2000,0030	CS		

Modality Performed Procedure Step SOP Class				
Attribute Name	Tag	VR	Value	Comment
>Film Size ID	2010,0050	CS		
>Number of Films	2100,0170	IS		

The behavior of the Azurion R3.1 for status codes in an MPPS N-SET response is presented in Table 26. In case of the retransmission attempt each message stored in the persistent queue is sent over a separate association

**Table 26: MPPS N-SET Response Status Handling Behavior**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Successful operation.	Association will be released. The notify status of the related examination is Updated (set to notified). The examination status is Set to COMPLETED and it is logged.
Failure	0213	Resource Limitation	The message content is made persistent and the Message is added to the persistent queue and waits for the next retransmission attempt. The examination status is set to CLOSED.
*	Any other status code	*	Association will be released. If this response status is reported during initial transmission the message contents is made persistent and the message is added to the persistent queue. If this response status is the result of the retransmission attempt related examination is updated to the state as if the transmission succeeded. Then the notify status of the related examination is updated (set to notified). The response status is logged as a warning. The examination status is set to COMPLETED.

#### 4.2.1.3.4. (Real-World) Activity – Image Export

##### 4.2.1.3.4.1. Description and Sequencing of Activities

The operator can select images (and presentation states) and request them to be sent to (pre-configure) multiple destinations. Each request is forwarded to the job queue and processed as individual request to Transfer Images (and Presentation States). If background image and presentation state transfer is configured, the Azurion R3.1 sends the acquired images and presentation states automatically. It can be configured which instances will be automatically marked and the destinations where the instances are automatically sent to. The background image and presentation state transfer are triggered by the image acquisition event and/or by the close examination event in Azurion R3.1. For each request to Transfer Images (and Presentation States) (i.e., transfer job), one association towards the remote system is established. Within the association, for each image or presentation state, a C-STORE request is transmitted. Once the responses are received, the association is closed. A possible sequence of interactions between the Azurion R3.1 and a remote AE with only one C-STORE request is presented in Figure 8.

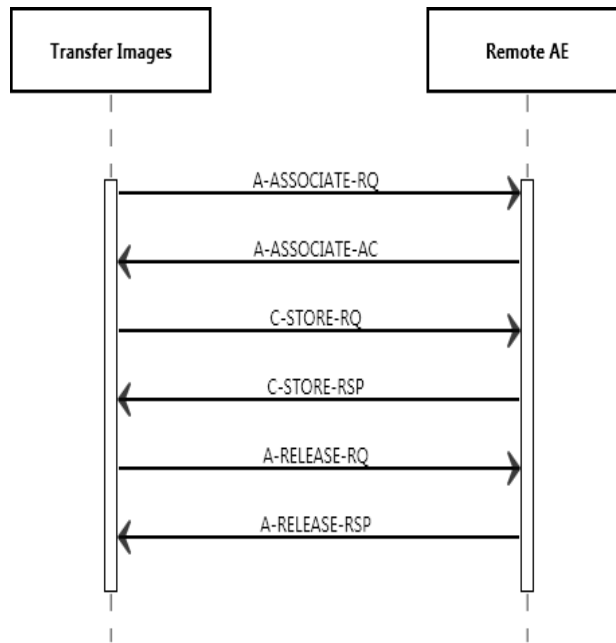


Figure 8: (Real World) Activity – Image Export

4.2.1.3.4.2. Proposed Presentation Contexts

Each time an association is initiated, the Azurion R3.1 proposes two presentation contexts to be used on that association. The presentation context proposed by the Azurion R3.1 for Transfer Images is defined in Table 27.

The implementation proposes each SOP Class only once in the abstract syntax specifying all possible transfer syntaxes for that SOP Class. Due to the fact that the SCP has to react with a chosen transfer syntax, as per SOP Class used transfer syntax is forced by the SCP.

Table 27: Proposed Presentation Contexts for (Real-World) Activity Image Export

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Secondary Capture Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14)	1.2.840.10008.1.2.4.70		
Grayscale Softcopy Presentation State Storage SOP Class	1.2.840.10008.5.1.4.1.1.11.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
X-Ray Angiographic Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.12.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14)	1.2.840.10008.1.2.4.70		
X-Ray Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.67	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

**4.2.1.3.4.3. SOP Specific Conformance for Storage SOP Classes**

Azurion R3.1 can exchange image data in the following formats:

- X-Ray Angiographic images can either be sent with raw pixel data or processed pixel data.
- Standard Secondary Capture (1.2.840.10008.5.1.4.1.1.7)
- Standard Grayscale Softcopy Presentation State SOP Class (1.2.840.10008.5.1.4.1.1.11.1)

Furthermore, the Azurion R3.1 can exchange non-image data in the following format:

- X-Ray Radiation Dose Structured Report (1.2.840.10008.5.1.4.1.1.88.67)

The behavior of Azurion R3.1 for status codes in a C-STORE response is summarized in Table 28.

**Table 28: Storage C-STORE Response Status Handling Behavior**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Successful operation	The SCP has successfully stored the SOP Instances. If all SOP Instances in a send job have status success, then the job is marked as completed. Success is logged.
Refused	A700	Out of Resources	The association is released, and the send job is marked as failed. An error message is logged.
Error	A900	Data Set does not match SOP Class	The association is released, and the send job is marked as failed. An error message is logged.
	C000-CFFF	Cannot Understand	The association is released, and the send job is marked as failed. An error message is logged.
Warning	B000	Coercion of Data Elements	The association is released, and the send job is marked as failed. An error message is logged.
	B006	Elements discarded	The association is released, and the send job is marked as failed. An error message is logged.
	B007	Data set does not match SOP class	The association is released, and the send job is marked as failed. An error message is logged.
*	Any other status code	*	The association is released, and the send job is marked as failed.

The behavior of Azurion R3.1 during communication failure is summarized in Table below.

Table 29: Storage Communication Failure Behavior

Exception	Behavior
Timeout	The send job is marked as failed. An error message is logged.
Association aborted	The send job is marked as failed. An error message is logged.
Association rejected	The send job is marked as failed. An error message is logged.

4.2.1.3.5. (Real-World) Activity – Storage Commitment Push Model AS SCU

4.2.1.3.5.1. Description and Sequencing of Activities

Azurion R3.1 Storage Commitment as a SCU service. It accepts a storage commitment notification (N-EVENT-REPORT) from systems that send them.

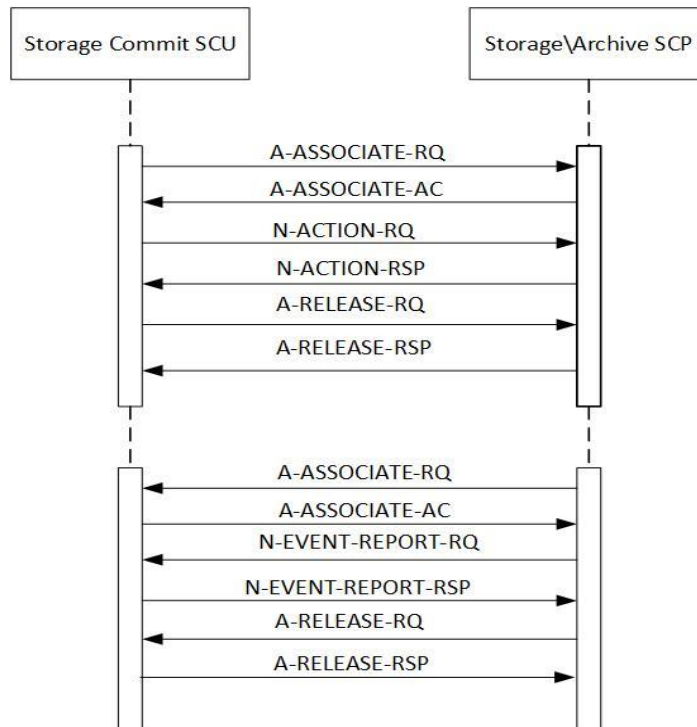


Figure 9: Data Flow Diagram – Commit Image (Asynchronous)

4.2.1.3.5.2. Proposed Presentation Contexts

The presentation contexts are defined in the Table below.

Table 30: Proposed Presentation Contexts for (Real-World) Activity – Storage Commitment Push Model as SCU

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Storage Commitment Push	1.2.840.10008.3.1.2.3.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Model SOP Class		Explicit VR Big Endian	1.2.840.10008.1.2.2		

**4.2.1.3.5.3. SOP Specific Conformance for Storage Commitment Push Model SOP Class**

This section and sub-section include the manufacturer SOP and Dataset specific information as well the status codes and their corresponding behavior.

**4.2.1.3.5.3.1. Dataset Specific Conformance for Storage Commitment Push Model SOP Class N-ACTION-SCU**

Details regarding the Dataset Specific response behavior will be reported in this section.

**Table 31: N-ACTION-RQ Dataset Specification**

Storage Commitment Push Model SOP Class			
Attribute Name	Tag	VR	Comment
<b>SOP Common Module</b>			
SOP Class UID	0008,0016	UI	
SOP Instance UID	0008,0018	UI	
<b>Storage Commitment Module</b>			
Transaction UID	0008,1195	UI	
Referenced SOP Sequence	0008,1199	SQ	
>Referenced SOP Class UID	0008,1150	UI	
>Referenced SOP Instance UID	0008,1155	UI	

The details regarding the response behavior to status codes are provided in Table below.

**Table 32: Storage Commitment N-ACTION Response Status Handling Behavior**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Successful operation	The storage commitment request has been successfully sent. The storage commitment request job is marked as completed. Success is logged.

**Table 33: Storage Commitment N-EVENT-REPORT Behavior**

Event Type	Event Type ID	Behavior
Storage Commitment Request Successful	1	The Examination is marked as completed and it becomes a candidate for an automatic deletion from the local database if local resources become scarce.
Storage Commitment Request Complete – Failures Exist	2	The failure is reported to the operator by not marking the examination as completed. The operator may re-transfer the image data (which was previously transferred to the PACS).

### 4.2.1.3.5.3.2. Dataset Specific Conformance for Storage Commitment Push Model SOP Class N-EVENT-REPORT-SCP

Details regarding the Dataset Specific response behavior will be reported in this section.

**Table 34: N-EVENT-REPORT-RSP Dataset Specification**

Storage Commitment Push Model SOP Class			
Attribute Name	Tag	VR	Comment
SOP Common Module			
SOP Class UID	0008,0016	UI	
SOP Instance UID	0008,0018	UI	

The details regarding the response behavior to status codes are provided in Table below.

**Table 35: Storage Commitment N-EVENT-REPORT Response Status Handling Behavior**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Successful operation	The storage commitment result has been successfully received. The SCP has successfully stored the SOP Instances. The examination is marked as completed.

**Table 36: Storage Commitment N-EVENT-REPORT Response Status**

Event Type	Event Type ID	Behavior
Storage Commitment Request Successful	1	The Examination is marked as completed and it becomes a candidate for an automatic deletion from the local database if local resources become scarce.
Storage Commitment Request Complete – Failures Exist	2	The failure is reported to the operator by not marking the examination as completed. The operator may re-transfer the image data (which was previously transferred to the PACS).

### 4.2.1.3.6. (Real-World) Activity – FIND as SCU

#### 4.2.1.3.6.1. Description and Sequencing of Activities

The operator is able to query a (pre-configured) remote database. The ACP AE initiates an association to the selected Remote AE and uses it to send C-FIND requests (and receive the associated find replies). For each query a number of C-FIND requests is established in one association to the peer entity, which is released when all query results are received. An example sequencing of Activities is presented in Figure 10 and Figure 11.



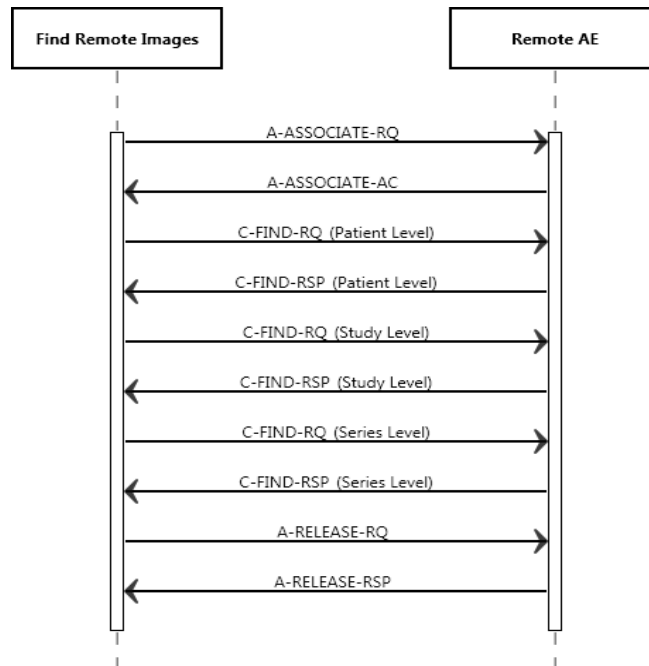


Figure 10: Sequencing of RWA (Patient Root Q/R Information Model)

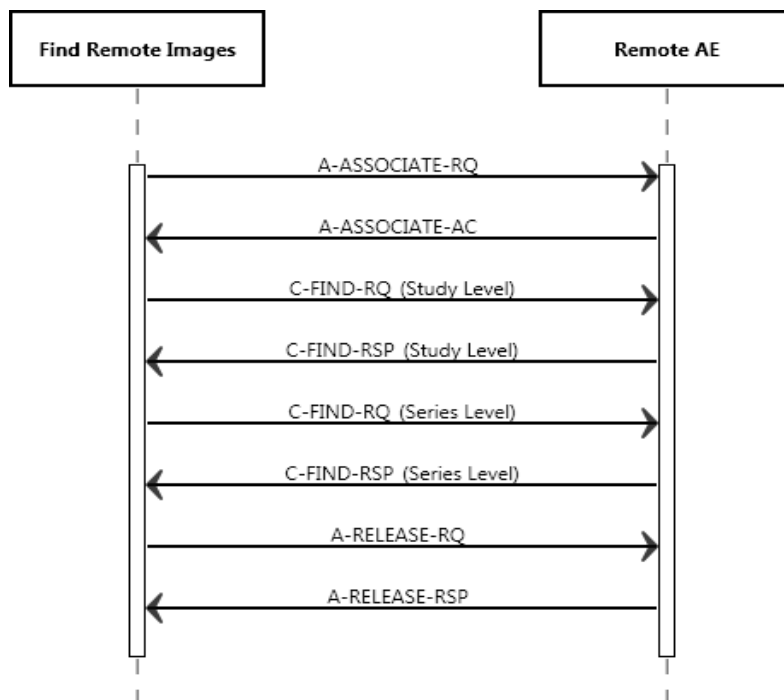


Figure 11: Sequencing of RWA (Study Root Q/R Information Model)

The clinical user may cancel the query to the PACS or Workstation. As a result, the Azurion R3.1 sends a C-FIND Cancel Request to the PACS or Workstation.

**4.2.1.3.6.2. Proposed Presentation Contexts**

Each time an association is initiated, the ACP AE proposes two presentation contexts to be used on that association. The presentation context proposed by the ACP AE for Find Remote Images is defined in Table 37.

**Table 37: Proposed Presentation Contexts for (Real-World) Activity – FIND As SCU**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Patient Root QR Information Model – FIND SOP Class	1.2.840.10008.5.1.4.1.2 .1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Study Root QR Information Model – FIND SOP Class	1.2.840.10008.5.1.4.1.2 .2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

**4.2.1.3.6.3. SOP Specific Conformance for Patient Root QR Information Model – FIND SOP Class**

The Azurion R3.1 provides standard conformance to this SOP class. The Azurion R3.1 AE does not generate queries containing optional keys and it does not generate relational queries.

**4.2.1.3.6.3.1. Dataset Specific Conformance for Patient Root QR Information Model - FIND SOP Class C-FIND-SCU**

In Table below the supported query keys for each query level are described. Universal matching is supported by default.

**Table 38: Supported Query Keys for Patient Root Information Model**

Patient Root Information Model				
Attribute Name	Tag	VR	Value	Comment
<b>SOP Common Module</b>				
Query/Retrieve Level	0008,0052	CS	Single Value	PATIENT, STUDY, SERIES
Specific Character Set	0008,0005	CS		
<b>Q/R Patient Level</b>				
Patient’s Name	0010,0010	PN	Single value matching or wild card matching or universal matching	
Patient ID	0010,0020	LO	Single value matching or wild card matching or universal matching	
Patient’s Birth Date	0010,0030	DA	Single value matching or universal matching	
Patient’s Sex	0010,0040	CS	Universal matching only	
<b>Q/R Study level</b>				
Study Date	0008,0020	DA	Range matching or universal matching	
Study Time	0008,0030	TM	Universal matching only	

Patient Root Information Model				
Attribute Name	Tag	VR	Value	Comment
Accession Number	0008,0050	SH	Value matching or wild card matching or universal matching	
Query/Retrieve Level	0008,0052	CS	Single	
Modalities in Study	0008,0061	CS	Single	
Study Description	0008,1030	LO	Universal matching	
Patient's Name	0010,0010	PN	Single value matching or wild card matching or universal matching	
Patient ID	0010,0020	LO	Single value matching or universal matching	
Patient's Birth Date	0010,0030	DA	Single value matching or universal matching	
Patient's Sex	0010,0040	CS	Universal matching only	
Patient Size	0010,1020	DS	Universal matching	
Patient Weight	0010,1030	DS	Universal matching	
Patient Comment	0010,4000	LT	Universal matching	
Study ID	0020,0010	SH	Universal matching only	
Study Instance UID	0020,000D	UI	Universal matching only	
Number Of Study Related Series	0020,1206	IS	Universal matching	
Q/R Series level				
Modality	0008,0060	CS	Universal matching only	
Series Description	0008,103E	LO	Universal matching	
Number Of Series Related Instances	0008,1050	PN	Universal matching only	
Study Instance UID	0020,000D	UI	Single value matching only	
Series Instance UID	0020,000E	UI	Universal matching only	
Series Number	0020,0011	IS	Universal matching only	

The behavior of the Azurion R3.1 for status codes in C-FIND response is summarized in Table below.

**Table 39: Status Response**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Matching is complete – No final Identifier is supplied.	Stops with processing the C-Find Response(s) from the SCP. All results are displayed to the operator.
Refused	A700	Out of Resources	The association is released, and the send job is marked as failed. An error message is logged.
Failed	A900	Identifier Does Not Match SOP Class	The association is released, and the send job is marked as failed. An error message is logged.
	CXXX	Unable to process	The association is released, and the send job is marked as failed. An error message is logged.
Cancel	FE00	Matching terminated due to Cancel Match request	Stops with processing the C-Find Response(s) from the SCP. Results already received up to that point are displayed to the operator.

Service Status	Error Code	Further Meaning	Behavior
Pending	FF00	Matches are continuing – Current Match is supported in the same manner as supplied and any Optional Keys were Required Keys.	Continues with processing of the C-Find Response(s) from the SCP
	FF01	Matches are continuing – Warning that one or more Optional Keys were not supported for existence for this Identifier.	Continues with processing of the C-Find Response(s) from the SCP.
*	Any other status code	*	The association is aborted using A-ABORT. The reason is logged, and the failure is reported to the user.

The behavior of the Azurion R3.1 during communication failure is summarized in below table.

**Table 40: DICOM Command Communication Failure Behavior**

Exception	Behavior
Timeout	The send job is marked as failed. An error message is logged.
Association aborted	The send job is marked as failed. An error message is logged.
Association rejected	The send job is marked as failed. An error message is logged.

**4.2.1.3.6.4. SOP Specific Conformance for Study Root QR Information Model – FIND SOP Class**

The Azurion R3.1 provides standard conformance to this SOP class. The Azurion R3.1 AE does not generate queries containing optional keys and it does not generate relational queries.

**4.2.1.3.6.4.1. Dataset Specific Conformance for Study Root QR Information Model - FIND SOP Class C-FIND-SCU**

In table below the supported query keys for each query level are described. Universal matching is supported as default.

**Table 41: Supported Query Keys for Study Root Information Model**

Study Root Information Model				
Attribute Name	Tag	VR	Value	Comment
<b>SOP Common Module</b>				
Query/Retrieve Level	0008,0052	CS	Single Value	STUDY, SERIES
Specific Character Set	0008,0005	CS		
<b>Q/R Study level</b>				
Study Date	0008,0020	DA	Range matching or universal matching	
Study Time	0008,0030	TM	Universal matching only	
Accession Number	0008,0050	SH	Value matching or wild card matching or universal matching	
Query/Retrieve Level	0008,0052	CS	Single	STUDY
Modalities in Study	0008,0061	CS	Single	
Study Description	0008,1030	LO	Universal matching	

Study Root Information Model				
Attribute Name	Tag	VR	Value	Comment
Patient's Name	0010,0010	PN	Single value matching or wild card matching or universal matching	
Patient ID	0010,0020	LO	Single value matching or universal matching	
Patient's Birth Date	0010,0030	DA	Single value matching or universal matching	
Patient's Sex	0010,0040	CS	Universal matching only	
Patient Size	0010,1020	DS	Universal matching	
Patient Weight	0010,1030	DS	Universal matching	
Patient Comment	0010,4000	LT	Universal matching	
Study ID	0020,0010	SH	Universal matching only	
Study Instance UID	0020,000D	UI	Universal matching only	
Number Of Study Related Series	0020,1206	IS	Universal matching	
Referring Physician name	0008,0090	PN	Universal matching	
Q/R Series level				
Modality	0008,0060	CS	Universal matching only	
Series Description	0008,103E	LO	Universal matching	
Number Of Series Related Instances	0008,1050	PN	Universal matching only	
Study Instance UID	0020,000D	UI	Single value matching only	
Series Instance UID	0020,000E	UI	Universal matching only	
Series Number	0020,0011	IS	Universal matching only	

The behavior of the Azurion R3.1 for status codes in C-FIND response is summarized in below table.

**Table 42: Status Response**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Matching is complete – No final Identifier is supplied.	Stops with processing the C-Find Response(s) from the SCP. All results are displayed to the operator.
Refused	A700	Out of Resources	The association is released, and the send job is marked as failed. An error message is logged.
Failed	A900	Identifier Does Not Match SOP Class	The association is released, and the send job is marked as failed. An error message is logged.
	CXXX	Unable to process	The association is released, and the send job is marked as failed. An error message is logged.
Cancel	FE00	Matching terminated due to Cancel Match request	Stops with processing the C-Find Response(s) from the SCP. Results already received up to that point are displayed to the operator.
Pending	FF00	Matches are continuing – Current Match is supported in the same manner as supplied and any Optional Keys were Required Keys.	Continues with processing of the C-Find Response(s) from the SCP

Service Status	Error Code	Further Meaning	Behavior
	FF01	Matches are continuing – Warning that one or more Optional Keys were not supported for existence for this Identifier.	Continues with processing of the C-Find Response(s) from the SCP.
*	Any other status code	*	The association is aborted using A-ABORT. The reason is logged, and the failure is reported to the user.

The behavior of the Azurion R3.1 during communication failure is summarized in below table.


**Table 43: DICOM Command Communication Failure Behavior**

Exception	Behavior
Timeout	The send job is marked as failed. An error message is logged.
Association aborted	The send job is marked as failed. An error message is logged.
Association rejected	The send job is marked as failed. An error message is logged.

### 4.2.1.3.7. (Real-World) Activity – MOVE as SCU

#### 4.2.1.3.7.1. Description and Sequencing of Activities

The request to move remote images is forwarded to the job queue. For each move job, one association towards the remote system is established, and C-MOVE requests are transmitted. Once the responses are received, the association is closed. An example of sequencing of activities is presented in Figure C-MOVE requests are done on the series level.

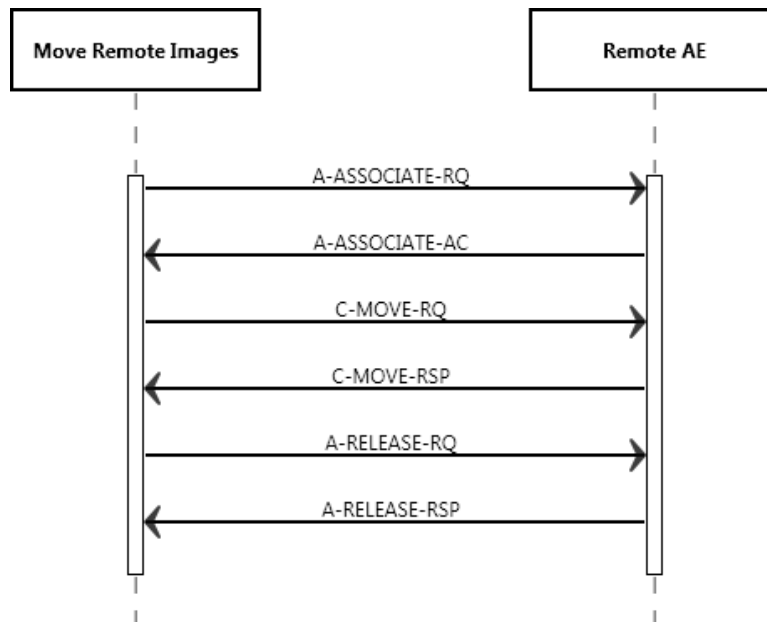

**Figure 12: Sequencing of RWA – MOVE as SCU**

The clinical user may cancel the move operation. As a result, the Azurion R3.1 Sends a C-MOVE Cancel Request to the PACS or Workstation.

**4.2.1.3.7.2. Proposed Presentation Contexts**

The presentation contexts for MOVE as SCU are defined in table below.

**Table 44: Proposed Presentation Contexts for (Real-World) Activity – MOVE As SCU**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Patient Root QR Information Model – MOVE SOP Class	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Study Root QR Information Model – MOVE SOP Class	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

The implementation proposes each SOP Class only ones in the abstract syntax specifying all possible transfer syntaxes for that SOP Class. Due to the fact that the SCP has to react with a chosen transfer syntax, the per SOP Class used transfer syntax is forced by the SCP.

**4.2.1.3.7.3. SOP Specific Conformance for SOP Classes**

Selecting a query result can retrieve only whole examinations. It is not possible to retrieve information if Patient ID contains the sign “greater than” or “less than” (> or <).

A C-MOVE can be done with the keys presented in Table 45 or Table 48.

**4.2.1.3.7.4. SOP Specific Conformance for Patient Root QR Information Model - MOVE SOP Class**

The Azurion R3.1 provides standard conformance for the Patient Root QR Information Model – MOVE SOP Class.

**4.2.1.3.7.4.1. Dataset Specific Conformance for Patient Root QR Information Model - MOVE SOP Class C-MOVE-SCU**

The behavior of the Identifiers for MOVE is summarized in this section.

**Table 45: Identifiers for MOVE Patient Root Information Model as SCU**

Patient Root Information Model			
Attribute Name	Tag	VR	Comment
<b>SOP Common Module</b>			
Query/Retrieve Level	0008,0052	CS	Applied value: Series
<b>Q/R Series level</b>			
Patient ID	0010,0020	PN	
Study Instance UID	0020,000D	UI	
Series Instance UID	0020,000E	UI	

The DICOM C-MOVE Patient Root Information Model Command Status Response Handling is shown in the Table below.

**Table 46: Status Response for C-MOVE Patient Root Information Model**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Sub-operations Complete No Failures	The move job is marked as completed. The association is released. Success is logged.
Refused	A701	Out of Resources – Unable to calculate number of matches	The association is released, and the send job is marked as failed.
	A702	Out of Resources – Unable to perform sub operations	An error message is logged. The reason is logged and reported to the user.
	A801	Move Destination Unknown	
Failed	A900	Identifier Does Not Match SOP Class	The association is released, and the send job is marked as failed.
	CXXX	Unable to process	An error message is logged
Cancel	FE00	Sub-operations terminated due to Cancel Indication	The move job is marked as cancelled. The association is released. The reason is logged and reported to the user.
Warning	B000	Sub-operations Complete – One or more Failures	The association is released, and the send job is marked as failed. An error message is logged
*	Any other status code	*	The association is released, and the send job is marked as failed. An error message is logged

The possible Communication Failures during a C-MOVE as SCU are shown in the Table below.

**Table 47: DICOM Command Communication Failure Behavior for C-MOVE Patient Root Information Model**

Exception	Behavior
Timeout	The send job is marked as failed. An error message is logged.
Association aborted	The send job is marked as failed. An error message is logged.
Association rejected	The send job is marked as failed. An error message is logged.

**4.2.1.3.7.5. SOP Specific Conformance for Study Root QR Information Model - MOVE SOP Class**

The Azurion R3.1 provides standard conformance to this SOP class.

**4.2.1.3.7.5.1. Dataset Specific Conformance for Study Root QR Information Model - MOVE SOP Class C-MOVE-SCU**

The identifiers for C-MOVE as SCU are listed in the Table below.

**Table 48: Identifiers for MOVE Study Root Information Model as SCU**

Study Root Information Model			
Attribute Name	Tag	VR	Comment
<b>SOP Common Module</b>			
Query/Retrieve Level	0008,0052	CS	Applied value: SERIES
<b>Q/R Series level</b>			
Series Instance UID	0020,000E	UI	
Study Instance UID	0020,000D	UI	



The DICOM C-MOVE Study Root Information Model Command Status Response Handling is shown in the Table below.

**Table 49: Status response for Study Root Information Model C-MOVE-SCU**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Sub-operations Complete No Failures	The SCP has successfully stored the SOP Instances. If all SOP Instances in a send job have status success, then the job is marked as completed. Success is logged.
Refused	A701	Out of Resources – Unable to calculate number of matches	The association is released, and the send job is marked as failed. An error message is logged.
	A702	Out of Resources – Unable to perform sub operations	
	A801	Move Destination Unknown	
Failed	A900	Identifier Does Not Match SOP Class	The association is released, and the send job is marked as failed. An error message is logged
	CXXX	Unable to process	
Cancel	FE00	Sub-operations terminated due to Cancel Indication	The move job is marked as cancelled. The association is released. The reason is logged and reported to the user.
Warning	B000	Sub-operations Complete – One or more Failures	The association is released, and the send job is marked as failed. An error message is logged.
*	Any other status code	*	The association is released, and the send job is marked as failed. An error message is logged.

The possible Communication Failures for C-MOVE as SCU are shown in the Table below.

**Table 50: DICOM Command Communication Failure Behavior for Study Root Information Model C-MOVE-SCU**

Exception	Behavior
Timeout	The send job is marked as failed. An error message is logged.
Association aborted	The send job is marked as failed. An error message is logged.
Association rejected	The send job is marked as failed. An error message is logged.

#### 4.2.1.3.8. (Real-World) Activity – Print Management as SCU

##### 4.2.1.3.8.1. Description and Sequencing of Activities

The operator can select images and request them to be printed on a printer (out of choice list of configured printers). Each request is forwarded to the job queue and processed as individual request to Print Images. The print job consists of data describing the images and graphics to be printed as well as the requested layout and other parameters. One print job on Azurion R3.1 may result in a number of film sessions with the printer equal to the number of printed film sheets. Each film sheet within the print job is internally processed, converted to a STANDARD/1, 1 page and then an association towards the remote Print Server is established and the page image is sent to that Print Server. Once the transmission of the film sheet is completed, the association is closed. A sequence of interactions between the Azurion R3.1 and a remote AE to print one film sheet is presented in Figure 13.

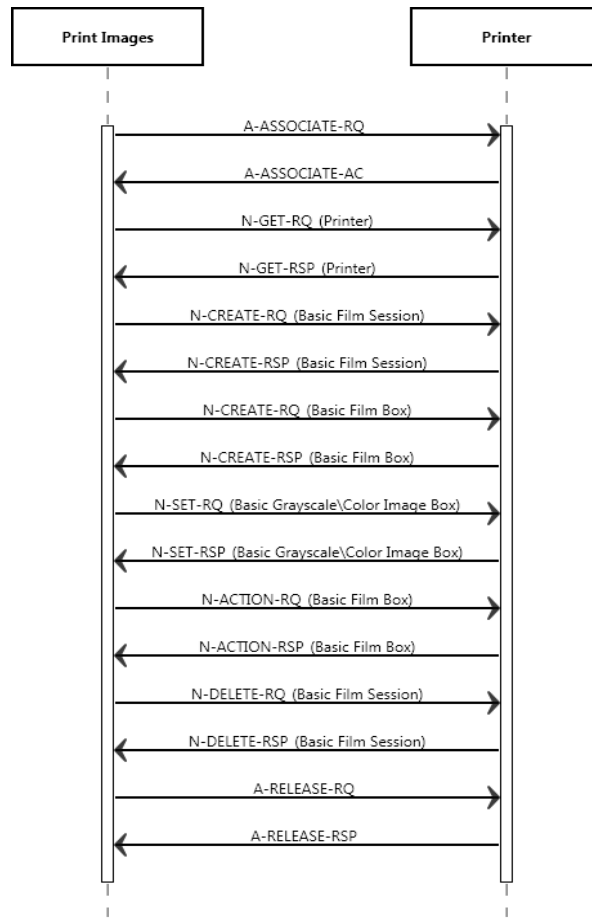


Figure 13: Sequencing of RWA – Print Management as SCU

The following implementation remarks are important to achieve successful printing:

- Each film session will be in a single association with one or more film boxes and one or more film sheets
- The number of images per Film Box is one. The images to be printed on one film are rendered by the Azurion R3.1 into one logical image. This logical image is very large, depending on the pixel matrix size (pixels per line, lines per image). A rough indication is 20 Mbytes. One should take this into account when selecting the DICOM printer and the printer configuration (e.g., the amount of memory).
- The Azurion R3.1 will request for releasing the association when the print command is given (i.e., the N-ACTION Request). The association is not kept open for receiving N-EVENT-REPORT of the Printer SOP Class.

Table 51: The Applied Order of Print Service Elements

Service Element of SOP Class	Description
N-GET of the Printer SOP Class	Purpose is to retrieve printer information.
N-CREATE of the Basic Film Session SOP Class	Specifies the DICOM Printer about some general presentation parameters, applicable for all films in the Film Session. Applied attributes are Number of Copies, Print Priority, Medium Type, Film Destination
N-CREATE of the Basic Film Box SOP Class	Specifies the DICOM Printer about some general presentation parameters, applicable for all images in the Film Box. Applied attributes are Film Orientation, Film Size ID, Magnification Type, Max. Density, Configuration Information, Trim.

Service Element of SOP Class	Description
N-SET of the Basic Grayscale Image Box SOP Class	Images to be printed. Applied attributes are Polarity
N-ACTION of the Basic Film Box SOP Class	Triggers the DICOM Printer to print. This actual print action is done at film box level. No attributes are present.

Table 52: Media Services

Service Element of SOP Class	Description
N-EVENT-REPORT of the Printer SOP Class	When N-EVENT-REPORT is received, no printer status polling on a separate connection is executed.

4.2.1.3.8.2. Proposed Presentation Contexts

Each time an association is initiated, the Azurion R3.1 proposes presentation contexts to be used on that association. The presentation contexts proposed by the Azurion R3.1 for Print Images is defined in Table 53.

The implementation proposes the SOP Class only ones in the abstract syntax specifying all possible transfer syntaxes for that SOP Class. Due to the fact that the SCP has to react with a chosen transfer syntax, as per SOP Class used transfer syntax is forced by the SCP.

Table 53: Proposed Presentation Contexts for (Real-World) Activity – Print Management as SCU

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Basic Grayscale Print Management Meta SOP Class	1.2.840.10008.5.1.1.9	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
>Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
>Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
>Basic Grayscale Image Box SOP Class	1.2.840.10008.5.1.1.4	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
>Printer SOP Class	1.2.840.10008.5.1.1.16	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Basic Color Print Management Meta SOP Class	1.2.840.10008.5.1.1.18	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
>Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
>Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
>Basic Color Image Box SOP Class	1.2.840.10008.5.1.1.4.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
>Printer SOP Class	1.2.840.10008.5.1.1.16	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

#### 4.2.1.3.8.3. SOP Specific Conformance for Basic Film Session SOP Class of the Basic Grayscale Print Management Meta SOP Class

The Azurion R3.1 provides standard conformance to the Basic Grayscale Print Management Meta SOP Class.

A description and the applied optional (i.e., non-mandatory attributes as Print SCU) attributes in these Service Elements are specified as well. Note that the Service Elements order is not specified by the DICOM standard. Azurion R3.1 sends the N-DELETE request for the film session. Overlay, annotation (showing the values of some major identifying attributes) and shutter information is processed in the images sent to the printer, all the processing including annotations will be part of the image.

This section and sub-section include the manufacturer SOP and Dataset specific information as well the status codes and their Corresponding behavior.

#### 4.2.1.3.8.3.1. Dataset Specific Conformance for Basic Film Session SOP Class for Basic Grayscale Print Meta N-CREATE-SCU

Table 54: N-CREATE-RQ Dataset Specification

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Number of Copies	2000,0010	IS	Between 1 and 100	ALWAYS	USER	
Print Priority	2000,0020	CS	MED	ALWAYS	AUTO	
Medium Type	2000,0030	CS	PAPER, BLUE FILM,	ALWAYS	AUTO	
Film Destination	2000,0040	CS	CLEAR FILM	ALWAYS	USER	
Film Session Label	2000,0050	LO	Human readable label that identifies the film session	ANAP	AUTO	

The details regarding the response behavior to status codes are provided in Table below.

Table 55: Status Response

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Successful operation	The print job continues.

Service Status	Error Code	Further Meaning	Behavior
Warning	0116	Any warning	The print job continues, and the warning is logged.
Error	0105	Any error	The association is aborted using A-ABORT. The print job will keep resubmitting the failed sheets until the error is solved or the retry timeout is exceeded.
	0106	Any error	The association is aborted using A-ABORT. The print job will keep resubmitting the failed sheets until the error is solved or the retry timeout is exceeded.

**4.2.1.3.8.4. SOP Specific Conformance for Basic Film Box SOP Class for the Basic Grayscale Print Management Meta SOP Class**

**4.2.1.3.8.4.1. Dataset Specific Conformance for Basic Film Box SOP Class for Basic Grayscale Print Meta N-CREATE-SCU**

The behavior of the Azurion R3.1 for status codes in an N-CREATE response is summarized in Table below.

**Table 56: N-CREATE-RQ Dataset Specification**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Image Display Format	2010,0010	ST	STANDARD\1,1	ANAP	AUTO	
Workstation Format	2010,0010	ST	STANDARD\C,R, CUSTOM\i	ANAP	AUTO	
Film Orientation	2010,0040	CS	LANDSCAPE, PORTRAIT	ANAP	USER	
Film Size ID	2010,0050	CS	DICOM specifies a number of Defined Terms; more values are possible and is print configuration dependent.	ANAP	USER	
Border Density	2010,0100	CS	BLACK	ANAP	USER	
Magnification Type	2010,0060	CS	Normally sent out, however sometimes send out empty Because some DICOM printers are not able to handle (Value NONE for) this attribute. Applied value(s): NONE	ANAP	AUTO	
Max Density	2010,0130	US	Maximum density of the images on the film, expressed in hundredths of OD. If Max Density is higher than maximum printer density than Max Density is set to maximum printer density.	ANAP	AUTO	
Trim	2010,0140	CS	NO	ANAP	AUTO	
Configuration Information	2010,0150	ST	Contains a vendor specific Lookup-table (LUT); should be applied by the DICOM printer if LUT data is present.	ANAP	AUTO	
Illumination	2010,015E	US		ANAP	AUTO	
Reflected Ambient Light	2010,0160	US		ANAP	AUTO	
Referenced Film Session Sequence	2010,0500	SQ		ANAP	AUTO	

>Referenced SOP Class UID	0008,1150	UI		ALWAYS	AUTO	
>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	AUTO	
Referenced Presentation LUT Sequence	2050,0500	SQ		ANAP	AUTO	

The details regarding the response behavior to status codes are provided in Table below.

**Table 57: Status Response**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Successful operation	The print job continues.
Warning	0116	Any warning	The print job continues, and the warning is logged.
Error	0105	Any error	The association is aborted using A-ABORT. The print job will keep resubmitting the failed sheets until the error is solved or the retry timeout is exceeded.
	0106	Any error	The association is aborted using A-ABORT. The print job will keep resubmitting the failed sheets until the error is solved or the retry timeout is exceeded.

#### 4.2.1.3.8.5. SOP Specific Conformance for Basic Grayscale Image Box SOP Class of the Basic Grayscale Print Management Meta SOP Class

##### 4.2.1.3.8.5.1. Dataset Specific Conformance for Basic Grayscale Image Box SOP Class for Basic Grayscale Print Meta N-SET-SCU

This application entity supports the attributes described in the table below.

**Table 58: N-SET-RQ Dataset Specification**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
SOP Class UID	0008,0016	UI		ALWAYS	AUTO	
SOP Instance UID	0008,0018	UI		ALWAYS	AUTO	
Image Box Position	2020,0010	US	1	ALWAYS	AUTO	
Polarity	2020,0020	CS	NORMAL	ALWAYS	AUTO	
Basic Grayscale Image Sequence	2020,0110	SQ		ALWAYS	AUTO	
>Samples Per Pixel	0028,0002	US	1	ANAP	AUTO	
>Photometric Interpretation	0028,0004	CS	MONOCHROME2	ANAP	AUTO	
>Rows	0028,0010	US	Depending on the selected printer type and film size.	ANAP	AUTO	
>Columns	0028,0011	US	Depending on the selected printer type and film size.	ANAP	AUTO	
>Pixel Aspect Ratio	0028,0034	IS		ANAP	AUTO	

>Bits Allocated	0028,0100	US	8 or 16	ANAP	AUTO	
>Bits Stored	0028,0101	US	8 or 12	ANAP	AUTO	
>High Bit	0028,0102	US	7 or 11	ANAP	AUTO	
>Pixel Representation	0028,0103	US	0X0000	ANAP	AUTO	
>Pixel Data	7FE0,0010	OW /OB		ANAP	AUTO	

The details regarding the response behavior to status codes are provided in Table below.

**Table 59: Status Response**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Successful operation	The print job continues.
Warning	0107	Any warning	The print job continues, and the warning is logged.
Error	0105	Any error	The association is aborted using A-ABORT. The print job will keep resubmitting the failed sheets until the error is solved or the retry timeout is exceeded.
	0106	Any error	The association is aborted using A-ABORT. The print job will keep resubmitting the failed sheets until the error is solved or the retry timeout is exceeded.

**4.2.1.3.8.6. SOP Specific Conformance for Basic Grayscale Image Box SOP Class for Basic Grayscale Print Management Meta SOP Class**

**4.2.1.3.8.6.1. Dataset Specific Conformance for Printer SOP Class for Basic Grayscale Print Meta N-GET-SCU**

This application entity supports the attributes described in the Table below.

**Table 60: N-GET-RQ Dataset Specification**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
SOP Class UID	0008,0016	UI		ALWAYS	AUTO	
SOP Instance UID	0008,0018	UI		ALWAYS	AUTO	
Printer Status	2110,0010	CS		ANAP	AUTO	
Printer Status Info	2110,0020	CS		ANAP	AUTO	
Print Priority	2000,0020	CS		ALWAYS	AUTO	
Execution Status	2100,0020	CS		ALWAYS	AUTO	
Execution Status Info	2100,0030	CS		ALWAYS	AUTO	

**4.2.1.3.8.6.2. Dataset Specific Conformance for Printer SOP Class for Basic Grayscale Print Meta N-EVENT-REPORT-SCP**

This application entity supports the attributes described in the below table.

**Table 61: N-EVENT-REPORT-RSP Dataset Specification**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
SOP Class UID	0008,0016	UI		ALWAYS	AUTO	
SOP Instance UID	0008,0018	UI		ALWAYS	AUTO	
Printer Status	2110,0010	CS		ANAP	AUTO	
Printer Status Info	2110,0020	CS		ANAP	AUTO	

**4.2.1.3.8.7. SOP Specific Conformance for Basic Color Print Management Meta SOP Class**

The Azurion R3.1 provides standard conformance to the Basic Color Print Management Meta SOP Class. A description and the applied optional (i.e., non-mandatory attributes as Print SCU) attributes in these Service Elements are specified as well. Note that the Service Elements order is not specified by the DICOM standard. Azurion R3.1 sends the N-DELETE request for the film session. Overlay, annotation (showing the values of some major identifying attributes) and shutter information is processed in the images sent to the printer, all the processing including annotations will be part of the image.

**4.2.1.3.8.8. SOP Specific Conformance for Basic Film Session SOP Class for Basic Color Print Management Meta SOP Class**

**4.2.1.3.8.8.1. Dataset Specific Conformance for Basic Film Session SOP Class for Basic Color Print Meta N-CREATE-SCU**

This application entity supports the attributes described in the Table below.

**Table 62: N-CREATE-RQ Dataset Specification**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Number of Copies	2000,0010	IS	Between 1 and 100	ALWAYS	USER	
Print Priority	2000,0020	CS	MED	ALWAYS	AUTO	
Medium Type	2000,0030	CS	PAPER, BLUE FILM, CLEAR FILM	ALWAYS	USER	
Film Destination	2000,0040	CS	MAGAZINE, PROCESSOR	ALWAYS	AUTO	
Film Session Label	2000,0050	LO	Human readable label that identifies the film session	ANAP	AUTO	

The details regarding the response behavior to status codes are provided in Table below.

**Table 63: Status Response**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Successful operation	The print job continues.
Warning	0107	Any warning	The print job continues, and the warning is logged.
Error	0105	Any error	The association is aborted using A-ABORT. The print job will keep resubmitting the failed sheets until the error is solved or the retry timeout is exceeded.
	0106	Any error	The association is aborted using A-ABORT. The print job will keep resubmitting the failed sheets until the error is solved or the retry timeout is exceeded.



**4.2.1.3.8.9. SOP Specific Conformance for Basic Film Box SOP Class for Basic Color Print Meta Management SOP Class**

**4.2.1.3.8.9.1. Dataset Specific Conformance for Basic Film Box SOP Class for Basic Color Print Meta N-CREATE-SCU**

The behavior of the Azurion R3.1 for status codes in an N-CREATE response is summarized in Table below.

**Table 64: N-CREATE-RQ Dataset Specification**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
SOP Class UID	0008,0016	UI		ALWAYS	AUTO	
SOP Instance UID	0008,0018	UI		ALWAYS	AUTO	
Workstation Format	2010,0010	ST	STANDARD\C, R, CUSTOM\i	ALWAYS	AUTO	
Film Orientation	2010,0040	CS	PORTRAIT, LANDSCAPE	ALWAYS	USER	
Film Size ID	2010,0050	CS	DICOM specifies a number of Defined Terms; more values are possible and is print configuration dependent.	ALWAYS	USER	
Magnification Type	2010,0060	CS	Normally sent out, however sometimes send out empty Because some DICOM printers are not able to handle (Value NONE for) this attribute. Applied value(s): NONE	ALWAYS	AUTO	
Max Density	2010,0130	US	Maximum density of the images on the film, expressed in hundredths of OD. If Max Density is higher than maximum printer density than Max Density is set to maximum printer density.	ALWAYS	AUTO	
Trim	2010,0140	CS	NO	ALWAYS	AUTO	
Configuration Information	2010,0150	ST	Contains a vendor specific Lookup-table (LUT); should be applied by the DICOM printer if LUT data is present.	ALWAYS	AUTO	
Reflected Ambient Light	2010,0160	US		ALWAYS	AUTO	
Referenced Film Session Sequence	2010,0500	SQ	Parent Film Session	ALWAYS	AUTO	
>Referenced SOP Class UID	0008,1150	UI	1.2.840.10008.5.1.1.1	ALWAYS	AUTO	
>Referenced SOP Instance UID	0008,1155	UI	UID of Parent Film Session	ALWAYS	AUTO	
Referenced Image Box Sequence	2010,0510	SQ		ALWAYS	AUTO	
Referenced Basic Annotation Box Sequence	2010,0520	SQ		VNAP	AUTO	

Referenced Presentation LUT Sequence	2050,0500	SQ		VNAP	AUTO	
--------------------------------------	-----------	----	--	------	------	--

The details regarding the response behavior to status codes are provided in Table below.

**Table 65: Status Response**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Successful operation	The print job continues.
Warning	0107	Any warning	The print job continues, and the warning is logged.
Error	0105	Any error	The association is aborted using A-ABORT. The print job will keep resubmitting the failed sheets until the error is solved or the retry timeout is exceeded.
	0106	Any error	The association is aborted using A-ABORT. The print job will keep resubmitting the failed sheets until the error is solved or the retry timeout is exceeded.

**4.2.1.3.8.9.2. Dataset Specific Conformance for Basic Film Box SOP Class for Basic Color Print Meta N-ACTION-SCU**

The behavior of the Azurion R3.1 for status codes in an N-ACTION response is summarized in Table below.

**Table 66: N-ACTION-RQ Dataset Specification**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
SOP Class UID	0008,0016	UI		ALWAYS	AUTO	
SOP Instance UID	0008,0018	UI		ALWAYS	AUTO	

**4.2.1.3.8.10. SOP Specific Conformance for Basic Color Image Box SOP Class for Basic Color Print Management Meta SOP Class**

**4.2.1.3.8.10.1. Dataset Specific Conformance for Basic Color Image Box SOP Class for Basic Color Print Meta N-SET-SCU**

This application entity supports the attributes described in the Table below.

**Table 67: N-SET-RQ Dataset Specification**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
SOP Class UID	0008,0016	UI		ALWAYS	AUTO	
SOP Instance UID	0008,0018	UI		ALWAYS	AUTO	
Image Box Position	2020,0010	US		ANAP	AUTO	
Polarity	2020,0020	CS		ANAP	AUTO	
Samples Per Pixel	0028,0002	US		ANAP	AUTO	
Photometric Interpretation	0028,0004	CS		ANAP	AUTO	
Rows	0028,0010	US		ANAP	AUTO	
Columns	0028,0011	US		ANAP	AUTO	
Pixel Aspect Ratio	0028,0034	IS		ANAP	AUTO	

Bits Allocated	0028,0100	US		ANAP	AUTO	
Bits Stored	0028,0101	US		ANAP	AUTO	
High Bit	0028,0102	US		ANAP	AUTO	
Pixel Representation	0028,0103	US		ANAP	AUTO	
Pixel Data	7FE0,0010	OW/OB		ANAP	AUTO	

The details regarding the response behavior to status codes are provided in Table below.

**Table 68: Status Response**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Successful operation	The print job continues.
Warning	0107	Any warning	The print job continues, and the warning is logged.
Error	0105	Any error	The association is aborted using A-ABORT. The print job will keep resubmitting the failed sheets until the error is solved or the retry timeout is exceeded.
	0106	Any error	The association is aborted using A-ABORT. The print job will keep resubmitting the failed sheets until the error is solved or the retry timeout is exceeded.

#### 4.2.1.3.8.11. SOP Specific Conformance for Basic Color Image Box SOP Class for Basic Color Print Management Meta SOP Class

##### 4.2.1.3.8.11.1. Dataset Specific Conformance for Printer SOP Class for Basic Color Print Meta N-EVENT-REPORT-SCP

This application entity supports the attributes described in the Table below.

**Table 69: N-EVENT-REPORT-RSP Dataset Specification**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
SOP Class UID	0008,0016	UI		ALWAYS	AUTO	
SOP Instance UID	0008,0018	UI		ALWAYS	AUTO	

#### 4.2.1.4. Association Acceptance Policy

The Application Entity will respond to a received Association rejection as shown in the Table below.

**Table 70: Association Reject response**

Result	Source	Reason/Diagnosis	Behavior
1 - rejected-permanent	1 - DICOM UL service-user	1 - no-reason-given	Log entry.
		2 - application-context-name-not supported	Log entry.
		3 - calling-AE-title-not-recognized	Log entry.
		7 - called-AE-title-not-recognized	Log entry.
	2 - DICOM UL service-provider (ACSE related function)	1 - no-reason-given	Log entry.
		2 - protocol-version-not-supported	Log entry.
	3 - DICOM UL service-provider (Presentation related function)	1 - temporary-congestion	Log entry.
		2 - local-limit-exceeded	Log entry.

Result	Source	Reason/Diagnosis	Behavior
2 – rejected - transient	1 - DICOM UL service-user	1 - no-reason-given	Log entry.
		2 - application-context-name-not-supported	Log entry.
		3 - calling-AE-title-not-recognized	Log entry.
		7 - called-AE-title-not-recognized	Log entry.
	2 - DICOM UL service-provider (ACSE related function)	1 - no-reason-given	Log entry.
		2 - protocol-version-not-supported	Log entry.
	3 - DICOM UL service-provider (Presentation related function)	1 - temporary-congestion	Log entry.
2 - local-limit-exceeded		Log entry.	

The behavior of the Azurion R3.1 during Abort Handling is summarized in Table below.


**Table 71: Association Abort Handling**

Source	Reason/Diagnosis	Behavior
0 - DICOM UL service-user (initiated abort)	0 - reason-not-specified	Log entry.
2 - DICOM UL service-provider (initiated abort)	0 - reason-not-specified	Log entry.
	1 - unrecognized-PDU	Log entry.
	2 - unexpected-PDU	Log entry.
	4 - unrecognized-PDU-parameter	Log entry.
	5 - unexpected-PDU-parameter	Log entry.
	6 - invalid-PDU-parameter-value	Log entry.

**4.2.1.4.1. (Real-World) Activity – Verification as SCP**

**4.2.1.4.1.1. Description and Sequencing of Activities**

A remote system requests verification from Azurion R3.1 using the C-ECHO command.

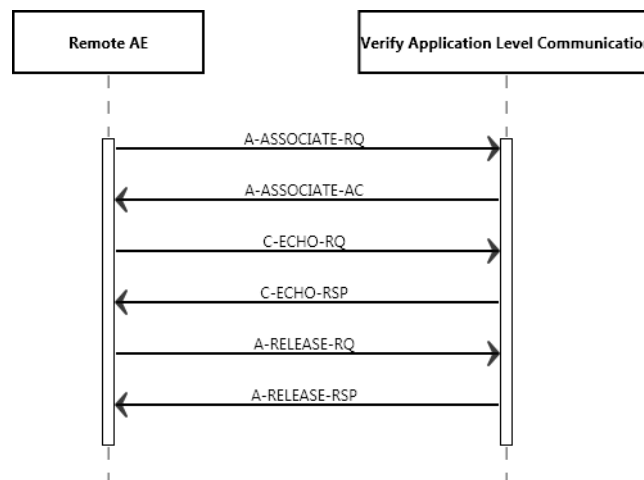

**Figure 14: (Real World) Activity – Verification as SCP Accepted Presentation Contexts**

**4.2.1.4.1.2. Accepted Presentation Contexts**

The presentation contexts are defined in the next table.

Table 72: Acceptable Presentation Contexts for (Real-World) Activity – Verification as SCP

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Verification SOP Class	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

4.2.1.4.1.3. SOP Specific Conformance for Verification SOP Class

Azurion R3.1 (C-ECHO SCP) provides standard conformance to the DICOM V3.0 verification SOP Class.

4.2.1.4.1.3.1. Dataset Specific Conformance for Verification C-ECHO SCP

This part of the section includes the dataset specific behavior, i.e., error codes, error and exception handling, time-outs, etc.

Table 73: Status Response

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Success	C-ECHO command was successful received.

4.2.1.4.2. (Real-World) Activity – Image Import

4.2.1.4.2.1. Description and Sequencing of Activities

The real world activity associated with the C-STORE operation is the storage of the image in the memory of the system upon which Azurion R3.1 is running in order to make it available for immediate processing by applications. Azurion R3.1 will issue a failure status if it is unable to store the image in the memory.

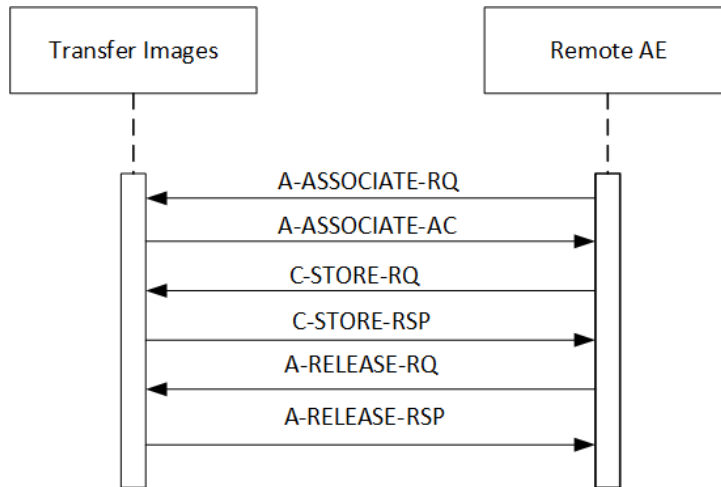


Figure 15: (Real World) Activity – Image Import

4.2.1.4.2.2. Accepted Presentation Contexts

The presentation contexts are defined in next table.

**Table 74: Acceptable Presentation Contexts for (Real-World) Activity – Image Import**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Secondary Capture Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14)	1.2.840.10008.1.2.4.70		
Grayscale Softcopy Presentation State Storage SOP Class	1.2.840.10008.5.1.4.1.1.11.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
X-Ray Angiographic Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.12.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14)	1.2.840.10008.1.2.4.70		

**4.2.1.4.2.3. SOP Specific Conformance for Storage SOP Classes**

This section and sub-section include the manufacturer SOP and Dataset specific information as well the status codes and their corresponding behavior.

Azurion R3.1 provides standard conformance to the DICOM V3.0 Storage Service Class as a SCP. Azurion R3.1 conforms to the SOPs of the Storage Service Class at Level 2 (Full). In case of a successful C-STORE, the stored image may be accessed by the processing applications.

**4.2.1.4.2.3.1. Dataset Specific Conformance for C-STORE-RSP**

This includes the dataset specific behavior, i.e., error codes, error and exception handling, time-outs, etc.

**Table 75: Status Response**

Service Status	Error Code	Further Meaning	Behavior
Success	0000	Successful stored	Whenever the store operation succeeded.
Failure	Cxxx	Failed	Whenever the store operation failed.
Failure	A901	Data set does not match SOP class	When the import operation has failed.
*	Any other status	Unsuccessful operation	Operation not completed, and reason is logged.

**4.3. Network Interfaces**

**4.3.1. Physical Network Interfaces**

The System provides only DICOM V3.0 TCP/IP Network Communication Support as defined in PS 3.8 of the standard.

TCP/IP is the only protocol stack supported.  
 Supported physical medium include:  
 IEEE 802.3-1995, 10BASE-T  
 IEEE 802.3-1995, 100BASE-TX (Fast Ethernet)  
 IEEE 802.3, 1000BASE-X (Fiber Optic Gigabit Ethernet).

The TCP/IP Stack as supported by the underlying Operating System.  
 The API is the WinSock 2 interface as supported by the underlying Operating System.

**4.3.2. Additional Protocols**

**4.3.2.1. Basic Application-Level Confidentiality Profile**

See Section 7.2.4.

**4.3.3. IPv4 and IPv6 Support**

Azurion R3.1 supports DICOM communication, as per DICOM standards/specifications, for both IPv4 and IPv6. However, not both IP versions at the same time. For BCP 195 secure connection see section 7.2.2.

**4.4. Configuration**

Any implementation's DICOM conformance may be dependent upon configuration, which takes place at the time of installation. Issues concerning configuration are addressed in this section.

**4.4.1. AE Title/Presentation Address Mapping**

An important installation issue is the translation from AE title to presentation address. How this is to be performed is described here.

**4.4.1.1. Local AE Titles**

The local AE title mapping and configuration are specified as:

**Table 76: AE Title configuration table**

Application Entity	Default AE Title	Default TCP/IP Port
IENGINE_SCU	IENGINE_SCU	29536

**4.4.1.2. Remote AE Title/Presentation Address Mapping**

All relevant remote applications that should be able to set up a DICOM association with Azurion R3.1 and that should be able to accept a DICOM association from Azurion R3.1 must be configured during the configuration time of Azurion R3.1.

**4.4.2. Parameters**

The specification of important operational parameters, their default value and range (if configurable) are specified here.

**Table 77: Configuration Parameters**

Local Parameters	Configurable	Default Value
AE Title	Yes	IENGINE_SCU
Port number	Yes	29536
IP host name/address	Yes	-



## 5. Media Interchange

### 5.1. Implementation model

The implementation model identifies the DICOM Application Entities for Media in specific implementation and relates the Application Entities to Real-World Activities.

#### 5.1.1. Application Data Flow Diagram

As part of the implementation model, an application data flow diagram is included. The next Figure shows the media interchange application data flow as a functional overview of the Media AE for DICOM CD and DVD.



Figure 16: Application Data Flow Diagram

The Media AE acts as a FSC for CD-R and DVD, when writing the selected images in a patient folder onto the medium.

#### 5.1.2. Functional Definitions of AE's

The Azurion R3.1 implements the following functions for DICOM media.

- Write a DICOM file-set onto the medium.
- Create a DICOMDIR file.

#### 5.1.3. Sequencing of Real World Activities

Not applicable.

## 5.2. AE Specifications

This section in the DICOM Conformance Statement specifies a set of Media Application Entities.

### 5.2.1. Media - Specification

This section contains general policies that apply to all of the Application Entities described in subsequent section. The Azurion R3.1 provides standard conformance to the DICOM interchange option of the media storage service class, and follows the specifications as defined in the DICOM standard – Media Storage and File Format for Data Interchange (PS 3.10) and Media Storage Application Profiles (PS 3.11).

The Azurion R3.1 supports multi-patient and multi-session for CD-R media (both reading and writing). For one or more Application Profiles, the following table shows the Real-World Activities and the roles of each of these Real-World Activities.

Table 78: AE Media Storage related Application Profiles, Real-World Activities and Roles

Supported Application Profile	Identifier	Real-World Activities	Roles
General Purpose CD-R Interchange	STD-GEN-CD	Create File-set	FSC/FSR

Supported Application Profile	Identifier	Real-World Activities	Roles
General Purpose Interchange on DVD-RAM Media	STD-GEN-DVD-RAM	Create File-set	FSC/FSR
General Purpose USB Media Interchange	STD-GEN-USB	Create File-set	FSC/FSR/FSU
General Purpose CD-R Interchange	STD-GEN-CD	Create File-set	FSC/FSR

### 5.2.1.1. DICOM File Meta Information for the Media

**Table 79: Implementation Identifying Information**

Implementation Class UID	1.3.46.670589.7.29.3.1.1
Implementation Version Name	Azurion

### 5.2.1.2. Real-World Activities

The AE specification contains a description of the Real-World Activities, which invoke the particular AE.

#### 5.2.1.2.1. RWA - Read File-set

Azurion R3.1 can read SC, XA and GSPS objects.

##### 5.2.1.2.1.1. Media Storage Application Profile

Refer to the table in section 5.2.1, Table 78: AE Media Storage related Application Profiles, Real-World Activities and Roles.

###### 5.2.1.2.1.1.1. Options

Not applicable.

#### 5.2.1.2.2. RWA - Create File-set

This Media Application Entity has a File-set Creator functionality which is described here.

##### Write Images

The Azurion R3.1 acts as an FSC when writing DICOM objects onto DICOM media. The Azurion R3.1 can also store private attributes.

When the Azurion R3.1 has to write objects to DICOM media, it can encounter the following situation. The objects were previously received via C-STORE operations. Some attributes in the received images have a zero-length value (Type 2 attributes). However, the Application Profile specifies some of these attributes as type 1: they must have a value. In such cases the Azurion R3.1 supplies a value for the following attributes (if necessary):

- Patient ID;
- Study ID;
- Series Number;
- Instance number;
- Study Date;
- Study Time.

The mechanism of generating a value for Patient ID is to create a new value (i.e., Study Instance UID) for each new study written to the medium, even if this study belongs to a patient recorded earlier. Study ID is assigned the

value of the first Requested Procedure ID (0040, 1001) encountered in the Request Attributes Sequence (0040, 0275).

#### **5.2.1.2.2.1. Media Storage Application Profile**

Refer to the table in section 5.2.1, Table 78: AE Media Storage related Application Profiles, Real-World Activities and Roles.

##### **5.2.1.2.2.1.1. Options**

Not applicable.

#### **5.2.1.2.3. RWA - Update File-set**

Not applicable.

#### **5.2.1.2.3.1. Media Storage Application Profile**

Refer to the table in section 5.2.1, Table 78: AE Media Storage related Application Profiles, Real-World Activities and Roles.

##### **5.2.1.2.3.1.1. Options**

Not applicable.

### **5.3. Augmented and Private Application Profiles**

Not applicable.

### **5.4. Media Configuration**

Not applicable.

## 6. Support of Character Sets

Any support for character sets in Network and Media services is described here.

**Table 80: Supported DICOM Character Sets**

Character Set Description	Defined Term	ESC Sequence	ISO Registration Number	Code Element	Character Set
Latin alphabet No. 1	ISO_IR 100	-	ISO-IR 6	G0	ISO 646
		-	ISO-IR 100	G1	Supplementary set of ISO 8859
Japanese	ISO 2022 IR 159	ESC 02/04 02/0804/04	ISO-IR 159	G0	JIS X 0212: Supplementary Kanji set
Japanese	ISO 2022 IR 87	ESC 02/04 04/02	ISO-IR 87	G0	JIS X 0208: Kanji and Hiragana
Japanese		ESC 02/09 04/09	ISO-IR 13	G1	JIS X 0201: Katakana
		ESC 02/08 04/10	ISO-IR 14	G0	JIS X 0201: Romaji (only for the patient's name)
Chinese	GB18030	-	GB18030	-	-

## 7. Security

### 7.1. Introduction

The security section describes security features implemented by this product. It includes description of non-DICOM network protocols, list of supported DICOM security profiles as well other applicable security related profiles.

### 7.2. DICOM Security Profile Support

#### 7.2.1. Secure Use and User Identity Profiles

Table 81: Secure Use and User Identity Profiles

Profile	Creator/Sender	Consumer/Receiver	Reference
Audit Trail Message Format	Yes	N/A	7.2.1.1.1
Audit Trail Message Transmission Profile - SYSLOG-TLS	Yes	N/A	7.2.1.1.1

#### 7.2.1.1. DICOM Security Profiles Details

##### 7.2.1.2. Audit Trail Messages

The Audit Trail Component is a component of Azurion R3.1 and can create messages according to the ATNA, IHE defined standard. Actors are information systems or components of information systems that produce, manage, or act on categories of information required by operational activities in the enterprise. The Audit Trail Component allows security officers in an institution to audit activities, to detect non-compliant behavior in the enterprise, and to facilitate detection of improper creation, access, modification and deletion of Protected Health Information (PHI), where PHI data is considered as information records (Registration, Order, Study/Procedure, Reports and to a lesser degree Images/Presentation States), and not the flow of information between the systems. This includes information exported to and imported from every secured node in the “secured domain”.

The messages will be created and sent to a syslog server according to the syslog protocol. The time that is used will be the local time of the system which is synchronized with the NTP Time Server. The timeserver and syslog server are elements of the Hospital infrastructure

The following table specifies the DICOM Audit Messages that Azurion R3.1 can detect and report. It defines the list of triggers that will cause audit message to be generated if these triggers can be configured or not. It also specifies if the content of the Audit message can be configured or not.

Table 82: DICOM Specific Audit Messages

Audit Message	Used
Data Export	Y
Data Import	Y
User Created	Y
User Deleted	Y
User Updated	Y
User Group Mapping Changed	Y
Begin Transferring DICOM Instances	Y
DICOM Instances Accessed	Y

Audit Message	Used
DICOM Instances Transferred	Y
Study Created	Y
Emergency Study Created	Y
Study Updated	Y
DICOM Study Deleted	Y
Series Updated	Y
Procedure Open With	Y
Procedure Started	Y
Procedure Complete	Y
Procedure Suspend	Y
Security Alert	Y
User Authentication - User Login	Y
User Authentication - User Logged Off	Y
Node Added	Y
Node Removed	Y
Patient Deleted	Y
Application Activity	Y

### 7.2.2. Security Transport Connection Profiles

Azurion R3.1 supports BCP 195 TLS Secure Transport Connection Profile.

**Table 83: Secure Transport Connections Profiles**

Profile	Secured AE	Sender	Receiver
BCP195 TLS Secure Transport Connection	ALL	Y	Y

The Azurion R3.1 supports X.509 certificates. The following TLS Certification checks will be done (TLS Handshake). The machine (either server or client) that will send its certificate will:

- Choose the certificate according to Common Name (CN) value in the Subject-field.
- This name is case-sensitive. All present certificates should have unique CN names.

The server verifies:

- That the client certificate is a X.509 certificate which is not tampered with
- That the client certificate is in the list of trusted certificates
- That the client certificate is not expired (present time is between “Valid From” and “Valid To” fields of the X.509 certificate)
- That the client certificate has the correct purpose (at least the Client Authentication purpose)

The client verifies:

- That the server certificate is a X.509 certificate which is not tampered with
- That the server certificate is in the list of trusted certificates
- That the server certificate is not expired (present time is between “Valid From” and “Valid To” fields of the X.509 certificate)
- That the server certificate has the correct purpose (at least Server Authentication purpose)

No verification is done on:

- Revocation of certificates
- Limiting the connection to a limited set of IP-addresses

Node authentication with or without encryption is only possible when both nodes have:

- An access to their own private keys
- An access to a copy of the certificate of the other node containing its public key

The Azurion R3.1 can only read certificates from the certificate stores of the HKEY\_LOCAL\_MACHINE registry key. It is the responsibility of the Hospital to setup and maintain the certificate stores. This includes the removal of revoked certificates and certificate updates prior to their expiration. Since neither X.500 directories, Lightweight Directory Access Protocol (LDAP) nor Certificate Revocation Lists (CRLs) are supported, the whole certificate chain needs to be replaced after a security breach.

The following figure presents the message flow of TLS handshake supported.

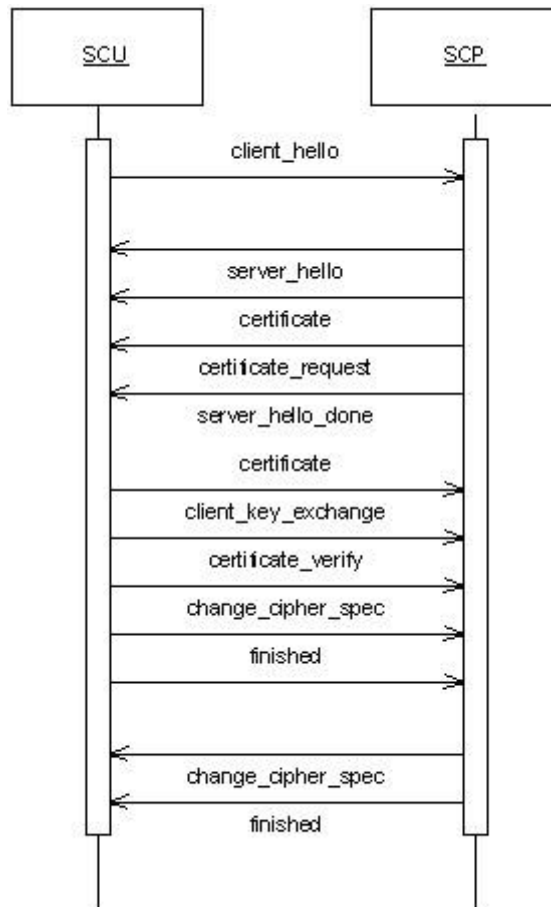


Figure 17: Message flow of TLS handshake

Azurion R3.1 supports Secure communication as a “mode of operation”. This functionality will be used by the DICOM nodes, which can authenticate each other before they exchange DICOM information. For secure communication, the TLS protocol v1.0,1.1 &1.2 are used which provides message authentication, integrity, confidentiality, and replay protection. Confidentiality is optional and can be controlled by the encryption settings. The system supports a secure negotiation using the following Cipher Suites.

**Table 84: Secure Transport Connections and Cipher Suites**

Profile	Cipher Suite
BCP 195 TLS Secure Transport Connection	TLS_ECDHE_ECDSA_WITH_AES_256_GCM_SHA384
	TLS_ECDHE_ECDSA_WITH_AES_128_GCM_SHA256
	TLS_ECDHE_RSA_WITH_AES_256_GCM_SHA384
	TLS_ECDHE_RSA_WITH_AES_128_GCM_SHA256
	TLS_DHE_RSA_WITH_AES_256_GCM_SHA384
	TLS_DHE_RSA_WITH_AES_128_GCM_SHA256
	TLS_ECDHE_ECDSA_WITH_AES_256_CBC_SHA384
	TLS_ECDHE_ECDSA_WITH_AES_128_CBC_SHA256
	TLS_ECDHE_RSA_WITH_AES_256_CBC_SHA384
	TLS_ECDHE_RSA_WITH_AES_128_CBC_SHA256
	TLS_ECDHE_ECDSA_WITH_AES_256_CBC_SHA
	TLS_ECDHE_ECDSA_WITH_AES_128_CBC_SHA
	TLS_ECDHE_RSA_WITH_AES_256_CBC_SHA
	TLS_ECDHE_RSA_WITH_AES_128_CBC_SHA
	TLS_RSA_WITH_AES_256_GCM_SHA384
	TLS_RSA_WITH_AES_128_GCM_SHA256
	TLS_RSA_WITH_AES_256_CBC_SHA256
	TLS_RSA_WITH_AES_128_CBC_SHA256
	TLS_RSA_WITH_AES_256_CBC_SHA
	TLS_RSA_WITH_AES_128_CBC_SHA
	TLS_DHE_RSA_WITH_AES_256_CBC_SHA
	TLS_DHE_RSA_WITH_AES_128_CBC_SHA
	TLS_DHE_DSS_WITH_AES_256_CBC_SHA256
	TLS_DHE_DSS_WITH_AES_128_CBC_SHA256
	TLS_DHE_DSS_WITH_AES_256_CBC_SHA
	TLS_DHE_DSS_WITH_AES_128_CBC_SHA

**Note:** Cipher suites that include cryptographic MD5, RC4, DES or 3DES are not supported by the system.

### 7.2.3. Media Storage Security Profiles

Not applicable.

### 7.2.4. Attribute Confidentiality Profiles

Azurion R3.1 conforms to the Basic Application-Level Confidentiality Profile as a de-identifier. This functionality is targeted towards creating a special purpose, de-identified version of an already existing Data set.

**Table 85: Attribute Confidentiality Profiles**

Profile	Option	AE	De-identifier	Re-identifier	Configurable
Basic Application-Level Confidentiality	Basic Profile	ALL	Y	N	Y

Table presents all attributes that can be de-identified by the Azurion R3.1. Each Attribute to be protected has its value replaced by a different “replacement value” which does not allow identification of the patient.



**Table 86: De-identified Attributes**

Attribute Name	Tag	VR	Replacement Value
Patient Name	0010,0010	PN	Assign user-specified value
Patient ID	0010,0020	LO	Generate and provide a new ID
Patient’s Birth Date	0010,0030	DA	Make Empty
Patient’s Sex	0010,0040	CS	Make Empty
Other Patient Ids	0010,1000	LO	Make Empty
Patient’s Size	0010,1020	DS	Make Empty
Patient Weight	0010,1030	DS	Make Empty
Ethnic Group	0010,2160	SH	Make Empty
Additional Patient’s History	0010,21B0	LT	Make Empty
Patient Comments	0010,4000	LT	Make Empty
SOP Instance UID	0008,0018	UI	Generate and provide new ID
Accession Number	0008,0050	SH	Make Empty
Institution Name	0008,0080	LO	Make Empty
Referring Physician’s Name	0008,0090	PN	Make Empty
Device Serial Number	0008,1000	LO	Make Empty
Station Name	0008,1010	SH	Make Empty
Institutional Department Name	0008,1040	LO	Make Empty
Performing Physician’s Name	0008,1050	PN	Make Empty
Operators’ Name	0008,1070	PN	Make Empty
Referenced SOP Instance UID	0008,1155	UI	Generate and provide a new ID
Protocol Name	0018,1030	LO	Make Empty
Study ID	0020,0010	SH	Make Empty
Study Instance UID	0020,000D	UI	Generate and provide a new ID
Series Instance UID	0020,000E	UI	Generate and provide a new ID
Performed Procedure Step Description	0040,0254	LO	Make Empty
Request Attributes Sequence	0040,0275	SQ	Generate and provide dummy value
Series Description	0008,103E	LO	Make Empty

**7.2.5. Digital Signature Profiles**

Not applicable.

**7.2.6. Basic Network Address Management Profiles**

Not applicable.

**7.2.7. Application Configuration Management Profiles**

Not applicable.

**7.2.8. Time Synchronization Profiles**

Azurion R3.1 conforms to the IHE Consistent Time Profile as time client. It is possible to synchronize time with the NTP Timeserver using serviceability. The NTP Timeserver is an element of Hospital Infrastructure.

### 7.3. Association Level Security

The Azurion R3.1 accepts associations from any AE-Title but only for Storage Commit N-Event-Report, and C-Store as SCP services. If Azurion R3.1 is configured to use secure mode, then the incoming associations (for Azurion R3.1 as SCP) should follow secure mode.

### 7.4. Application Level Security

The Azurion R3.1 allows the use of either a conventional (non-secure) DICOM communication or a secure DICOM communication based on the Transport Layer Security (TLS) protocol [TLS]. If configured, the Azurion R3.1 supports security Measures for:

- Secure authentication of a node
- Integrity and confidentiality of transmitted data
- Replay protection
- Generation of audit trail records
- Access control and user authentication.

## 8. Annexes

### 8.1. IOD Contents

#### 8.1.1. Created SOP Instance

This section specifies each IOD created by this application and specifies the content for each IOD created (including private IODs).

For each attribute in the IOD the following information is supplied:

- Attribute name
- Tag
- VR – Value representation
- Value – specifies possible values
- Presence of value – specifies if attribute is always present or only under specific conditions
- Source of value – specifies the source of the value
- Comment – gives additional information on the attribute

**Abbreviations used in the IOD tables for the column "Presence of Module" are:**

ALWAYS            The module is always present  
 CONDITIONAL    The module is used under specified condition

**Abbreviations used in the Module table for the column "Presence of Value" are:**

ALWAYS            The attribute is always present with a value  
 EMPTY            The attribute is always present without any value (attribute sent zero length)  
 VNAP              The attribute is always present and its Value is Not Always Present (attribute sent zero length if no value is present)  
 ANAP              The attribute is present under specified condition – if present then it will always have a value

**The abbreviations used in the Module table for the column "Source" are:**

AUTO                The attribute value is generated automatically  
 CONFIG            The attribute value source is a configurable parameter  
 COPY                The attribute value source is another SOP instance  
 FIXED              The attribute value is hard-coded in the application  
 IMPLICIT          The attribute value source is a user-implicit setting  
 MPPS                The attribute value is the same as that use for Modality Performed Procedure Step  
 MWL                The attribute value source is a Modality Worklist  
 USER              The attribute value source is explicit user input

#### 8.1.1.1. List of created SOP Classes

**Table 87: List of created SOP Classes**

SOP Class Name	SOP Class UID
Secondary Capture Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.7
Grayscale Softcopy Presentation State Storage SOP Class	1.2.840.10008.5.1.4.1.1.11.1
X-Ray Angiographic Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.12.1
X-Ray Radiation Dose Structured Report SOP Class	1.2.840.10008.5.1.4.1.1.88.67

**8.1.1.1.1. Secondary Capture Image Storage SOP Class**

**Table 88: SOP Class Modules**

Information Entity	Module	Presence Of Module
Patient	Patient Module	ALWAYS
Study	General Study Module	ALWAYS
	Patient Study Module	ALWAYS
Series	General Series Module	ALWAYS
Equipment	General Equipment Module	ALWAYS
	SC Equipment Module	ALWAYS
Image	General Image Module	ALWAYS
	Image Pixel Module	ALWAYS
	General Reference Module	CONDITIONAL
	SC Image Module	ALWAYS
	VOI LUT Module	ALWAYS
	SOP Common Module	ALWAYS

**Table 89: Patient Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Referenced Patient Sequence	0008,1120	SQ		ANAP	MWL	
>Referenced SOP Class UID	0008,1150	UI		ALWAYS	MWL	
>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	MWL	
Patient's Name	0010,0010	PN		VNAP	MWL, USER	
Patient ID	0010,0020	LO		VNAP	MWL, USER	
Patient's Birth Date	0010,0030	DA		VNAP	MWL, USER	
Patient's Sex	0010,0040	CS		VNAP	MWL, USER	
Other Patient IDs	0010,1000	LO		ANAP	MWL, USER	
Ethnic Group	0010,2160	SH		ANAP	MWL	
Patient Comments	0010,4000	LT		ANAP	MWL	

**Table 90: General Study Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Study Date	0008,0020	DA		VNAP	AUTO	
Study Time	0008,0030	TM		VNAP	AUTO	
Accession Number	0008,0050	SH		VNAP	MWL	
Referring Physician's Name	0008,0090	PN		VNAP	MWL	
Study Description	0008,1030	LO		VNAP	USER, MWL	Copied from Requested procedure step description
Procedure Code Sequence	0008,1032	SQ		VNAP	AUTO, MWL	
>Code Value	0008,0100	SH		ALWAYS	AUTO, MWL	
>Coding Scheme Designator	0008,0102	SH		ALWAYS	AUTO, MWL	

>Coding Scheme Version	0008,0103	SH		ALWAYS	AUTO, MWL	
>Code Meaning	0008,0104	LO		ALWAYS	AUTO, MWL	
Referenced Study Sequence	0008,1110	SQ		ALWAYS	AUTO, MWL	
>Referenced SOP Class UID	0008,1150	UI		ALWAYS	AUTO, MWL	
>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	AUTO, MWL	
Study Instance UID	0020,000D	UI		ALWAYS	AUTO, MWL	
Study ID	0020,0010	SH		VNAP	AUTO, MWL, USER	In case Study ID is empty, accession number is used. If that is also empty then the system generates a value for it

Table 91: Patient Study Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Patient's Size	0010,1020	DS		ALWAYS	MWL, USER	When received from the MWL SCP, the value can still be modified
Patient's Weight	0010,1030	DS		ALWAYS	MWL, USER	When received from the MWL SCP, the value can still be modified
Medical Alerts	0010,2000	LO		VNAP	MWL, USER	
Allergies	0010,2110	LO		VNAP	MWL, USER	
Additional Patient History	0010,21B0	LT		VNAP	MWL	

Table 92: General Series Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Series Date	0008,0021	DA		ANAP	AUTO	
Series Time	0008,0031	TM		ANAP	AUTO	
Modality	0008,0060	CS		ALWAYS	AUTO	Applied values: OT and XA
Series Description	0008,103E	LO		ANAP	AUTO	
Performing Physicians' Name	0008,1050	PN		ANAP	MWL, USER	
Operators' Name	0008,1070	PN		ANAP	MWL, USER	
Referenced Performed Procedure Step Sequence	0008,1111	SQ	Identifies the MPPS SOP Instance to which this image is related	VNAP	AUTO, MPPS	
>Referenced SOP Class UID	0008,1150	UI	MPPS SOP Class UID	ALWAYS	MPPS	
>Referenced SOP Instance UID	0008,1155	UI	MPPS SOP Instance UID	ALWAYS	MPPS	
Protocol Name	0018,1030	LO		ANAP	AUTO	

Series Instance UID	0020,000E	UI		ALWAYS	AUTO	
Series Number	0020,0011	IS		VNAP	AUTO	
Laterality	0020,0060	CS		ANAP	AUTO	
Performed Procedure Step Start Date	0040,0244	DA		ANAP	AUTO	
Performed Procedure Step Start Time	0040,0245	TM		ANAP	AUTO	
Performed Procedure Step ID	0040,0253	SH		ANAP	AUTO, MWL	
Performed Procedure Step Description	0040,0254	LO		ANAP	MWL	
Request Attributes Sequence	0040,0275	SQ		ANAP	MWL	
>Accession Number	0008,0050	SH		ANAP	MWL	
>Requested Procedure Description	0032,1060	LO		ANAP	MWL	
>Requested Procedure Code Sequence	0032,1064	SQ		ANAP	MWL	
>>Code Value	0008,0100	SH		ALWAYS	MWL	
>>Coding Scheme Designator	0008,0102	SH		ALWAYS	MWL	
>>Coding Scheme Version	0008,0103	SH		ALWAYS	MWL	
>>Code Meaning	0008,0104	LO		ALWAYS	MWL	
>Scheduled Procedure Step Description	0040,0007	LO		ALWAYS	MWL	
> Scheduled Protocol Code Sequence	0040,0008	SQ		ALWAYS	MWL	
>>Code Value	0008,0100	SH		ALWAYS	MWL	
>>Coding Scheme Designator	0008,0102	SH		ALWAYS	MWL	
>>Coding Scheme Version	0008,0103	SH		ALWAYS	MWL	
>>Code Meaning	0008,0104	LO		ALWAYS	MWL	
>Scheduled Procedure Step ID	0040,0009	SH		ANAP	MWL	
>Requested Procedure ID	0040,1001	SH		ANAP	MWL	

**Table 93: General Equipment Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Manufacturer	0008,0070	LO	Philips	ALWAYS	FIXED	
Institution Name	0008,0080	LO		VNAP	CONFIG	
Station Name	0008,1010	SH		VNAP	CONFIG	
Institutional Department Name	0008,1040	LO		VNAP	AUTO	
Manufacturer’s Model Name	0008,1090	LO	Azurion	ALWAYS	AUTO	

Device Serial Number	0018,1000	LO		VNAP	AUTO	
Software Versions	0018,1020	LO	3.1.x	ALWAYS	AUTO	“x” represents the Level release number from current software version.

Table 94: SC Equipment Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Modality	0008,0060	CS		ANAP	AUTO	Applied values: OT and XA
Conversion Type	0008,0064	CS	WSD	ALWAYS	AUTO	

Table 95: General Image Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Image Type	0008,0008	CS	DERIVED\PRIMARY	ALWAYS	AUTO	
Content Date	0008,0023	DA		ALWAYS	AUTO	
Content Time	0008,0033	TM		ALWAYS	AUTO	
Instance Number	0020,0013	IS		ALWAYS	AUTO	
Patient Orientation	0020,0020	CS		VNAP	AUTO	
Lossy Image Compression	0028,2110	CS	00	ALWAYS	AUTO	

Table 96: General Reference Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Derivation Description	0008,2111	ST		ANAP	AUTO	

Table 97: Image Pixel Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Samples per Pixel	0028,0002	US		ALWAYS	AUTO	
Photometric Interpretation	0028,0004	CS	RGB	ALWAYS	AUTO	
Planar Configuration	0028,0006	US		ANAP	AUTO	
Rows	0028,0010	US		ALWAYS	AUTO	
Columns	0028,0011	US		ALWAYS	AUTO	
Bits Allocated	0028,0100	US	8 or 16 Note: For Snapshot function, this number is 8	ALWAYS	AUTO	
Bits Stored	0028,0101	US	8 or 12 Note: For Snapshot function, this number is 8	ALWAYS	AUTO	
High Bit	0028,0102	US		ALWAYS	AUTO	
Pixel Representation	0028,0103	US	0000H	ALWAYS	AUTO	
Smallest Image Pixel Value	0028,0106	US /SS		ANAP	AUTO	

Largest Image Pixel Value	0028,0107	US /SS		ANAP	AUTO	
Pixel Data	7FE0,0010	O W/OB		ALWAYS	AUTO	

Table 98: SC Image Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Date of Secondary Capture	0018,1012	DA		ANAP	AUTO	
Time of Secondary Capture	0018,1014	TM		ANAP	AUTO	
Nominal Scanned Pixel Spacing	0018,2010	DS		ANAP	AUTO	
Pixel Spacing Calibration Type	0028,0A02	CS		ANAP	AUTO	

Table 99: VOI LUT Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Window Center	0028,1050	DS		ALWAYS	AUTO	
Window Width	0028,1051	DS		ALWAYS	AUTO	

Table 100: SOP Common Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Specific Character Set	0008,0005	CS		ANAP	AUTO	
Instance Creation Date	0008,0012	DA		ANAP	AUTO	
Instance Creation Time	0008,0013	TM		ANAP	AUTO	
SOP Class UID	0008,0016	UI	1.2.840.10008.5.1.4.1.1.7	ALWAYS	FIXED	
SOP Instance UID	0008,0018	UI		ALWAYS	AUTO	
Instance Number	0020,0013	IS		ANAP	AUTO	

### 8.1.1.1.2. Grayscale Softcopy Presentation State Storage SOP Class

Table 101: SOP Class Modules

Information Entity	Module	Presence Of Module
Patient	Patient Module	ALWAYS
Study	General Study Module	ALWAYS
	Patient Study Module	ALWAYS
Series	General Series Module	ALWAYS
	Presentation Series Module	ALWAYS
Equipment	General Equipment Module	ALWAYS
Presentation State	Presentation State Identification Module	ALWAYS
	Presentation State Relationship Module	ALWAYS
	Presentation State Shutter Module	ALWAYS
	Display Shutter Module	ALWAYS
	Displayed Area Module	ALWAYS
	Graphic Layer Module	ALWAYS



Softcopy Presentation LUT Module	ALWAYS
Softcopy VOI LUT module	ALWAYS
SOP Common Module	ALWAYS

Table 102: Patient Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Referenced Patient Sequence	0008,1120	SQ		ANAP	MWL	
>Referenced SOP Class UID	0008,1150	UI		ALWAYS	MWL	
>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	MWL	
Patient's Name	0010,0010	PN		VNAP	MWL, USER	
Patient ID	0010,0020	LO		VNAP	MWL, USER	
Patient's Birth Date	0010,0030	DA		VNAP	MWL, USER	
Patient's Sex	0010,0040	CS		VNAP	MWL, USER	
Other Patient IDs	0010,1000	LO		ANAP	MWL, USER	
Ethnic Group	0010,2160	SH		ANAP	MWL	
Patient Comments	0010,4000	LT		ANAP	MWL	

Table 103: General Study Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Study Date	0008,0020	DA		VNAP	AUTO	
Study Time	0008,0030	TM		VNAP	AUTO	
Accession Number	0008,0050	SH		VNAP	MWL	
Referring Physician's Name	0008,0090	PN		VNAP	MWL	
Study Description	0008,1030	LO		VNAP	USER, MWL	Copied from Requested procedure step description
Procedure Code Sequence	0008,1032	SQ		AVNAP	AUTO, MWL	
>Code Value	0008,0100	SH		ALWAYS	AUTO, MWL	
>Coding Scheme Designator	0008,0102	SH		ALWAYS	AUTO, MWL	
>Coding Scheme Version	0008,0103	SH		ALWAYS	AUTO, MWL	
>Code Meaning	0008,0104	LO		ALWAYS	AUTO, MWL	
Referenced Study Sequence	0008,1110	SQ		ANAP	MWL	
>Referenced SOP Class UID	0008,1150	UI		ALWAYS	MWL	
>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	MWL	
Study Instance UID	0020,000D	UI		ALWAYS	AUTO	
Study ID	0020,0010	SH		VNAP	AUTO, MWL, USER	In case Study ID is empty, accession number is used. If that is also empty then the system generates a value for it

**Table 104: Patient Study Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Patient's Size	0010,1020	DS		ALWAYS	MWL, USER	In meters. When received from the MWL SCP, the value can still be modified
Patient's Weight	0010,1030	DS		ALWAYS	MWL, USER	In kilograms. When received from the MWL SCP, the value can still be modified
Medical Alerts	0010,2000	LO		VNAP	MWL, USER	
Allergies	0010,2110	LO		VNAP	MWL, USER	
Additional Patient History	0010,21B0	LT		VNAP	MWL	

**Table 105: General Series Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Series Date	0008,0021	DA		ANAP	AUTO	
Series Time	0008,0031	TM		ANAP	AUTO	
Modality	0008,0060	CS	PR	ALWAYS	AUTO	
Series Description	0008,103E	LO		ALWAYS	AUTO	
Performing Physicians' Name	0008,1050	PN		ANAP	MWL, USER	
Operators' Name	0008,1070	PN		ANAP	MWL, USER	
Referenced Performed Procedure Step Sequence	0008,1111	SQ	Identifies the MPPS SOP Instance to which this image is related	AVNAP	AUTO, MPPS	
>Referenced SOP Class UID	0008,1150	UI	MPPS SOP Class UID	ALWAYS	MWL	
>Referenced SOP Instance UID	0008,1155	UI	MPPS SOP Instance UID	ALWAYS	MWL	
Protocol Name	0018,1030	LO		ANAP	AUTO	
Series Instance UID	0020,000E	UI		ALWAYS	AUTO	
Series Number	0020,0011	IS		VNAP	AUTO	
Laterality	0020,0060	CS		EMPTY	AUTO	
Performed Procedure Step Start Date	0040,0244	DA		ALWAYS	AUTO	
Performed Procedure Step Start Time	0040,0245	TM		ALWAYS	AUTO	
Performed Procedure Step ID	0040,0253	SH	Same as MPPS	ALWAYS	AUTO, USER	
Performed Procedure Step Description	0040,0254	LO		ANAP	MWL	
Request Attributes Sequence	0040,0275	SQ		ANAP	MWL	

>Accession Number	0008,0050	SH		ANAP	MWL	
>Issuer of Accession Number Sequence	0008,0051	SQ		ANAP	MWL	
>Referenced Study Sequence	0008,1110	SQ		ANAP	MWL	
>>Referenced SOP Class UID	0008,1150	UI		ALWAYS	MWL	
>>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	MWL	
>Study Instance UID	0020,000D	UI		ANAP	MWL	
>Requested Procedure Description	0032,1060	LO		ANAP	MWL	
>Requested Procedure Code Sequence	0032,1064	SQ		ANAP	MWL	
>>Code Value	0008,0100	SH		ALWAYS	MWL	
>>Coding Scheme Designator	0008,0102	SH		ALWAYS	MWL	
>>Coding Scheme Version	0008,0103	SH		ALWAYS	MWL	
>>Code Meaning	0008,0104	LO		ALWAYS	MWL	
> Scheduled Procedure Step Description	0040,0007	LO		ALWAYS	MWL	
> Scheduled Protocol Code Sequence	0040,0008	SQ		ALWAYS	MWL	
>>Code Value	0008,0100	SH		ALWAYS	MWL	
>>Coding Scheme Designator	0008,0102	SH		ALWAYS	MWL	
>>Coding Scheme Version	0008,0103	SH		ALWAYS	MWL	
>>Code Meaning	0008,0104	LO		ALWAYS	MWL	
>>Protocol Context Sequence	0040,0440	SQ		ANAP	MWL	
>>>Value Type	0040,A040	CS		ALWAYS	MWL	
>>>Concept Name Code Sequence	0040,A043	SQ		ALWAYS	MWL	
>>>>Code Value	0008,0100	SH		ALWAYS	MWL	
>>>>Coding Scheme Designator	0008,0102	SH		ALWAYS	MWL	
>>>>Code Meaning	0008,0104	LO		ALWAYS	MWL	
>Reason for the Requested Procedure	0040,1002	LO		ANAP	MWL	
>Reason for Requested Procedure Code Sequence	0040,100A	SQ		ANAP	MWL	
>>Code Value	0008,0100	SH		ALWAYS	MWL	
>>Coding Scheme Designator	0008,0102	SH		ALWAYS	MWL	
>>Context Identifier	0008,010F	CS		ANAP	MWL	
>>Context UID	0008,0117	UI		ANAP	MWL	

>Scheduled Procedure Step ID	0040,0009	SH		ALWAYS	MWL	
>Requested Procedure ID	0040,1001	SH		ALWAYS	MWL	

Table 106: Presentation Series Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Modality	0008,0060	CS	PR	ALWAYS	AUTO	

Table 107: General Equipment Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Manufacturer	0008,0070	LO	Philips	ALWAYS	FIXED	
Institution Name	0008,0080	LO		VNAP	CONFIG	
Station Name	0008,1010	SH		VNAP	CONFIG	
Institutional Department Name	0008,1040	LO		VNAP	AUTO	
Manufacturer’s Model Name	0008,1090	LO	Azurion	ALWAYS	AUTO	
Device Serial Number	0018,1000	LO		VNAP	AUTO	
Software Versions	0018,1020	LO	3.1.x	ALWAYS	AUTO	“x” represents the Level release number from current software version.

Table 108: Presentation State Identification Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Instance Number	0020,0013	IS		ALWAYS	AUTO	
Content Label	0070,0080	CS	AS LAST SEEN	ALWAYS	FIXED	
Content Description	0070,0081	LO		VNAP	AUTO	
Presentation Creation Date	0070,0082	DA		ALWAYS	AUTO	
Presentation Creation Time	0070,0083	TM		ALWAYS	AUTO	
Content Creator’s Name	0070,0084	PN		VNAP	AUTO	

Table 109: Presentation State Relationship Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Referenced Series Sequence	0008,1115	SQ		ALWAYS	AUTO	
>Referenced Image Sequence	0008,1140	SQ		ALWAYS	AUTO	
>>Referenced SOP Class UID	0008,1150	UI		ALWAYS	AUTO	
>>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	AUTO	
>Series Instance UID	0020,000E	UI		ALWAYS	AUTO	

Table 110: Presentation State Shutter Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Shutter Presentation Value	0018,1622	US		ALWAYS	AUTO	

Table 111: Display Shutter Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Shutter Shape	0018,1600	CS	RECTANGULAR	ALWAYS	FIXED	
Shutter Left Vertical Edge	0018,1602	IS		ANAP	AUTO	
Shutter Right Vertical Edge	0018,1604	IS		ANAP	AUTO	
Shutter Upper Horizontal Edge	0018,1606	IS		ANAP	AUTO	
Shutter Lower Horizontal Edge	0018,1608	IS		ANAP	AUTO	
Shutter Presentation Value	0018,1622	US		ANAP	AUTO	

Table 112: Displayed Area Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Displayed Area Selection Sequence	0070,005A	SQ		ALWAYS	AUTO	
>Referenced Image Sequence	0008,1140	SQ		ANAP	AUTO	
>>Referenced SOP Class UID	0008,1150	UI		ALWAYS	AUTO	
>>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	AUTO	
>>Referenced Frame Number	0008,1160	IS		ALWAYS	AUTO	
>Displayed Area Top Left Hand Corner	0070,0052	SL		ALWAYS	AUTO	calculated by the system but initiated by user i.e. without user zoom and pan displayed area does not have any meaning
>Displayed Area Bottom Right Hand Corner	0070,0053	SL		ALWAYS	AUTO	
>Presentation Size Mode	0070,0100	CS	SCALE TO FIT	ALWAYS	AUTO	
>Presentation Pixel Aspect Ratio	0070,0102	IS		ANAP	AUTO	

Table 113: Graphic Layer Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Graphic Layer Sequence	0070,0060	SQ		ALWAYS	AUTO	
>Graphic Layer	0070,0002	CS	GRAPHICS	ALWAYS	AUTO	
>Graphic Layer Order	0070,0062	IS	1	ALWAYS	AUTO	

Table 114: Softcopy Presentation LUT Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Presentation LUT Shape	2050,0020	CS	IDENTITY	ALWAYS	AUTO	

Table 115: Softcopy VOI LUT Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Softcopy VOI LUT Sequence	0028,3110	SQ		ALWAYS	AUTO	

>Window Center	0028,1050	DS		ALWAYS	AUTO	
>Window Width	0028,1051	DS		ALWAYS	AUTO	

Table 116: SOP Common Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Specific Character Set	0008,0005	CS		ANAP	AUTO	
Instance Creation Date	0008,0012	DA		ANAP	AUTO	
Instance Creation Time	0008,0013	TM		ANAP	AUTO	
SOP Class UID	0008,0016	UI	1.2.840.10008.5.1.4.1.1.11.1	ALWAYS	AUTO	
SOP Instance UID	0008,0018	UI		ALWAYS	AUTO	
Instance Number	0020,0013	IS		ANAP	AUTO	

8.1.1.1.3. X-Ray Angiographic Image Storage SOP Class

Table 117: SOP Class Modules

Information Entity	Module	Presence Of Module
Patient	Patient Module	ALWAYS
Study	General Study Module	ALWAYS
	Patient Study Module	ALWAYS
Series	General Series Module	ALWAYS
Equipment	General Equipment Module	ALWAYS
Acquisition	General Acquisition Module	ALWAYS
Image	General Image Module	ALWAYS
	General Reference Module	ALWAYS
	Image Pixel Module	ALWAYS
	Contrast/Bolus Module	ALWAYS
	Cine Module	ALWAYS
	Multi-Frame Module	ALWAYS
	Display Shutter Module	ALWAYS
	X-Ray Image Module	ALWAYS
	X-Ray Acquisition Module	ALWAYS
	X-Ray Table Module	ALWAYS
	XA Positioner Module	ALWAYS
	Modality LUT Module	ALWAYS
	VOI LUT Module	ALWAYS
	Curve Module	CONDITIONAL This is present only when ECG signals are present in the data
	SOP Common Module	ALWAYS

Table 118: Patient Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Referenced Patient Sequence	0008,1120	SQ		ANAP	MWL	

>Referenced SOP Class UID	0008,1150	UI		ALWAYS	MWL	
>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	MWL	
Patient's Name	0010,0010	PN		VNAP	MWL, USER	
Patient ID	0010,0020	LO		VNAP	MWL, USER	
Patient's Birth Date	0010,0030	DA		VNAP	MWL, USER	
Patient's Sex	0010,0040	CS		VNAP	MWL, USER	
Other Patient IDs	0010,1000	LO		ANAP	MWL, USER	
Ethnic Group	0010,2160	SH		ANAP	MWL	
Patient Comments	0010,4000	LT		ANAP	MWL	

Table 119: General Study Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Study Date	0008,0020	DA		VNAP	AUTO	
Study Time	0008,0030	TM		VNAP	AUTO	
Accession Number	0008,0050	SH		VNAP	MWL	
Referring Physician's Name	0008,0090	PN		VNAP	MWL	
Study Description	0008,1030	LO		VNAP	USER, MWL	Copied from Requested procedure step description
Procedure Code Sequence	0008,1032	SQ		VNAP	AUTO, MWL	
>Code Value	0008,0100	SH		ALWAYS	AUTO, MWL	
>Coding Scheme Designator	0008,0102	SH		ALWAYS	AUTO, MWL	
>Coding Scheme Version	0008,0103	SH		ALWAYS	AUTO, MWL	
>Code Meaning	0008,0104	LO		ALWAYS	AUTO, MWL	
Referenced Study Sequence	0008,1110	SQ		ANAP	MWL	
>Referenced SOP Class UID	0008,1150	UI		ALWAYS	MWL	
>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	MWL	
Study Instance UID	0020,000D	UI		ALWAYS	AUTO, MWL	
Study ID	0020,0010	SH		VNAP	MWL	In case Study ID is empty, accession number is used. If that is also empty then the system generates a value for it

Table 120: Patient Study Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Patient's Size	0010,1020	DS		ALWAYS	MWL, USER	In meters. When received from the MWL SCP, the value can still be modified.

Patient's Weight	0010,1030	DS		ALWAYS	MWL, USER	In kilograms. When received from the MWL SCP, the value can still be modified.
Medical Alerts	0010,2000	LO		VNAP	MWL, USER	
Allergies	0010,2110	LO		VNAP	MWL, USER	
Additional Patient History	0010,21B0	LT		VNAP	MWL	

Table 121: General Series Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Series Date	0008,0021	DA		ANAP	AUTO	
Series Time	0008,0031	TM		ANAP	AUTO	
Modality	0008,0060	CS	XA	ALWAYS	AUTO	
Series Description	0008,103E	LO		ANAP	AUTO	
Performing Physicians' Name	0008,1050	PN		ANAP	MWL, USER	
Operators' Name	0008,1070	PN		ANAP	MWL, USER	
Referenced Performed Procedure Step Sequence	0008,1111	SQ	Identifies the MPPS SOP Instance to which this image is related	VNAP	AUTO, MPPS	
>Referenced SOP Class UID	0008,1150	UI	MPPS SOP Class UID	ALWAYS	AUTO	
>Referenced SOP Instance UID	0008,1155	UI	MPPS SOP Instance UID	ALWAYS	AUTO	
Protocol Name	0018,1030	LO		ANAP	AUTO	
Series Instance UID	0020,000E	UI		ALWAYS	AUTO	
Series Number	0020,0011	IS		VNAP	AUTO	
Laterality	0020,0060	CS		EMPTY	AUTO	
Performed Procedure Step Start Date	0040,0244	DA		ANAP	AUTO,	
Performed Procedure Step Start Time	0040,0245	TM		ANAP	AUTO	
Performed Procedure Step ID	0040,0253	SH	Same as MPPS	ANAP	AUTO, USER	
Performed Procedure Step Description	0040,0254	LO	Same as MPPS	ANAP	AUTO, USER	
Request Attributes Sequence	0040,0275	SQ		ANAP	MWL	
>Accession Number	0008,0050	SH		ANAP	MWL	
>Issuer of Accession Number Sequence	0008,0051	SQ		ANAP	MWL	
>Referenced Study Sequence	0008,1110	SQ		ANAP	MWL	



>>Referenced SOP Class UID	0008,1150	UI		ALWAYS	MWL	
>>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	MWL	
>Study Instance UID	0020,000D	UI		ANAP	MWL	
>Requested Procedure Description	0032,1060	LO		ANAP	MWL	
>Requested Procedure Code Sequence	0032,1064	SQ		ANAP	MWL	
>>Code Value	0008,0100	SH		ALWAYS	MWL	
>>Coding Scheme Designator	0008,0102	SH		ALWAYS	MWL	
>>Coding Scheme Version	0008,0103	SH		ALWAYS	MWL	
>>Code Meaning	0008,0104	LO		ALWAYS	MWL	
>>Context Identifier	0008,010F	CS		ANAP	MWL	
>>Context UID	0008,0117	UI		ANAP	MWL	
>Scheduled Procedure Step Description	0040,0007	LO		ANAP	MWL	
>Scheduled Protocol Code Sequence	0040,0008	SQ		ANAP	MWL	
>>Code Value	0008,0100	SH		ALWAYS	MWL	
>>Coding Scheme Designator	0008,0102	SH		ALWAYS	MWL	
>>Coding Scheme Version	0008,0103	SH		ALWAYS	MWL	
>>Code Meaning	0008,0104	LO		ALWAYS	MWL	
>>Context Identifier	0008,010F	CS		ANAP	MWL	
>>Context UID	0008,0117	UI		ANAP	MWL	
>>Protocol Context Sequence	0040,0440	SQ		ANAP	MWL	
>>>Content Item Modifier Sequence	0040,0441	SQ		ANAP	MWL	
>>>>Value Type	0040,A040	CS		ALWAYS	MWL	
>>>>Concept Name Code Sequence	0040,A043	SQ		ALWAYS	MWL	
>>>>Code Value	0008,0100	SH		ALWAYS	MWL	
>>>>Coding Scheme Designator	0008,0102	SH		ALWAYS	MWL	
>>>>Code Meaning	0008,0104	LO		ALWAYS	MWL	
>>>Value Type	0040,A040	CS		ALWAYS	MWL	
>>>Concept Name Code Sequence	0040,A043	SQ		ALWAYS	MWL	
>>>>Code Value	0008,0100	SH		ALWAYS	MWL	
>>>>Coding Scheme Designator	0008,0102	SH		ALWAYS	MWL	

>>>>Code Meaning	0008,0104	LO		ALWAYS	MWL	
>>>>Context Identifier	0008,010F	CS		ANAP	MWL	
>>>>Context UID	0008,0117	UI		ANAP	MWL	
>Scheduled Procedure Step ID	0040,0009	SH		ANAP	MWL	
>Reason for Requested Procedure Code Sequence	0040,100A	SQ		ANAP	MWL	
>>Code Value	0008,0100	SH		ALWAYS	MWL	
>>Coding Scheme Designator	0008,0102	SH		ALWAYS	MWL	
>>Code Meaning	0008,0104	LO		ALWAYS	MWL	
>>Context Identifier	0008,010F	CS		ANAP	MWL	
>>Context UID	0008,0117	UI		ANAP	MWL	
>Requested Procedure ID	0040,1001	SH		ALWAYS	MWL	

**Table 122: General Equipment Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Manufacturer	0008,0070	LO	Philips	ALWAYS	FIXED	
Institution Name	0008,0080	LO		VNAP	CONFIG	
Station Name	0008,1010	SH		VNAP	CONFIG	
Institutional Department Name	0008,1040	LO		VNAP	AUTO	
Manufacturer’s Model Name	0008,1090	LO	Azurion	ANAP	AUTO	
Device Serial Number	0018,1000	LO		VNAP	AUTO	
Software Versions	0018,1020	LO	3.1.x	AALWAYS	AUTO	“x” represents the Level release number from current software version.

**Table 123: General Acquisition Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Acquisition Date	0008,0022	DA		ANAP	AUTO	
Acquisition Time	0008,0032	TM		ANAP	AUTO	
Irradiation Event UID	0008,3010	UI		ANAP	AUTO	

Table 124: General Image Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Image Type	0008,0008	CS	Applied value(s): <b>Value 1:</b> ORIGINAL or DERIVED (if subtraction has been processed into the image) <b>Value 2:</b> PRIMARY <b>Value 3:</b> SINGLE PLANE (if the image is a single plane acquisition) BIPLANE A (if the image is the first plane of a Bi-plane acquisition) BIPLANE B (if the image is the second plane of a Bi-plane acquisition) <b>Value 4:</b> SINGLE A (if the image is derived from plane A of a biplane image and sent as a SINGLE PLANE image) SINGLE B (if the image is derived from plane B of a biplane image and sent as a SINGLE PLANE image)	ANAP	AUTO	
Content Date	0008,0023	DA		ANAP	AUTO	
Content Time	0008,0033	TM		ANAP	AUTO	
Instance Number	0020,0013	IS		VNAP	AUTO	
Patient Orientation	0020,0020	CS		ANAP	AUTO	
Lossy Image Compression	0028,2110	CS	00	ANAP	AUTO	
Presentation LUT Shape	2050,0020	CS	IDENTITY	ALWAYS	AUTO	

Table 125: General Reference Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Referenced Image Sequence	0008,1140	SQ		ANAP	AUTO	
>Referenced SOP Class UID	0008,1150	UI		ALWAYS	AUTO	
>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	AUTO	
Derivation Description	0008,2111	ST		VNAP	AUTO	
Source Image Sequence	0008,2112	SQ		ANAP	AUTO	
> Referenced SOP Class UID	0008,1150	UI		ALWAYS	AUTO	Documentation of source images for derived images. This will be present only for Derived images.

>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	AUTO	
>Referenced Frame Number	0008,1160	IS		ALWAYS	AUTO	

Table 126: Image Pixel Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Samples per Pixel	0028,0002	US	1	ALWAYS	AUTO	
Photometric Interpretation	0028,0004	CS	MONOCHROME2: Upon import, only images with a photometric interpretation MONOCHROME1 or MONOCHROME2 are accepted.	ALWAYS	AUTO	
Rows	0028,0010	US		ALWAYS	AUTO	
Columns	0028,0011	US		ALWAYS	AUTO	
Bits Allocated	0028,0100	US	8 or 16 Note: For Snapshot function, this number is 8	ALWAYS	AUTO	
Bits Stored	0028,0101	US	8 or 12 Note: For Snapshot function, this number is 8	ALWAYS	AUTO	
High Bit	0028,0102	US	7	ALWAYS	AUTO	
Pixel Representation	0028,0103	US	0000H	ALWAYS	AUTO	
Pixel Data	7FE0,0010	OW /OB		ANAP	AUTO	

Table 127: SC Image Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Contrast/Bolus Agent	0018,0010	LO		VNAP	AUTO	

Table 128: Cine Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Recommended Display Frame Rate	0008,2144	IS		ANAP	AUTO	
Cine Rate	0018,0040	IS		ANAP	AUTO	
Frame Time Vector	0018,1065	DS		ANAP	AUTO	
Frame Time	0018,1063	DS		ANAP	AUTO	Either frame time vector or Frame time will be present
Frame Delay	0018,1066	DS		ANAP	AUTO	

Table 129: Multi-Frame Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Number of Frames	0028,0008	IS		ALWAYS	AUTO	
Frame Increment Pointer	0028,0009	AT		ALWAYS	AUTO	

Table 130: Display Shutter Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Shutter Shape	0018,1600	CS	RECTANGULAR	ALWAYS	AUTO	
Shutter Left Vertical Edge	0018,1602	IS		ALWAYS	AUTO	
Shutter Right Vertical Edge	0018,1604	IS		ALWAYS	AUTO	
Shutter Upper Horizontal Edge	0018,1606	IS		ALWAYS	AUTO	
Shutter Lower Horizontal Edge	0018,1608	IS		ALWAYS	AUTO	

Table 131: X-Ray Image Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Image Type	0008,0008	CS		ALWAYS	AUTO	
Derivation Description	0008,2111	ST		VNAP	AUTO	
Scan Options	0018,0022	CS		ANAP	AUTO	ROTA
Referenced Image Sequence	0008,1140	SQ		ALWAYS	AUTO	
>Referenced SOP Class UID	0008,1150	UI		ALWAYS	AUTO	
>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	AUTO	
Samples per Pixel	0028,0002	US	1	ALWAYS	AUTO	
Photometric Interpretation	0028,0004	CS	MONOCHROME2 Upon import, only images with a photometric interpretation MONOCHROME1 or MONOCHROME2 are accepted.	ALWAYS	AUTO	
Frame Increment Pointer	0028,0009	AT		ALWAYS	AUTO	
Bits Allocated	0028,0100	US	8 or 16 Note: For Snapshot function, this number is 8	ALWAYS	AUTO	
Bits Stored	0028,0101	US	8 or 12 Note: For Snapshot function, this number is 8	ALWAYS	AUTO	
High Bit	0028,0102	US	11	ALWAYS	AUTO	

Pixel Representation	0028,0103	US	0000H	ALWAYS	AUTO	
Pixel Intensity Relationship	0028,1040	CS		ALWAYS	AUTO	
Lossy Image Compression	0028,2110	CS	00	ALWAYS	AUTO	

Table 132: X-Ray Acquisition Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
KVP	0018,0060	DS		ALWAYS	AUTO	
Exposure Time	0018,1150	IS	Only sent if Exposure (0018, 1152) is not sent.	ANAP	AUTO	
X-Ray Tube Current	0018,1151	IS	Only sent if Exposure (0018, 1152) is not sent.	ANAP	AUTO	
Average Pulse Width	0018,1154	DS		ANAP	AUTO	
Exposure	0018,1152	IS	Only sent if Exposure Time (0018, 1150) and X-Ray Tube Current (0018, 1151) are not sent.	ANAP	AUTO	
Radiation Setting	0018,1155	CS		ALWAYS	AUTO	
Imager Pixel Spacing	0018,1164	DS		ANAP	AUTO	
X-Ray Tube Current in $\mu$ A	0018,8151	DS		ANAP	AUTO	
Pixel Spacing	0028,0030	DS		ALWAYS	AUTO	

Table 133: X-Ray Table Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Table Motion	0018,1134	CS	STATIC, DYNAMIC	VNAP	AUTO	
Table Vertical Increment	0018,1135	DS	Incremental change (per frame) in vertical position relatively to the first frame of Multi-Frame image in mm	ANAP	AUTO	
Table Lateral Increment	0018,1136	DS	Incremental change (per frame) in lateral position relatively to the first frame of Multi-Frame image in mm	ANAP	AUTO	
Table Longitudinal Increment	0018,1137	DS	Incremental change (per frame) in longitudinal position relatively to the first frame of Multi-Frame image in mm	ANAP	AUTO	

Table Angle	0018,1138	DS	Angle of table plane in degrees relative to horizontal plane (gravity plane). Positive values indicate that the head of the table is upwards.	ANAP	AUTO	
-------------	-----------	----	---	------	------	--

**Table 134: XA Positioner Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Distance Source to Detector	0018,1110	DS		ALWAYS	AUTO	
Distance Source to Patient	0018,1111	DS		ALWAYS	AUTO	
Estimated Radiographic Magnification Factor	0018,1114	DS		ALWAYS	AUTO	
Positioner Motion	0018,1500	CS	STATIC, DYNAMIC	ALWAYS	AUTO	
Positioner Primary Angle	0018,1510	DS		ALWAYS	AUTO	
Positioner Secondary Angle	0018,1511	DS		ALWAYS	AUTO	
Positioner Primary Angle Increment	0018,1520	DS	An array that contains the Positioner Primary Angle Increments between the n-th frame and the previous frame for a Multi-frame image.	ANAP	AUTO	
Positioner Secondary Angle Increment	0018,1521	DS	An array that contains the Positioner Secondary Angle Increments between the n-th frame and the previous frame for a Multi-frame image.	ANAP	AUTO	

**Table 135: Modality LUT Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Modality LUT Sequence	0028,3000	SQ		ANAP	AUTO	
>LUT Descriptor	0028,3002	US/SS		ANAP	AUTO	
>Modality LUT Type	0028,3004	LO		ANAP	AUTO	
>LUT Data	0028,3006	UN		ANAP	AUTO	

**Note:** Modality LUT and pixel intensity “LOG” only when X-Ray Angiographic images are sent with unprocessed pixel data.

-No Modality LUT and pixel intensity “LIN” when X-Ray Angiographic images are sent with processed pixel data

Table 136: VOI LUT Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Window Center	0028,1050	DS		ALWAYS	AUTO	
Window Width	0028,1051	DS		ALWAYS	AUTO	

Table 137: Curve Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Curve Dimensions	5000,0005	US		ALWAYS	AUTO	
Number Of Points	5000,0010	US		ALWAYS	AUTO	
Type Of Data	5000,0020	CS		ALWAYS	AUTO	
Axis Units	5000,0030	SH	DPPS\NONE	ALWAYS	AUTO	
Data Value Representation	5000,0103	US		ALWAYS	AUTO	
Minimum Coordinate Value	5000,0104	US		ALWAYS	AUTO	
Maximum Coordinate Value	5000,0105	US		ALWAYS	AUTO	
Curve Data Descriptor	5000,0110	US		ALWAYS	AUTO	
Coordinate Start Value	5000,0112	US		ALWAYS	AUTO	
Coordinate Step Value	5000,0114	US		VNAP	AUTO	
Curve Data	5000,3000	OW		ALWAYS	AUTO	

Table 138: SOP Common Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Specific Character Set	0008,0005	CS		ANAP	AUTO	
Instance Creation Date	0008,0012	DA		ALWAYS	AUTO	
Instance Creation Time	0008,0013	TM		ALWAYS	AUTO	
SOP Class UID	0008,0016	UI	1.2.840.10008.5.1.4.1.1.12.1	ALWAYS	AUTO	
SOP Instance UID	0008,0018	UI	Generated by device	ALWAYS	AUTO	
Instance Number	0020,0013	IS		ALWAYS	AUTO	

8.1.1.1.4. X-Ray Radiation Dose SR

Table 139: SOP Class Modules

Information Entity	Module	Presence Of Module
Patient	Patient Module	ALWAYS
Study	General Study Module	ALWAYS
	Patient Study Module	ALWAYS
Series	SR Document Series Module	ALWAYS
Equipment	General Equipment Module	ALWAYS
	Enhanced General Equipment Module	ALWAYS
Document	SR Document General Module	ALWAYS
	SR Document Content Module	ALWAYS
	SOP Common Module	ALWAYS



Table 140: Patient Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Referenced Patient Sequence	0008,1120	SQ		ANAP	MWL	
>Referenced SOP Class UID	0008,1150	UI		ALWAYS	MWL	
>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	MWL	
Patient's Name	0010,0010	PN		ALWAYS	MWL, USER	
Patient ID	0010,0020	LO		ALWAYS	MWL, USER	
Patient's Birth Date	0010,0030	DA		VNAP	MWL, USER	
Patient's Sex	0010,0040	CS		VNAP	MWL, USER	
Other Patient IDs	0010,1000	LO		ANAP	MWL, USER	
Ethnic Group	0010,2160	SH		ANAP	MWL, USER	
Patient Comments	0010,4000	LT		ANAP	MWL, USER	

Table 141: General Study Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Study Date	0008,0020	DA		ALWAYS	MWL, AUTO	
Study Time	0008,0030	TM		ALWAYS	MWL, AUTO	
Accession Number	0008,0050	SH		ALWAYS	MWL	
Referring Physician's Name	0008,0090	PN		VNAP	MWL	
Study Description	0008,1030	LO		VNAP	USER, MWL	Copied from Requested procedure step description
Procedure Code Sequence	0008,1032	SQ		VNAP	MWL, AUTO	
Referenced Study Sequence	0008,1110	SQ		ANAP	MWL	
>Referenced SOP Class UID	0008,1150	UI		ALWAYS	MWL	
>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	MWL	
Study Instance UID	0020,000D	UI		ALWAYS	AUTO	
Study ID	0020,0010	SH		VNAP	AUTO, MWL, USER	In case Study ID is empty, accession number is used. If that is also empty then the system generates a value for it

Table 142: Patient Study Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Patient's Size	0010,1020	DS		ANAP	MWL, USER	When received from the MWL SCP, the value can still be modified.
Patient's Weight	0010,1030	DS		ANAP	MWL, USER	

Medical Alerts	0010,2000	LO		ANAP	MWL, USER	
Allergies	0010,2110	LO		ANAP	MWL, USER	
Additional Patient History	0010,21B0	LT		ANAP	MWL	

**Table 143: SR Document Series Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Series Date	0008,0021	DA		ANAP	AUTO	
Series Time	0008,0031	TM		ANAP	AUTO	
Modality	0008,0060	CS	SR	ALWAYS	AUTO	
Series Description	0008,103E	LO	“Radiation Dose Information”	ANAP	AUTO	
Referenced Performed Procedure Step Sequence	0008,1111	SQ		VNAP	AUTO	
>Referenced SOP Class UID	0008,1150	UI		ANAP	AUTO	
>Referenced SOP Instance UID	0008,1155	UI		ANAP	AUTO	
Protocol Name	0018,1030	LO		ALWAYS	AUTO	
Series Instance UID	0020,000E	UI		ALWAYS	AUTO	
Series Number	0020,0011	IS		ALWAYS	AUTO	

**Table 144: General Equipment Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Manufacturer	0008,0070	LO	Philips	ALWAYS	FIXED	
Institution Name	0008,0080	LO		ANAP	CONFIG	
Station Name	0008,1010	SH		ANAP	CONFIG	
Institutional Department Name	0008,1040	LO		ANAP	CONFIG	
Manufacturer’s Model Name	0008,1090	LO	Azurion	ANAP	AUTO	
Device Serial Number	0018,1000	LO		ANAP	AUTO	
Software Versions	0018,1020	LO	3.1.x	ALWAYS	AUTO	“x” represents the Level release number from current software version.

**Table 145: Enhanced General Equipment Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Manufacturer	0008,0070	LO	Philips	ALWAYS	FIXED	
Manufacturer's Model Name	0008,1090	LO	Azurion	ALWAYS	AUTO	
Device Serial Number	0018,1000	LO		ALWAYS	AUTO	

Software Version(s)	0018,1020	LO	3.1.x	ALWAYS	AUTO	“x” represents the Level release number from current software version.
---------------------	-----------	----	-------	--------	------	--

Table 146: SR Document General Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Content Date	0008,0023	DA		ALWAYS	AUTO	
Content Time	0008,0033	TM		ALWAYS	AUTO	
Instance Number	0020,0013	IS		ALWAYS	AUTO	
Referenced Request Sequence	0040,A370	SQ		ANAP	AUTO	
>Accession Number	0008,0050	SH		ALWAYS	MWL	
>Referenced Study Sequence	0008,1110	SQ		VNAP	MWL	
>Referenced SOP Class UID	0008,1150	UI		ALWAYS	AUTO	
>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	AUTO	
>Study Instance UID	0020,000D	UI		ALWAYS	MWL	
>Requested Procedure Description	0032,1060	LO		VNAP	AUTO	
>Requested Procedure Code Sequence	0032,1064	SQ		VNAP	MWL	
>>Code Value	0008,0100	SH		ALWAYS	MWL	
>>Coding Scheme Designator	0008,0102	SH		ALWAYS	MWL	
>>Coding Scheme Version	0008,0103	SH		ALWAYS	MWL	
>>Code Meaning	0008,0104	LO		ALWAYS	MWL	
>Requested Procedure ID	0040,1001	SH		VNAP	AUTO	
>Reason for the Requested Procedure	0040,1002	LO		ANAP	AUTO	
>Placer Order Number/Imaging Service Request	0040,2016	LO		VNAP	AUTO	
>Filler Order Number/Imaging Service Request	0040,2017	LO		VNAP	AUTO	
>Referenced Instance Sequence	0008,114A	SQ		VNAP	MWL	
>>Referenced SOP Class UID	0008,1150	UI		ALWAYS	AUTO	
>>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	AUTO	
Performed Procedure Code Sequence	0040,A372	SQ		VNAP	AUTO	
Current Requested Procedure Evidence Sequence	0040,A375	SQ		ANAP	AUTO	
>Referenced Series Sequence	0008,1115	SQ		ALWAYS	AUTO	
>>Referenced SOP Sequence	0008,1199	SQ		ALWAYS	AUTO	
>>>Referenced SOP Class UID	0008,1150	UI		ALWAYS	AUTO	
>>>Referenced SOP Instance UID	0008,1155	UI		ALWAYS	AUTO	

>>Series Instance UID	0020,000E	UI		ALWAYS	AUTO	
>Study Instance UID	0020,000D	UI		ALWAYS	AUTO	
Completion Flag	0040,A491	CS	COMPLETE	ALWAYS	AUTO	
Completion Flag Description	0040,A492	LO	“Complete X-Ray Radiation Dose Structured Report”	ANAP	AUTO	
Verification Flag	0040,A493	CS	UNVERIFIED	ALWAYS	AUTO	

**Table 147: SR Document Content Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Value Type	0040,A040	CS	CONTAINER	ALWAYS	AUTO	
Concept Name Code Sequence	0040,A043	SQ		ANAP	AUTO	
>Code Value	0008,0100	SH		ALWAYS	AUTO	
>Coding Scheme Designator	0008,0102	SH		ALWAYS	AUTO	
>Code Meaning	0008,0104	LO		ALWAYS	AUTO	
Content Template Sequence	0040,A504	SQ		ANAP	AUTO	
>Template Identifier	0040,DB00	CS		ALWAYS	AUTO	
>Mapping Resource	0008,0105	CS		ALWAYS	AUTO	
Continuity of Content	0040,A050	CS		ALWAYS	AUTO	
Content Sequence	0040,A730	SQ		ANAP	AUTO	
>Measured Value Sequence	0040,A300	SQ		VNAP	AUTO	
>>Measurement Units Code Sequence	0040,08EA	SQ		ALWAYS	AUTO	
>>>Code Value	0008,0100	SH		VNAP	AUTO	
>>>Coding Scheme Designator	0008,0102	SH		VNAP	AUTO	
>>>Code Meaning	0008,0104	LO		ALWAYS	AUTO	
>>Numeric Value	0040,A30A	DS		ALWAYS	AUTO	
>Relationship Type	0040,A010	CS		ALWAYS	AUTO	
>Text Value	0040,A160	UT		ANAP	AUTO	
>Value Type	0040,A040	CS		ALWAYS	AUTO	
>Concept Name Code Sequence	0040,A043	SQ		ANAP	AUTO	
>>Code Value	0008,0100	SH		ALWAYS	AUTO	
>>Coding Scheme Designator	0008,0102	SH		ALWAYS	AUTO	
>>Code Meaning	0008,0104	LO		ALWAYS	AUTO	
>Concept Code Sequence	0040,A168	SQ		ALWAYS	AUTO	
>>Code Value	0008,0100	SH		ALWAYS	AUTO	
>>Coding Scheme Designator	0008,0102	SH		ALWAYS	AUTO	
>>Code Meaning	0008,0104	LO		ALWAYS	AUTO	

**Table 148: SOP Common Module**

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Specific Character Set	0008,0005	CS		ANAP	AUTO	

Instance Creation Date	0008,0012	DA		ANAP	AUTO	
Instance Creation Time	0008,0013	TM		ANAP	AUTO	
SOP Class UID	0008,0016	UI	1.2.840.10008.5.1.4.1.1.88.67	ALWAYS	AUTO	
SOP Instance UID	0008,0018	UI		ALWAYS	AUTO	
Instance Number	0020,0013	IS		ANAP	AUTO	

**8.1.2. Attribute Mapping**

Not applicable.

**8.1.3. Coerced/Modified fields**

Not applicable.

**8.2. Data Dictionary of Private Attributes**

Not applicable.

**8.3. Coded Terminology and Templates**

Not applicable.


**8.3.1. Context Groups**

Not applicable.

**8.3.2. Template Specifications**

**X-RAY RADIATION DOSE STRUCTURED REPORT IOD TEMPLATES**

The templates comply SCP the X-Ray Radiation Dose please refer the figure below:

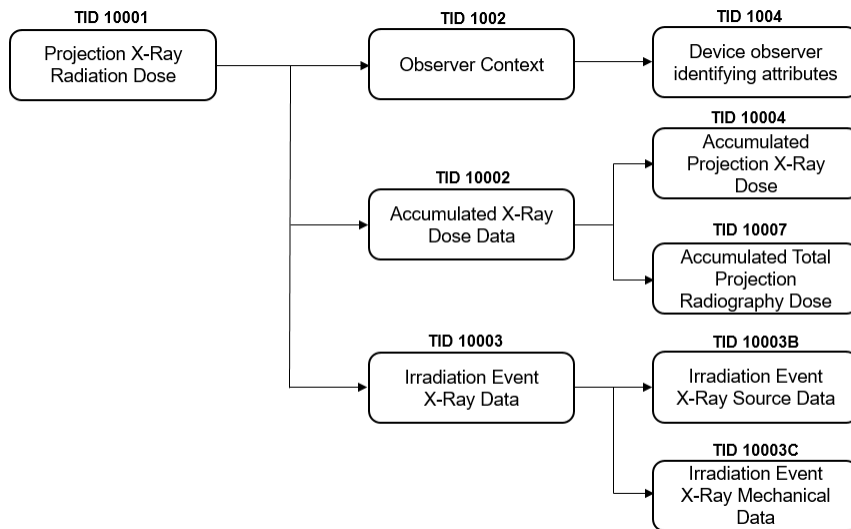

**Figure 18: X-Ray Radiation Dose Structured Report IOD Template Structure**

This section describes the content of all the templates used in the X-Ray Radiation Dose Reporting SR.

**Table 149: Used Templates for X-Ray Radiation Dose Reporting**

Template Name	Template ID
Projection X-Ray Radiation Dose	TID 10001
Accumulated X-Ray Dose	TID 10002
Irradiation Event X-Ray Data	TID 10003
Irradiation Event X-Ray Source Data (for Fluoroscopy Irradiation Event type)	TID 10003B
Irradiation Event X-Ray Source Data (for Stationary Acquisition Event type)	TID 10003B
Irradiation Event X-Ray Mechanical Data	TID 10003C
Accumulated Acquisition Projection X-Ray Dose (for Fluoroscopy Irradiation Event type)	TID 10004
Accumulated Acquisition Projection X-Ray Dose (for Stationary Acquisition Event type)	TID 10004
Accumulated Total Projection Radiography Dose	TID 10007
Observer Context	TID 1002
Device Observer Identifying Attributes	TID 1004

**8.3.2.1. TID 10001 Projection X-Ray Radiation Dose**

**Table 150: Projection X-Ray Radiation Dose**

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
		EV (113701, DCM, "X-Ray Radiation Dose Report")	CONTAINER	1	ALWAYS	
>	HAS CONCEPT MOD	EV (121058, DCM, "Procedure reported")	CODE	1	ALWAYS	(113704, DCM, "Projection X-Ray")
>>	HAS CONCEPT MOD	EV (363703001, SCT, "Has Intent")	CODE	1	ALWAYS	(1279505009, SCT, "Combined diagnostic and therapeutic intent (qualifier value)" )
>		DTID 1002 "Observer Context"	INCLUDE	1-n	ALWAYS	
>	HAS OBS CONTEXT	EV (113705, DCM, "Scope of Accumulation")	CODE	1	ALWAYS	(113016, DCM, "Performed Procedure Step")
>>	HAS PROPERTIES	121126, DCM, "Performed Procedure Step SOP Instance UID"	UIDREF	1	ALWAYS	
>	CONTAINS	113945, DCM, "X-Ray Detector Data Available"	CODE	1	ALWAYS	(373067005, SCT, "No")
>	CONTAINS	DTID 10002 "Accumulated X-Ray Dose"	INCLUDE	1	ALWAYS	(113622, DCM, "Single Plane") OR (113620, DCM, "Plane A") OR (113621, DCM, "Plane B")
>	CONTAINS	DTID 10003 "Irradiation Event X-Ray Data"	INCLUDE	1-n	ALWAYS	

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>	CONTAINS	EV (121106, DCM, "Comment")	TEXT	1	ALWAYS	X-Ray Radiation Dose Structured Report related to the Performed.
>	CONTAINS	EV (113854, DCM, "Source of Dose Information")	CODE	1-n	ALWAYS	(113856, DCM, Automated Data Collection)

**8.3.2.2. TID 10002 Accumulated X-Ray Dose**

**Table 151: Accumulated X-Ray Dose**

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
		EV (113702, DCM, "Accumulated X-Ray Dose Data")	CONTAINER	1	ALWAYS	
>	HAS CONCEPT MOD	EV (113764, DCM, "Acquisition Plane")	CODE	1	ALWAYS	(113622, DCM, "Single Plane") OR (113620, DCM, "Plane A") OR (113621, DCM, "Plane B")
>	CONTAINS	EV (122505, DCM, "Calibration")	CONTAINER	1	CONDITIONAL	
>>	HAS CONCEPT MOD	EV (113794, DCM, "Dose Measurement Device")	CODE	1	CONDITIONAL	(15869005, SCT, "Dosimeter")
>>	CONTAINS	EV (113723, DCM, "Calibration DateTime")	DATETIME	1	CONDITIONAL	
>>	CONTAINS	EV (122322, DCM, "Calibration Factor")	NUM	1	CONDITIONAL	Units: (1, UCUM, "no units")
>>	CONTAINS	EV (113763, DCM, "Calibration Uncertainty")	NUM	1	CONDITIONAL	Units: (% , UCUM, "Percent")
>>	CONTAINS	EV (113724, DCM, "Calibration Responsible Party")	TEXT	1	CONDITIONAL	
>>	CONTAINS	EV (113720, DCM, "Calibration Protocol")	TEXT	1	CONDITIONAL	
>	CONTAINS	(001, 99PHI-IXR-XPER, "Height of System")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>	CONTAINS	(002, 99PHI-IXR-XPER, "Focal Spot to ISO Center")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>	CONTAINS	DTID (10004) "Accumulated Projection X-Ray Dose"	INCLUDE	1	ALWAYS	TID (10001) Row 2 = (113704, DCM, "Projection X-Ray") AND TID (10001) Row 4 is absent
>	CONTAINS	DTID (10007) "Accumulated Total Projection Radiography Dose"	INCLUDE	1	ALWAYS	TID (10001) Row 2 = (113704, DCM, "Projection X-Ray") AND TID (10001) Row 4 is absent

**8.3.2.3. TID 10003 Irradiation Event X-Ray Data**

**Table 152: Irradiation Event X-Ray Data**

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
	CONTAINS	EV (113706, DCM, "Irradiation Event X-Ray Data")	CONTAINER	1	ALWAYS	
>	HAS CONCEPT MOD	EV (113764, DCM, "Acquisition Plane")	CODE	1	ALWAYS	(113622, DCM, "Single Plane") OR (113620, DCM, "Plane A") OR (113621, DCM, "Plane B")
>	CONTAINS	EV (113769, DCM, "Irradiation Event UID")	UIDREF	1	ALWAYS	
>	CONTAINS	DT (111526, DCM, "DateTime Started")	DATETIME	1	ALWAYS	
>	CONTAINS	EV (113721, DCM, "Irradiation Event Type")	CODE	1	ALWAYS	(113611, DCM, "Stationary Acquisition") OR (113613, DCM, "Rotational Acquisition") OR (113612, DCM, "Stepping Acquisition") OR (44491008, SCT, "Fluoroscopy")
>	CONTAINS	EV (125203, DCM, "Acquisition Protocol")	TEXT	1	ALWAYS	
>	CONTAINS	EV (113745, DCM, "Patient Table Relationship")	CODE	1	ALWAYS	
>	CONTAINS	EV (113743, DCM, "Patient Orientation")	CODE	1	ALWAYS	



NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>>	HAS CONCEPT MOD	EV (113744, DCM, "Patient Orientation Modifier")	CODE	1	ALWAYS	
>	CONTAINS	EV (123014, DCM, "Target Region")	CODE	1	ALWAYS	
>	CONTAINS	EV (122130, DCM, "Dose Area Product")	NUM	1	ALWAYS	Units: (Gy.m2, UCUM, "Gy.m2")
>	CONTAINS	EV (111638, DCM, "Patient Equivalent Thickness")	NUM	1	ALWAYS	
>	CONTAINS	EV (121106, DCM, "Comment")	TEXT	1	ALWAYS	
>	CONTAINS	DTID 10003B "Irradiation Event X-Ray Source Data"	INCLUDE	1	CONDITIONAL	TID (10001) Row 9 is absent
>	CONTAINS	DTID 10003C "Irradiation Event X-Ray Mechanical Data"	INCLUDE	1	CONDITIONAL	TID (10001) Row 10 is absent
>	CONTAINS	(003, 99PHI-IXR-XPER, "Number of Frames")	NUM	1	ALWAYS	Units: (1, UCUM, "no units")
>	CONTAINS	(004, 99PHI-IXR-XPER, "Sub Images per Frame")	NUM	1	ALWAYS	Units: (1, UCUM, "no units")
>>	CONTAINS	(005, 99PHI-IXR-XPER, "Wedges and Shutters")	CONTAINER	1	ALWAYS	Units: (mm, UCUM, "mm")
>>>	CONTAINS	(006, 99PHI-IXR-XPER, "Bottom Shutter")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>>>	CONTAINS	(007, 99PHI-IXR-XPER, "Left Shutter")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>>>	CONTAINS	(008, 99PHI-IXR-XPER, "Right Shutter")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>>>	CONTAINS	(009, 99PHI-IXR-XPER, "Top Shutter")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>>>	CONTAINS	(010, 99PHI-IXR-XPER, "Distance Wedge 1")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>>>	CONTAINS	(011, 99PHI-IXR-XPER, "Distance Wedge 2")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>>>	CONTAINS	(012, 99PHI-IXR-XPER, "Angle Wedge 1")	NUM	1	ALWAYS	Units: (deg, UCUM, "deg")
>>>	CONTAINS	(013, 99PHI-IXR-XPER, "Angle Wedge 2")	NUM	1	ALWAYS	Units: (deg, UCUM, "deg")
>>	CONTAINS	(014, 99PHI-IXR-XPER, "Beam Position")	CONTAINER	1	ALWAYS	Units: (mm, UCUM, "mm")
>>>	CONTAINS	(015, 99PHI-IXR-XPER, "Longitudinal Beam Position")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>>>	CONTAINS	(016, 99PHI-IXR-XPER, "Lateral Beam Position")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>>>	CONTAINS	(017, 99PHI-IXR-XPER, "Beam Angle")	NUM	1	ALWAYS	Units: (deg, UCUM, "deg")
>	CONTAINS	(018, 99PHI-IXR-XPER, "Final Distance Source to Detector")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>	CONTAINS	(019, 99PHI-IXR-XPER, "Final Table Cradle Angle")	NUM	1	ALWAYS	Units: (deg, UCUM, "deg")
>	CONTAINS	(021, 99PHI-IXR-XPER, "Table Height Position")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>	CONTAINS	(022, 99PHI-IXR-XPER, "Final Table Tilt Angle")	NUM	1	ALWAYS	Units: (deg, UCUM, "deg")
>>	CONTAINS	(023, 99PHI-IXR-XPER, "Detector Field Size")	CONTAINER	1	ALWAYS	Units: (mm, UCUM, "mm")
>>>	CONTAINS	(024, 99PHI-IXR-XPER, "X Side")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>>>	CONTAINS	(025, 99PHI-IXR-XPER, "Y Side")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>	CONTAINS	(026, 99PHI-IXR-XPER, "Object Thickness")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>	CONTAINS	(121114, DCM, "Performing Physician")	TEXT	1	ALWAYS	
>	CONTAINS	(029, 99PHI-IXR-XPER, "Application Name")	TEXT	1	ALWAYS	Left Coronary 15 fps Medium
>	CONTAINS	(030, 99PHI-IXR-XPER, "Fluoro Flavour")	TEXT	1	ALWAYS	Medium

**8.3.2.4. TID 10003B Irradiation Event X-Ray Source Data (for Fluoroscopy Irradiation Event type)**

**Table 153: Irradiation Event X-Ray Source Data**

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>	CONTAINS	EV (113738, DCM, "Dose (RP)")	NUM	1	ALWAYS	Units: (Gy, UCUM, "Gy")
>	CONTAINS	EV(113780, DCM, "Reference Point Definition")	TEXT	1	ALWAYS	15 cm below BeamIsocenter
>	CONTAINS	EV (113732, DCM, "Fluoro Mode")	CODE	1	ALWAYS	(113630, DCM, "Continuous") OR (113631, DCM, "Pulsed")
>	CONTAINS	EV (113768, DCM, "Number of Pulses")	NUM	1	ALWAYS	Units: (1, UCUM, "no units")

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>	CONTAINS	EV (113793, DCM, "Pulse Width")	NUM	1	ALWAYS	Units: (ms, UCUM, "ms")
>	CONTAINS	EV (113742, DCM, "Irradiation Duration")	NUM	1	ALWAYS	Units: (s, UCUM, "s")
>	CONTAINS	EV (113733, DCM, "KVP")	NUM	1	ALWAYS	Units: (kV, UCUM, kV)
>	CONTAINS	EV (113734, DCM, "X-Ray Tube Current")	NUM	1	ALWAYS	Units: (mA, UCUM, mA)
>	CONTAINS	EV (113767, DCM, "Average X-Ray Tube Current")	NUM	1	ALWAYS	Units: (mA, UCUM, mA)
>	CONTAINS	EV (113736, DCM, "Exposure")	NUM	1	CONDITIONAL	Units: (uA.s, UCUM, uA.s)
>	CONTAINS	EV (113766, DCM, "Focal Spot Size")	NUM	1	CONDITIONAL	Units: (mm, UCUM, mm)
>	CONTAINS	(113771, DCM, "X-Ray Filters")	CONTAINER	1-n	ALWAYS	
>	CONTAINS	EV (113772, DCM, "X-Ray Filter Type")	CODE	1	ALWAYS	
>	CONTAINS	EV (113757, DCM, "X-Ray Filter Material")	CODE	1	ALWAYS	(12503006, SCT,Aluminum) OR (71128006, SCT,Molybdenum) OR (66925006, SCT, "Copper") OR (59801003, SCT, Rhodium") OR (767776000, SCT,"Niobium") OR (767775001, SCT,"Europium") OR (88488004, SCT, "Lead") OR (45215009, SCT,"Tantalum") OR (41967008, SCT, "Silver")
>	CONTAINS	EV (113758, DCM, "X-Ray Filter Thickness Minimum")	NUM	1	ALWAYS	Units: (mm, UCUM, mm)
>	CONTAINS	EV (113773, DCM, "X-Ray Filter Thickness Maximum")	NUM	1	ALWAYS	Units: (mm, UCUM, mm)
>	CONTAINS	EV (113790, DCM, "Collimated Field Area")	NUM	1	ALWAYS	Units: (m2, UCUM, m2)

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>	CONTAINS	EV (113788, DCM, "Collimated Field Height")	NUM	1	ALWAYS	Units: (mm, UCUM, mm)
>	CONTAINS	EV (113789, DCM, "Collimated Field Width")	NUM	1	ALWAYS	Units: (mm, UCUM, mm)

**8.3.2.5. TID 10003B Irradiation Event X-Ray Source Data (for Stationary Acquisition Irradiation Event type)**

**Table 154: Irradiation Event X-Ray Source Data**

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>	CONTAINS	EV (113738, DCM, "Dose (RP)")	NUM	1	ALWAYS	Units: (Gy, UCUM, "Gy")
>	CONTAINS	EV(113780, DCM, "Reference Point Definition")	TEXT	1	ALWAYS	15 cm below BeamIsocenter
>	CONTAINS	EV (113768, DCM, "Number of Pulses")	NUM	1	ALWAYS	Units: (1, UCUM, "no units")
>	CONTAINS	EV (113793, DCM, "Pulse Width")	NUM	1	ALWAYS	Units: (ms, UCUM, "ms")
>	CONTAINS	EV (113742, DCM, "Irradiation Duration")	NUM	1	ALWAYS	Units: (s, UCUM, "s")
>	CONTAINS	EV (113733, DCM, "KVP")	NUM	1	ALWAYS	Units: (kV, UCUM, kV)
>	CONTAINS	EV (113734, DCM, "X-Ray Tube Current")	NUM	1	ALWAYS	Units: (mA, UCUM, mA)
>	CONTAINS	EV (113767, DCM, "Average X-Ray Tube Current")	NUM	1	ALWAYS	Units: (mA, UCUM, mA)
>	CONTAINS	EV (113736, DCM, "Exposure")	NUM	1	ALWAYS	Units: (uA.s, UCUM, uA.s)
>	CONTAINS	EV (113766, DCM, "Focal Spot Size")	NUM	1	ALWAYS	Units: (mm, UCUM, mm)
>	CONTAINS	(113771, DCM, "X-Ray Filters)	CONTAINER	1-n	ALWAYS	
>	CONTAINS	EV (113772, DCM, "X-Ray Filter Type")	CODE	1	ALWAYS	

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>	CONTAINS	EV (113757, DCM, "X-Ray Filter Material")	CODE	1	ALWAYS	(12503006, SCT, "Aluminum") OR (71128006, SCT, "Molybdenum") OR (66925006, SCT, "Copper") OR (59801003, SCT, "Rhodium") OR (767776000, SCT, "Niobium") OR (767775001, SCT, "Europium") OR (88488004, SCT, "Lead") OR (45215009, SCT, "Tantalum") OR (41967008, SCT, "Silver")
>	CONTAINS	EV (113758, DCM, "X-Ray Filter Thickness Minimum")	NUM	1	ALWAYS	Units: (mm, UCUM, mm)
>	CONTAINS	EV (113773, DCM, "X-Ray Filter Thickness Maximum")	NUM	1	ALWAYS	Units: (mm, UCUM, mm)
>	CONTAINS	EV (113790, DCM, "Collimated Field Area")	NUM	1	ALWAYS	Units: (m2, UCUM, m2)
>	CONTAINS	EV (113788, DCM, "Collimated Field Height")	NUM	1	ALWAYS	Units: (mm, UCUM, mm)
>	CONTAINS	EV (113789, DCM, "Collimated Field Width")	NUM	1	ALWAYS	Units: (mm, UCUM, mm)

8.3.2.6. TID 1003C Irradiation Event X-Ray Mechanical Data

Table 155: Irradiation Event X-Ray Mechanical Data

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
		EV (112011, DCM, "Positioner Primary Angle")	NUM	1	CONDITIONAL	Units: (deg, UCUM, deg)
		EV (112012, DCM, "Positioner Secondary Angle")	NUM	1	CONDITIONAL	Units: (deg, UCUM, deg)
		EV (113754, DCM, "Table Head Tilt Angle")	NUM	1	ALWAYS	Units: (deg, UCUM, deg)
		EV (113755, DCM, "Table Horizontal Rotation Angle")	NUM	1	ALWAYS	Units: (deg, UCUM, deg)

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
		EV (113756, DCM, "Table Cradle Tilt Angle")	NUM	1	ALWAYS	Units: (deg, UCUM, deg)
		(113748, DCM, "Distance Source to Isocenter")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
		(113737, DCM, "Distance Source to Reference Point")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
		(113750, DCM, "Distance Source to Detector")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
		(113751, DCM, "Table Longitudinal Position")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
		(113752, DCM, "Table Lateral Position")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
		(113753, DCM, "Table Height Position")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")

**8.3.2.7. TID 10004 Accumulated Projection X-Ray Dose (for Fluoroscopy Irradiation Event type)**

**Table 156: Accumulated Projection X-Ray Dose**

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>>	CONTAINS	EV (113726, DCM, "Fluoro Dose Area Product Total")	NUM	1	ALWAYS	Units: (Gy.m2, UCUM, "Gy.m2")
>>	CONTAINS	EV (113728, DCM, "Fluoro Dose (RP) Total")	NUM	1	ALWAYS	Units: (Gy, UCUM, "Gy")
>>	CONTAINS	EV (113730, DCM, "Total Fluoro Time")	NUM	1	ALWAYS	Units: (s, UCUM, "s")

**8.3.2.8. TID 10004 Accumulated Projection X-Ray Dose (for Stationary Acquisition Irradiation Event type)**

**Table 157: Accumulated Projection X-Ray Dose**

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>>	CONTAINS	EV (113727, DCM, "Acquisition Dose Area Product Total")	NUM	1	ALWAYS	Units: (Gy.m2, UCUM, "Gy.m2")
>>	CONTAINS	EV (113729, DCM, "Acquisition Dose (RP) Total")	NUM	1	CONDITIONAL	Units: (Gy, UCUM, "Gy")
>>	CONTAINS	EV (113855, DCM, "Total Acquisition Time")	NUM	1	ALWAYS	Units: (s, UCUM, "s")

**8.3.2.9. TID 10007 Accumulated Total Projection Radiography Dose**

**Table 158: Accumulated Total Projection Radiography Dose**

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>	CONTAINS	EV (113722, DCM, "Dose Area Product Total")	NUM	1	ALWAYS	Units: (Gy.m2, UCUM, Gy.m2)
>	CONTAINS	EV (113725, DCM, "Dose (RP) Total")	NUM	1	ALWAYS	Units: (Gy, UCUM, Gy)
>	CONTAINS	EV (113737, DCM, "Distance Source to Reference Point")	NUM	1	ALWAYS	Units: (mm, UCUM, "mm")
>	CONTAINS	EV (113731, DCM, "Total Number of Radiographic Frames")	NUM	1	ALWAYS	Units: (1, UCUM, no units)
>	CONTAINS	EV (113780, DCM, "Reference Point Definition")	TEXT	1	ALWAYS	15 cm below BeamIsocenter

### 8.3.2.10. TID 1002 Observer Context

Table 159: Observer Context

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>	HAS OBS CONTEXT	EV (121005, DCM, "Observer Type")	CODE	1	ALWAYS	(121007, DCM, "Device")
	HAS OBS CONTEXT	DTID 1004 "Device Observer Identifying Attributes"	INCLUDE	1	ALWAYS	

### 8.3.2.11. TID 1004 Device Observer Identifying Attributes

Table 160: Device Observer Identifying Attributes

NL	Relation with Parent	Concept Name	VT	VM	Presence of Value	Value
>	HAS OBS CONTEXT	EV (121012, DCM, "Device Observer UID")	UIDREF	1	ALWAYS	
>	HAS OBS CONTEXT	EV (121013, DCM, "Device Observer Name")	TEXT	1	CONDITIONAL	
>	HAS OBS CONTEXT	EV (121014, DCM, "Device Observer Manufacturer")	TEXT	1	ALWAYS	Philips
>	HAS OBS CONTEXT	EV (121015, DCM, "Device Observer Model Name")	TEXT	1	ALWAYS	Azurion
>	HAS OBS CONTEXT	EV (121016, DCM, "Device Observer Serial Number")	TEXT	1	ALWAYS	

**8.3.3. Private code definitions**

Not applicable.

**8.4. Grayscale Image consistency**

The monitors and printers attached to the product can be calibrated by using the Service Application.

**8.5. Standard Extended/Specialized/Private SOP Classes**

Not applicable.

**8.6. Private Transfer Syntaxes**

Not applicable.



*- This part of the page is left intentionally empty -*

**Issued by:**

IGT:

Philips Medical Systems Nederland B.V.

Veenpluis 6

5684 PC Best

The Netherlands

Note that the address is also known as “Veenpluis 4-6”, which refers to the same physical location

Internet: <https://www.philips.com/dicom>

Doc Id: HSDP-1471478

Date: 10-July-2024

