

**Philips Medical Systems
DICOM Conformance Statement**

DSI Release 4.4

Document Number 4522 220 84061
6 June 1997

© Copyright Philips Medical Systems Nederland B.V. 1997

All rights reserved

Philips
Medical
Systems



PHILIPS

Issued by:

Philips Medical Systems Nederland B.V.
Integrated Clinical Solutions, Marketing & Communications
Building QP-0233
P.O. Box 10.000
5680 DA Best
The Netherlands
Tel.: +31 40 2763827
Fax.: +31 40 2763810
email: dicom@best.ms.philips.com
Internet: <http://www.philips.com/ms/solution/connect>
ftp://ftp.philips.com/pub/ms/dicom/Conformance_Stmnts

Table of Contents

1	Introduction	1
1.1	Scope and field of application	1
1.2	Intended audience	1
1.3	Contents and structure	1
1.4	Used definitions, terms and abbreviations	1
1.5	References	2
1.6	Important note to the reader	2
2	Implementation model	3
2.1	Application Data Flow Diagram	3
2.1.1	Description of the DSI DICOM Export Functionality	4
2.1.2	Description of the DSI DICOM Modality Worklist Functionality ..	5
2.2	Functional definition of Application Entities	5
2.3	Sequencing of Real World Activities	5
3	AE Specifications	6
3.1	DSI DICOM AE Specification	6
3.1.1	Association Establishment Policies	6
3.1.2	Association Initiation Policy	7
3.1.3	Association Acceptance Policy	12
4	Communication Profiles	13
4.1	TCP/IP Stack	13
4.1.1	Physical Media Support	13
5	Extensions/Specializations/Privatizations	13
6	Configuration	13
6.1	AE Title/Presentation Address mapping	13
6.1.1	Local AE Titles and Presentation Addresses	13
6.1.2	Remote AE Titles and Presentation Addresses	13
6.2	Configurable parameters	13
7	Support of Extended Character Sets	14
8	Overview of the applied X-Ray Fluoroscopy (XRF) Image IOD	15
9	Overview of the applied Secondary Capture (SC) Image IOD	19
10	Overview of the applied Modality Worklist IOD	23
11	Overview of the applied Study Component Management IOD	24

1 Introduction

This chapter provides general information about the purpose, scope and contents of this Conformance Statement.

1.1 Scope and field of application

The scope of this DICOM Conformance Statement is to facilitate data exchange with equipment of Philips Medical Systems. This document specifies the compliance to the DICOM standard (formally called the NEMA PS 3.X-1993 standards). It contains a short description of the applications involved and provides technical information about the data exchange capabilities of the equipment. The main elements describing these capabilities are: the supported DICOM Service Object Pair (SOP) Classes, Roles, Information Object Definitions (IOD) and Transfer Syntaxes.

The field of application is the integration of the Philips Medical Systems equipment into an environment of medical devices.

This Conformance Statement should be read in conjunction with the DICOM standard and its addenda. The conformance to the DICOM standard is a key element of the Inturis Program (see [INTURIS]).

1.2 Intended audience

This Conformance Statement is intended for:

- (potential) customers,
- system integrators of medical equipment,
- marketing staff interested in system functionality,
- software designers implementing DICOM interfaces.

It is assumed that the reader is familiar with the DICOM standard.

1.3 Contents and structure

The DICOM Conformance Statement is contained in chapter 2 through 7 and follows the contents and structuring requirements of DICOM PS 3.2-1993 and Supplement 2 (in case of Media specifications).

Additionally, the chapters following 7 specify the details of the applied IODs.

1.4 Used definitions, terms and abbreviations

DICOM definitions, terms and abbreviations are used throughout this Conformance Statement. For a description of these, see NEMA PS 3.3-1993 and PS 3.4-1994.

The word Philips in this document refers to Philips Medical Systems.

1.5 References

- [DICOM] The Digital Imaging and Communications in Medicine (DICOM) standard:
NEMA PS 3.X (X refers to the part 1 - 13) and Supplements
National Electrical Manufacturers Association (NEMA) Publication Sales
1300 N. 17th Street, Suite 1847
Rosslyn, Va. 22209, United States of America
- [INTURIS] Philips Inturis Program
Integrated Clinical Solutions
Philips Medical Systems Nederland B.V. (see address at page ii)

1.6 Important note to the reader

This Conformance Statement by itself does not guarantee successful interoperability of Philips equipment with non-Philips equipment. The user (or user's agent) should be aware of the following issues:

- **Interoperability**

Interoperability refers to the ability of application functions, distributed over two or more systems, to work successfully together. The integration of medical devices into a networked environment may require application functions that are not specified within the scope of DICOM. Consequently, using only the information provided by this Conformance Statement does not guarantee interoperability of Philips equipment with non-Philips equipment. It is the user's responsibility to analyse thoroughly the application requirements and to specify a solution that integrates Philips equipment with non-Philips equipment.

- **Validation**

Philips equipment has been carefully tested to assure that the actual implementation of the DICOM interface corresponds with this Conformance Statement.

Where Philips equipment is linked to non-Philips equipment, the first step is to compare the relevant Conformance Statements. If the Conformance Statements indicate that successful information exchange should be possible, additional validation tests will be necessary to ensure the functionality, performance, accuracy and stability of image and image related data. It is the responsibility of the user (or user's agent) to specify the appropriate test suite and to carry out the additional validation tests.

- **New versions of the DICOM Standard**

The DICOM Standard will evolve in future to meet the user's growing requirements and to incorporate new features and technologies. Philips is actively involved in this evolution and plans to adapt its equipment to future versions of the DICOM Standard. In order to do so, Philips reserves the right to make changes to its products or to discontinue its delivery. The user should ensure that any non-Philips provider linking to Philips equipment, also adapts to future versions of the DICOM Standard. If not, the incorporation of DICOM enhancements into Philips equipment may lead to loss of connectivity (in case of networking) and incompatibility (in case of media).

2 Implementation model

The DSI (Digital Spot Imaging) is a digital fluorography modality. It is part of an X-ray system. The main functions are:

- image acquisition and display
- image review and processing
- image handling, storage and networking
- administration of patient, physician and examination data

The main application areas are:

- R/F examinations
- vascular and non-vascular examinations
- angiography examinations
- tomography examinations
- interventional procedures

DSI Release 4.4 contains a DICOM Export function (to transfer DSI image data to a remote system) and a DICOM RIS interface (to retrieve an up-to-date Worklist from Radiology Information System).

2.1 Application Data Flow Diagram

The DSI contains one Application Entity able to export DICOM images and handle Modality Worklists. The related Implementation Model is shown in Figure 2-1 on page 3.

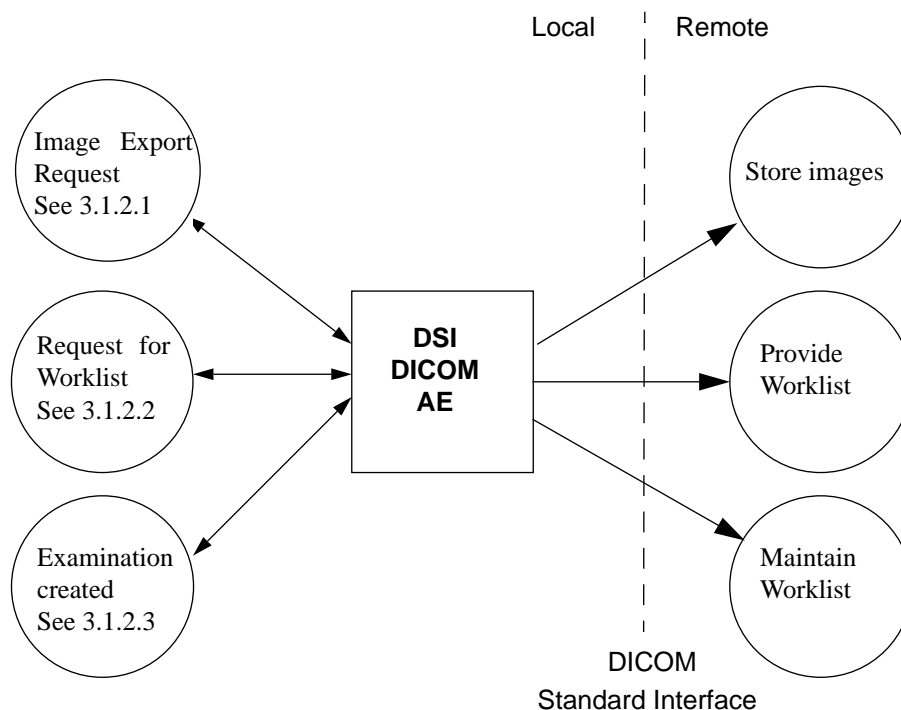


Figure 2-1: DSI DICOM Implementation Model

2.1.1 Description of the DSI DICOM Export Functionality

The DSI DICOM Export function is activated by an operator request. A remote destination is selected from the user interface, followed by the selection of the examination.

With DSI systems an examination corresponds to the DICOM Patient and Study level. Each examination contains one or more runs, corresponding to the DICOM Series level. Each run contains one or more images, corresponding to the DICOM Image level. This relationship is depicted in Figure 2-2 on page 4. DSI can contain up to 14 examinations, maximum 1280 runs per examination and maximum 1280 images per run.

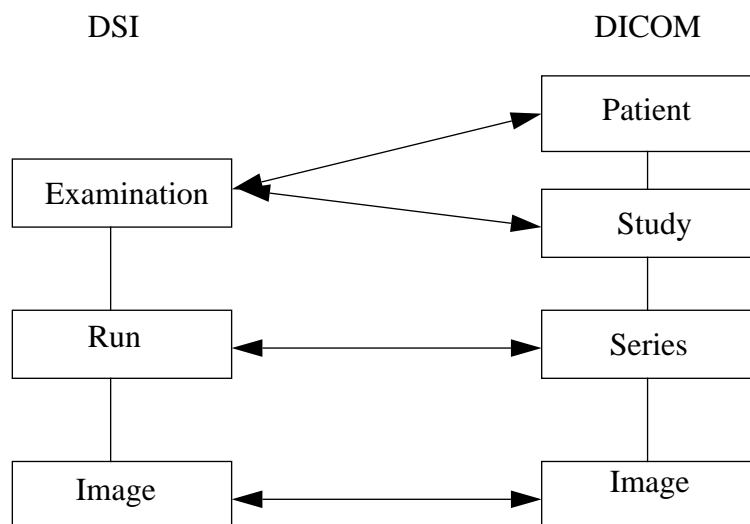


Figure 2-2: Relationship between the DSI and DICOM levels

The DSI DICOM Export transfers a complete examination to a remote DICOM node. The transfer of a subset of images in an examination is not possible. During the DICOM store operation it is possible to perform a cancel operation on the store.

Image data to be transferred are instances of the DICOM X-Ray Radiofluoroscopic (XRF) or Secondary Capture (SC) classes. The following cases can be distinguished:

- The remote system supports both XRF and SC classes.
Result will be that all fluoroscopy and exposure images are exported as XRF images and all other images (like external video) as SC images.
- The remote system supports the XRF class only.
Result will be that all fluoroscopy and exposure images are exported as XRF images and all other images (like external video) are **not** exported.
- The remote system supports the SC class only.
Result will be that all images are exported as SC images.
- The remote system supports neither the XRF nor SC class.
Result will be that none of the image types can be exported.

During the DICOM export of an exposure or fluoroscopy image as XRF image the following image processing is performed by DSI: video invert, subtraction, pixel shift.

During the DICOM export of an exposure or fluoroscopy image as SC image the following image processing is performed by DSI: video invert, contrast, brightness, edge enhancement, subtraction, pixel shift.

During the DICOM export of an external video image as SC image the following image processing is performed by DSI: video invert, contrast, brightness, edge enhancement.

In case of a subtracted run the DICOM Export first stores the mask image, followed by the subtracted images from that run. No explicit indication is sent with the subtracted images, as to which image was used as the mask image. The image number in the run can be used as an implicit indication.

Images shown zoomed on the DIS are exported as normal (i.e. non zoomed) images. Annotations on zoomed images are not sent. DSI annotations on normal images are exported as Image Comments.

The images are intended for viewing purpose only.

The compatibility of image data re-imported (by media exchange) of the exported DICOM image data in an earlier stage is not defined.

DSI logs certain events related to the DICOM export at three different levels, see the service manual of the DSI system.

2.1.2 Description of the DSI DICOM Modality Worklist Functionality

DSI is able to retrieve the modality Worklist from a RIS. This is done at request of the operator. From the received list a selection of one Worklist item is made; the examination to be performed.

After selecting a Worklist item, the RIS is informed about this creation of the study component.

2.2 Functional definition of Application Entities

The DSI DICOM Application Entity acts as a Service Class User (SCU) of the Storage Service Class. After invoking it will open an Association to the remote system. For each image to be transported a retrieve action from the DSI storage will take place followed by the conversion to a DICOM message to be transferred to the remote system.

The DSI DICOM Application Entity acts also as a Service Class User (SCU) of the Basic Worklist Management Service Class and the Study Management Service Class. After invoking it will open an Association to the remote system (usually a RIS) to request for the up-to-date modality Worklist.

After selecting a Worklist item, a new Association to the remote system is opened and that system is informed about the creation of a Study Component.

2.3 Sequencing of Real World Activities

The Request for Worklist should be done first, before a Study Component can be created.

Then the generated images may be exported. However, export of DICOM images is also possible without the Worklist and Study Component activities.

3 AE Specifications

DSI contains one Application Entity.

3.1 DSI DICOM AE Specification

The DSI DICOM Application Entity provides Standard Conformance to the following DICOM 3.0 SOP classes as an SCU:

Table 3-1: Supported SOP classes by the DSI DICOM AE as SCU

<i>SOP class Name</i>	<i>UID</i>
Secondary Capture Image Storage ^a	1.2.840.10008.5.1.4.1.1.7
X-Ray Radiofluoroscopic Image Storage ^a	1.2.840.10008.5.1.4.1.1.12.2
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31
Study Component Management	1.2.840.10008.3.1.2.3.2

- a. See section 2.1 on page 3 for the mapping of the DSI image types to these DICOM XRF and SC SOP Classes.

The DSI DICOM Application Entity does not support DICOM 3.0 SOP classes as an SCP.

3.1.1 Association Establishment Policies

3.1.1.1 General

The maximum PDU size of DSI is fixed on 16K (is 16384 bytes). See also the important remark about the PDU size of the remote systems in section 6.2 on page 13.

3.1.1.2 Number of Associations

DSI will attempt to establish one Association at a time. DSI does not accept Associations.

3.1.1.3 Asynchronous Nature

DSI does not support asynchronous operations and will not perform asynchronous window negotiation.

3.1.1.4 Implementation Identifying Information

The Implementation Class UID is: "1.3.46.670589.6.1.1.4.4.1".
The Implementation Version Name is: "DSI R441, 970303".

3.1.2 Association Initiation Policy

DSI initiates Associations as a result of the following events:

- The DSI operator requests for DICOM export, see section 3.1.2.1 on page 7;
- The DSI operator requests for the DSI Worklist, see section 3.1.2.2 on page 10;
- The DSI operator has selected a Worklist item from the received DSI Worklist (i.e. an examination to perform), see section 3.1.2.3 on page 12.

3.1.2.1 Export from DSI system

3.1.2.1.1 Associated Real-World Activity

The DSI operator is able to request for export of one examination or a list of examinations to a remote system. See section 2.1 on page 3 for the definition of an examination. The complete examination is transferred to the remote system.

The DSI DICOM Export function will be accessible through the DSI F2 Copy page. With the F4 Config page the remote DICOM system is selected from a list of maximum of five configurable nodes.

The current transfer can be aborted by the DSI F2 Cancel function.

After the transfer the Association is released.

3.1.2.1.2 Proposed Presentation Contexts

DSI will propose the following presentation contexts:

Table 3-2: Proposed Presentation Contexts at Image Export

<i>Presentation Context table</i>					
<i>Abstract Syntax</i>		<i>Transfer Syntax</i>		<i>Role</i>	<i>Extended Negotiation</i>
<i>Name</i>	<i>UID</i>	<i>Name List</i>	<i>UID List</i>		
See Note ^a	See Note ^a	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
See Note ^a	See Note ^a	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
See Note ^a	See Note ^a	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

- a. Any of the Image Storage SOP classes listed in Table 3-1, "Supported SOP classes by the DSI DICOM AE as SCU," on page 6

3.1.2.1.2.1 SOP Specific Conformance to Storage SOP Classes

DSI provides standard conformance.

Extended negotiation is not supported.

Table 3-3 lists the applied optional modules and attributes in the XRF images.

AE Specifications

Conditional attributes Laterality (type 2C), Patient Orientation (type 2C), Image Date (type 2C), Image Time (type 2C), Exposure (type 2C), Window Width (type 1C) are always present. A detailed overview of the applied XRF Image IOD is given section 8 on page 15.

Table 3-3: Applied optional Modules and Attributes of the XRF Image IOD

<i>IE</i>	<i>Module</i>	<i>Optional Attributes</i>
Patient	Patient	-
Study	General Study	Study Description
Series	General Series	Series Date, Series Time, Performing Physician's Name, Protocol Name
Equipment	General Equipment	Institution Name, Station Name, Manufacturer's Model name, Device Serial Number, Software Version(s)
Image	General Image	Acquisition Number, Acquisition Date, Acquisition Time, Image Comments
	Image Pixel	-
	Display Shutter (applied optional Module)	-
	X-Ray Image	-
	X-Ray Acquisition	-
	VOI LUT (applied optional Module)	Window Center
	SOP Common	Specific Character Set

Table 3-4 lists the applied optional modules and attributes in the SC images.

Conditional attributes Laterality (type 2C), Patient Orientation (type 2C), Image Date (type 2C), Image Time (type 2C) are always present. A detailed overview of the applied SC Image IOD is given section 9 on page 19.

Table 3-4: Applied optional Modules and Attributes of the SC Image IOD

<i>IE</i>	<i>Module</i>	<i>Optional Attributes</i>
Patient	Patient	-
Study	General Study	Study Description
Series	General Series	Series Date, Series Time, Performing Physician's Name, Protocol Name

Table 3-4: Applied optional Modules and Attributes of the SC Image IOD (Continued)

<i>IE</i>	<i>Module</i>	<i>Optional Attributes</i>
Equipment	SC Equipment	Secondary Capture Device Manufacturer, Secondary Capture Device Manufacturer's Model Name, Secondary Capture Software Version(s)
Image	General Image	Acquisition Number, Acquisition Date, Acquisition Time, Image Comments
	Image Pixel	-
	SC Image	Date of Secondary Capture, Time of Secondary Capture
	SOP Common	Specific Character Set

During the selection and export of an examination, the user interface shows the status:

Export flag	examination flagged for DICOM export
Export busy	examination being exported
Export done	examination exported successfully
Export error	error while exporting examination
Export cancel	export of examination being cancelled
Not exported	export of examination cancelled

DSI will stop the transfer of the image data and release the Association as soon as it receives an unsuccessful or warning C-STORE Response status, or when the Association is aborted by the remote system. The reason will be logged, the user interface of the DSI console will show the status "Export Error".

If a RIS connection is present, Patient and Study related information will be retrieved by DSI from the RIS and will be put in the image headers of the exported images. See also section 8 on page 15 and section 9 on page 19.

The UIDs in the composite images are generated when the related Study, Series and Image are created. This means that two exports of the same image will have the same UIDs. The Study UID may be retrieved from the RIS via the Worklist.

3.1.2.2 Request for a Modality Worklist

3.1.2.2.1 Associated Real-World Activity

This DSI function will be triggered at request of the operator. An Association will be set-up to the pre-configured remote system (the RIS). After receiving the Worklist the Association is released.

3.1.2.2.1.1 Proposed Presentation Contexts

DSI will propose the following presentation contexts:

Table 3-5: Proposed Presentation Contexts for Request for Modality Worklist

<i>Presentation Context table</i>					
<i>Abstract Syntax</i>		<i>Transfer Syntax</i>		<i>Role</i>	<i>Extended Negotiation</i>
<i>Name</i>	<i>UID</i>	<i>Name List</i>	<i>UID List</i>		
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

3.1.2.2.1.2 SOP Specific Conformance to Modality Worklist Management

DSI provides standard conformance.

No optional Matching keys are supported (i.e. no optional Matching Keys will be present in the C-FIND Requests).

No optional Return Keys are supported (i.e. no optional Return Keys will be present in the C-FIND Requests) except the optional attribute Code Meaning (0008, 0104) in the Requested Procedure Code Sequence.

If more than 42 worklist items are received (via C-FIND Responses) as result of a worklist request, DSI will cancel the request by sending a C-CANCEL-FIND Request.

A detailed overview of all requested Matching and Return keys with additional attribute information is given in section 10 on page 23. The possibly used matching types (like Single Value, Wildcarding, Range matching) are specified there too.

The status of the C-FIND Responses (Success, Refused, Error, Warning) is logged. Only general status messages are displayed on the user interface, like "RIS not responding" and "No patient available from RIS".

The following non-printable characters (hexa-decimal coded) are not supported in the received Worklist data:

00H through 1FH,

7FH
80H through 9FH,
A0H, A6H, A8H, A9H, AAH, AEH
B1H, B4H, B8H, B9H, BEH
C0H, C1H, C2H, C3H, C8H, CAH, CBH, CCH, CDH, CEH, CFH
D0H, D2H, D3H, D4H, D5H, D9H, DAH, DBH, DDH, DEH
E3H
F0H, F5H, FDH, FEH

If one or more of these non-printable characters are present in the strings of received Worklist data, the string is not accepted.

If non-printable characters are present in the Patient Name or if this attribute is empty, the worklist entry is not accepted. In case the Patient Name only contains spaces, this Worklist entry and all succeeding Worklist entries will be skipped.

3.1.2.3 Create a Study Component

3.1.2.3.1 Associated Real-World Activity

This DSI function will be triggered when a Worklist item is selected, i.e. a Study Component will be created. An Association will be set-up to the pre-configured remote system (usually a RIS). After informing the remote system about the created Study Component, the Association is released.

3.1.2.3.1.1 Proposed Presentation Contexts

DSI will propose the following presentation contexts:

Table 3-6: Proposed Presentation Contexts for Create a Study Component

<i>Presentation Context table</i>					
<i>Abstract Syntax</i>		<i>Transfer Syntax</i>		<i>Role</i>	<i>Extended Negotiation</i>
<i>Name</i>	<i>UID</i>	<i>Name List</i>	<i>UID List</i>		
Study Component Management SOP Class	1.2.840.10008.3.1.2.3.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Study Component Management SOP Class	1.2.840.10008.3.1.2.3.2	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Study Component Management SOP Class	1.2.840.10008.3.1.2.3.2	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

3.1.2.3.1.2 SOP Specific Conformance to Study Component Management

DSI provides standard conformance.

Only the N-CREATE Service Element is used (as SCU), so no use of the N-GET and N-SET Service Elements.

No optional attributes are applied in the N-CREATE Service Element. The Specific Character Set (conditional in DICOM) will always be present.

A detailed overview of all applied attributes with additional attribute information is given in section 11 on page 24.

The status of the DIMSE Responses (Success, Refused, Error, Warning) is logged. No status messages are displayed on the user interface.

3.1.3 Association Acceptance Policy

DSI does not accept Associations.

4 Communication Profiles

4.1 TCP/IP Stack

DSI provides DICOM 3.0 TCP/IP Network Communication Support as defined in Part 8 of the DICOM 3.0 Standard.

4.1.1 Physical Media Support

The DSI system supports ISO 8802-3 10BASE5 Ethernet.

5 Extensions/Specializations/Privatizations

Not applicable.

6 Configuration

The configuration of a DSI system is done by means of a configuration program. It is intended to be used by Philips service engineers only.

6.1 AE Title/Presentation Address mapping

6.1.1 Local AE Titles and Presentation Addresses

The local (so of DSI itself) Application Entity Title, local System Name and local (System) IP Address are selected by the service configuration program.

6.1.2 Remote AE Titles and Presentation Addresses

All remote applications to be selected as image export destination or as Worklist supplier are configurable for the following items:

- The Application Entity Title of the remote application.
- The IP Address and Port Number at which the remote application should accept Association requests.
- The Remote Host Name (i.e. System name) of the system on which the remote application resides.

The Remote Host Name is used in the remote DICOM system list with the F4 Config page.

6.2 Configurable parameters

The PDU size of DSI (i.e. the maximum allowed size of PDU messages received by DSI) is fixed on 16K.

For optimal performance of the communication DSI - remote system, it is advised to configure the PDU size on the remote system as large as possible: unlimited and 64K are preferred (in that order). PDU size of 32K on the remote system should **not** be taken due to an implementation restriction of DSI.

7 Support of Extended Character Sets

DSI supports the Extended Character Set “ISO_IR 100” (Latin alphabet No 1, supplementary set) for the Image Export function.

The support of characters at import of Modality Worklist data is specified in section 3.1.2.2.1.2 on page 10.

Overview of the applied X-Ray Fluoroscopy (XRF) Image IOD

8 Overview of the applied X-Ray Fluoroscopy (XRF) Image IOD

The modules selected from the IOD module table of DICOM 3.0 are given in the table below.

Table 8-1: Applied Modules in the XRF IOD

<i>Information Entity</i>	<i>Module</i>
Patient	Patient
Study	General Study
Series	General Series
Equipment	General Equipment
Image	General Image
	Image Pixel
	X-Ray Image
	Display Shutter
	X-Ray Acquisition
	VOI LUT
	SOP Common

The details of these applied modules are given in the tables below. The list of possible values are given (if applicable). The situation that an attribute is present conditionally/optionally or that an attribute may contain a zero length value, is indicated too. Conditions and Defined/Enumerated Values of DICOM 3.0 are applicable but are not shown in the tables.

Table 8-2: Patient Module

<i>Attribute Description</i>	<i>Tag</i>	<i>Note</i>
Patient's Name	0010,0010	Received from RIS or entered by user
Patient ID	0010,0020	Received from RIS or entered by user
Patient's Birth Date	0010,0030	Received from RIS or entered by user
Patient's Sex	0010,0040	Received from RIS or entered by user

Overview of the applied X-Ray Fluoroscopy (XRF) Image IOD

Table 8-3: General Study Module

<i>Attribute Description</i>	<i>Tag</i>	<i>Note</i>
Study Instance UID	0020,000D	Generated at creation of the Study (Component) or received from RIS
Study Date	0008,0020	
Study Time	0008,0030	
Referring Physician's Name	0008,0090	Zero length value if not received from RIS
Study ID	0020,0010	Zero length value if not received from RIS
Accession Number	0008,0050	Zero length value if not received from RIS
Study Description	0008,1030	Not present if not entered by user

Table 8-4: General Series Module

<i>Attribute Description</i>	<i>Tag</i>	<i>Note</i>
Modality	0008,0060	RF
Series Instance UID	0020,000E	Generated at creation of the Series
Series Number	0020,0011	
Series Date	0008,0021	
Series Time	0008,0031	
Performing Physician's Name	0008,1050	Received from RIS, entered by user or is empty if not known.
Protocol Name	0018,1030	Not present if not entered by user
Laterality	0020,0060	Always zero length value

Table 8-5: General Equipment Module

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
Manufacturer	0008,0070	Philips Medical Systems
Institution Name	0008,0080	
Station name	0008,1010	
Manufacturer's Model Name	0008,1090	In format DSI<release number>
Device Serial Number	0018,1000	
Software Version(s)	0018,1020	

Overview of the applied X-Ray Fluoroscopy (XRF) Image IOD

Table 8-6: General Image Module

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
Image Number	0020,0013	1
Patient Orientation	0020,0020	Always zero length value
Image Date	0008,0023	
Image Time	0008,0033	
Acquisition Number	0020,0012	
Acquisition Date	0008,0022	
Acquisition Time	0008,0032	
Image Comments	0020,4000	Contains also the DSI image annotations on normal (i.e. non zoomed) images in the format "(x,y) <text>". This attribute is not present if not entered by user and if no annotations are present.

Table 8-7: Image Pixel Module and X-Ray Image Module^a

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
Image Type	0008,0008	ORIGINAL\PRIMARY\SINGLE PLANE
Pixel Intensity Relationship	0028,1040	DISP
Samples per Pixel	0028,0002	1
Photometric Interpretation	0028,0004	MONOCHROME2
Rows	0028,0010	512 or 1024 The actual image size in 60 Hz DSI systems is smaller: 480 or 960.
Columns	0028,0011	equal to the value of Rows (512 or 1024). The actual image size in 60 Hz DSI systems is smaller: 480 or 960.
Bits Allocated	0028,0100	8
Bits Stored	0028,0101	8
High Bit	0028,0102	7
Pixel Representation	0028,0103	0000H
Pixel Data	7FE0,0010	

a. These two modules are combined because some attributes are present in both modules.

Overview of the applied X-Ray Fluoroscopy (XRF) Image IOD

Table 8-8: Display Shutter Module

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
Shutter Shape	0018,1600	CIRCULAR or CIRCULAR\RECTANGULAR
Shutter Left Vertical Edge	0018,1602	
Shutter Right Vertical Edge	0018,1604	
Shutter Upper Horizontal Edge	0018,1606	
Shutter Lower Horizontal Edge	0018,1608	
Center of Circular Shutter	0018,1610	
Radius of Circular Shutter	0018,1612	

Table 8-9: X-Ray Acquisition Module

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
KVP	0018,0060	Always zero length value
Exposure	0018,1152	Always zero length value
Radiation Setting	0018,1155	SC or GR

Table 8-10: VOI LUT Module

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
Window Center	0028,1050	This attribute is related to the DSI Contrast / Brightness.
Window Width	0028,1051	This attribute is related to the DSI Contrast / Brightness.

Table 8-11: SOP Common Module

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
SOP Class UID	0008,0016	1.2.840.10008.5.1.4.1.1.12.2
SOP Instance UID	0008,0018	Generated at creation of the image
Specific Character Set	0008,0005	ISO_IR 100

Overview of the applied Secondary Capture (SC) Image IOD

9 Overview of the applied Secondary Capture (SC) Image IOD

The modules selected from the IOD module table of DICOM 3.0 are given in the table below.

Table 9-1: Applied Modules in the SC IOD

<i>Information Entity</i>	<i>Module</i>
Patient	Patient
Study	General Study
Series	General Series
Equipment	SC Equipment
Image	General Image
	Image Pixel
	SC Image
	SOP Common

The details of these applied modules are given in the tables below. The list of possible values are given (if applicable). The situation that an attribute is present conditionally/optionally or that an attribute may contain a zero length value, is indicated too. Conditions and Defined/Enumerated Values of DICOM 3.0 are applicable but are not shown in the tables.

Table 9-2: Patient Module

<i>Attribute Description</i>	<i>Tag</i>	<i>Note</i>
Patient's Name	0010,0010	Received from RIS or entered by user
Patient ID	0010,0020	Received from RIS or entered by user
Patient's Birth Date	0010,0030	Received from RIS or entered by user
Patient's Sex	0010,0040	Received from RIS or entered by user

Table 9-3: General Study Module

<i>Attribute Description</i>	<i>Tag</i>	<i>Note</i>
Study Instance UID	0020,000D	Generated at creation of the Study (Component) or received from RIS
Study Date	0008,0020	
Study Time	0008,0030	

Table 9-3: General Study Module (Continued)

<i>Attribute Description</i>	<i>Tag</i>	<i>Note</i>
Referring Physician's Name	0008,0090	Zero length value if not received from RIS.
Study ID	0020,0010	Zero length value if not received from RIS.
Accession Number	0008,0050	Zero length value if not received from RIS.
Study Description	0008,1030	Not present if not entered by user

Table 9-4: General Series Module

<i>Attribute Description</i>	<i>Tag</i>	<i>Note</i>
Modality	0008,0060	OT
Series Instance UID	0020,000E	Generated at creation of the Series
Series Number	0020,0011	
Series Date	0008,0021	
Series Time	0008,0031	
Performing Physician's Name	0008,1050	Received from RIS, entered by user or is empty if not known.
Protocol Name	0018,1030	Not present if not entered by user
Laterality	0020,0060	Always zero length value

Table 9-5: SC Equipment Module

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
Conversion Type	0008,0064	DV
Secondary Capture Device Manufacturer	0018,1016	Philips Medical Systems
Secondary Capture Device Manufacturer's Model Name	0018,1018	In format DSI<release number>
Secondary Capture Software Version(s)	0018,1019	

Table 9-6: General Image Module

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
Image Number	0020,0013	1
Patient Orientation	0020,0020	Always zero length value
Image Date	0008,0023	

Overview of the applied Secondary Capture (SC) Image IOD

Table 9-6: General Image Module (Continued)

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
Image Time	0008,0033	
Acquisition Number	0020,0012	
Acquisition Date	0008,0022	
Acquisition Time	0008,0032	
Image Comments	0020,4000	Contains also the DSI image annotations on normal (i.e. non zoomed) images in the format "(x,y) <text>". This attribute is not present if not entered by user and if no annotations are present.

Table 9-7: Image Pixel Module

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
Samples per Pixel	0028,0002	1
Photometric Interpretation	0028,0004	MONOCHROME2
Rows	0028,0010	512 or 1024 The actual image size in 60 Hz DSI systems is smaller: 480 or 960.
Columns	0028,0011	Equal to the value of Rows (512 or 1024) The actual image size in 60 Hz DSI systems is smaller: 480 or 960.
Bits Allocated	0028,0100	8
Bits Stored	0028,0101	8
High Bit	0028,0102	7
Pixel Representation	0028,0103	0000H
Pixel Data	7FE0,0010	

Table 9-8: SC Image Module

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
Date of Secondary Capture	0018,1012	
Time of Secondary Capture	0018,1014	

Table 9-9: SOP Common Module

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
SOP Class UID	0008,0016	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	0008,0018	Generated at creation of the image
Specific Character Set	0008,0005	ISO_IR 100

Overview of the applied Modality Worklist IOD

10 Overview of the applied Modality Worklist IOD

This chapter specifies in detail the applied attributes in the C-FIND Service Element of this supported SOP Class.

The list of possible values are given (if applicable). The situation that an attribute is present conditionally/optionally or that an attribute may contain a zero length value, is indicated too.

Table 10-1: Modality Worklist Information Model - FIND SOP Class - C-FIND

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
Patient's Name	0010,0010	Return key
Patient ID	0010,0020	Return key
Patient's Birth Date	0010,0030	Return key
Patient's Sex	0010,0040	Return key
Scheduled Procedure Step Sequence	0040,0100	Return key
> Modality	0008,0060	Fixed Single Value matching is applied. Applied value(s): RF
> Scheduled Station AE Title	0040,0001	Fixed Single Value matching is applied (which is the configured Application Name)
> Scheduled Procedure Step Start Time	0040,0003	Return key
> Scheduled Performing Physician's Name	0040,0006	Return key
Study Instance UID	0020,000D	Return key
Requested Procedure Code Sequence	0032,1064	Return key
> Code Value	0008,0100	Return key
> Coding Scheme Designator	0008,0102	Return key
> Code Meaning	0008,0104	Return key
Requested Procedure ID	0040,1001	Return key
Accession Number	0008,0050	Return key
Referring Physician's Name	0008,0090	Return key

11 Overview of the applied Study Component Management IOD

This chapter specifies in detail the applied attributes in the N-CREATE Service Element of this supported SOP Class.

The list of possible values are given (if applicable). The situation that an attribute is present conditionally/optionally or that an attribute may contain a zero length value, is indicated too.

Table 11-1: Study Component Management SOP Class - N-CREATE

<i>Attribute Name</i>	<i>Tag</i>	<i>Note</i>
Specific Character Set	0008,0005	Applied value(s): ISO_IR 100
Referenced Series Sequence	0008,1115	Is always empty
Study ID	0020,0010	Is always empty
Referenced Study Sequence	0008,1110	
> Referenced SOP Class UID	0008,1150	Applied value(s): 1.2.840.10008.3.1.2.3.1
> Referenced SOP Instance UID	0008,1155	Value from Study Instance UID in C-FIND Response of Modality Worklist.
Modality	0008,0060	Applied value(s): RF, RG
Study Description	0008,1030	Description of the classification of the Study (Component) performed, entered by institution.
Procedure Code Sequence	0008,1032	
> Code Value	0008,0100	Applied value(s): DSI
> Coding Scheme Designator	0008,0102	Applied value(s): 99DSI
> Code Meaning	0008,0104	Applied value(s): DSI CREATED CODE
Study Component Status ID	0032,1055	Applied value(s): COMPLETED