


DICOM Conformance Statement

Application Annex:

3D-RA R6.6

On Interventional Workspot R1.6

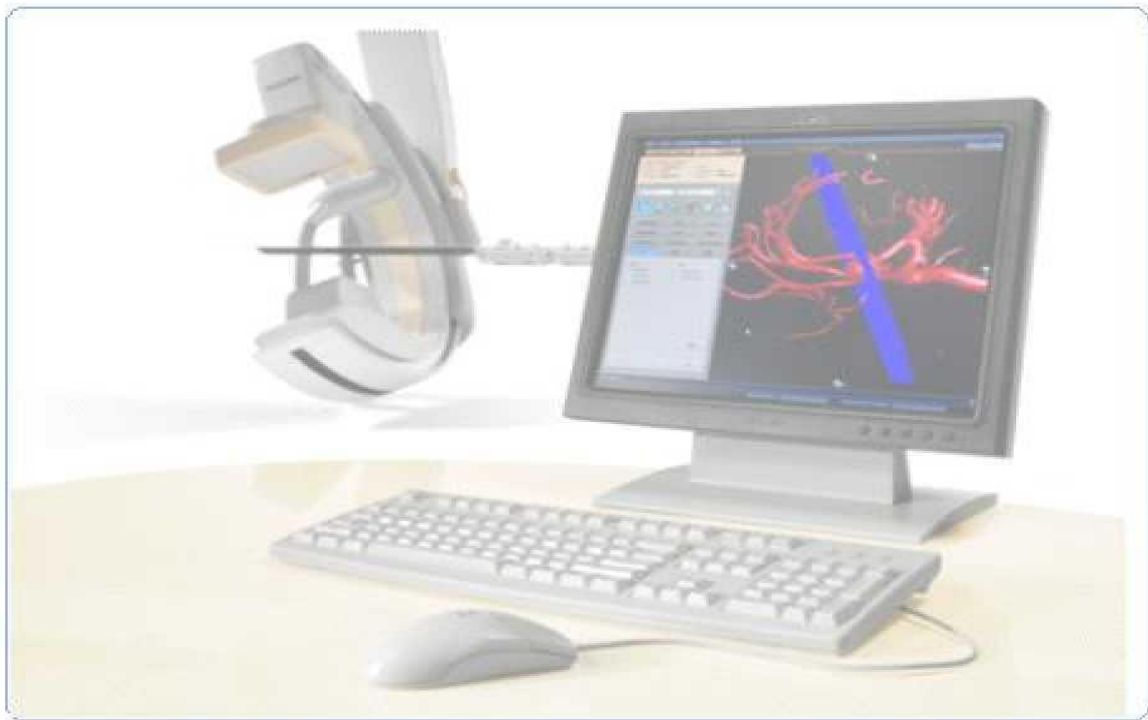

Issued by:

Philips Medical Systems Nederland BV, a Philips Healthcare company,

P.O. Box 10.000
5680 DA Best
The Netherlands

Internet: www.philips.com/dicom

Document Number: ICAP-PF.0046232

Date: 02-March-2020

Table of Contents

1. INTRODUCTION	4
1.1. REVISION HISTORY	4
1.2. TERMINOLOGY	4
2. DATA SPECIFICATIONS	5
2.1. SUPPORTED IOD'S	5
2.1.1. Acceptance Criteria	5
2.1.2. Contents of Created IOD's	6
2.1.2.1. List of created SOP Classes	6
2.1.2.2. CT Image Storage SOP Class	7
2.1.2.3. Secondary Capture Image Storage SOP class	10
2.1.2.4. Multiframe True Color Secondary Capture Image Storage SOP class	12
2.1.2.5. X-Ray Angiographic Image Storage SOP Class	15
2.1.2.6. X-Ray 3D Angiographic Image Storage	18
2.1.2.7. Raw data Storage SOP class	22
3. VERSION HISTORY	ERROR! BOOKMARK NOT DEFINED.

1. Introduction

This DICOM Conformance Statement annex is applicable to the **3D-RA R6.6** later referred to as 3D-RA R6.6 Application. In general **3D-RA R6.6** Application allows for generating three-dimensional volumes from XA data and for viewing and analyzing XA images and derived data.

The following analysis packages are offered by **3D-RA R6.6** Application (licensing might be applicable):

- Advanced Vessel Analysis (AVA)
- Virtual Stenting

1.1. Revision History

The revision history below provides dates and differences among individual document versions.

Table 1: Revision History

Document Version	Date of Issue	Status	Description
00	02-March-2020	Approved	Final Version

1.2. Terminology

DICOM	Digital Imaging and Communications in Medicine
IOD	Information Object Definition
UID	Unique Identifier
VR	Value Representation
XA	X-Ray Angiography
AVA	Advanced Vessel Analysis

2. Data Specifications

2.1. Supported IOD's

This section specifies each IOD accepted and / or created by 3D-RA R6.6 Application.

- ACCEPTED** The applicable IOD is accepted for storage in the repository of the hosting platform and supported for import 3D-RA R6.6 Application for viewing and analysis.
- CREATED** The 3D-RA R6.6 Application supports generation of derived data by using the applicable IOD and is able to store this data in the repository of the hosting platform.

Table 2: Supported IOD's

IOD		Support	
Name	UID	ACCEPTED	CREATED
X-Ray 3D Angiographic Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.13.1.1	No	Yes
CT Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.2	Yes	Yes
Raw Data Storage SOP Class	1.2.840.10008.5.1.4.1.1.66	No	Yes
X-Ray Angiographic Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.12.1	Yes	Yes
MR Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.4	Yes	No
Secondary Capture Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.7	No	Yes
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	No	Yes
Embedded Document	1.3.46.670589.2.8.1.1	No	Yes

2.1.1. Acceptance Criteria

This section specifies the acceptance criteria applied by 3D-RA R6.6/3D-RA R6.6 Application to which a dataset should adhere before it can be imported into the application. This can be criteria on the highest level (e.g. data from a certain manufacturer or system model) or certain DICOM attributes mandatory to be present into the dataset holding a specific value. In case one or more Philips private attributes are required, then a list of supported Philips system models will be mentioned.

Table 3: Accepted system models

Manufacturer	Modality	System Model Name(s)
Not applicable	Not applicable	Not applicable

Table 4: Accepted transfer syntaxes per IOD

IOD		Transfer Syntax	
Name	UID	Name	UID
CT Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		JPEG 2000 Image Compression	1.2.840.10008.1.2.4.91
		JPEG 2000 Image Compression (Lossless Only)	1.2.840.10008.1.2.4.90
		JPEG Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Non-Hierarchical, FOP (Process 14)	1.2.840.10008.1.2.4.70
RLE Lossless	1.2.840.10008.1.2.5		
X-Ray Angiographic Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.12.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1

		JPEG 2000 Image Compression JPEG 2000 Image Compression (Lossless Only) JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical, FOP (Process 14) RLE Lossless	1.2.840.10008.1.2.4.91 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.5
MR Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.4	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian JPEG 2000 Image Compression (Lossless Only) JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical, FOP (Process 14) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.4.91 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.5

Table 5: Accepted attribute values

Attribute Name	Attribute Number	Values / Comments
Not applicable	Not applicable	Not applicable

2.1.2. Contents of Created IOD's

This section specifies in detail the attribute contents of created data objects. Attributes are grouped together by its corresponding module as specified by DICOM standard. Philips private attributes are excluded for specification.

Abbreviations used in the Module table for the column "Presence of Value" are:

ALWAYS	The attribute is always present with a value
EMPTY	The attribute is always present without any value (attribute sent zero length)
VNAP	The attribute is always present and its Value is Not Always Present (attribute sent zero length if no value is present)
ANAP	The attribute is present under specified condition – if present then it will always have a value

The abbreviations used in the Module table for the column "Source" are:

AUTO	The attribute value is generated automatically
CONFIG	The attribute value source is a configurable parameter
COPY	The attribute value source is another SOP instance
FIXED	The attribute value is hard-coded in the application
IMPLICIT	The attribute value source is a user-implicit setting
MPPS	The attribute value is the same as that use for Modality Performed Procedure Step
MWL	The attribute value source is a Modality Worklist
USER	The attribute value source is explicit user input

2.1.2.1. List of created SOP Classes

Table 6: List of created SOP Classes

SOP Class Name	SOP Class UID
CT Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.2
Secondary Capture Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.7
Multiframe True Color Secondary Capture Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.7.4
X-Ray Angiographic Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.12.1

X-Ray 3D Angiographic Image Storage SOP Class	1.2.840.10008.5.1.4.1.1.13.1.1
Raw Data Storage SOP Class	1.2.840.10008.5.1.4.1.1.66

2.1.2.2. CT Image Storage SOP Class

Table 7: IOD of Created CT Image Storage SOP Class Instances

Information Entity	Module	Presence Of Module
Patient	Patient Module	ALWAYS
Study	General Study Module	ALWAYS
Patient Study	Patient Study Module	ALWAYS
Series	General Series Module	ALWAYS
Frame of Reference	Frame of Reference Module	ALWAYS
Equipment	General Equipment Module	ALWAYS
Image	Image Plane Module	ALWAYS
	General Image Module	ALWAYS
	Image Pixel Module	ALWAYS
	CT Image Module	ALWAYS
	VOI LUT Module	ALWAYS
	SOP Common Module	ALWAYS

Table 8: Patient Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Patient's Name	0010,0010	PN		ALWAYS	COPY	copied from source data
Patient ID	0010,0020	LO		ALWAYS	COPY	copied from source data
Issuer of Patient ID	0010,0021	LO		VNAP		
Patient's Birth Date	0010,0030	DA		VNAP	COPY	copied from source data
Patient's Sex	0010,0040	CS		ALWAYS	COPY	copied from source data

Table 9: General Study Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Study Date	0008,0020	DA		ALWAYS	COPY	copied from source data
Study Time	0008,0030	TM		ALWAYS	COPY	copied from source data
Accession Number	0008,0050	SH			COPY	copied from source data
Referring Physician's Name	0008,0090	PN		VNAP	COPY	copied from source data
Study Instance UID	0020,000D	UI		ALWAYS	COPY	copied from source data
Study ID	0020,0010	SH		ALWAYS	COPY	copied from source data

Table 10: Patient Study Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Admitting Diagnoses Description	0008,1080	LO		ALWAYS	COPY	copied from source data

Table 11: General Series Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Series Date	0008,0021	DA		ALWAYS	COPY	copied from source data
Series Time	0008,0031	TM		ALWAYS	COPY	copied from source data
Modality	0008,0060	CS		ALWAYS	COPY	copied from source data
Performing Physician's Name	0008,1050	PN		ALWAYS	COPY	copied from source data
Patient Position	0018,5100	CS		EMPTY	COPY	copied from source data
Series Instance UID	0020,000E	UI		ALWAYS	COPY	copied from source data
Series Number	0020,0011	IS		ALWAYS	COPY	copied from source data
Laterality	0020,0060	CS		ANAP	COPY	copied from source data
Performed Procedure Step Start Date	0040,0244	DA		ALWAYS	COPY	copied from source data
Performed Procedure Step Start Time	0040,0245	TM		ALWAYS	COPY	copied from source data
Performed Procedure Step ID	0040,0253	SH		ALWAYS	COPY	copied from source data

Table 12: Frame of Reference Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Frame of Reference UID	0020,0052	UI		ALWAYS	COPY	copied from source data
Position Reference Indicator	0020,1040	LO		VNAP	COPY	copied from source data

Table 13: General Equipment Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Manufacturer	0008,0070	LO	Philips	ALWAYS	FIXED	
Institution Name	0008,0080	LO		VNAP	COPY	copied from source data
Station Name	0008,1010	SH				
Manufacturer's Model Name	0008,1090	LO	Interventional Workspot	ALWAYS	CONFIG	
Device Serial Number	0018,1000	LO		ANAP	COPY	copied from source data
Software Versions	0018,1020	LO	1.6.x	ALWAYS	CONFIG	where "x" is the detailed application SW version.

Table 14: General Image Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Image Type	0008,0008	CS		VNAP		
Content Date	0008,0023	DA		ANAP		
Content Time	0008,0033	TM		ANAP		
Acquisition Number	0020,0012	IS		VNAP		
Instance Number	0020,0013	IS		ANAP		
Burned in Annotation	0028,0301	CS		VNAP		
Lossy Image Compression	0028,2110	CS		VNAP		

Table 15: Image Plane Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Slice Thickness	0018,0050	DS		VNAP		
Image Position (Patient)	0020,0032	DS		ALWAYS		
Image Orientation (Patient)	0020,0037	DS		ALWAYS		
Slice Location	0020,1041	DS		ANAP		
Pixel Spacing	0028,0030	DS		ALWAYS		

Table 16: Image Pixel Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Rows	0028,0010	US		ALWAYS	COPY	copied from source data
Columns	0028,0011	US		ALWAYS	COPY	copied from source data
Pixel Representation	0028,0103	US	0000	ALWAYS	COPY	copied from source data
Samples per Pixel	0028,0002	US	1	ALWAYS	FIXED	
Bits Allocated	0028,0100	US	16	ALWAYS	FIXED	
Bits Stored	0028,0101	US	16	ALWAYS	FIXED	
High Bit	0028,0102	US	15	ALWAYS	FIXED	
Pixel Data	7FE0,0010	OW/OB		ALWAYS	COPY	copied from source data

Table 17: CT Image Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Image Type	0008,0008	CS	DERIVED, SECONDARY	ALWAYS	FIXED	
KVP	0018,0060	DS		VNAP	COPY	copied from source data
Acquisition Number	0020,0012	IS		VNAP		
Samples per Pixel	0028,0002	US	1	ALWAYS	FIXED	
Photometric Interpretation	0028,0004	CS	MONOCHROME2	ALWAYS	FIXED	
Bits Allocated	0028,0100	US	16	ALWAYS	FIXED	
Bits Stored	0028,0101	US	16	ALWAYS	FIXED	
High Bit	0028,0102	US	15	ALWAYS	FIXED	
Rescale Intercept	0028,1052	DS		ALWAYS	COPY	copied from source data
Rescale Slope	0028,1053	DS		ALWAYS	COPY	copied from source data
Rescale Type	0028,1054	LO	US	ALWAYS		

Table 18: VOI LUT Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Window Center	0028,1050	DS	Value 1: 3D-RA R6.6/3D-RA R6.6 Window Width as set in histogram, converted to Hounsfield, XperCT Abdominal:60, XperCT Neuro:40	ALWAYS	COPY	copied from source data
Window Width	0028,1051	DS		ALWAYS	COPY	copied from source data

Table 19: SOP Common Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Specific Character Set	0008,0005	CS		ALWAYS	FIXED	As supported by hosting platform
Instance Creation Date	0008,0012	DA		ALWAYS		
Instance Creation Time	0008,0013	TM		ALWAYS		
SOP Class UID	0008,0016	UI	1.2.840.10008.5.1.4.1.1.2	ALWAYS	FIXED	
SOP Instance UID	0008,0018	UI		ALWAYS	COPY	copied from source data
Instance Number	0020,0013	IS		ALWAYS		

2.1.2.3. Secondary Capture Image Storage SOP class

Table 20: IOD of Created Secondary Capture Image Storage SOP Class Instances

Information Entity	Module	Presence Of Module
Patient	Patient Module	ALWAYS
Study	General Study Module	ALWAYS
Series	General Series Module	ALWAYS
Equipment	General Equipment Module	CONDITIONAL
	SC Equipment Module	ALWAYS
Image	General Image Module	ALWAYS
	Image Pixel Module	ALWAYS
	SOP Common Module	ALWAYS

Table 21: Patient Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Patient's Name	0010,0010	PN		ALWAYS	COPY	copied from source data
Patient ID	0010,0020	LO		ALWAYS	COPY	copied from source data
Patient's Birth Date	0010,0030	DA		ALWAYS	COPY	copied from source data
Patient's Sex	0010,0040	CS		ALWAYS	COPY	copied from source data

Table 22: General Study Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Study Date	0008,0020	DA		ALWAYS	COPY	copied from source data
Study Time	0008,0030	TM		ALWAYS	COPY	copied from source data
Accession Number	0008,0050	SH		VNAP		
Referring Physician's Name	0008,0090	PN		VNAP	COPY	copied from source data
Study Instance UID	0020,000D	UI		ALWAYS	COPY	copied from source data
Study ID	0020,0010	SH		ALWAYS	COPY	copied from source data

Table 23: General Series Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Series Date	0008,0021	DA		ALWAYS	COPY	copied from source data
Series Time	0008,0031	TM		ALWAYS	COPY	copied from source data
Modality	0008,0060	CS		ALWAYS	COPY	copied from source data
Series Instance UID	0020,000E	UI		ALWAYS	COPY	copied from source data
Series Number	0020,0011	IS		VNAP	COPY	copied from source data
Related Series Sequence	0008,1250	SQ		VNAP		
>Study Instance UID	0020,000D	UI		ALWAYS		
>Series Instance UID	0020,000E	UI		ALWAYS		
>Purpose of Reference Code Sequence	0040,A170	SQ		EMPTY		

Table 24: General Equipment Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Manufacturer	0008,0070	LO	Philips	ALWAYS	FIXED	
Institution Name	0008,0080	LO		VNAP	COPY	copied from source data
Station Name	0008,1010	SH				
Manufacturer's Model Name	0008,1090	LO	Interventional Workspot	ALWAYS	CONFIG	
Device Serial Number	0018,1000					
Software Versions	0018,1020	LO	1.6.x	ALWAYS	CONFIG	where "x" is the detailed application SW version

Table 25 : SC Equipment Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Modality	0008,0060	CS		ANAP		
Conversion Type	0008,0064	CS	WSD	ALWAYS		

Table 26: General Image Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Instance Number	0020,0013	IS		ALWAYS		
Patient Orientation	0020,0020	CS		VNAP		

Table 27: Image Pixel Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Samples per Pixel	0028,0002	US		ALWAYS		
Photometric Interpretation	0028,0004	CS		ALWAYS		
Planar Configuration	0028,0006	US		ALWAYS		
Rows	0028,0010	US		ALWAYS	COPY	copied from source data
Columns	0028,0011	US		ALWAYS	COPY	copied from source data
Bits Allocated	0028,0100	US	8	ALWAYS		
Bits Stored	0028,0101	US	8	ALWAYS		
High Bit	0028,0102	US	7	ALWAYS		
Pixel Representation	0028,0103	US	0000	ALWAYS	COPY	copied from source data
Pixel Data	7FE0,0010	OW/OB		ALWAYS	COPY	copied from source data

Table 28: SOP Common Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
SOP Class UID	0008,0016	UI	1.2.840.10008.5.1.4.1.1.7	ALWAYS	FIXED	
SOP Instance UID	0008,0018	UI		ALWAYS	COPY	copied from source data
Instance Creation Date	0008,0012	DA		ANAP	COPY	copied from source data
Instance Creation Time	0008,0013	TM		ANAP	COPY	copied from source data
Instance Number	0020,0013	IS		ANAP	COPY	copied from source data

2.1.2.4. Multiframe True Color Secondary Capture Image Storage SOP class

Table 29: IOD of Created Multiframe True Color Secondary Capture Image Storage SOP Class Instances

Information Entity	Module	Presence Of Module
Patient	Patient Module	ALWAYS
Study	General Study Module	ALWAYS
Series	General Series Module	ALWAYS
Equipment	General Equipment Module	CONDITIONAL
	SC Equipment Module	ALWAYS
Image	General Image Module	ALWAYS
	Image Pixel Module	ALWAYS
	Cine Module	CONDITIONAL
	Multi-Frame Module	ALWAYS
	Multi-Frame Functional Groups Module	OPTIONAL

SC Multi-frame Image Module	ALWAYS
SOP Common Module	ALWAYS

Table 30: Patient Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Patient's Name	0010,0010	PN		VNAP	COPY	copied from source data
Patient ID	0010,0020	LO		VNAP	COPY	copied from source data
Patient's Birth Date	0010,0030	DA		VNAP	COPY	copied from source data
Patient's Sex	0010,0040	CS		VNAP	COPY	copied from source data

Table 31: General Study Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Study Date	0008,0020	DA		VNAP	COPY	copied from source data
Study Time	0008,0030	TM		VNAP	COPY	copied from source data
Accession Number	0008,0050	SH		VNAP		
Referring Physician's Name	0008,0090	PN		VNAP	COPY	copied from source data
Study Instance UID	0020,000D	UI		ALWAYS	COPY	copied from source data
Study ID	0020,0010	SH		VNAP	COPY	copied from source data

Table 32: General Series Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Series Date	0008,0021	DA		ANAP	COPY	copied from source data
Series Time	0008,0031	TM		ANAP	COPY	copied from source data
Modality	0008,0060	CS		ALWAYS	COPY	copied from source data
Series Instance UID	0020,000E	UI		ALWAYS	COPY	copied from source data
Series Number	0020,0011	IS		ANAP	COPY	copied from source data
Related Series Sequence	0008,1250	SQ		ANAP		
>Study Instance UID	0020,000D	UI		ALWAYS		
>Series Instance UID	0020,000E	UI		ALWAYS		
>Purpose of Reference Code Sequence	0040,A170	SQ		VNAP		

Table 33: General Equipment Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Manufacturer	0008,0070	LO	Philips	ALWAYS	FIXED	

Institution Name	0008,0080	LO		VNAP	COPY	copied from source data
Station Name	0008,1010	SH				
Manufacturer's Model Name	0008,1090	LO	Interventional Workspot	ALWAYS	CONFIG	
Device Serial Number	0018,1000					
Software Versions	0018,1020	LO	1.6.x	ALWAYS	CONFIG	where "x" is the detailed application SW version.

Table 34 : SC Equipment Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Modality	0008,0060	CS		ANAP		
Conversion Type	0008,0064	CS	WSD	ALWAYS		

Table 35: General Image Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Instance Number	0020,0013	IS		VNAP		
Patient Orientation	0020,0020	CS		VNAP		
Burned in Annotation	0028,0301	CS		ANAP		

Table 36: Image Pixel Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Samples per Pixel	0028,0002	US		ALWAYS		
Photometric Interpretation	0028,0004	CS		ALWAYS		
Planar Configuration	0028,0006	US		ALWAYS		
Rows	0028,0010	US		ALWAYS	COPY	copied from source data
Columns	0028,0011	US		ALWAYS	COPY	copied from source data
Bits Allocated	0028,0100	US	8	ALWAYS		
Bits Stored	0028,0101	US	8	ALWAYS		
High Bit	0028,0102	US	7	ALWAYS		
Pixel Representation	0028,0103	US	0000	ALWAYS	COPY	copied from source data
Pixel Data	7FE0,0010	OW/OB		ALWAYS	COPY	copied from source data

Table 37: Cine Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Frame Time	0018,1063	DS		ALWAYS	COPY	copied from source data

Table 38: Multi-Frame Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Number of Frames	0028,0008	DS		ALWAYS	COPY	copied from source data
Frame Increment Pointer	0028,0009	AT		ALWAYS	COPY	copied from source data

Table 39: Multi-Frame Functional Groups Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Instance Number	0020,0013	IS		ALWAYS	COPY	copied from source data
Number of Frames	0028,0008	IS		ALWAYS	COPY	copied from source data

Table 40: SC Multi-Frame Image Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Frame Increment Pointer	0028,0009	AT		ALWAYS	COPY	copied from source data
Burned In Annotation	0028,0301	CS		ALWAYS	COPY	copied from source data

Table 41: SOP Common Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
SOP Class UID	0008,0016	UI	1.2.840.10008.5.1.4.1.1.7.4	ALWAYS	FIXED	
SOP Instance UID	0008,0018	UI		ALWAYS	COPY	copied from source data
Instance Creation Date	0008,0012	DA		ANAP	COPY	copied from source data
Instance Creation Time	0008,0013	TM		ANAP	COPY	copied from source data
Instance Number	0020,0013	IS		ANAP	COPY	copied from source data

2.1.2.5. X-Ray Angiographic Image Storage SOP Class**Table 42: IOD of Created X-Ray 3D Angiographic Image Storage Instances**

Information Entity	Module	Presence Of Module
Patient	Patient Module	ALWAYS
Study	General Study Module	ALWAYS
Series	General Series Module	ALWAYS
Equipment	General Equipment Module	ALWAYS
Image	General Image Module	ALWAYS
	Image Pixel Module	ALWAYS
	Cine Module	ALWAYS
	Multi-Frame Module	ALWAYS
	X-Ray Image Module	ALWAYS
	X-Ray Acquisition Module	ALWAYS
	XA Positioner Module	ALWAYS

VOI LUT Module	ALWAYS
SOP Common Module	ALWAYS

Table 43: Patient Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Patient's Name	0010,0010	PN		VNAP		
Patient ID	0010,0020	LO		VNAP		
Patient's Birth Date	0010,0030	DA		VNAP		
Patient's Sex	0010,0040	CS		VNAP		

Table 44: General Study Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Study Date	0008,0020	DA		VNAP		
Study Time	0008,0030	TM		VNAP		
Accession Number	0008,0050	SH		VNAP		
Referring Physician's Name	0008,0090	PN		VNAP		
Study Instance UID	0020,000D	UI		ALWAYS		
Study ID	0020,0010	SH		VNAP		

Table 45: General Series Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Series Date	0008,0021	DA		ANAP		
Series Time	0008,0031	TM		ANAP		
Modality	0008,0060	CS		ALWAYS		
Performing Physician's Name	0008,1050	PN		ANAP		
Related Series Sequence	0008,1250	SQ		ANAP		
>Study Instance UID	0020,000D	UI		ALWAYS		
>Series Instance UID	0020,000E	UI		ALWAYS		
>Purpose of Reference Code Sequence	0040,A170	SQ		VNAP		
Series Instance UID	0020,000E	UI		ALWAYS		
Series Number	0020,0011	IS		VNAP		
Laterality	0020,0060	CS		ANAP		

Table 46: General Equipment Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Manufacturer	0008,0070	LO	Philips	VNAP		
Institution Name	0008,0080	LO		ANAP		
Station Name	0008,1010	SH		ANAP		
Manufacturer's Model Name	0008,1090	LO	Interventional Workspot	ANAP		
Device Serial Number	0018,1000	LO		ANAP		
Software Versions	0018,1020	LO	1.6.x	ANAP		where "x" is the detailed application SW version

Table 47: General Image Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Instance Number	0020,0013	IS		VNAP		
Patient Orientation	0020,0020	CS		ANAP		
Icon Image Sequence	0088,0200	SQ		ANAP		
>Samples per Pixel	0028,0002	US		ALWAYS		
>Photometric Interpretation	0028,0004	CS		ALWAYS		
>Rows	0028,0010	US		ALWAYS		
>Columns	0028,0011	US		ALWAYS		
>Bits Allocated	0028,0100	US		ALWAYS		
>Bits Stored	0028,0101	US		ALWAYS		
>High Bit	0028,0102	US		ALWAYS		
>Pixel Representation	0028,0103	US		ALWAYS		
>Pixel Data	7FE0,0010	UN		ANAP		

Table 48: Image Pixel Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Rows	0028,0010	US		ALWAYS		
Columns	0028,0011	US		ALWAYS		
>Samples per Pixel	0028,0002	US		ALWAYS		
Photometric Interpretation	0028,0004	CS		ALWAYS		
Bits Allocated	0028,0100	US		ALWAYS		
Bits Stored	0028,0101	US		ALWAYS		
High Bit	0028,0102	US		ALWAYS		
Pixel Representation	0028,0103	US		ALWAYS		
Pixel Data	7FE0,0010	UN		ANAP		

Table 49: Cine Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Frame Time	0018,1063	DS		ANAP		

Table 50: Multi-Frame Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Number of Frames	0028,0008	IS		ALWAYS		
Frame Increment Pointer	0028,0009	AT		ALWAYS		

Table 51: X-Ray Image Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Image Type	0008,0008	CS		ALWAYS		
Samples per Pixel	0028,0002	US		ALWAYS		
Photometric Interpretation	0028,0004	CS		ALWAYS		
Frame Increment Pointer	0028,0009	AT		ANAP		
Bits Allocated	0028,0100	US		ALWAYS		
Bits Stored	0028,0101	US		ALWAYS		
High Bit	0028,0102	US		ALWAYS		
Pixel Representation	0028,0103	US		ALWAYS		
Pixel Intensity Relationship	0028,1040	CS		ALWAYS		

Table 52: X-Ray Acquisition Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
KVP	0018,0060	DS		VNAP		
Exposure Time	0018,1150	IS		ANAP		
X-Ray Tube Current	0018,1151	IS		ANAP		
Radiation Setting	0018,1155	CS		ALWAYS		

Table 53: XA Positioner Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Positioner Motion	0018,1500	CS		ANAP		
Positioner Primary Angle	0018,1510	DS		VNAP		
Positioner Secondary Angle	0018,1511	DS		VNAP		

Table 54: VOI LUT Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Window Center	0028,1050	DS		ANAP		
Window Width	0028,1051	DS		ANAP		

Table 55: SOP Common Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
SOP Class UID	0008,0016	UI	1.2.840.10008.5.1.4.1.1.12.1	ALWAYS		
SOP Instance UID	0008,0018	UI		ALWAYS		
Instance Number	0020,0013	IS		ANAP		

2.1.2.6. X-Ray 3D Angiographic Image Storage

Information Entity	Module	Presence Of Module
Patient	Patient Module	ALWAYS
Study	General Study Module	ALWAYS
Series	General Series Module	ALWAYS
	Enhanced Series Module	ALWAYS

Image	Frame Of Reference Module	ALWAYS
	General Equipment Module	ALWAYS
	Enhanced General Equipment Module	ALWAYS
	Image Pixel Module	ALWAYS
	Acquisition Context Module	ALWAYS
	Multi-frame Functional Groups Module	ALWAYS
	X-Ray 3D Image Module	ALWAYS
	X-Ray 3D Reconstruction Module	ALWAYS
	SOP Common Module	ALWAYS

Table 56: Patient Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Patient's Name	0010,0010	PN		VNAP		
Patient ID	0010,0020	LO		VNAP		
Patient's Birth Date	0010,0030	DA		VNAP		
Patient's Sex	0010,0040	CS		VNAP		

Table 57: General Study Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Study Date	0008,0020	DA		VNAP		
Study Time	0008,0030	TM		VNAP		
Accession Number	0008,0050	SH		VNAP		
Referring Physician's Name	0008,0090	PN		VNAP		
Study Instance UID	0020,000D	UI		ALWAYS		
Study ID	0020,0010	SH		VNAP		

Table 58: General Series Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Series Date	0008,0021	DA		ANAP		
Series Time	0008,0031	TM		ANAP		
Modality	0008,0060	CS	XA	ALWAYS		
Performing Physician's Name	0008,1050	PN		ANAP		
Related Series Sequence	0008,1250	SQ		ANAP		
>Study Instance UID	0020,000D	UI		ALWAYS		
>Series Instance UID	0020,000E	UI		ALWAYS		
>Purpose of Reference Code Sequence	0040,A170	SQ		VNAP		
Series Instance UID	0020,000E	UI		ALWAYS		
Laterality	0020,0060	CS		ANAP		
Performed Procedure Step Start Date	0040,0244	DA		ANAP		
Performed Procedure Step Start Time	0040,0245	TM		ANAP		
Performed Procedure Step ID	0040,0253	SH		ANAP		

Table 59: Enhanced Series Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Series Number	0020,0011	IS		ALWAYS		

Table 60: Frame of Reference Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Frame of Reference UID	0020,0052	UI		ALWAYS		
Position Reference Indicator	0020,1040	LO		VNAP		

Table 61: General Equipment Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Manufacturer	0008,0070	LO	Philips	VNAP		
Institution Name	0008,0080	LO		ANAP		
Station Name	0008,1010	SH		ANAP		
Manufacturer's Model Name	0008,1090	LO	Interventional Workspot	ANAP		
Device Serial Number	0018,1000	LO		ANAP		
Software Versions	0018,1020	LO	1.6.x	ANAP		where "x" is the detailed application SW version

Table 62: Enhanced General Equipment Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Manufacturer	0008,0070	LO	Philips	ALWAYS	FIXED	
Institution Name	0008,0080	LO		VNAP	COPY	copied from source data
Station Name	0008,1010	SH				
Manufacturer's Model Name	0008,1090	LO	Interventional Workspot	ALWAYS	CONFIG	
Device Serial Number	0018,1000					
Software Versions	0018,1020	LO	1.6.x	ALWAYS	CONFIG	where "x" is the detailed application SW version.

Table 63: Image Pixel Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Samples per Pixel	0028,0002	US		ALWAYS		
Photometric Interpretation	0028,0004	CS	MONOCHROME2	ALWAYS		
Rows	0028,0010	US		ALWAYS		
Columns	0028,0011	US		ALWAYS		
Bits Allocated	0028,0100	US		ALWAYS		
Bits Stored	0028,0101	US		ALWAYS		
High Bit	0028,0102	US		ALWAYS		
Pixel Representation	0028,0103	US		ALWAYS		
Pixel Data	7FE0,0010	UN		ANAP		

Table 64: Acquisition Context Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Acquisition Context Sequence	0040,0555	SQ		VNAP		
Concept Name Code Sequence	0040,A043	SQ		ALWAYS		

Table 65: Multi-frame Functional Groups Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Content Date	0008,0023	DA		ALWAYS		

Content Time	0008,0033	TM		ALWAYS		
Instance Number	0020,0013	IS		ALWAYS		
Number of Frames	0028,0008	IS		ALWAYS		
Shared Functional Groups Sequence	5200,9229	SQ		VNAP		
>Pixel Measures Sequence	0028,9110	SQ		ALWAYS		
>>Slice Thickness	0018,0050	DS		ALWAYS		
>>Pixel Spacing	0028,0030	DS		ALWAYS		
>Frame Anatomy Sequence	0020,9071	SQ		ALWAYS		
>>Frame Laterality	0020,9072	CS		ALWAYS		
>>Anatomic Region Sequence	0008,2218	SQ		ALWAYS		
>>>Code Value	0008,0100	SH		ALWAYS		
>>>Coding Scheme Designator	0008,0102	SH		ALWAYS		
>>>Code Meaning	0008,0104	LO		ALWAYS		
Per-frame Functional Groups Sequence	5200,9230	SQ		ALWAYS		
>Frame Content Sequence	0020,9111	SQ		ALWAYS		
>Plane Position Sequence	0020,9113	SQ		ALWAYS		
>>Image Position (Patient)	0020,0032	DS		ANAP		
>Plane Orientation Sequence	0020,9116	SQ		ALWAYS		
>>Image Orientation (Patient)	0020,0037	DS		ANAP		
>Derivation Image Sequence	0008,9124	SQ		ANAP		
>>Source Image Sequence	0008,2112	SQ		VNAP		
>>Derivation Code Sequence	0008,9215	SQ		ALWAYS		
>>>Code Value	0008,0100	SH		ALWAYS		
>>>Coding Scheme Designator	0008,0102	SH		ALWAYS		
>>>Code Meaning	0008,0104	LO		ALWAYS		
>Frame VOI LUT Sequence	0028,9132	SQ		ALWAYS		
>>Window Center	0028,1050	DS		ALWAYS		
>>Window Width	0028,1051	DS		ALWAYS		
>X-Ray 3D Frame Type Sequence	0018,9504	SQ		ANAP		
>>Frame Type	0008,9007	CS	DERIVED\PRIMARY\ VOLUME\NONE	ALWAYS		
>>Reconstruction Index	0020,9536	US		ALWAYS		
>>Pixel Presentation	0008,9205	CS	MONOCHROME	ALWAYS		
>>Volumetric Properties	0008,9206	CS	VOLUME	ALWAYS		
>>Volume Based Calculation Technique	0008,9207	CS	NONE	ALWAYS		

Table 66: X-Ray 3D Image Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Image Type	0008,0008	CS	DERIVED\SECONDARY\ AXIAL\3DRA_PROP	ALWAYS		
Content Qualification	0018,9004	CS	PRODUCT	ALWAYS		
Samples per Pixel	0028,0002	US		ALWAYS		
Photometric Interpretation	0028,0004	CS	MONOCHROME2	ALWAYS		
Bits Allocated	0028,0100	US		ALWAYS		
Bits Stored	0028,0101	US		ALWAYS		
High Bit	0028,0102	US		ALWAYS		
Burned In Annotation	0028,0301	CS	NO	ALWAYS		
Lossy Image Compression	0028,2110	CS	00	ALWAYS		
Icon Image Sequence	0088,0200	SQ		ANAP		

>Samples per Pixel	0028,0002	US		ALWAYS		
>Photometric Interpretation	0028,0004	CS	MONOCHROME2	ALWAYS		
>ROWS	0028,0010	US		ALWAYS		
>COLUMNS	0028,0011	US		ALWAYS		
>Bits Allocated	0028,0100	US		ALWAYS		
>Bits Stored	0028,0101	US		ALWAYS		
>High Bit	0028,0102	US		ALWAYS		
>Pixel Presentation	0008,9205	CS	MONOCHROME	ALWAYS		
>Pixel Data	7FE0,0010	OB		ALWAYS		
Presentation LUT Shape	2050,0020	CS	IDENTITY	ALWAYS		
Pixel Presentation	0008,9205	CS	MONOCHROME	ALWAYS		
Volumetric Properties	0008,9206	CS	VOLUME	ALWAYS		
Volume Based Calculation Technique	0008,9207	CS	NONE	ALWAYS		

Table 67: X-Ray 3D Reconstruction Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
X-Ray 3D Reconstruction Sequence	0018,9530	SQ		ALWAYS		
>Application Name	0018,9524	LO	Interventional Workspot	ALWAYS		
>Application Version	0018,9525	LO	1.6.0	ALWAYS		
>Application Manufacturer	0018,9526	LO	Philips	ALWAYS		
>Algorithm Type	0018,9527	CS	FILTER_BACK_PROJ	ALWAYS		
>Acquisition Index	0020,9518	US	1	ALWAYS		

Table 68: SOP Common Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Specific Character Set	0008,0005	CS		ALWAYS		As supported by hosting platform
SOP Class UID	0008,0016	UI	1.2.840.10008.5.1.4.1.1.13.1.1	ALWAYS	FIXED	
SOP Instance UID	0008,0018	UI		ALWAYS	COPY	copied from source data
Instance Creation Date	0008,0012	DA		ANAP	COPY	copied from source data
Instance Creation Time	0008,0013	TM		ANAP	COPY	copied from source data
Instance Number	0020,0013	IS		ANAP		

2.1.2.7. Raw data Storage SOP class

Table 69: IOD of Created Raw Data Storage SOP Class Instances

Information Entity	Module	Presence Of Module
Patient	Patient Module	ALWAYS
Study	General Study Module	ALWAYS
Series	General Series Module	ALWAYS
Frame of Reference	Frame of Reference	OPTIONAL
Equipment	General Equipment Module	ALWAYS
Image	Acquisition Context Module	ALWAYS
	Raw Data Module	ALWAYS

SOP Common Module

ALWAYS

Table 70 : Patient Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Patient's Name	0010,0010	PN		ALWAYS	COPY	copied from source data
Patient ID	0010,0020	LO		ALWAYS	COPY	copied from source data
Patient's Birth Date	0010,0030	DA		VNAP	COPY	copied from source data
Patient's Sex	0010,0040	CS		ALWAYS	COPY	copied from source data

Table 71 : General Study Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Study Date	0008,0020	DA		ALWAYS	COPY	copied from source data
Study Time	0008,0030	TM		ALWAYS	COPY	copied from source data
Referring Physician's Name	0008,0090	PN		VNAP	COPY	copied from source data
Study Instance UID	0020,000D	UI		ALWAYS	COPY	copied from source data
Study ID	0020,0010	SH		ALWAYS	COPY	copied from source data
Accession Number	0008,0050	SH		EMPTY	COPY, USER	copied from source data

Table 72 : General Series Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Series Date	0008,0021	DA		ANAP	COPY	copied from source data
Series Time	0008,0031	TM		ANAP	COPY	copied from source data
Modality	0008,0060	CS		ALWAYS	COPY	copied from source data
Series Description	0008,103E	LO		ANAP		
Performing Physicians' name	0008,1050	PN		ANAP		
Related Series Sequence	0008,1250	SQ		ANAP		
>Study Instance UID	0020,000D	UI		ALWAYS		
>Series Instance UID	0020,000E	UI		ALWAYS	COPY	copied from source data
>Purpose of Reference Code Sequence	0040,A170	SQ		VNAP		
Series Instance UID	0020,000E	UI		ALWAYS		
Series Number	0020,0011	IS		VNAP	COPY	copied from source data
Laterality	0020,0060	CS		ANAP		
Performed Procedure Step Start Date	0040,0244	DA		ANAP		
Performed Procedure Step Start Time	0040,0245	TM		ANAP		

Performed Procedure Step ID	0040,0253	SH		ANAP		
-----------------------------	-----------	----	--	------	--	--

Table 73: Frame of Reference Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Frame of Reference UID	0020,0052	UI		ALWAYS	COPY	copied from source data
Position Reference Indicator	0020,1040	LO		VNAP	COPY	copied from source data

Table 74: General Equipment Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Manufacturer	0008,0070	LO	Philips	ALWAYS	FIXED	
Institution Name	0008,0080	LO		VNAP	COPY	copied from source data
Station Name	0008,1010	SH				
Manufacturer's Model Name	0008,1090	LO	Interventional Workspot	ALWAYS	CONFIG	
Device Serial Number	0018,1000					
Software Versions	0018,1020	LO	1.6.x	ALWAYS	CONFIG	where "x" is the detailed application SW version.

Table 75: Acquisition Context Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Acquisition Context Sequence	0040,0555	SQ		VNAP	COPY	copied from source data

Table 76: Raw Data Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
Content Date	0008,0023	DA		ALWAYS	COPY	copied from source data
Content Time	0008,0033	TM		ALWAYS	COPY	copied from source data
Creator Version UID	0008,9123	UI		ALWAYS	COPY	copied from source data
Instance Number	0020,0013	IS		ANAP	COPY	copied from source data

Table 77: SOP Common Module

Attribute Name	Tag	VR	Value	Presence of Value	Source	Comment
SOP Class UID	0008,0016	UI	1.2.840.10008.5.1.4.1.1.66	ALWAYS	COPY	copied from source data
SOP Instance UID	0008,0018	UI		ALWAYS	COPY	copied from source data
Original Specialized SOP Class UID	0008,001B	UI		VNAP	COPY	copied from source data
Instance Creation Date	0008,0012	DA		VNAP	COPY	copied from source data

Instance Creation Time	0008,0013	TM		VNAP	COPY	copied from source data
Instance Number	0020,0013	IS		VNAP		