


# Precedence


## Preferred Room Layout

The layout shown below is based upon a typical equipment configuration and should be considered as a general design guideline. Site conditions, application requirements, customer preferences, and/or equipment configuration may significantly impact suite design and equipment layout. It is recommended to request site-specific drawings from a Philips representative early in the design process.

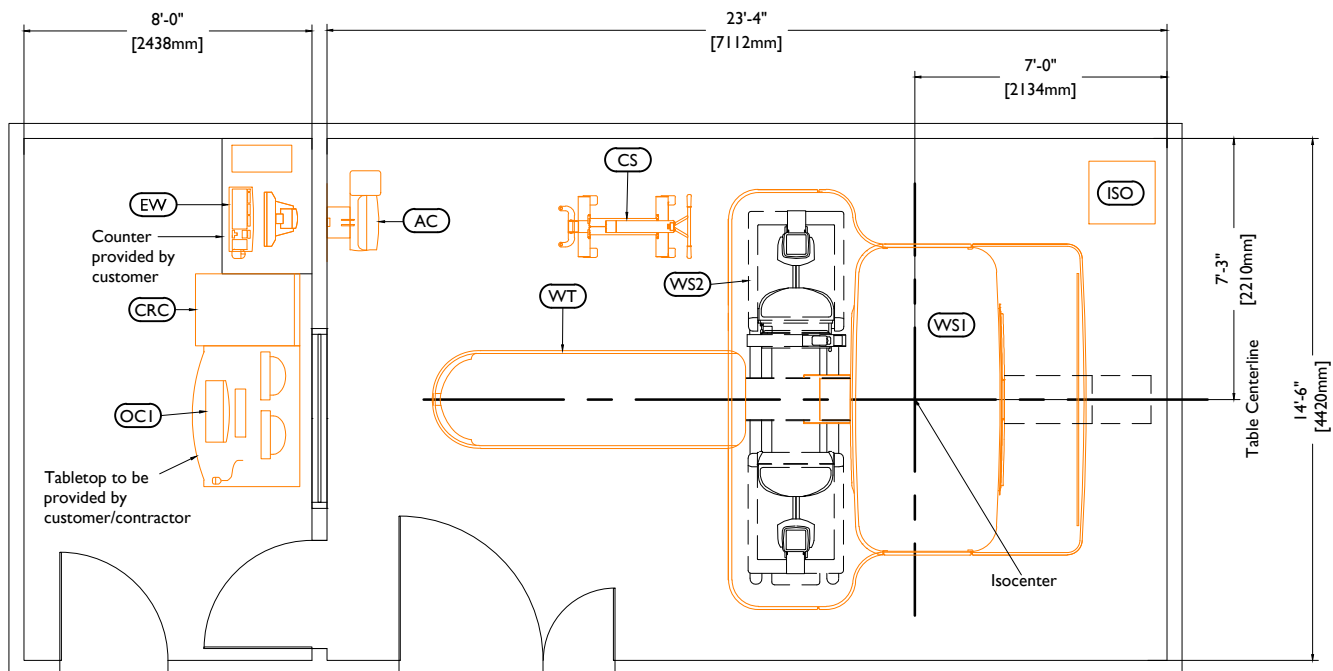

## Equipment Layout

Recommended Ceiling Height: 9'-6" (2896mm)



Equipment Legend

- A Furnished and installed by Philips
- B Furnished by customer/contractor and installed by customer/contractor
- C Installed by customer/contractor
- D Furnished by Philips and installed by contractor
- E Existing
- F Future
- G Optional item furnished by Philips

Equipment Designation

|   |       | Description                                | Weight<br>lbs [kg] | Heat Load<br>Btu/hr [W] |
|---|-------|--|--------------------|-------------------------|
| A | (WS1) | CT Scanner Gantry                          | 3295[1495]         | 23000[6741]             |
| A | (WS2) | SPECT Scanner Gantry                       | 5700[2586]         | 7000[2052]              |
| A | (WT)  | Patient Table                              | 900[409]           | -                       |
| A | (OCI) | Acquisition Station                        | 45 [20]            | 3572 [1046]             |
| A | (CRC) | CIRS Recon / COM Cabinet                   | 269 [122]          | -                       |
| A | (AC)  | Acquisition Terminal (wall mounted)        | 30[14]             | -                       |
| A | (CS)  | Collimator Server/Storer                   | 155[71]            | -                       |
| G | (EW)  | Extended Brilliance Workspace              | 90 [41]            | 1000 [293]              |
| D | (ISO) | Teal MCT 100 / 480 Isotran Plus Power Unit | 697 [316]          | 1950 [572]              |

## Environmental Requirements for General Equipment Locations

Operating temperature range within the CT Exam Room is 64°-75° F (18°-24° C) [ideal stable room temperature setting: 72° F (22° C)] at 35% to 70% relative humidity (non-condensing). Operating temperature change per hour throughout the CT Exam Room must not exceed 7.5° F (4.1° C).

Operating temperature range throughout the rest of the CT Suite is 59°-75° F (15°-24° C) [ideal stable room temperature setting: 72° F (22° C)] at 35% to 70% relative humidity (non-condensing). Operating temperature change per hour throughout the CT Suite must not exceed 9° F (5° C).

The above conditions must be maintained at all times including overnight, weekends, and holidays. Heat output in one area of the CT Suite must not affect temperature and humidity in other areas. It is strongly recommended that any definable areas within the suite, i.e. equipment closets, control areas, etc. (if applicable), be individually environmentally controlled as required to meet the ambient ranges specified.

## Power Requirements

|                        |  |
|------------------------|--|
| Supply Configuration:  | 3 phase Wye, 3 wire power, Earth 1 & 2, and neutral<br>(with Philips Line Filter/TVS Device) |
| Supply Configuration:  | 3 phase, 3 wire power, Earth<br>(with all other Philips approved power devices)              |
| Nominal Line Voltage:  | 480 VAC (+/- 10%), 50/60 Hz (+/- 3 Hz)   |
| Branch Power Capacity: | 112.5 kVA  |

## Remote Service Diagnostics

Medical Imaging equipment to be installed by Philips is equipped with a service diagnostic feature which allows for remote and on-site service diagnostics. To establish this feature, a RJ45 type Ethernet 10/100/1000 Mbit network connector must be installed. Access to customer's network via their remote access server is needed for Remote Service Network (RSN) connectivity. All costs with this feature are the responsibility of the customer.



© Koninklijke Philips Electronics N.V. 2011.  
All rights reserved.

Reproduction in whole or in part is  
prohibited without prior written consent of  
the copyright holder.

Rev. 11.00